

User: Galos, Marie
 Westchester Dept. of Labs & Research
 Date: 02/05/2002 Time: 11:39:58

Sample: AD31339
 Analysis: \$B1GCMS Blank for GCMS Scan
 Units: ug
 Started: 2/5/02 11:34 Ended: 2/5/02 11:34 Analyst: MG
 Result source: manual entry
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	n-Nitrosodimethylamine		< MDL		2.0
2	bis(2-Chloroethyl)ether		< MDL		2.0
3	1,3-Dichlorobenzene		< MDL		2.0
4	1,4-Dichlorobenzene		< MDL		2.0
5	1,2-Dichlorobenzene		< MDL		2.0
6	2,2'-oxybis(1-Chloropropane)		< MDL		2.0
7	n-Nitrosodi-n-propylamine		< MDL		2.0
8	Hexachloroethane		< MDL		2.0
9	Nitrobenzene		< MDL		2.0
10	Isophorone		< MDL		2.0
11	bis(2-Chloroethoxy)methane		< MDL		2.0
12	1,2,4-Trichlorobenzene		< MDL		2.0
13	Naphthalene		< MDL		2.0
14	Hexachlorobutadiene		< MDL		2.0
15	2-Chloronaphthalene		< MDL		2.0
16	Dimethylphthalate		< MDL		2.0
17	2,6-Dinitrotoluene		< MDL		2.0
18	Acenaphthylene		< MDL		2.0
19	Acenaphthene		< MDL		2.0
20	2,4-Dinitrotoluene		< MDL		2.0
21	Diethylphthalate		< MDL		2.0
22	4-Chlorophenylphenylether		< MDL		2.0
23	Fluorene		< MDL		2.0
24	Azobenzene/1,2-Diphenylhydraz		< MDL		2.0
25	n-Nitrosodiphenylamine		< MDL		2.0
26	4-Bromophenylphenylether		< MDL		2.0
27	Hexachlorobenzene		< MDL		2.0
28	Phenanthrene		< MDL		2.0
29	Anthracene		< MDL		2.0
30	Di-n-butylphthalate		< MDL		2.0
31	Fluoranthene		< MDL		2.0
32	Pyrene		< MDL		2.0
33	Butylbenzylphthalate		< MDL		2.0
34	Benzo(a)anthracene		< MDL		2.0
35	bis(2-Ethylhexyl)phthalate		< MDL		2.0
36	Chrysene		< MDL		2.0
37	Di-n-octylphthalate		< MDL		2.0
38	Benzo(b)fluoranthene		< MDL		2.0
39	Benzo(k)fluoranthene		< MDL		2.0
40	Benzo(a)pyrene		< MDL		2.0
41	Indeno(1,2,3-cd)pyrene		< MDL		2.0
42	Dibenz(a,h)anthracene		< MDL		2.0
43	Benzo(g,h,i)perylene		< MDL		2.0

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\JAN1502\LB.D

Vial: 4

Acq On : 15 Jan 2002 12:52 pm

Operator: 209 GALOS

Sample : gc/ms scan 12/26

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Feb 4 12:44 2002

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Tue Jan 22 11:56:23 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0103

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.50	152	657921	20.00	ug/l	-0.20
10) Naphthalene-d8	15.09	136	2553190	20.00	ug/l	-0.22
17) Acenaphthene-d10	20.36	164	1265310	20.00	ug/l	-0.22
29) Phenanthrene-d10	24.78	188	1684798	20.00	ug/l	-0.22
38) Chrysene-d12	32.80	240	990098	20.00	ug/l	-0.23
44) Perylene-d12	36.87	264	600275	20.00	ug/l	-0.25

System Monitoring Compounds

37) 2,4-DDD	29.85	235	93732	5.06	ug/mL	-0.22
Spiked Amount	5.000		Recovery	=	101.20%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	5.18	74	270	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.15	128	1919	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	21.88	149	100	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	

(#)=qualifier out of range (m)=manual integration

LB.D GCMS1126.M Mon Feb 04 12:45:36 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\JAN1502\LB.D
 Acq On : 15 Jan 2002 12:52 pm
 Sample : gc/ms scan 12/26
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Feb 4 12:44 2002

Vial: 4
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Tue Jan 22 11:56:23 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0103

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	24.85	178	356	N.D.		
34) Anthracene	24.85	178	356	N.D.		
35) Di-n-butylphthalate	26.80	149	9480	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	32.80	228	2530	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.10	149	1784	N.D.		
43) Chrysene	32.80	228	2530	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	36.88	252	2450	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

 (#) = qualifier out of range (m) = manual integration

LB.D GCMS1126.M Mon Feb 04 12:45:39 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\JAN1502\LB.D
 Acq On : 15 Jan 2002 12:52 pm
 Sample : gc/ms scan 12/26
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Feb 4 12:44 2002

Vial: 4
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: GCMS1126.RES

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Tue Jan 22 11:56:23 2002
 Response via : Initial Calibration

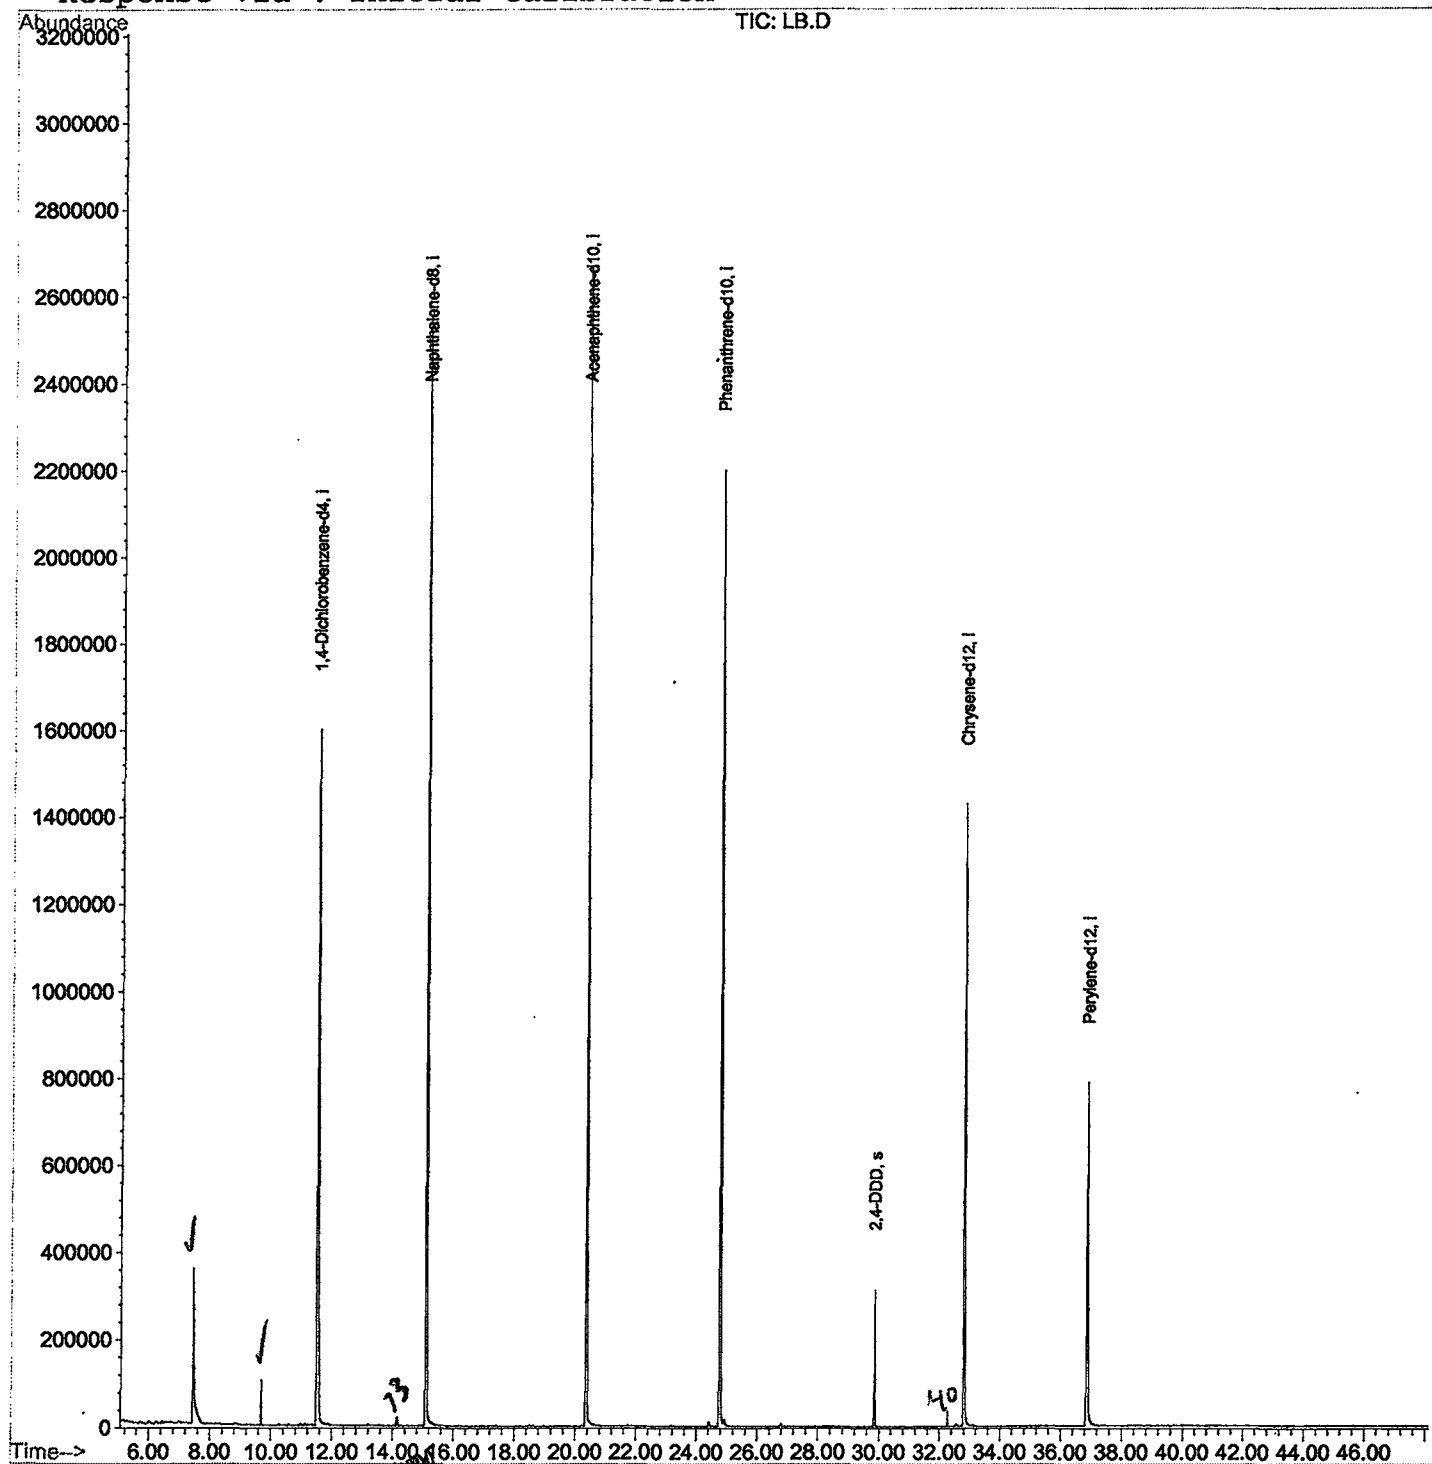

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\JAN1502\LB.D

Acq On : 15 Jan 2002 12:52 pm

Sample : gc/ms scan 12/26

Misc :

MS Integration Params: LSCINT.P

Vial: 4

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	7.443	257	261	298	rVB	353567	1091558	20.27%	4.069%
2	9.683	504	505	507	rBV	102981	57964	1.08%	0.216%
3	11.501	698	703	723	rBV	1597248	4194733	77.91%	15.636%
4	15.091	1089	1094	1114	rBV	2545972	5281774	98.10%	19.688%
5	20.360	1662	1668	1688	rBV	2666039	5383886	100.00%	20.069%
6	24.776	2142	2149	2159	rBV2	2198773	4784491	88.87%	17.834%
7	29.853	2697	2702	2710	rBV	311693	581889	10.81%	2.169%
8	32.799	3017	3023	3044	rBV2	1426711	3221735	59.84%	12.009%
9	36.866	3458	3466	3483	rBV2	786305	2229346	41.41%	8.310%


Sum of corrected areas: 26827376

LB.D GCMS1126.M

Mon Feb 04 15:12:18 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\JAN1502\LB.D
 Operator : 209 GALOS
 Acquired : 15 Jan 2002 12:52 pm using AcqMethod GCMS0103
 Instrument : GC/MS 209
 Sample Name: gc/ms scan 12/26
 Misc Info :
 Vial Number: 4
 Quant File :GCMS1126.RES (RTE Integrator)

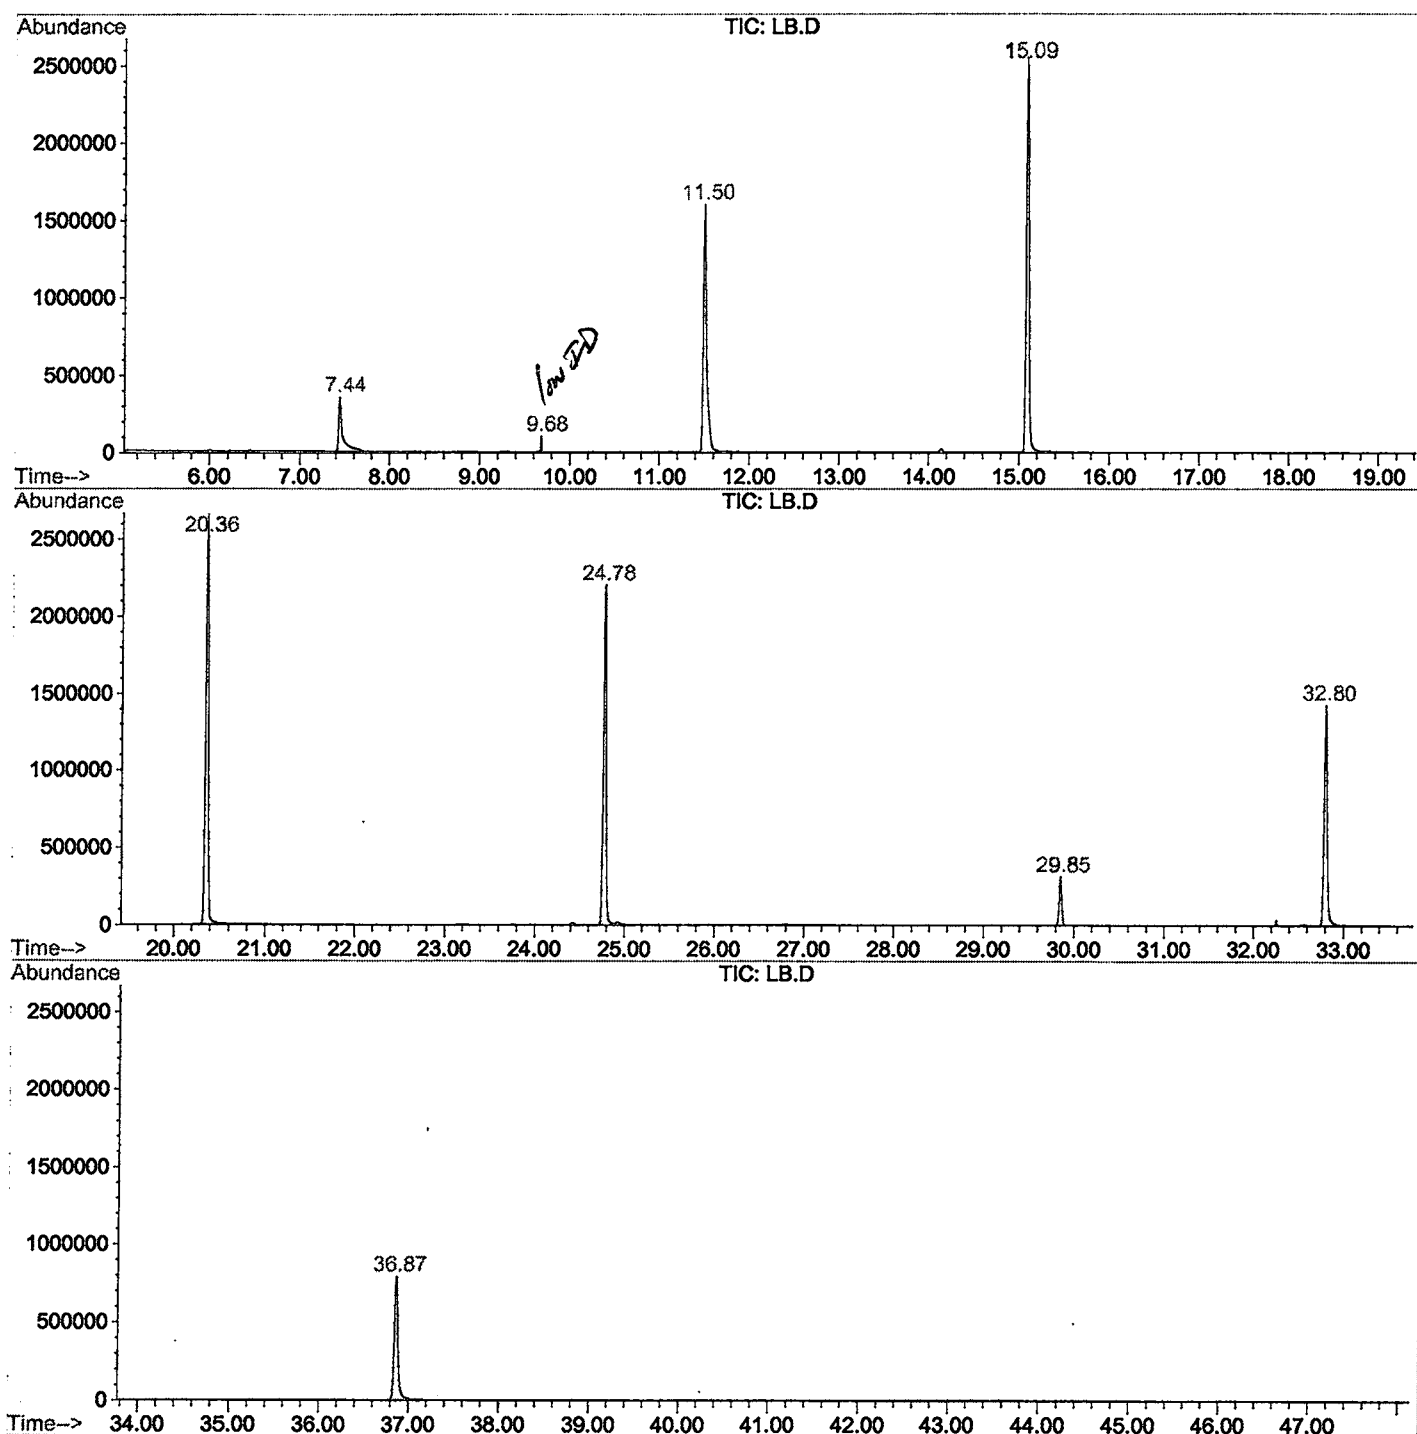

LB.D GCMS1126.M

Mon Feb 04 15:12:24 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\JAN1502\LB.D
Acq On : 15 Jan 2002 12:52 pm
Sample : gc/ms scan 12/26
Misc :
MS Integration Params: LSCINT.P



Vial: 4
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L


Peak Number 1 1-Butanamine, 3-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.44	5.20 ug/l	1091560	1,4-Dichlorobenzene-d4	11.50


Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Butanamine, 3-methyl-	87	C5H13N	000107-85-7	9
2			N-Ethylformamide	73	C3H7NO	000627-45-2	9
3			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	9
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	9

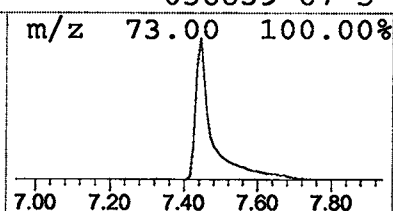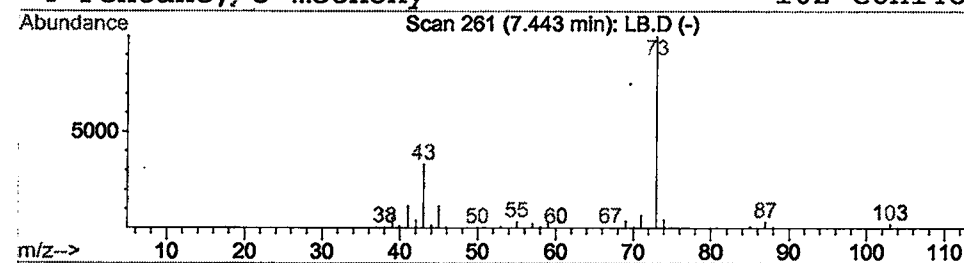


m/z 43.00 33.10%

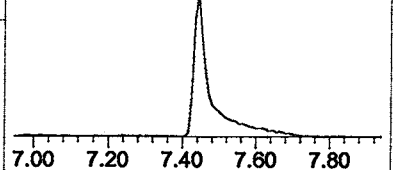





m/z 41.00 11.51%

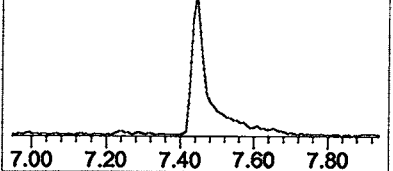

m/z 44.95 11.51%

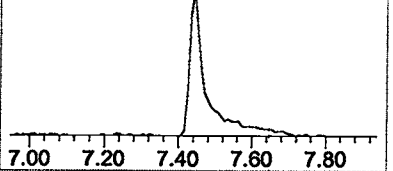

m/z 71.00 6.97%

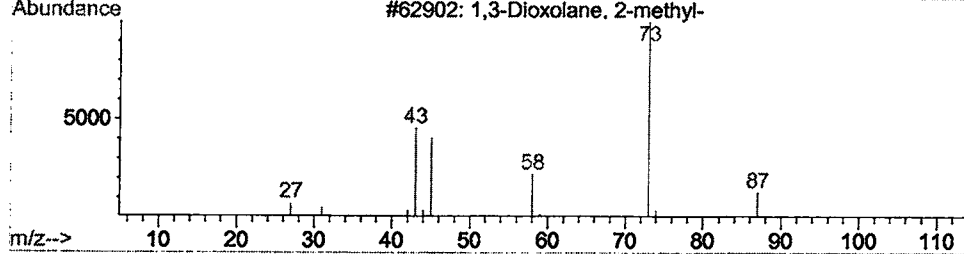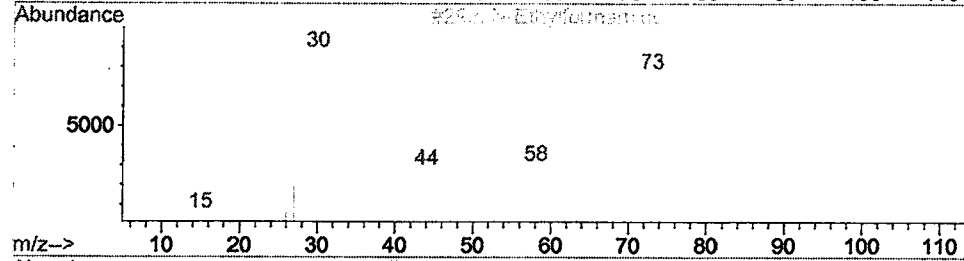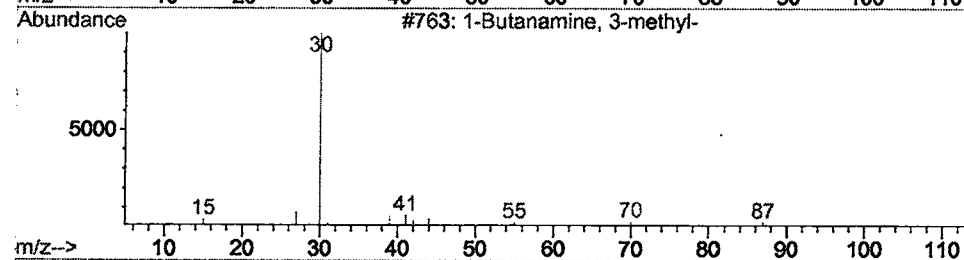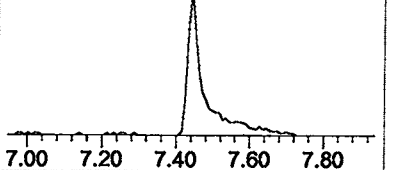

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\JAN1502\LB.D
 Acq On : 15 Jan 2002 12:52 pm
 Sample : gc/ms scan 12/26
 Misc :
 MS Integration Params: LSCINT.P


Vial: 4
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 2 Ethylene oxide Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.68	0.28 ug/l	57964	1,4-Dichlorobenzene-d4	11.50

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Ethylene oxide	44	C2H4O	000075-21-8	3
2		Acetaldehyde	44	C2H4O	000075-07-0	3
3		Propane	44	C3H8	000074-98-6	1
4		Carbanic acid, monoammonium salt	78	CH6N2O2	001111-78-0	1

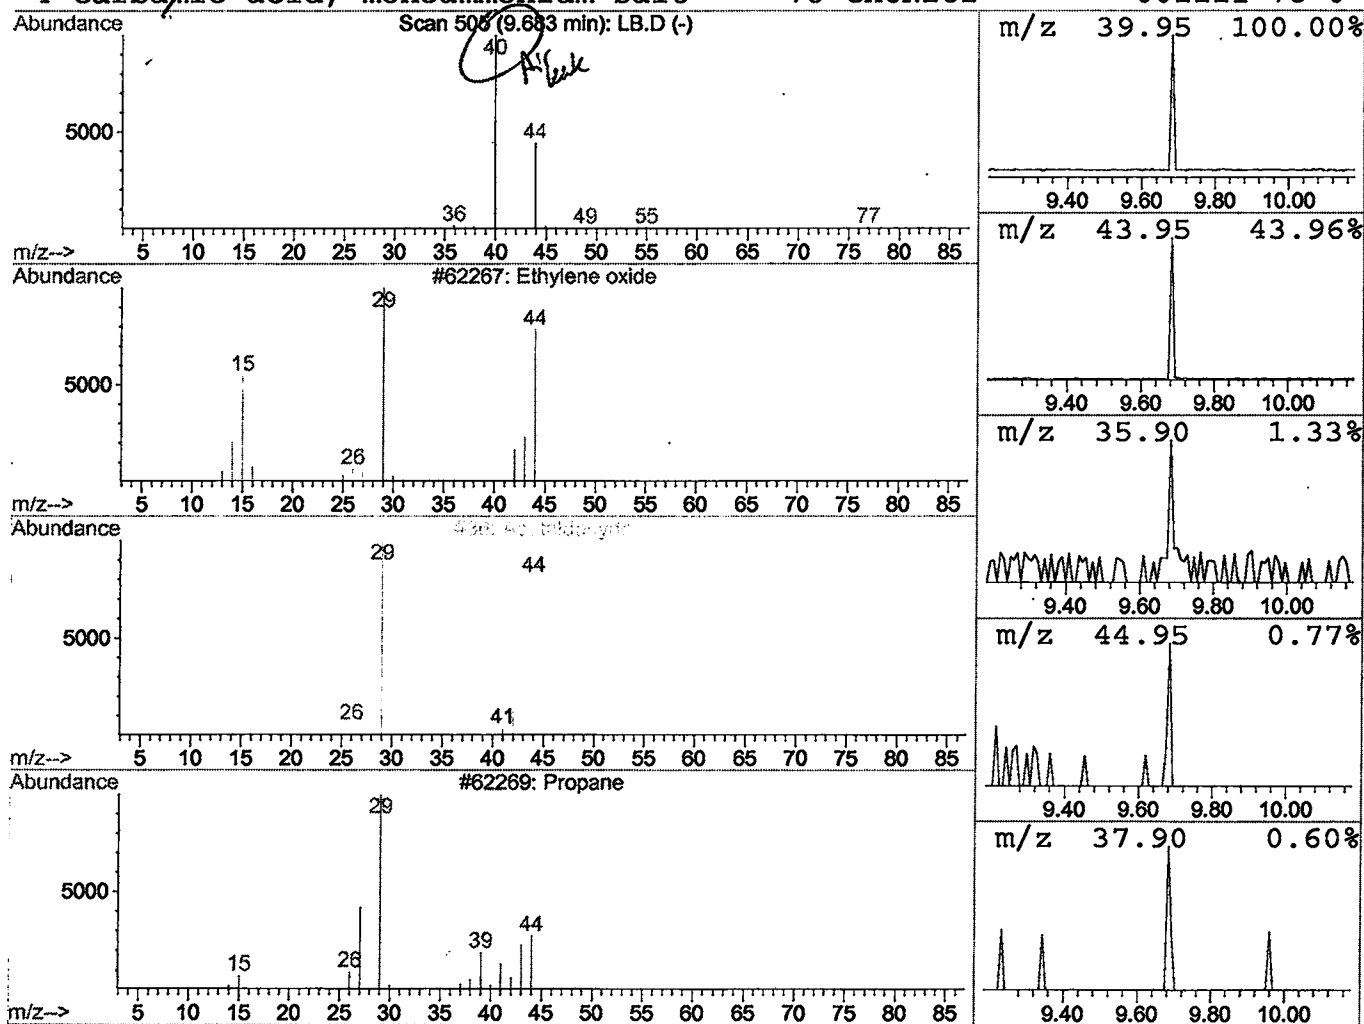

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 15 Jan 2002 12:52 pm
Data File: C:\HPCHEM\1\DATA\JAN1502\LB.D
Name: gc/ms scan 12/26
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
1-Butanamine, 3-meth	7.44	5.2	ug/l	1091560	ISTD01	11.50	4194730	20.0
Ethylene oxide	9.68	0.3	ug/l	57964	ISTD01	11.50	4194730	20.0

LB.D GCMS1126.M Mon Feb 04 15:12:38 2002