

Sequence Name: C:\HPCHEM\1\SEQUENCE\JAN1602.S

Comment: INST 209; 30Mx0.25umX0.50

Operator: 209 GALOS

Data Path: C:\HPCHEM\1\data\jan1602\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

☒ Full Method☐ Reprocessing Only

On A Barcode Mismatch

☒ Inject Anyway☐ Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
------	------	------	----------	--------	-------------

1	Sample	2	CAL10	GCMS0103	
2	Sample	4	LB	GCMS0103	gc/ms scan 12/27
3	Sample	5	REF	GCMS0103	gc/ms scan 12/27
4	Sample	6	31458	GCMS0103	gc/ms scan 12/27
5	Sample	7	31407	GCMS0103	gc/ms scan 12/27
6	Sample	8	31363	GCMS0103	gc/ms scan 12/27
7	Sample	9	31404	GCMS0103	gc/ms scan 12/27
8	Sample	10	31456	GCMS0103	gc/ms scan 12/27
9	Sample	11	31405	GCMS0103	gc/ms scan 12/27
10	Sample	12	31340	GCMS0103	gc/ms scan 12/27
11	Sample	13	31406	GCMS0103	gc/ms scan 12/27
12	Sample	14	31457	GCMS0103	gc/ms scan 12/27
13	Sample	15	31459	GCMS0103	gc/ms scan 12/27
14	Sample	16	31364	GCMS0103	gc/ms scan 12/27
15	Sample	17	LBA	GCMS0103	gc/ms scan 12/28
16	Sample	18	REFA	GCMS0103	gc/ms scan 12/28
17	Sample	19	31402	GCMS0103	gc/ms scan 12/28
18	Sample	20	31408	GCMS0103	gc/ms scan 12/28
19	Sample	21	31434	GCMS0103	gc/ms scan 12/28
20	Sample	22	31463	GCMS0103	gc/ms scan 12/28
21	Sample	23	31460	GCMS0103	gc/ms scan 12/28
22	Sample	24	31401	GCMS0103	gc/ms scan 12/28
23	Sample	1	DFTPP	GCMS0103	
24	Sample	25	31466	GCMS0103	gc/ms scan 12/28
25	Sample	26	31467	GCMS0103	gc/ms scan 12/28
26	Sample	27	31462	GCMS0103	gc/ms scan 12/28
27	Sample	28	31465	GCMS0103	gc/ms scan 12/28
28	Sample	29	31461	GCMS0103	gc/ms scan 12/28
29	Sample	2	CAL40	GCMS0103	

DFTPP

Data File : C:\HPCHEM\1\DATA\JAN1602\DFTPP.D

Acq On : 17 Jan 2002 11:06 am

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0103.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

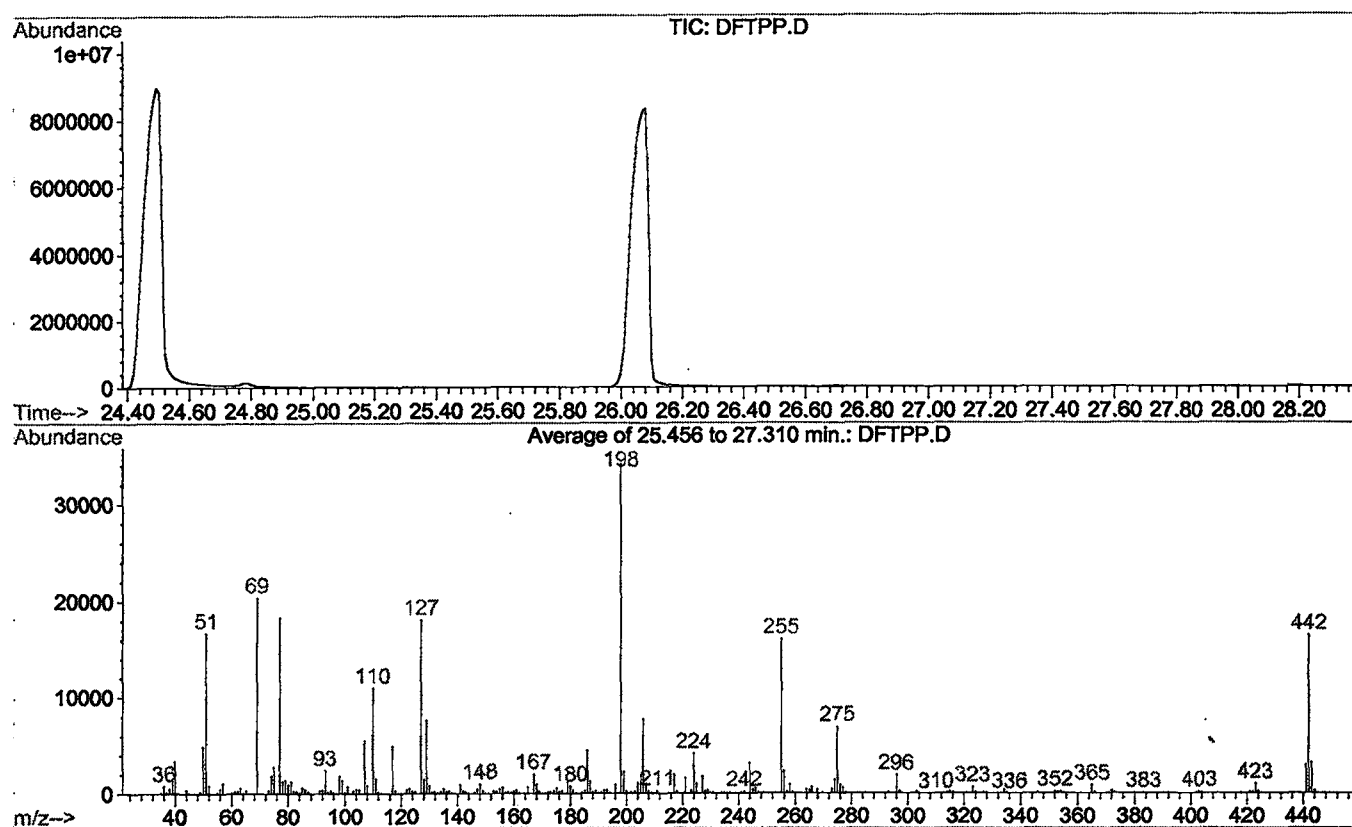

Spectrum Information: Average of 25.456 to 27.310 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	49.1	16758	PASS
68	69	0.00	2	0.0	3	PASS
69	198	0.00	100	59.9	20436	PASS
70	69	0.00	2	0.1	16	PASS
127	198	40	60	53.2	18135	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	34097	PASS
199	198	5	9	6.7	2275	PASS
275	198	10	30	20.3	6912	PASS
365	198	1	100	2.6	882	PASS
441	443	0.01	100	93.8	2971	PASS
442	198	40	110	48.3	16461	PASS
443	442	17	23	19.3	3169	PASS

DFTPP.D GCMS0103.M

Thu Feb 07 10:35:36 2002