

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 02/11/2002 Time: 17:31:46

Sample: AD31462
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 2/11/02 17:31 Ended: 2/11/02 17:31 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		85		5.0

Comments for Sample AD31462 - Analysis \$GCMS

Westchester Dept. of Labs & Research
User: Vinci, David L
Date: 02-11-2002 Time: 17:31:54

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

The recoveries for 3 of the 43 compounds in the LCS Standard were above their acceptance ranges.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\JAN1602\31462.D

Vial: 27

Acq On : 17 Jan 2002 2:02 pm

Operator: 209 GALOS

Sample : gc/ms scan 12/28

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Feb 7 12:21 2002

Quant Results File: GCMS0103.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0103.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Mon Jan 07 10:31:02 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0103

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.50	152	786686	20.00	ug/l	-0.02
10) Naphthalene-d8	15.09	136	3075516	20.00	ug/l	-0.02
17) Acenaphthene-d10	20.35	164	1542778	20.00	ug/l	-0.03
29) Phenanthrene-d10	24.77	188	2177542	20.00	ug/l	-0.03
38) Chrysene-d12	32.80	240	1409446	20.00	ug/l	-0.03
44) Perylene-d12	36.87	264	947350	20.00	ug/l	-0.02

System Monitoring Compounds

37) 2,4-DDD	29.86	235	106163	4.25	ug/mL	-0.21
Spiked Amount	5.000		Recovery	=	85.00%	

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.		
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.		
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.		
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.		
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.		
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.		
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.		
9) Hexachloroethane	0.00	117	0	N.D.		
11) Nitrobenzene	0.00	77	0	N.D.		
12) Isophorone	0.00	82	0	N.D.		
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.		
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
15) Naphthalene	15.15	128	1257	N.D.		
16) Hexachlorobutadiene	0.00	225	0	N.D.		
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
19) 2-Chloronaphthalene	0.00	162	0	N.D.		
20) Dimethylphthalate	0.00	163	0	N.D.		
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d	
22) Acenaphthylene	0.00	152	0	N.D.		
23) Acenaphthene	0.00	153	0	N.D.		
24) 2,4-Dinitrotoluene	20.76	165	208	N.D.		
25) Diethylphthalate	21.90	149	343	N.D.		
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.		
27) Fluorene	0.00	166	0	N.D.		
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.		

(#)=qualifier out of range (m)=manual integration

31462.D GCMS0103.M

Thu Feb 07 12:22:12 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\JAN1602\31462.D

Vial: 27

Acq On : 17 Jan 2002 2:02 pm

Operator: 209 GALOS

Sample : gc/ms scan 12/28

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Feb 7 12:21 2002

Quant Results File: GCMS0103.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0103.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Mon Jan 07 10:31:02 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0103

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	24.83	178	200	N.D.		
34) Anthracene	24.83	178	200	N.D.		
35) Di-n-butylphthalate	26.80	149	4068	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	32.80	228	3742	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.11	149	9525	N.D.		
43) Chrysene	32.80	228	3742	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	36.87	252	4177	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

 (#) = qualifier out of range (m) = manual integration

31462.D GCMS0103.M

Thu Feb 07 12:22:16 2002


Page 2

Quantitation Report

Data File : C:\HPCHEM\1\DATA\JAN1602\31462.D
Acq On : 17 Jan 2002 2:02 pm
Sample : gc/ms scan 12/28
Misc :
MS Integration Params: GOOFY.P
Quant Time: Feb 7 12:21 2002

Vial: 27
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00
Quant Results File: GCMS0103.RES

Method : C:\HPCHEM\1\METHODS\GCMS0103.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Mon Jan 07 10:31:02 2002
Response via : Initial Calibration

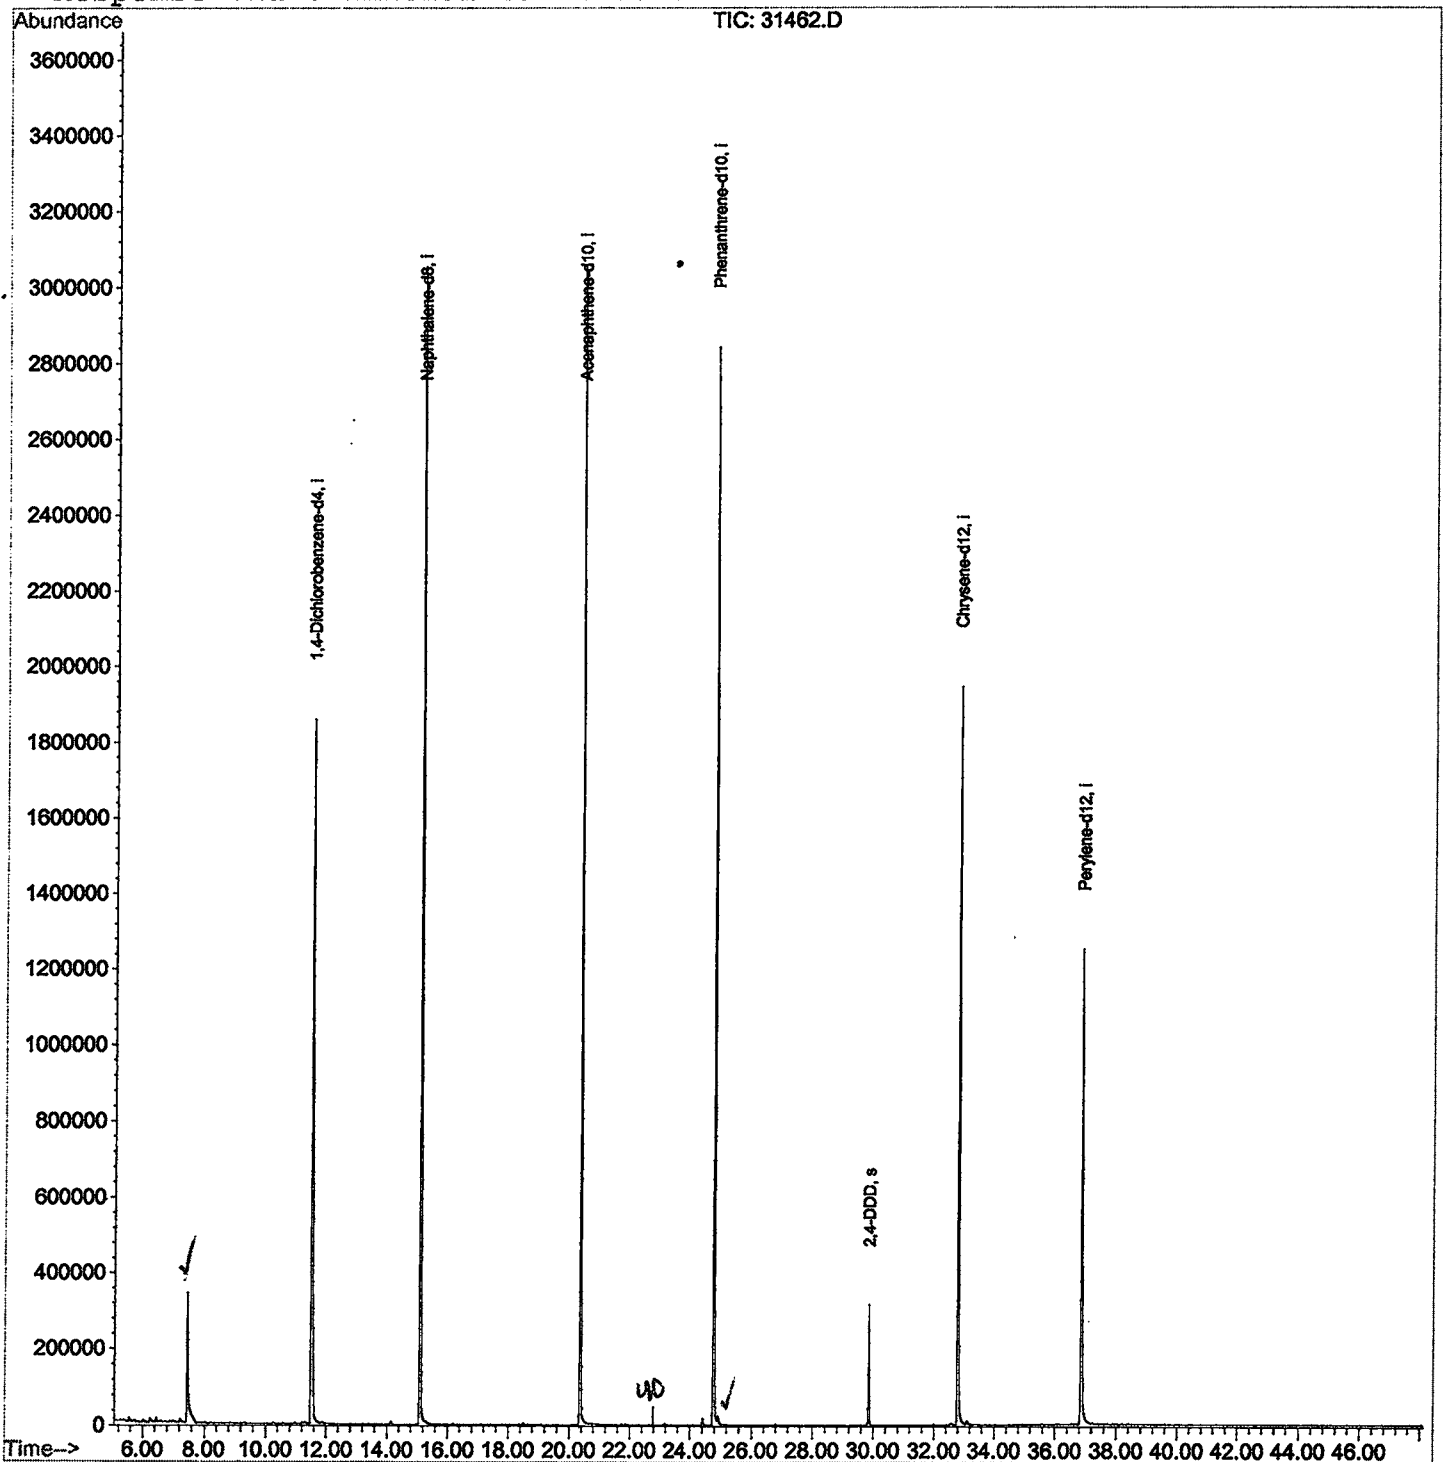

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\JAN1602\31462.D

Acq On : 17 Jan 2002 2:02 pm

Sample : gc/ms scan 12/28

Misc :

MS Integration Params: LSCINT.P

Vial: 27

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0103.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	7.447	258	262	295	rVB	340477	1018226	15.72%	3.028%
2	11.505	699	704	723	rBV	1856577	4950700	76.45%	14.723%
3	15.094	1089	1095	1114	rBV	3051376	6311142	97.45%	18.769%
4	20.354	1662	1668	1685	rBV	3058302	6475983	100.00%	19.259%
5	24.770	2143	2149	2162	rBV2	2842142	6117355	94.46%	18.193%
6	24.926	2162	2166	2179	rVB	22885	74461	1.15%	0.221%
7	29.847	2697	2702	2713	rBV	313599	659065	10.18%	1.960%
8	32.803	3017	3024	3045	rBV2	1944842	4525093	69.87%	13.457%
9	36.870	3457	3467	3488	rBV	1249168	3493074	53.94%	10.388%


Sum of corrected areas: 33625099

31462.D GCMS0103.M

Thu Feb 07 12:39:32 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\JAN1602\31462.D
 Operator : 209 GALOS
 Acquired : 17 Jan 2002 2:02 pm using AcqMethod GCMS0103
 Instrument : GC/MS 209
 Sample Name: gc/ms scan 12/28
 Misc Info :
 Vial Number: 27
 Quant File :GCMS0103.RES (RTE Integrator)

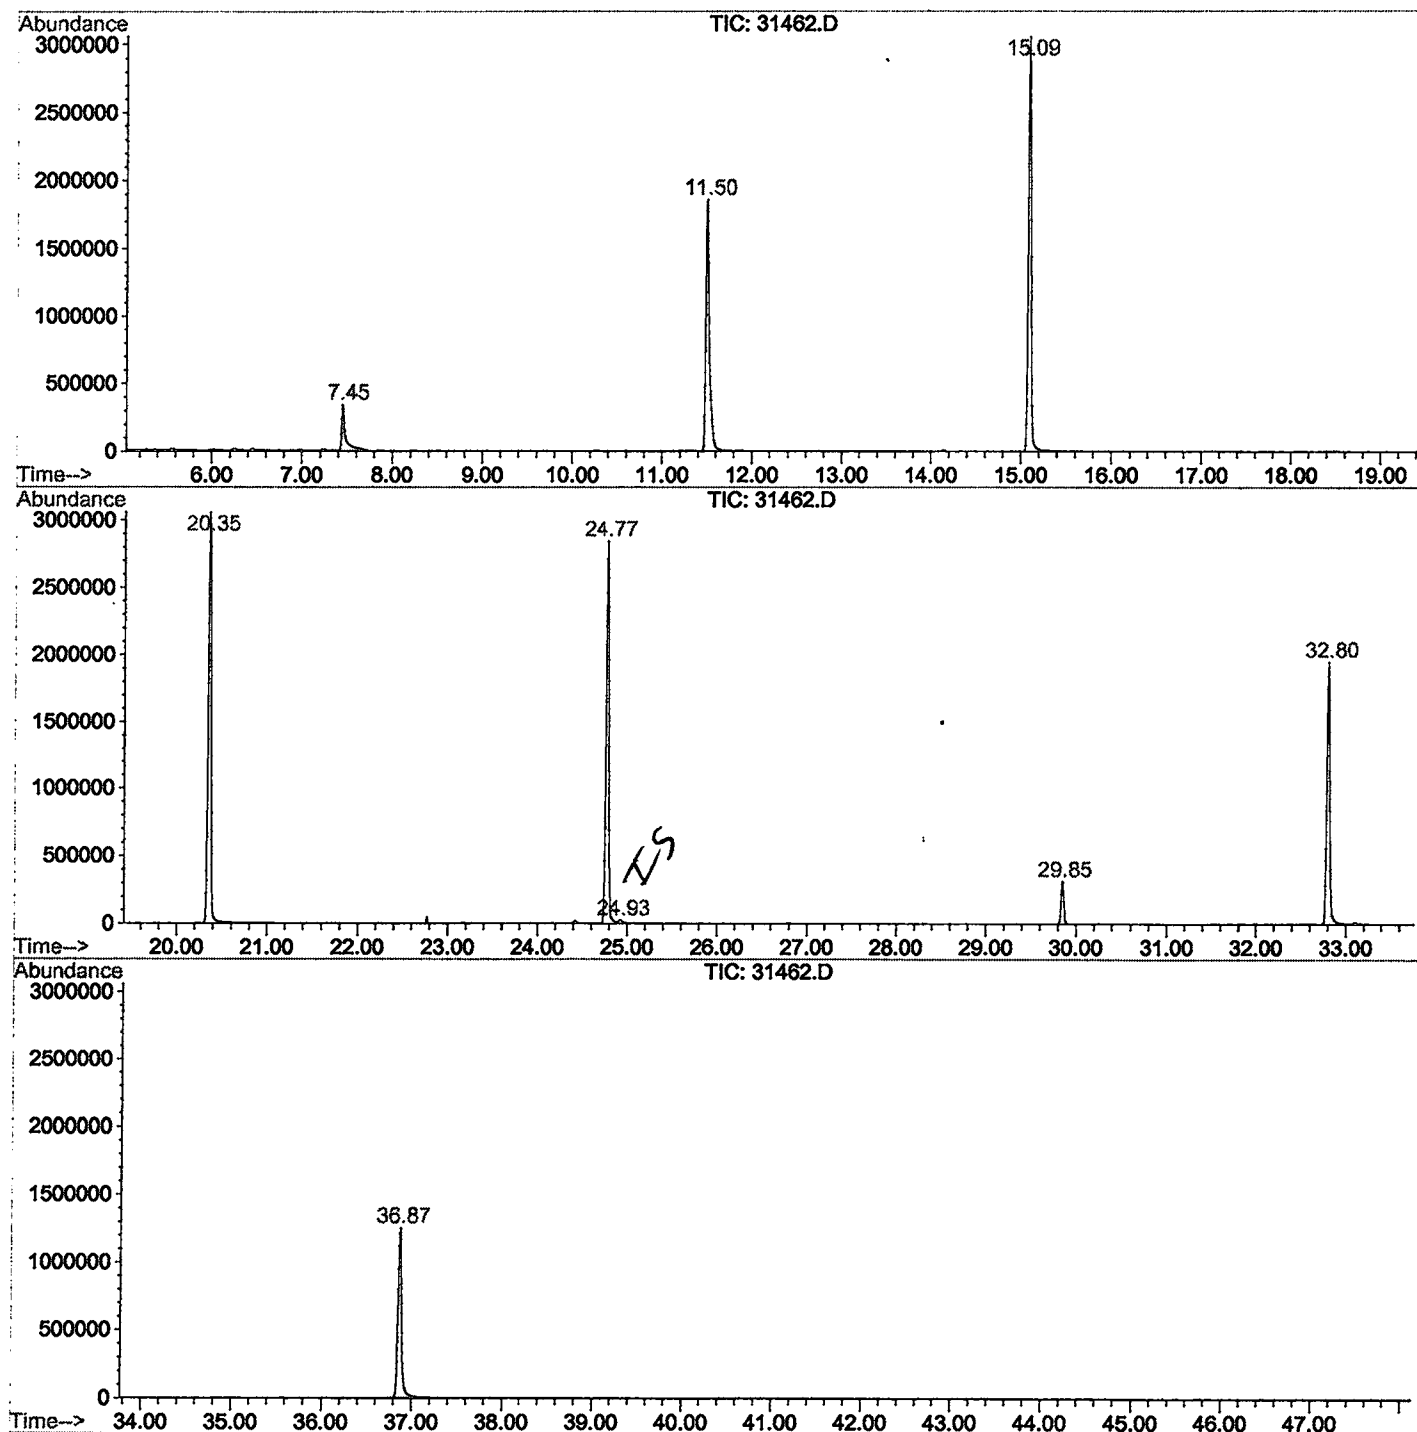

31462.D GCMS0103.M

Thu Feb 07 12:39:38 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\JAN1602\31462.D
Acq On : 17 Jan 2002 2:02 pm
Sample : gc/ms scan 12/28
Misc :
MS Integration Params: LSCINT.P










Vial: 27
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0103.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 Silane, tetramethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.45	4.11 ug/l	1018230	1,4-Dichlorobenzene-d4	11.50

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
2			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	9
3			1-Butanamine, 3-methyl-	87	C5H13N	000107-85-7	9
4			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	9

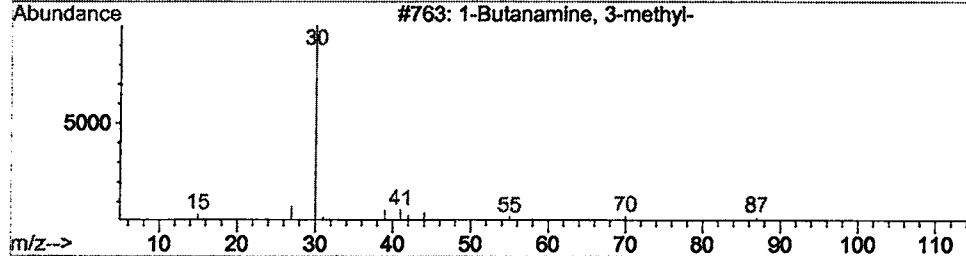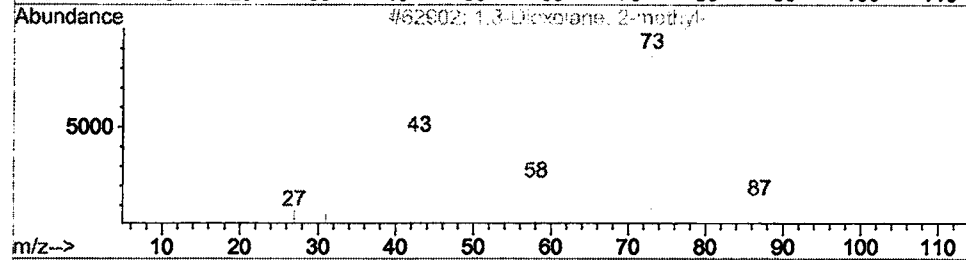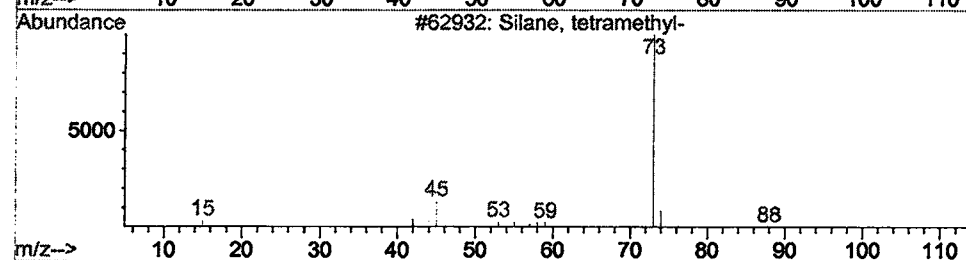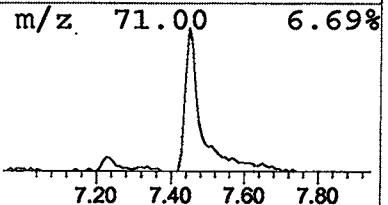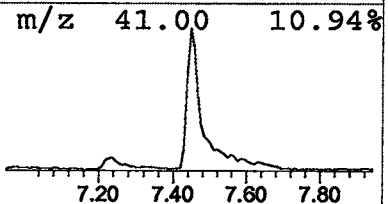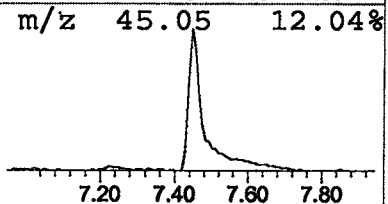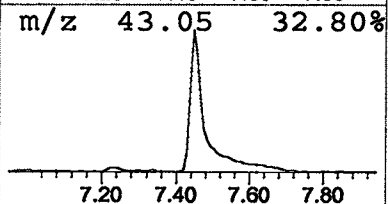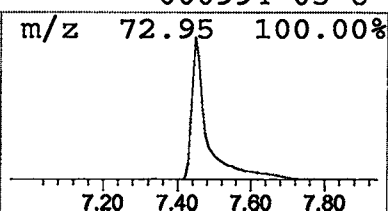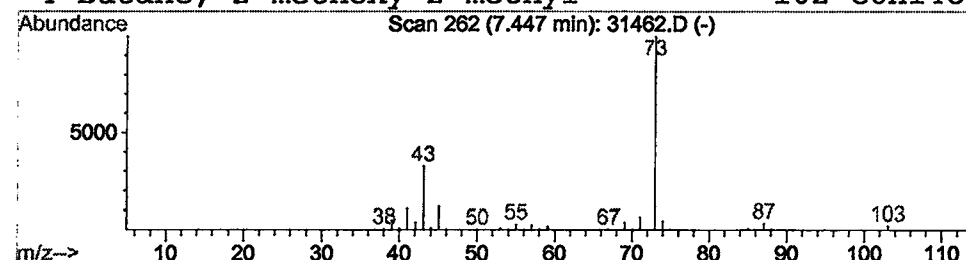

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\JAN1602\31462.D
 Acq On : 17 Jan 2002 2:02 pm
 Sample : gc/ms scan 12/28
 Misc :
 MS Integration Params: LSCINT.P


Vial: 27
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0103.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 2 Anthracene-d10- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
24.93	0.24 ug/l	74461	Phenanthrene-d10	24.77

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Anthracene-d10- <i>JS</i>	188	C14D10	001719-06-8	87
2			Antipyrine	188	C11H12N2O	000060-80-0	53
3			Phenanthrene-d10	188	C14D10	001517-22-2	50
4			4-Methyl-2-(4-fluorophenyl)pyrimidi	188	C11H9FN2	076128-67-1	42

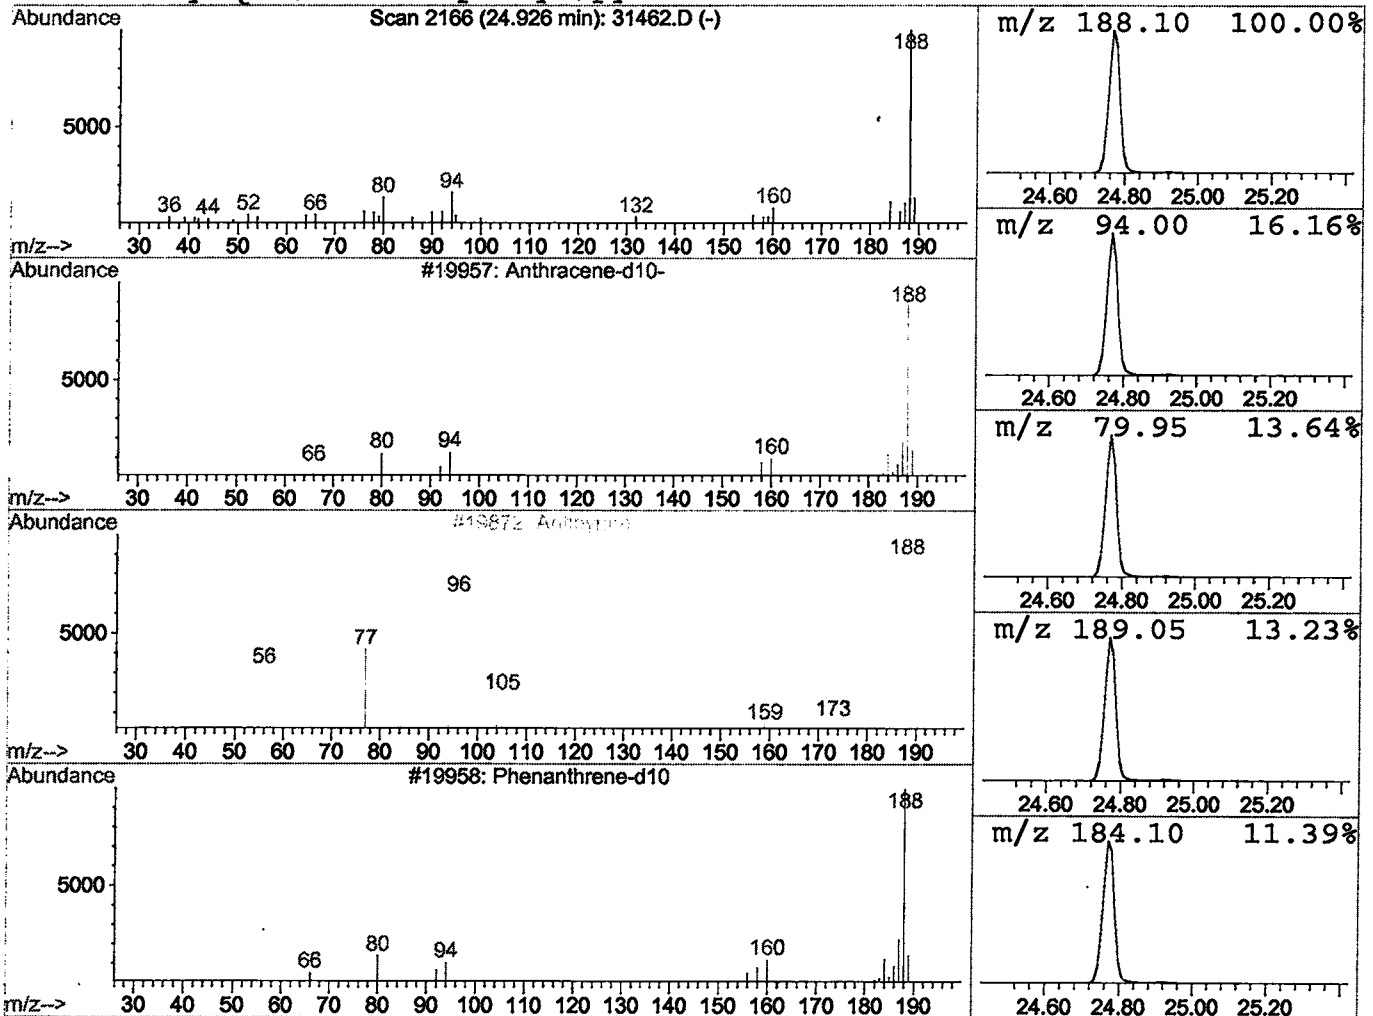

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 17 Jan 2002 2:02 pm
Data File: C:\HPCHEM\1\DATA\JAN1602\31462.D
Name: gc/ms scan 12/28
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0103.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
Silane, tetramethyl	7.45	4.1	ug/l	1018230	ISTD01	11.50	4950700	20.0
Anthracene d10 <i>IS</i>	24.93	0.2	ug/l	74461	ISTD04	24.77	6117360	20.0

31462.D GCMS0103.M Thu Feb 07 12:39:53 2002