

DFTPP

Data File : M:\INSTRU-1\209\DATA\JAN0802\DFTPP1.D

Vial: 1

Acq On : 9 Jan 2002 8:50 am

Operator: 209 GALOS

Sample :

Inst : GC/MS 209


Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

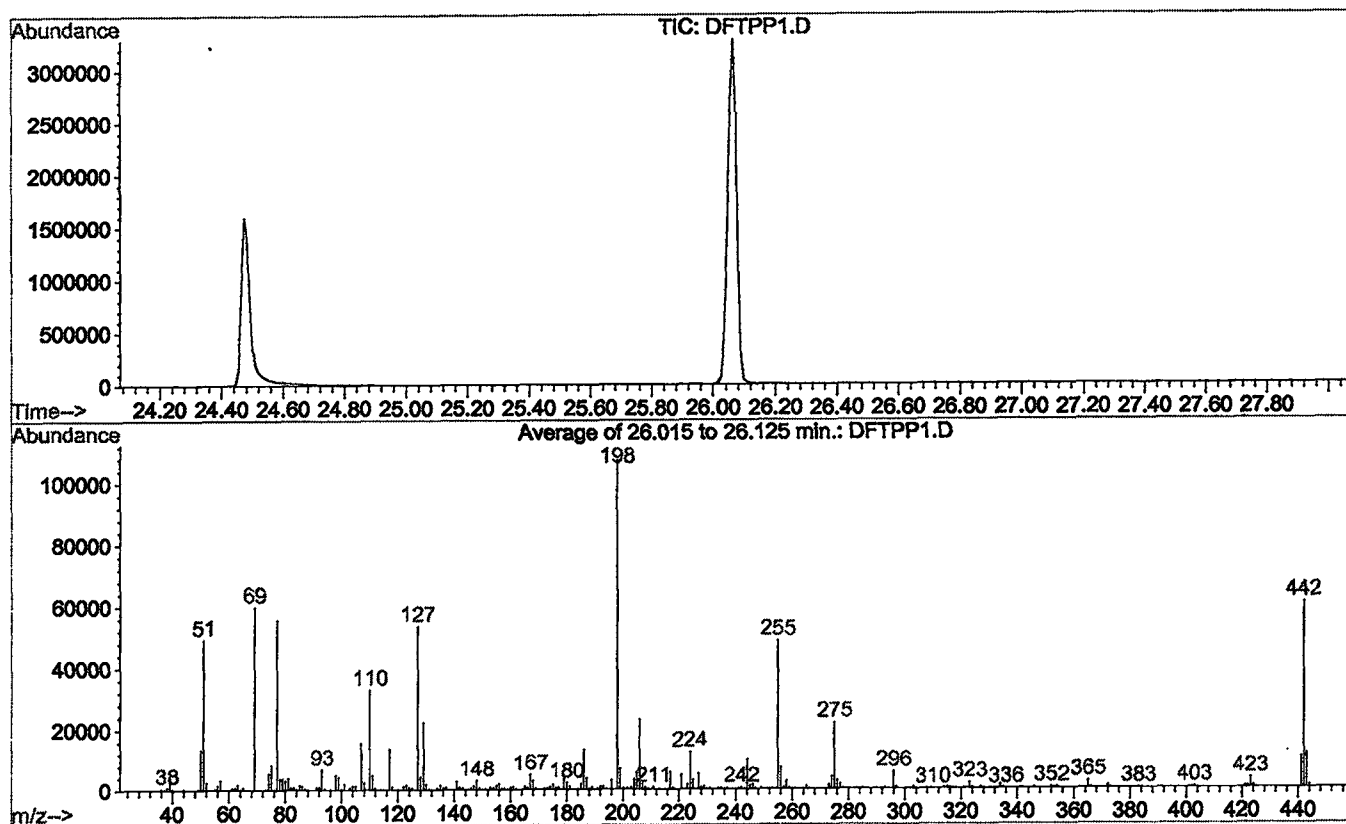

Spectrum Information: Average of 26.015 to 26.125 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	45.9	49298	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	55.9	60025	PASS
70	69	0.00	2	0.1	76	PASS
127	198	40	60	50.0	53606	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	107316	PASS
199	198	5	9	6.7	7156	PASS
275	198	10	30	20.5	22010	PASS
365	198	1	100	2.3	2474	PASS
441	443	0.01	100	89.0	10355	PASS
442	198	40	110	56.6	60774	PASS
443	442	17	23	19.1	11634	PASS