

Method 508 mod

Date Extracted 12/31/01

Page 99

REF

#GCM5-16527

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count	Rec'd
	LB	500ml		1ml			1ml	6A	7		
	REF				5ml			6B			
	31464							7B			
	31433							7A			
	31502							4A			
	31503							2A			
	31432							3B			
	31501							3A			
	31504							5A			
	31500							6B			
	31505							8B			
	31552							4B			
	31550							8A			
Remarks											
drip rate must be between 5-15 ml/min for liq-liq extractors											
drip rate -											
Extraction type		Solv. lot#		NaCl lot#		Na2SO4 lot#					
STANDARD		INT STD LOG#									
CALIBRATION											
REF SPIKE		91159									
MDL/MDRF											
Q. CHECK											
INT. STD.											
SURROGATE		121101		GCM5							
LPC											
ENDRIN/DDT											

Analyst

Reviewed by

Sequence Name: C:\HPCHEM\1\SEQUENCE\JAN1802.S

Comment: INST 209; 30Mx0.25umX0.50

Operator: 209 GALOS

Data Path: C:\HPCHEM\1\data\jan1802\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run	On A Barcode Mismatch
(X) Full Method	(X) Inject Anyway
() Reprocessing Only	() Don't Inject

Line Type	Vial	DataFile	Method	Sample Name
-----------	------	----------	--------	-------------

1 Sample	1	DFTPP	GCMS0103	
2 Sample	2	CAL40	GCMS0103	
3 Sample	3	30986	GCMS0103	
4 Sample	1	DFTPP1	GCMS0103	
5 Sample	2	CAL40A	GCMS0103	calib 40
6 Sample	3	30986A	GCMS0103	
7 Sample	4	LB	GCMS0103	gc/ms scan 12/31
8 Sample	5	REF	GCMS0103	gc/ms scan 12/31
9 Sample	6	31464	GCMS0103	gc/ms scan 12/31
10 Sample	7	31433	GCMS0103	gc/ms scan 12/31
11 Sample	8	31502	GCMS0103	gc/ms scan 12/31
12 Sample	9	31503	GCMS0103	gc/ms scan 12/31
13 Sample	10	31432	GCMS0103	gc/ms scan 12/31
14 Sample	11	31501	GCMS0103	gc/ms scan 12/31
15 Sample	12	31504	GCMS0103	gc/ms scan 12/31
16 Sample	13	31500	GCMS0103	gc/ms scan 12/31
17 Sample	14	31505	GCMS0103	gc/ms scan 12/31
18 Sample	15	31552	GCMS0103	gc/ms scan 12/31
19 Sample	16	31550	GCMS0103	gc/ms scan 12/31

DFTPP

Data File : C:\HPCHEM\1\DATA\JAN1802\DFTPP1.D

Acq On : 18 Jan 2002 3:24 pm

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

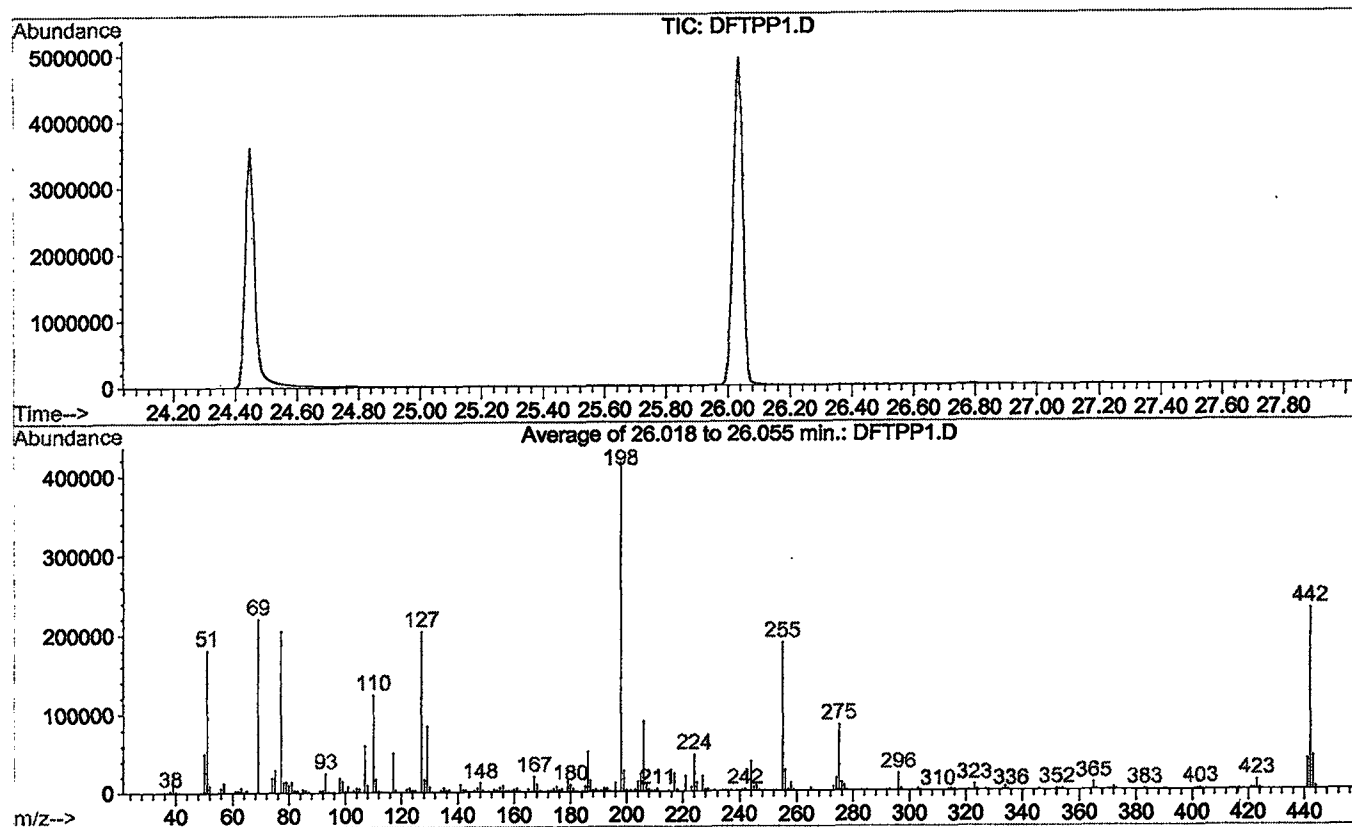

Spectrum Information: Average of 26.018 to 26.055 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	43.7	181672	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	53.1	220594	PASS
70	69	0.00	2	0.0	90	PASS
127	198	40	60	49.1	204190	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	415770	PASS
199	198	5	9	6.6	27289	PASS
275	198	10	30	20.4	84629	PASS
365	198	1	100	2.4	9798	PASS
441	443	0.01	100	89.6	40102	PASS
442	198	40	110	55.4	230238	PASS
443	442	17	23	19.4	44742	PASS