

Method 508 mod

Date Extracted 12/12/01

Page 60

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
✓ LB		500ml		1ml			1ml	10A	7			
✓ Ref					0.5ml			9B				
✓ 30111	✓ - ✓							9A				
✓ 30010	✓ - ✓							10A				
✓ 30107	✓ - ✓							10B				
✓ 30110	✓ - ✓							10A				
✓ 30109	✓ - ✓							10B				
✓ 30009	✓ - ✓							9A				
✓ 30025	✓ - ✓							9B				
✓ 30108	✓ - ✓							8B				
✓ 30253	✓ - ✓							7B				
✓ 30119	✓ - ✓							7A				
✓ H												
Remarks Sep funnel broke for LB, changed 30109 from 10B to 8A b/c 10B wasn't working.												
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate -												
Extraction type - <u>sep fun</u> Solv. lot# <u>V39960</u> NaCl lot# <u>V1599</u> Na2SO4 lot# <u>V391100</u>												
STANDARD	INT STD LOG#											
CALIBRATION												
REF/SPIKE	91759											
MDL/MDRF												
Q. CHECK												
INT. STD.												
SURROGATE	GCHS-121101											
LPC												
ENDRIN/DDT												

Analyst LF
revision 4/12/01

Verified by _____

Reviewed by DN
Date 1/9/02

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC1901\DFTPP1.D

Vial: 1

Acq On : 20 Dec 2001 9:14 am

Operator: 209 GALOS

Sample :

Inst : GC/MS 209


Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

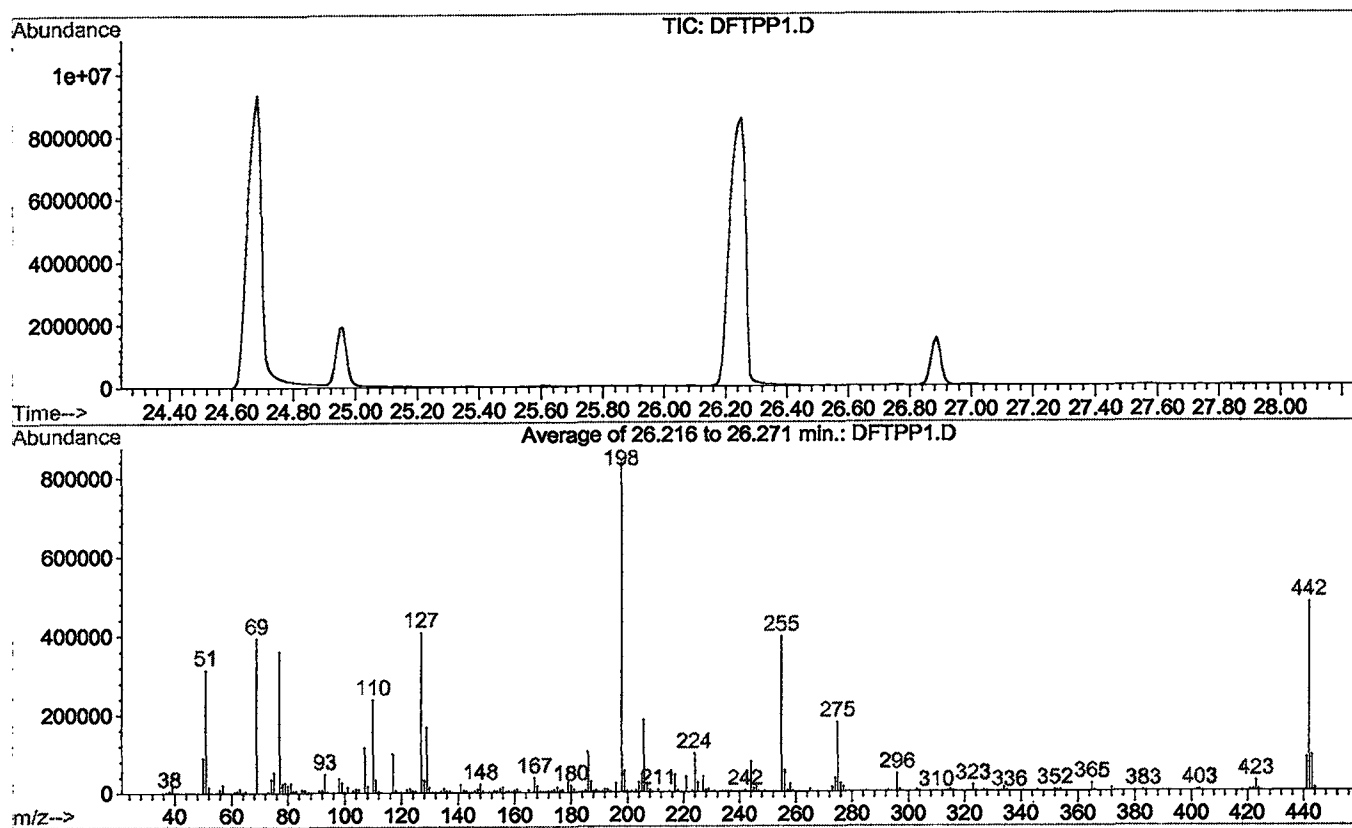

Spectrum Information: Average of 26.216 to 26.271 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	37.8	315479	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	47.3	394963	PASS
70	69	0.00	2	0.0	89	PASS
127	198	40	60	49.0	408897	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	835310	PASS
199	198	5	9	6.6	55542	PASS
275	198	10	30	21.3	178319	PASS
365	198	1	100	2.6	22047	PASS
441	443	0.01	100	93.7	86850	PASS
442	198	40	110	57.6	481088	PASS
443	442	17	23	19.3	92731	PASS

DFTPP1.D GCMS1126.M

Wed Jan 02 10:05:37 2002

DFTPP

Data File : C:\HPCHEM\1\DATA\JAN0302\DFTPP.D

Acq On : 3 Jan 2002 9:35 am

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

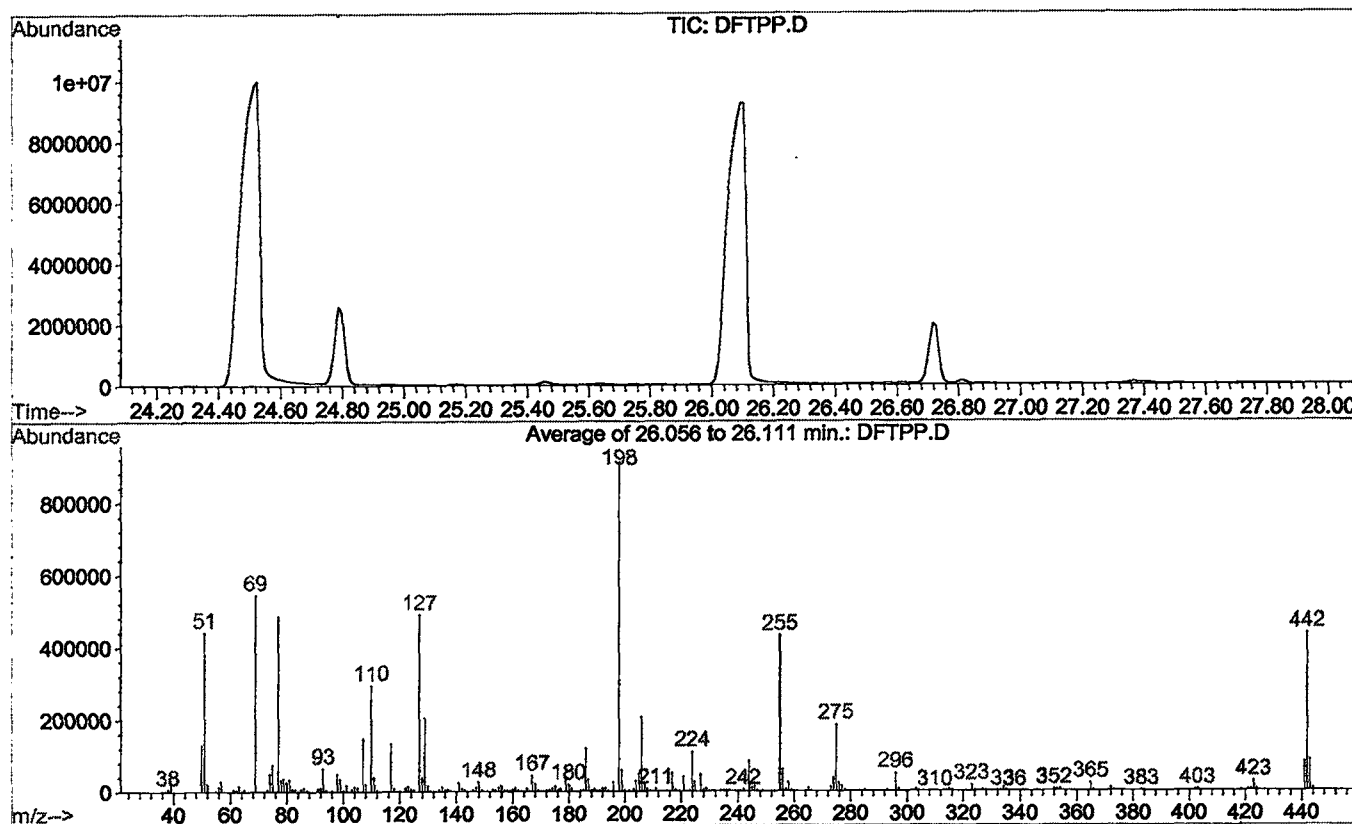

Spectrum Information: Average of 26.056 to 26.111 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	48.7	443154	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	59.9	545609	PASS
70	69	0.00	2	0.0	225	PASS
127	198	40	60	53.9	491127	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	910811	PASS
199	198	5	9	6.6	60463	PASS
275	198	10	30	20.4	185573	PASS
365	198	1	100	2.6	23897	PASS
441	443	0.01	100	95.4	81827	PASS
442	198	40	110	48.0	437111	PASS
443	442	17	23	19.6	85802	PASS

DFTPP.D GCMS1126.M

Thu Jan 03 13:09:30 2002