

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 01/09/2002 Time: 14:54:59

Sample: AD30111

Analysis: \$GCMS GCMS Scan For Unknowns

Units: ug

Started: 1/9/02 14:54 Ended: 1/9/02 14:54 Analyst: DLV

Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		113		5.0

Comments for Sample AD30111 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 01-09-2002 Time: 14:55:41

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\JAN0302\30111.D

Vial: 34

Acq On : 4 Jan 2002 6:41 pm

Operator: 209 GALOS

Sample : gcms scan 1/2a

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Jan 4 19:29 2002

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 28 15:11:00 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.52	152	733410	20.00	ug/l	-0.17
10) Naphthalene-d8	15.12	136	2860781	20.00	ug/l	-0.18
17) Acenaphthene-d10	20.39	164	1440494	20.00	ug/l	-0.18
29) Phenanthrene-d10	24.81	188	2026552	20.00	ug/l	-0.18
38) Chrysene-d12	32.83	240	1170282	20.00	ug/l	-0.20
44) Perylene-d12	36.90	264	642813	20.00	ug/l	-0.22

System Monitoring Compounds

37) 2,4-DDD	29.88	235	125766	5.64	ug/mL	-0.19
Spiked Amount	5.000		Recovery	=	112.80%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.18	128	1001	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	20.73	165	285	N.D.	
25) Diethylphthalate	21.93	149	564	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	

(#)=qualifier out of range (m)=manual integration

30111.D GCMS0103.M Mon Jan 07 11:35:42 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\JAN0302\30111.D

Vial: 34

Acq On : 4 Jan 2002 6:41 pm

Operator: 209 GALOS

Sample : gcms scan 1/2a

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Jan 4 19:29 2002

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 28 15:11:00 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	24.80	178	662	N.D.		
34) Anthracene	24.80	178	662	N.D.		
35) Di-n-butylphthalate	26.83	149	32917	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	32.83	228	3074	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.14	149	1393	N.D.		
43) Chrysene	32.83	228	3074	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	36.90	252	2862	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

30111.D GCMS0103.M Mon Jan 07 11:35:46 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\JAN0302\30111.D
Acq On : 4 Jan 2002 6:41 pm
Sample : gcms scan 1/2a
Misc :
MS Integration Params: GOOFY.P
Quant Time: Jan 4 19:29 2002

Vial: 34
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS1126.RES

Method : C:\HPCHEM\1\METHODS\GCMS0103.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Mon Jan 07 10:31:02 2002
Response via : Initial Calibration

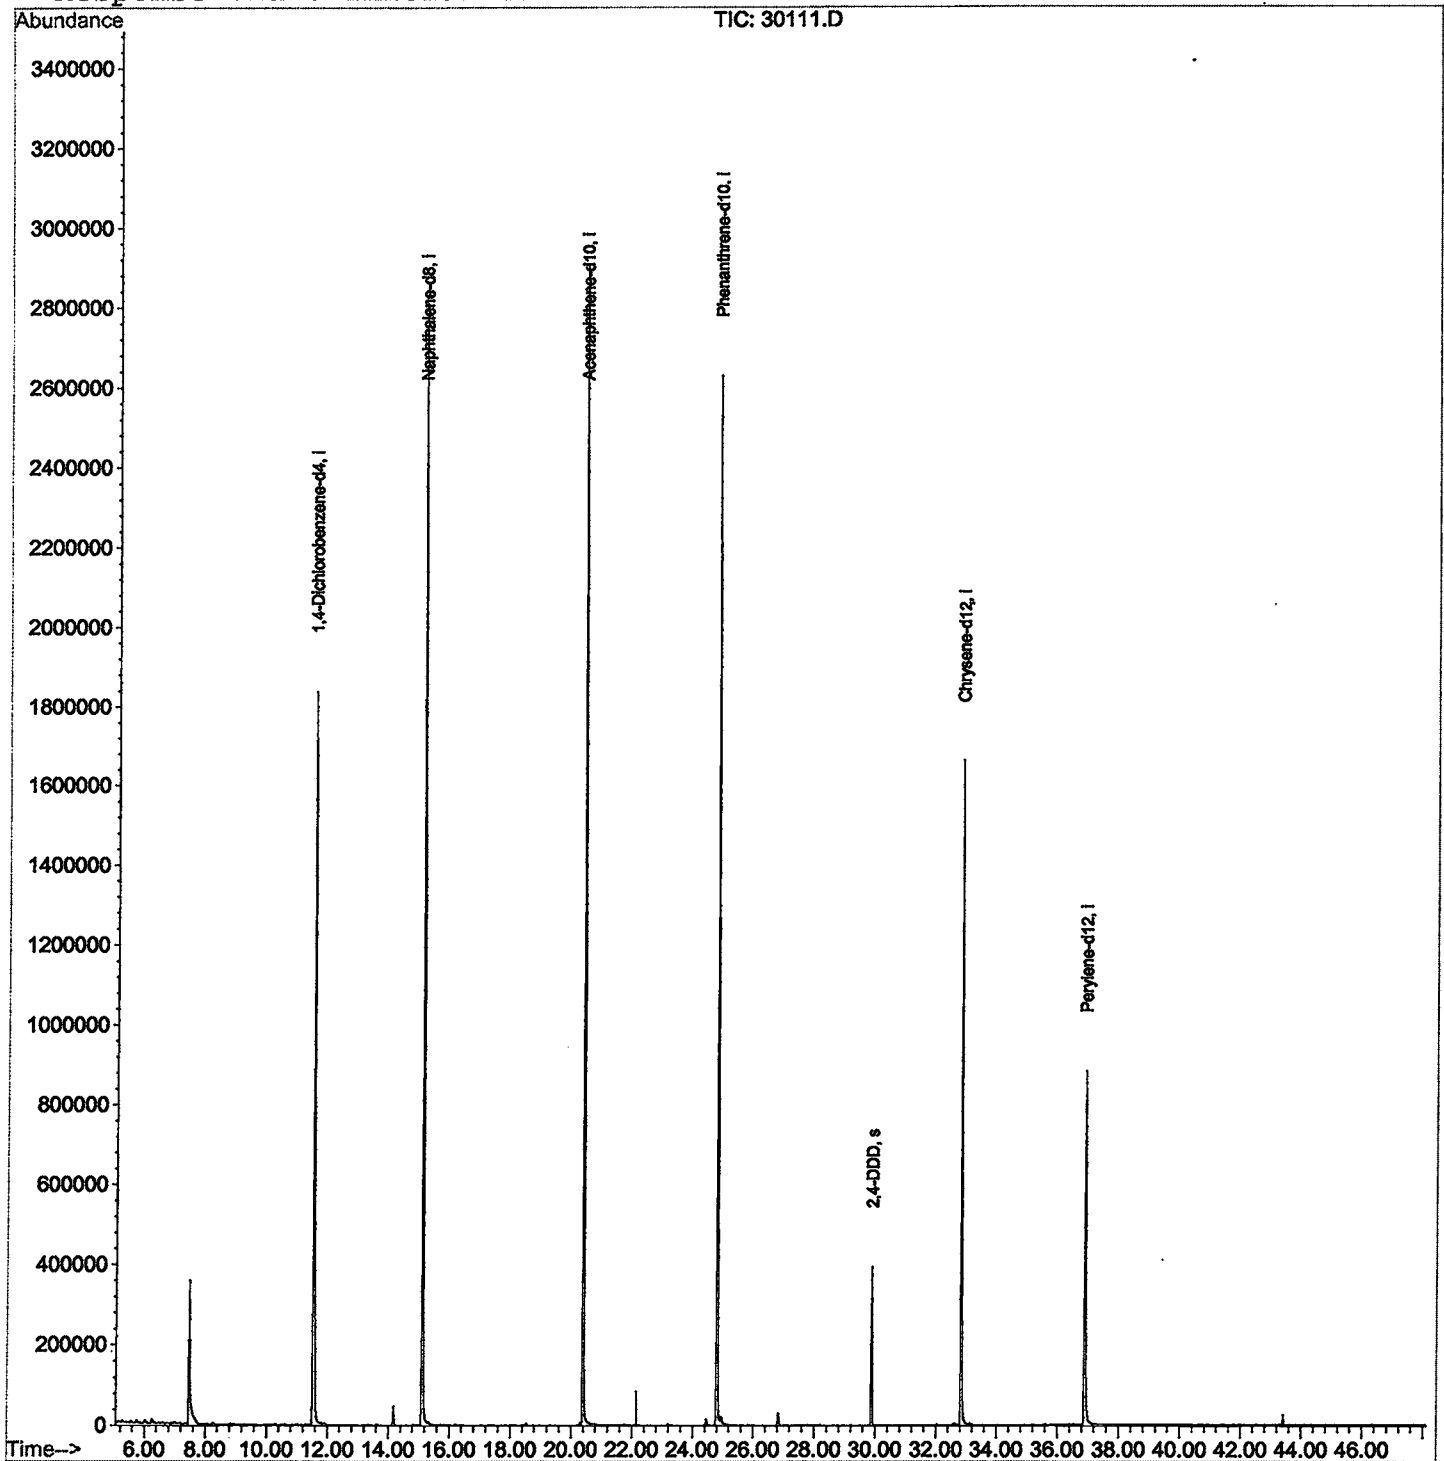

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\JAN0302\30111.D

Vial: 34

Acq On : 4 Jan 2002 6:41 pm

Operator: 209 GALOS

Sample : gcms scan 1/2a

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	7.466	260	264	295	rBV	356281	1064769	17.70%	3.518%
2	11.524	701	706	727	rBV	1838033	4590529	76.29%	15.165%
3	14.168	989	994	999	rVB2	48175	90689	1.51%	0.300%
4	15.122	1092	1098	1115	rBV	2809460	5821709	96.75%	19.233%
5	20.392	1666	1672	1687	rBV	2907505	6017058	100.00%	19.878%
6	24.808	2147	2153	2165	rBV2	2630154	5705137	94.82%	18.848%
7	29.884	2701	2706	2715	rBV	392639	784505	13.04%	2.592%
8	32.831	3021	3027	3048	rBV2	1662875	3784639	62.90%	12.503%
9	36.898	3463	3470	3493	rBV	880895	2410578	40.06%	7.964%


Sum of corrected areas: 30269613

30111.D GCMS1126.M

Mon Jan 07 11:47:03 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\JAN0302\30111.D
 Operator : 209 GALOS
 Acquired : 4 Jan 2002 6:41 pm using AcqMethod GCMS1126
 Instrument : GC/MS 209
 Sample Name: gcms scan 1/2a
 Misc Info :
 Vial Number: 34
 Quant File :GCMS1126.RES (RTE Integrator)

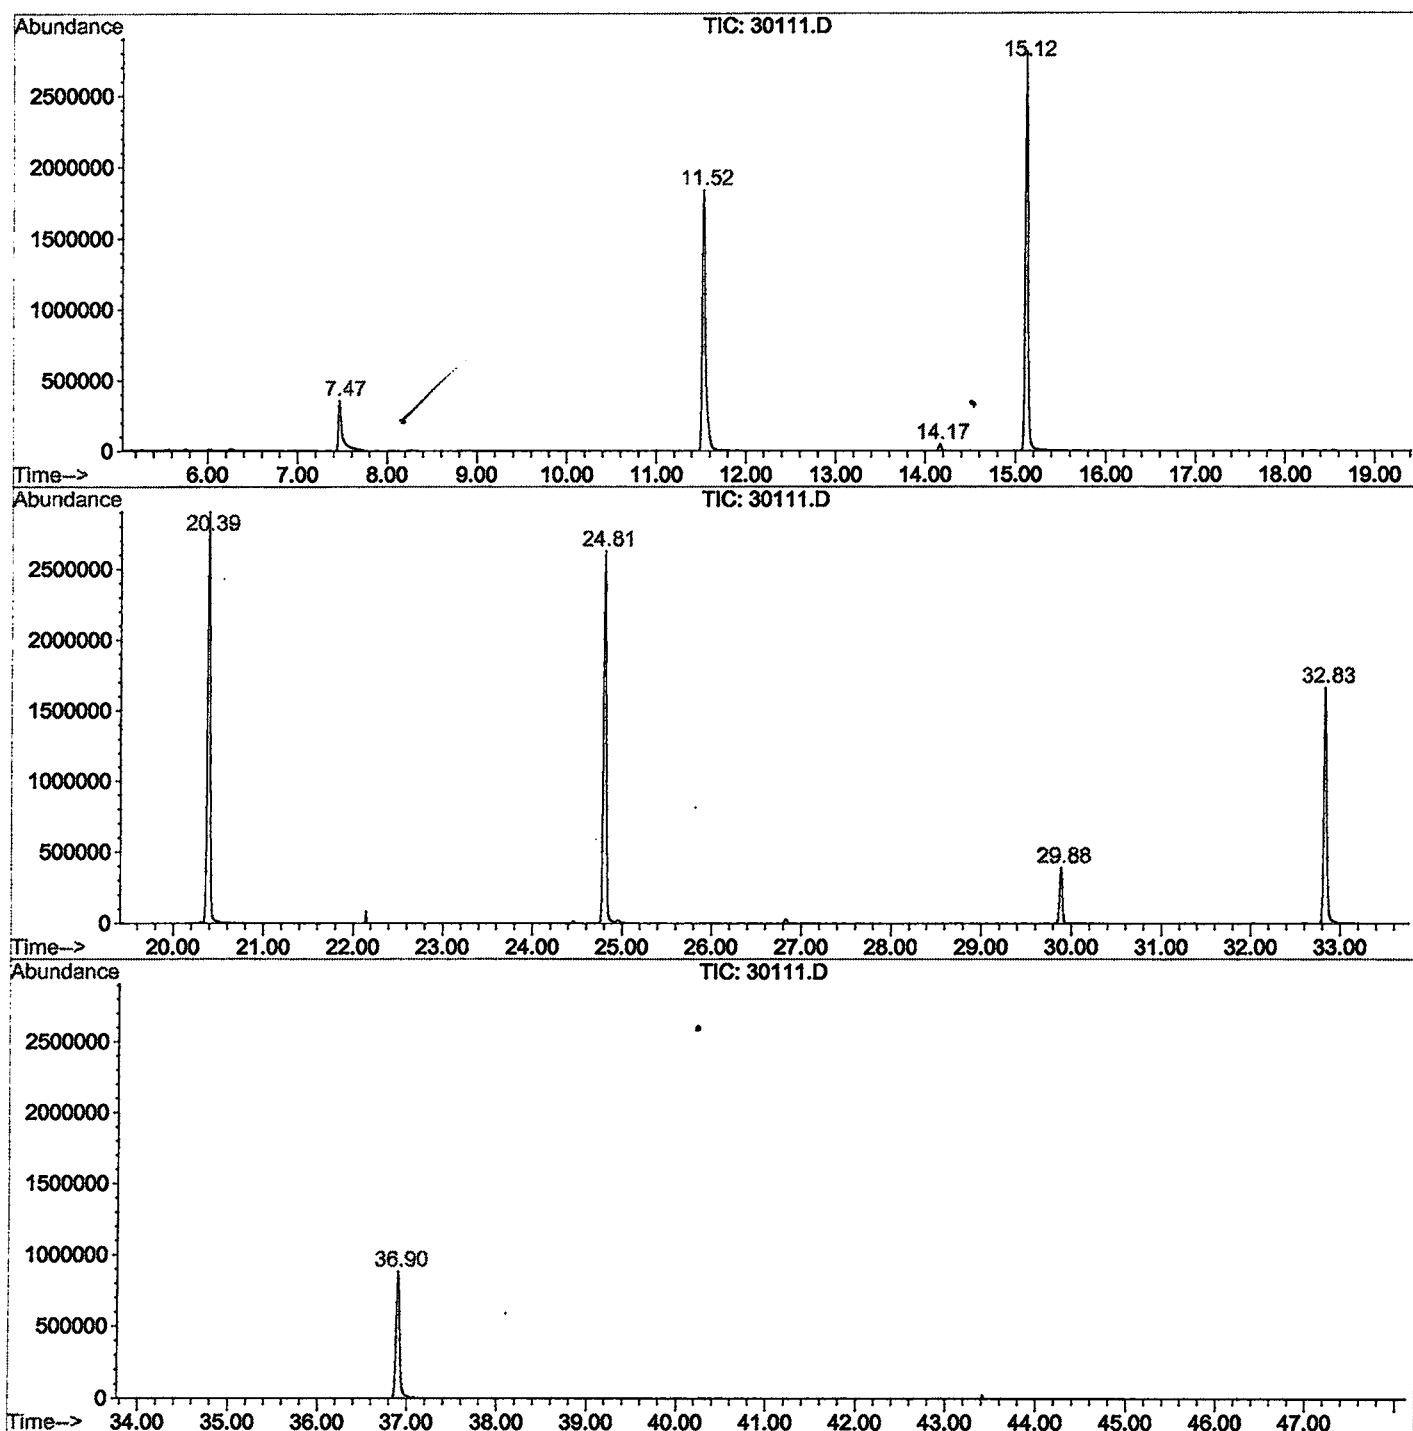

30111.D GCMS1126.M

Mon Jan 07 11:47:08 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\JAN0302\30111.D
Acq On : 4 Jan 2002 6:41 pm
Sample : gcms scan 1/2a
Misc :
MS Integration Params: LSCINT.P










Vial: 34
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 3-Pentanol, 3-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.47	4.64 ug/l	1064770	1,4-Dichlorobenzene-d4	11.52

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	33
2			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
3			N-Ethylformamide	73	C3H7NO	000627-45-2	9
4			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	9

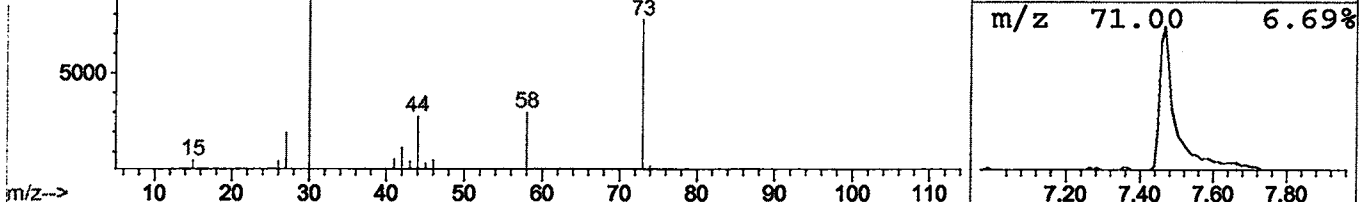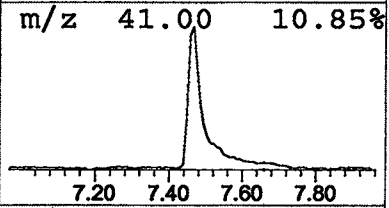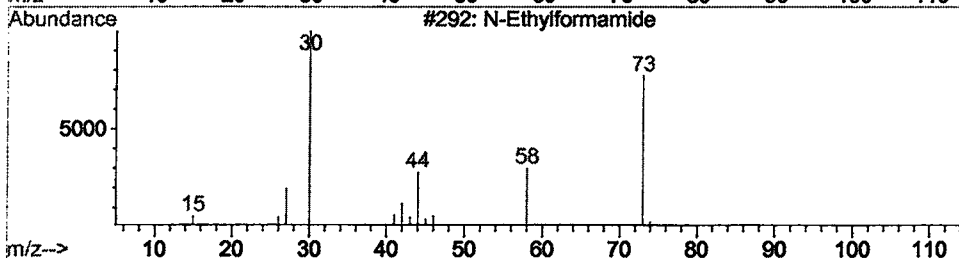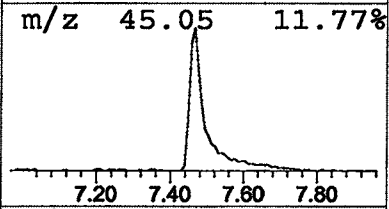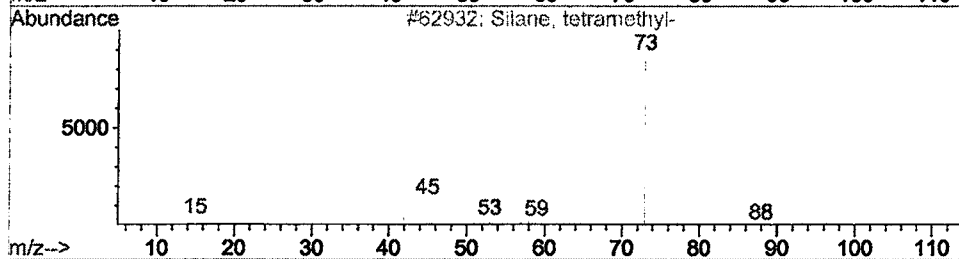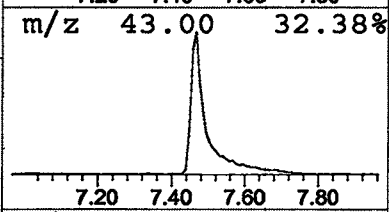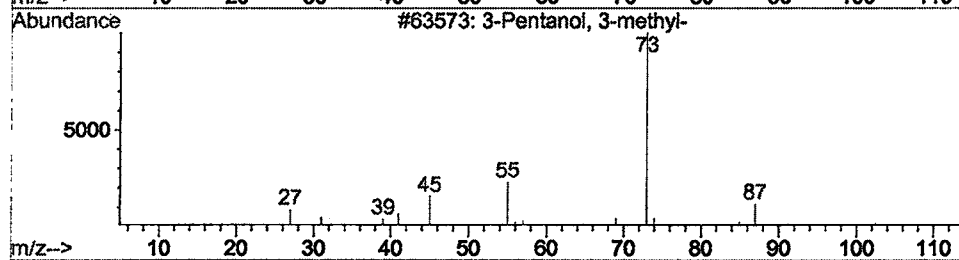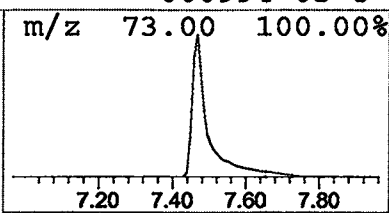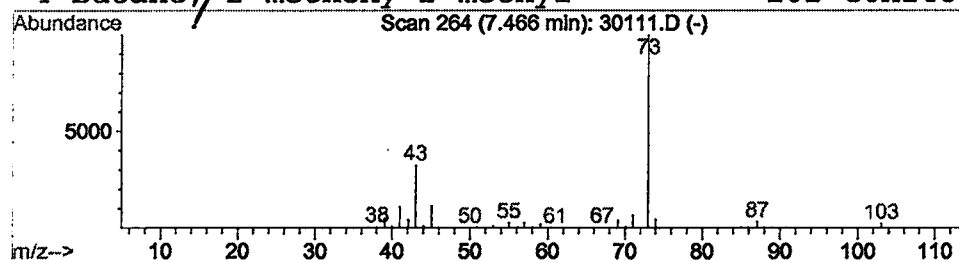

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 4 Jan 2002 6:41 pm
 Data File: C:\HPCHEM\1\DATA\JAN0302\30111.D
 Name: gcms scan 1/2a
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc

3-Pentanol, 3-methyl	7.47	4.6 ug/l		1064770	ISTD01	11.52	4590530	20.0
30111.D GCMS1126.M								
	Mon Jan 07 11:47:18 2002							