

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 01/09/2002 Time: 14:58:07

Sample: AD30023
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 1/9/02 14:57 Ended: 1/9/02 14:57 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		105		5.0

Comments for Sample AD30023 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 01-09-2002 Time: 14:58:22

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\JAN0302\30023.D

Vial: 37

Acq On : 4 Jan 2002 9:36 pm

Operator: 209 GALOS

Sample : gcms scan 1/2a

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Jan 4 22:24 2002

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 28 15:11:00 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.52	152	665142	20.00	ug/l	-0.18
10) Naphthalene-d8	15.12	136	2614886	20.00	ug/l	-0.19
17) Acenaphthene-d10	20.39	164	1302228	20.00	ug/l	-0.19
29) Phenanthrene-d10	24.80	188	1794805	20.00	ug/l	-0.19
38) Chrysene-d12	32.83	240	1015783	20.00	ug/l	-0.21
44) Perylene-d12	36.89	264	593094	20.00	ug/l	-0.22

System Monitoring Compounds

37) 2,4-DDD	29.89	235	103609	5.25	ug/mL	-0.18
Spiked Amount	5.000		Recovery	=	105.00%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.18	128	765	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	20.68	165	389	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	

(#)=qualifier out of range (m)=manual integration

30023.D GCMS0103.M Mon Jan 07 11:37:52 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\JAN0302\30023.D

Vial: 37

Acq On : 4 Jan 2002 9:36 pm

Operator: 209 GALOS

Sample : gcms scan 1/2a

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Jan 4 22:24 2002

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 28 15:11:00 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	24.80	178	599	N.D.		
34) Anthracene	24.80	178	599	N.D.		
35) Di-n-butylphthalate	26.83	149	17912	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	32.84	228	2636	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.14	149	3451	N.D.		
43) Chrysene	32.84	228	2636	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	36.90	252	2383	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

30023.D GCMS0103.M Mon Jan 07 11:37:55 2002

Page 2

Quantitation Report

Data File : C:\HPCHEM\1\DATA\JAN0302\30023.D

Vial: 37

Acq On : 4 Jan 2002 9:36 pm

Operator: 209 GALOS

Sample : gcms scan 1/2a

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Jan 4 22:24 2002


Quant Results File: GCMS1126.RES

Method : C:\HPCHEM\1\METHODS\GCMS0103.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Mon Jan 07 10:31:02 2002

Response via : Initial Calibration

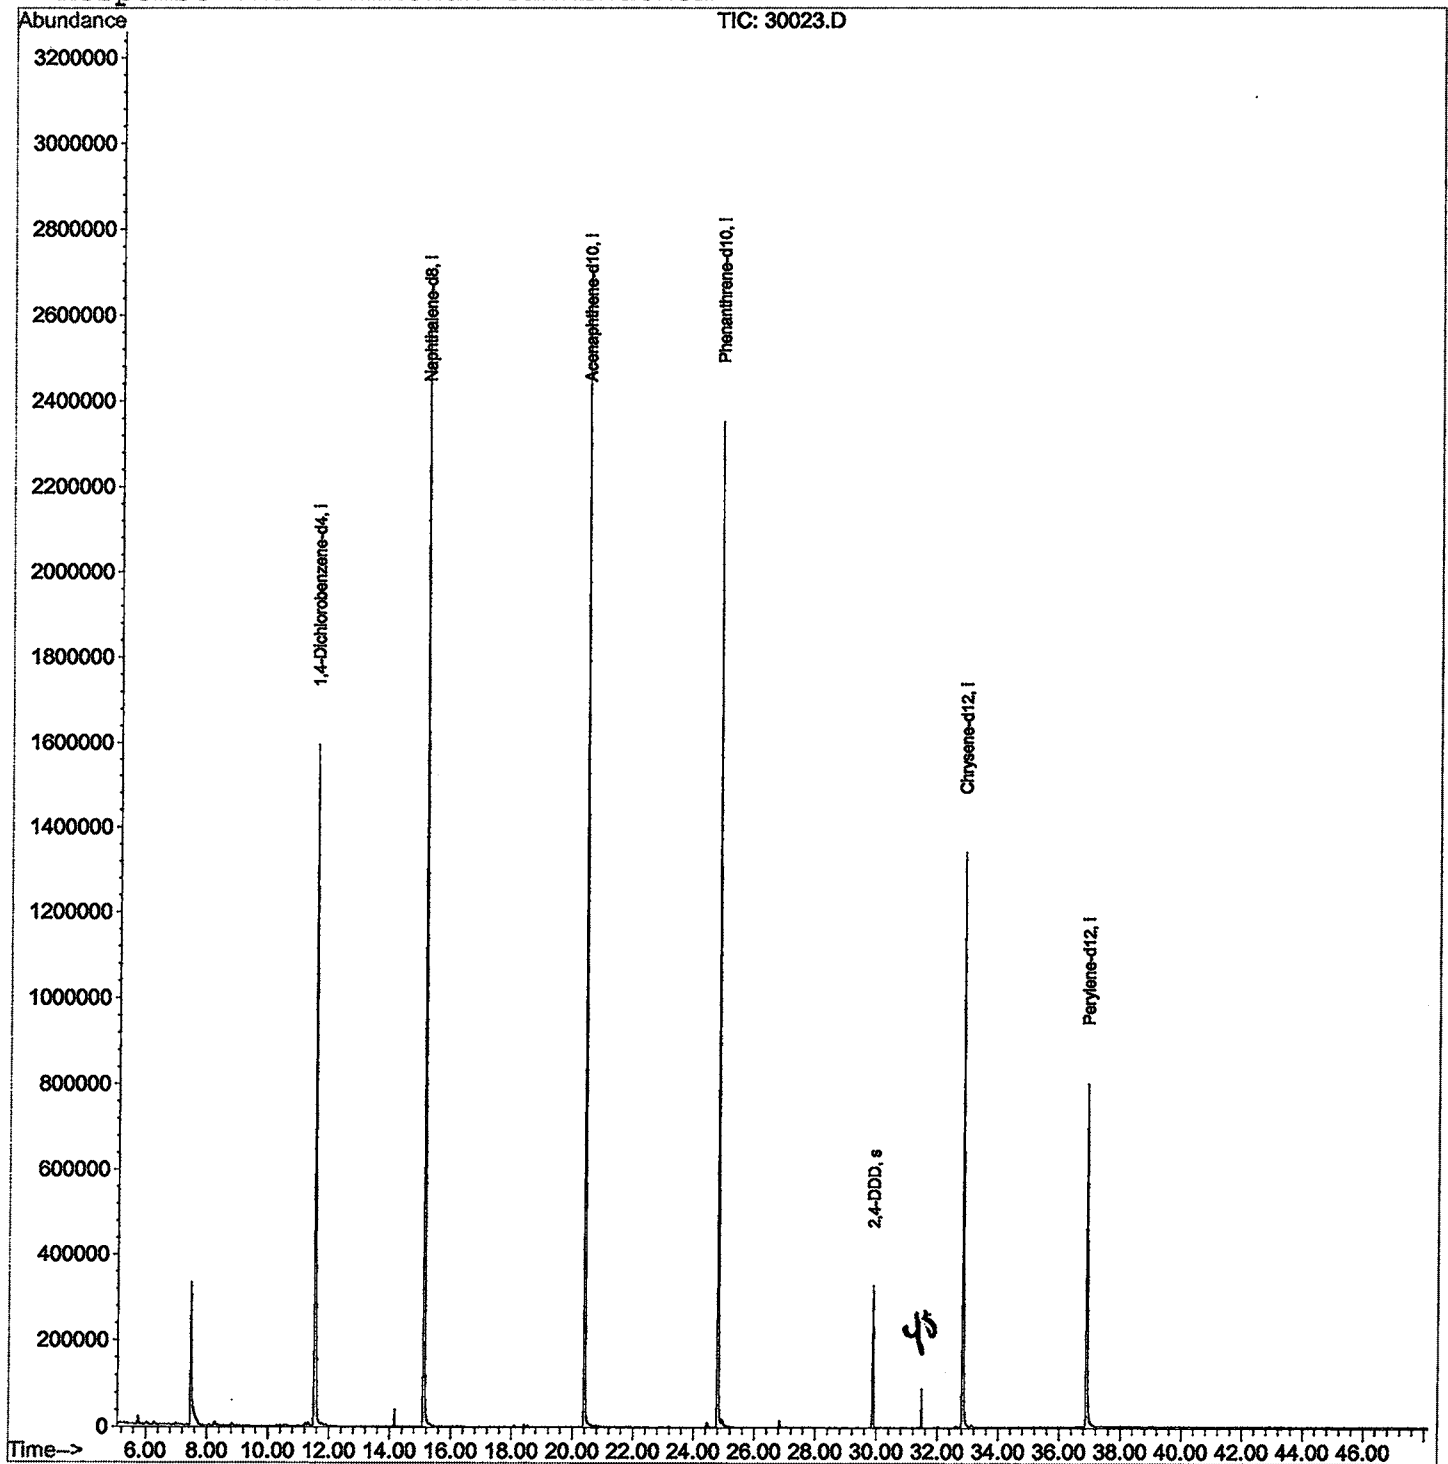

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\JAN0302\30023.D

Acq On : 4 Jan 2002 9:36 pm

Sample : gcms scan 1/2a

Misc :

MS Integration Params: LSCINT.P

Vial: 37

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	7.463	259	263	300	rBV	330547	990590	18.21%	3.643%
2	11.520	701	705	727	rBV	1591225	4196015	77.15%	15.433%
3	14.164	988	993	1000	rBV	39859	76373	1.40%	0.281%
4	15.119	1092	1097	1116	rBV	2581495	5335853	98.10%	19.625%
5	20.389	1665	1671	1690	rBV	2715358	5439033	100.00%	20.005%
6	24.804	2146	2152	2165	rBV2	2351856	5060445	93.04%	18.612%
7	29.881	2700	2705	2714	rBV	326639	646694	11.89%	2.379%
8	32.828	3020	3026	3047	rBV2	1340409	3257560	59.89%	11.981%
9	36.895	3463	3469	3482	rBV2	799082	2185988	40.19%	8.040%


Sum of corrected areas: 27188551

30023.D GCMS1126.M

Mon Jan 07 11:45:47 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\JAN0302\30023.D
Operator : 209 GALOS
Acquired : 4 Jan 2002 9:36 pm using AcqMethod GCMS1126
Instrument : GC/MS 209
Sample Name: gcms scan 1/2a
Misc Info :
Vial Number: 37
Quant File :GCMS1126.RES (RTE Integrator)

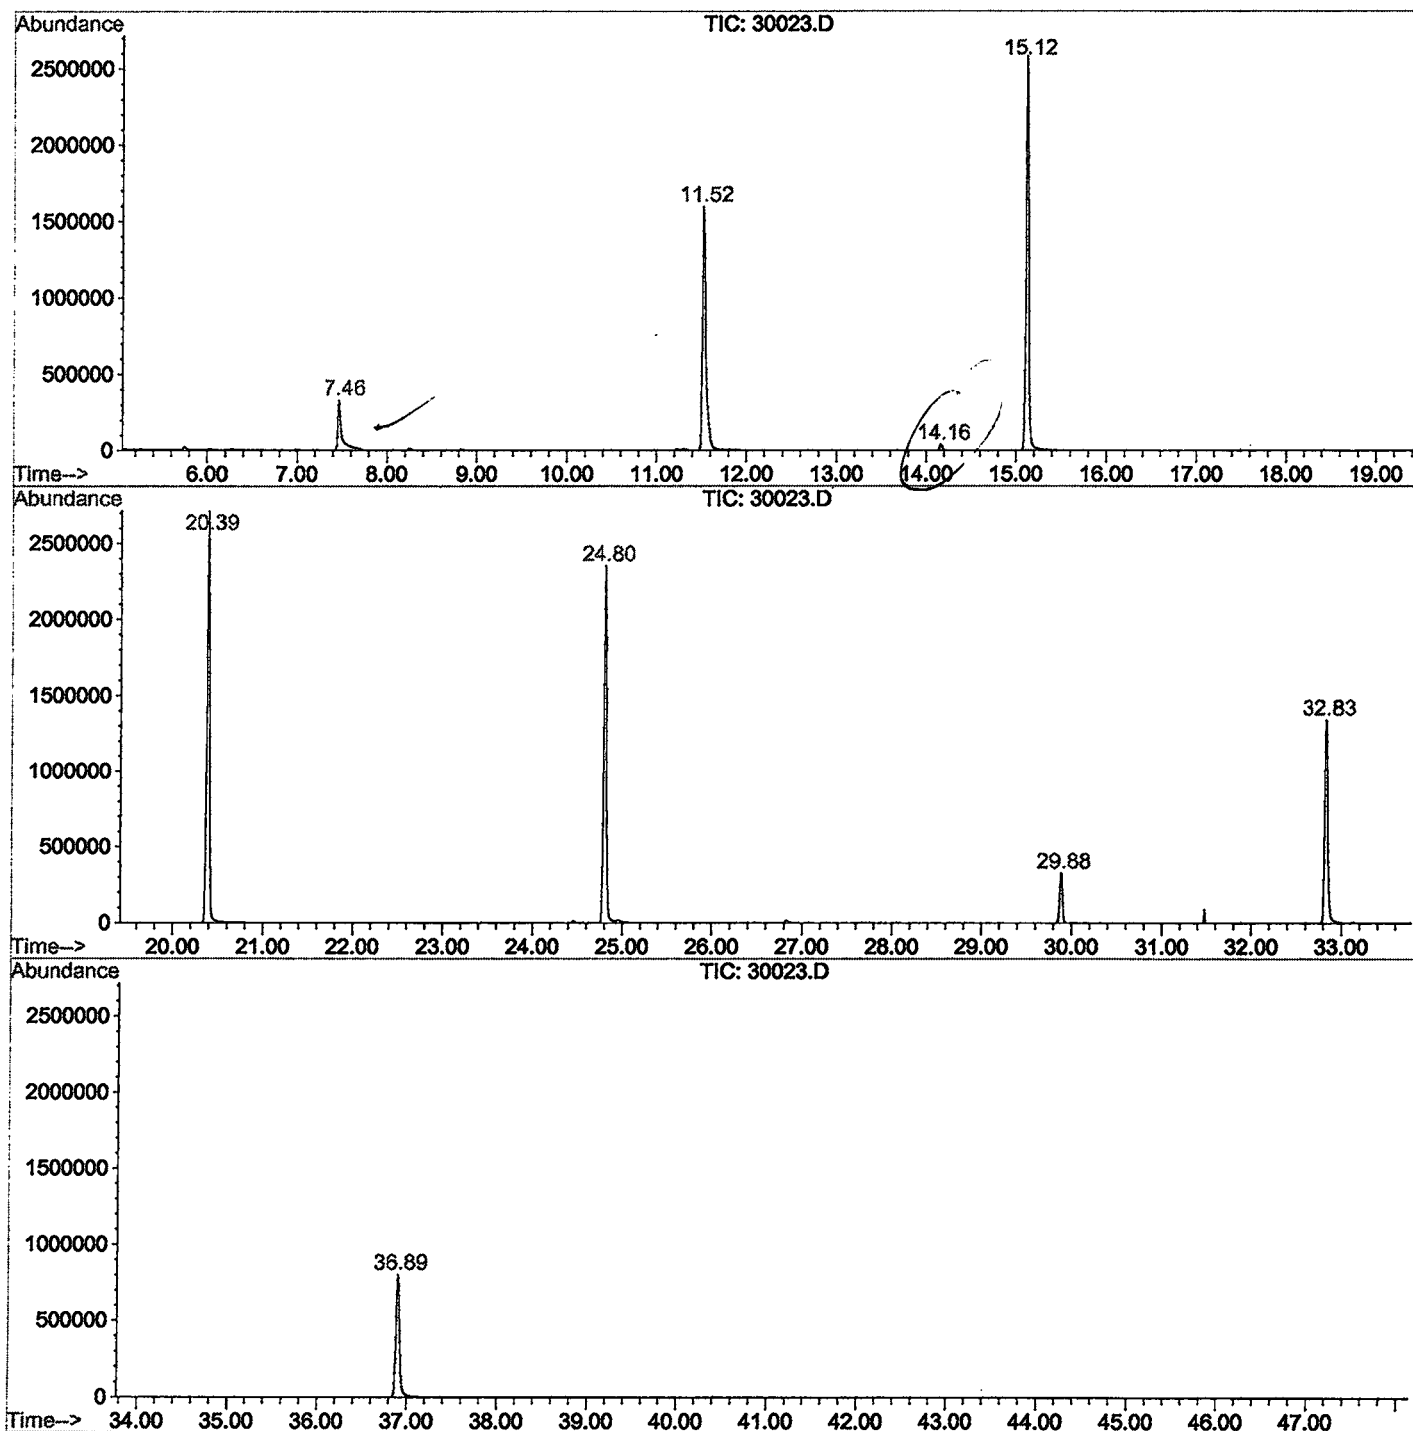

30023.D GCMS1126.M

Mon Jan 07 11:45:53 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\JAN0302\30023.D
 Acq On : 4 Jan 2002 9:36 pm
 Sample : gcms scan 1/2a
 Misc :
 MS Integration Params: LSCINT.P










Vial: 37
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 3-Pentanol, 3-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.46	4.72 ug/l	990590	1,4-Dichlorobenzene-d4	11.52

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	36
2			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
3			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	9
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	9

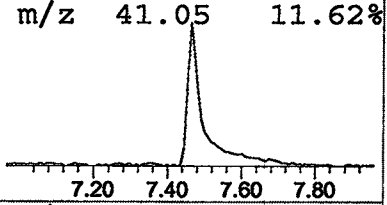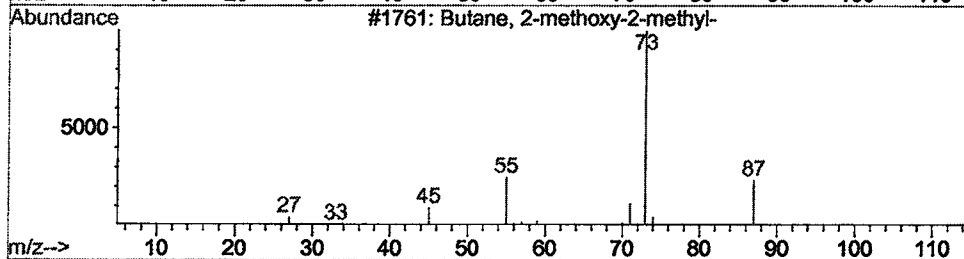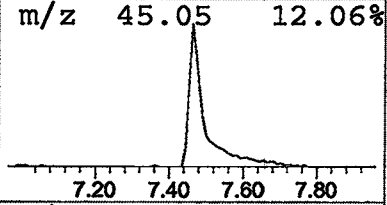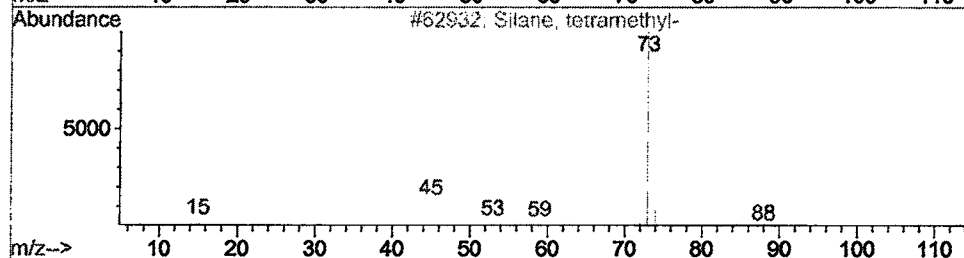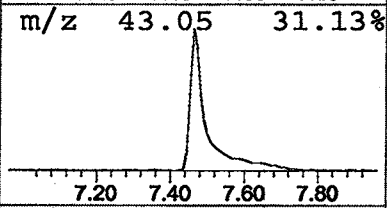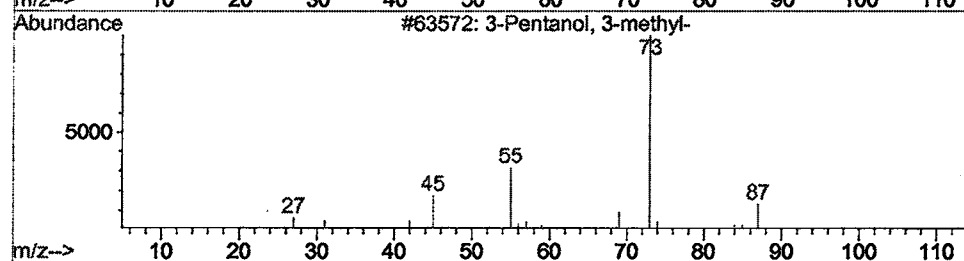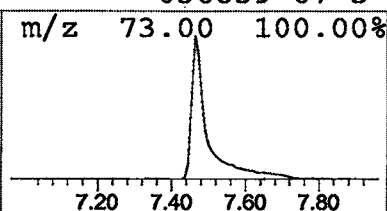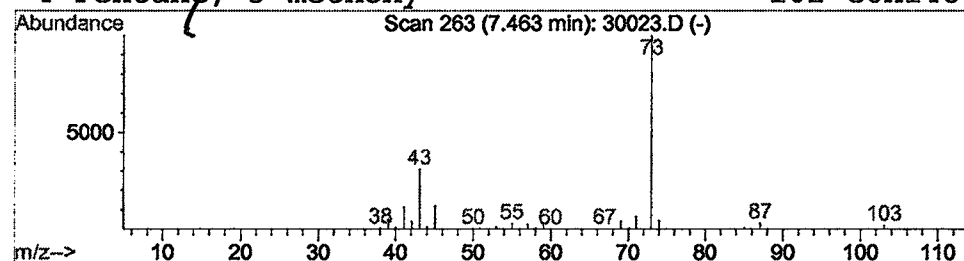

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 4 Jan 2002 9:36 pm
 Data File: C:\HPCHEM\1\DATA\JAN0302\30023.D
 Name: gcms scan 1/2a
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
----- 3-Pentanol , 3-methyl	7.46	4.7	ug/l	990590	ISTD01	11.52	4196020	20.0

30023.D GCMS1126.M Mon Jan 07 11:46:02 2002