

Method 508 modified Date Extracted 12/17/01

Page 67

#GCMS-16362

REF

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spt add	IS add	Final vol.	T.V. pos.	pH	Count		
✓ LB ✓		500 mL		1 mL			1 mL	3B	7			
✓ REF					5 mL			3A				
✓ 30601 ✓								5A				
✓ 30602 ✓								2A				
✓ 30603 ✓								9B				
✓ 30604 ✓								4B				
✓ 30605 *	dried out							4A				
✓ 30607 ✓								6A				
✓ 30608 ✓								5B				
✓ 30631 ✓	1/2/02 restructure							7A				
✓ 30632 ✓								7B				
✓ 30633 ✓								8A				
✓ 30634 ✓								6B				
Remarks: Sample # 30605 dried out so it has to be re-extracted.												
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate -												
Extraction type <u>SUP FM</u> Solv. lot# <u>N39466</u> NaCl lot# <u>V11599</u> Na2SO4 lot# <u>V39H00</u>												
STANDARD	INT STD LOG#											
CALIBRATION												
REF SPIKE	91759											
MDL/MDRF												
Q. CHECK												
INT. STD.												
SURROGATE	GCMS 12/11/01											
LPC												
ENDRIN/DDT												

Reviewed by,
CB 5/15/02

Analyst EH/AD
revision 4/12/01

Verified by _____

Reviewed by
Date 1/22/02

Sequence Name: C:\HPCHEM\1\SEQUENCE\Dec2701.S

Comment: INST 209; 30Mx0.25umX0.50

Operator: 209 GALOS

Data Path: C:\HPCHEM\1\data\dec2701\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run	On A Barcode Mismatch
(X) Full Method	(X) Inject Anyway
() Reprocessing Only	() Don't Inject

Line Type	Vial	DataFile	Method	Sample Name
1 Sample	1	DFTPP	GCMS1126	
2 Sample	2	CAL100	GCMS1126	
3 Sample	3	LB	GCMS1126	GC/MS SCAN 12/12
4 Sample	4	LBA	GCMS1126	GC/MS SCAN 12/13
5 Sample	4	REF	GCMS1126	GC/MS SCAN 12/13
6 Sample	5	30425	GCMS1126	GC/MS SCAN 12/13
7 Sample	6	30354	GCMS1126	GC/MS SCAN 12/13
8 Sample	35	SURR	GCMS1126	GC/MS SCAN 12/13
9 Sample	7	30355	GCMS1126	GC/MS SCAN 12/13
10 Sample	8	30251	GCMS1126	GC/MS SCAN 12/13
11 Sample	9	30023	GCMS1126	GC/MS SCAN 12/13
12 Sample	10	26477	GCMS1126	GC/MS SCAN 12/13
13 Sample	11	26827	GCMS1126	GC/MS SCAN 12/13
14 Sample	12	30009	GCMS1126	GC/MS SCAN 12/12A
15 Sample	13	30010	GCMS1126	GC/MS SCAN 12/12A
16 Sample	14	30110	GCMS1126	GC/MS SCAN 12/12A
17 Sample	15	30111	GCMS1126	GC/MS SCAN 12/12A
18 Sample	16	30107	GCMS1126	GC/MS SCAN 12/12A
19 Sample	17	30353	GCMS1126	GC/MS SCAN 12/13
20 Sample	18	30357	GCMS1126	GC/MS SCAN 12/13
21 Sample	19	30352	GCMS1126	GC/MS SCAN 12/13
22 Sample	20	30351	GCMS1126	GC/MS SCAN 12/13
23 Sample	21	30356	GCMS1126	GC/MS SCAN 12/13
24 Sample	1	DFTPP1	GCMS1126	
25 Sample	22	30252	GCMS1126	GC/MS SCAN 12/13
26 Sample	2	CAL100A	GCMS1126	
27 Sample	23	30426	GCMS1126	GC/MS SCAN 12/13
28 Sample	24	LBB	GCMS1126	GC/MS SCAN 12/17
29 Sample	25	30631	GCMS1126	GC/MS SCAN 12/17
30 Sample	26	30632	GCMS1126	GC/MS SCAN 12/17
31 Sample	27	30633	GCMS1126	GC/MS SCAN 12/17
32 Sample	28	30634	GCMS1126	GC/MS SCAN 12/17
33 Sample	29	30601	GCMS1126	GC/MS SCAN 12/17
34 Sample	30	30602	GCMS1126	GC/MS SCAN 12/17
35 Sample	31	30603	GCMS1126	GC/MS SCAN 12/17
36 Sample	32	30608	GCMS1126	GC/MS SCAN 12/17
37 Sample	33	30607	GCMS1126	GC/MS SCAN 12/17
38 Sample	34	30604	GCMS1126	GC/MS SCAN 12/17
39 Sample	36	29563	GCMS1126	GC/MS SCAN 12/7
40 Sample	37	29523	GCMS1126	GC/MS SCAN 12/7
41 Sample	1	DFTPP2	GCMS1126	
42 Sample	4	REFA	GCMS1126	GC/MS SCAN 12/13

Last Modified: Fri Dec 28 16:44:24 2001

Page: 1

DFTPP

Data File : C:\HPCHEM\1\DATA\JAN0302\DFTPP.D

Acq On : 3 Jan 2002 9:35 am

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0103.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

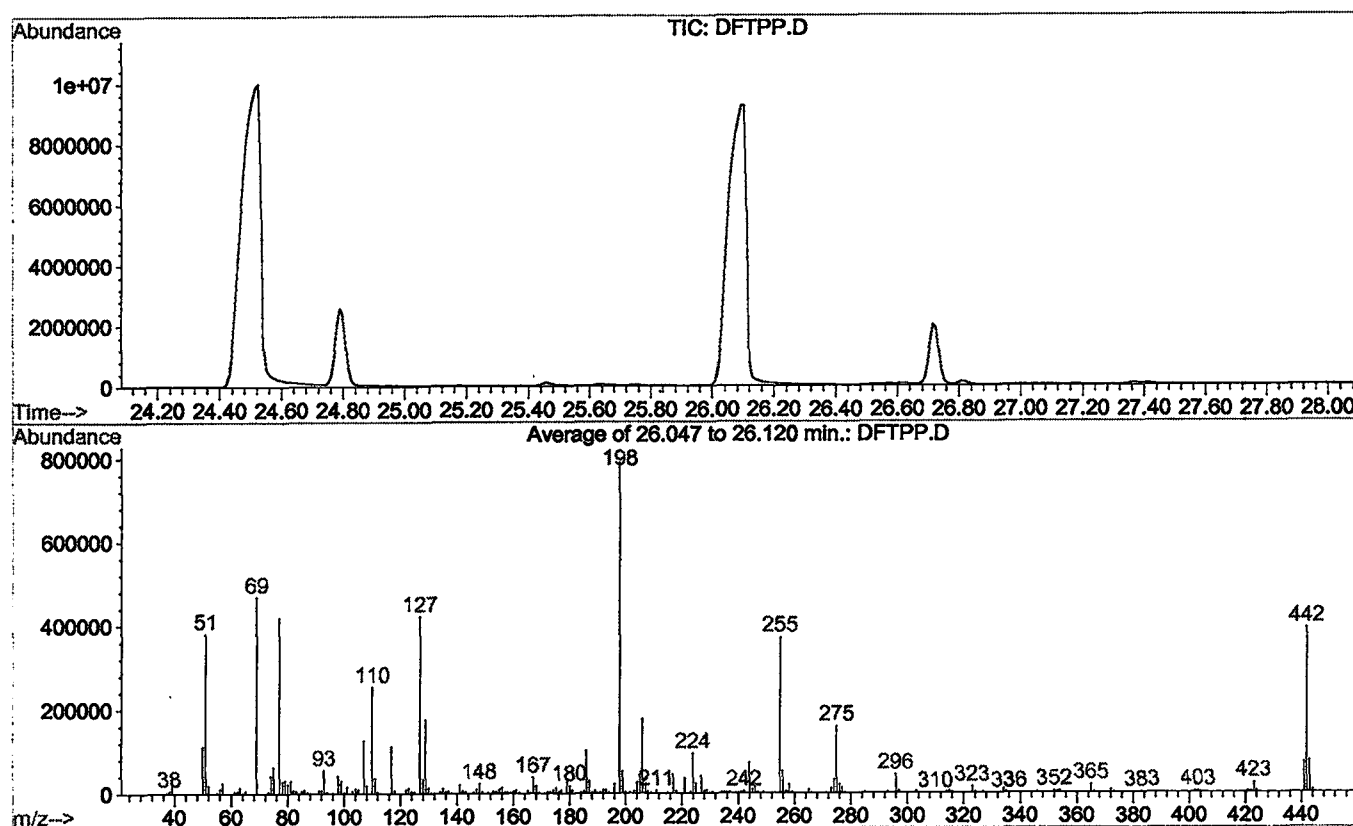

Spectrum Information: Average of 26.047 to 26.120 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	48.3	381035	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	59.5	469099	PASS
70	69	0.00	2	0.0	211	PASS
127	198	40	60	53.5	422351	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	788713	PASS
199	198	5	9	6.7	52678	PASS
275	198	10	30	20.3	160060	PASS
365	198	1	100	2.6	20380	PASS
441	443	0.01	100	94.8	72500	PASS
442	198	40	110	49.6	391054	PASS
443	442	17	23	19.6	76478	PASS

DFTPP.D GCMS0103.M

Thu Jan 10 09:56:04 2002