

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 01/22/2002 Time: 12:10:47

Sample: AD30631

Analysis: \$GCMS GCMS Scan For Unknowns

Units: ug

Started: 1/22/02 12:10 Ended: 1/22/02 12:10 Analyst: DLV

Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		81		5.0

Comments for Sample AD30631 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 01-22-2002 Time: 12:11:08

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report

(Not Reviewed)

Data File : C:\HPCHEM\1\DATA\JAN0302\30631.D

Vial: 30

Acq On : 4 Jan 2002 2:46 pm

Operator: 209 GALOS

Sample : gcms scan 1/2

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Jan 4 15:35 2002

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 28 15:11:00 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.53	152	652724	20.00	ug/l	-0.17
10) Naphthalene-d8	15.12	136	2555253	20.00	ug/l	-0.19
17) Acenaphthene-d10	20.39	164	1278051	20.00	ug/l	-0.19
29) Phenanthrene-d10	24.81	188	1763157	20.00	ug/l	-0.19
38) Chrysene-d12	32.83	240	983807	20.00	ug/l	-0.20
44) Perylene-d12	36.90	264	560709	20.00	ug/l	-0.22

System Monitoring Compounds

37) 2,4-DDD	29.88	235	78443	4.05	ug/mL	-0.19
Spiked Amount	5.000		Recovery	=	81.00%	

Target Compounds

				Qvalue
2) N-nitroso-dimethyl amine	5.11	74	104	N.D.
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.
9) Hexachloroethane	0.00	117	0	N.D.
11) Nitrobenzene	0.00	77	0	N.D.
12) Isophorone	0.00	82	0	N.D.
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.
15) Naphthalene	15.18	128	991	N.D.
16) Hexachlorobutadiene	0.00	225	0	N.D.
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.
19) 2-Chloronaphthalene	0.00	162	0	N.D.
20) Dimethylphthalate	0.00	163	0	N.D.
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.
22) Acenaphthylene	0.00	152	0	N.D.
23) Acenaphthene	0.00	153	0	N.D.
24) 2,4-Dinitrotoluene	20.70	165	363	N.D.
25) Diethylphthalate	21.92	149	511	N.D.
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.
27) Fluorene	0.00	166	0	N.D.
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.

(#)=qualifier out of range (m)=manual integration

30631.D GCMS0103.M Thu Jan 10 12:18:23 2002

Page 1

Data File : C:\HPCHEM\1\DATA\JAN0302\30631.D

Vial: 30

Acq On : 4 Jan 2002 2:46 pm

Operator: 209 GALOS

Sample : gcms scan 1/2

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Jan 4 15:35 2002

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 28 15:11:00 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	24.81	178	576	N.D.		
34) Anthracene	24.81	178	576	N.D.		
35) Di-n-butylphthalate	26.83	149	2245	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	32.83	228	2360	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.13	149	917	N.D.		
43) Chrysene	32.83	228	2360	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	36.90	252	2195	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

30631.D GCMS0103.M

Thu Jan 10 12:18:26 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\JAN0302\30631.D
Acq On : 4 Jan 2002 2:46 pm
Sample : gcms scan 1/2
Misc :
MS Integration Params: GOOFY.P
Quant Time: Jan 4 15:35 2002

Vial: 30
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS1126.RES

Method : C:\HPCHEM\1\METHODS\GCMS0103.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Mon Jan 07 10:31:02 2002
Response via : Initial Calibration

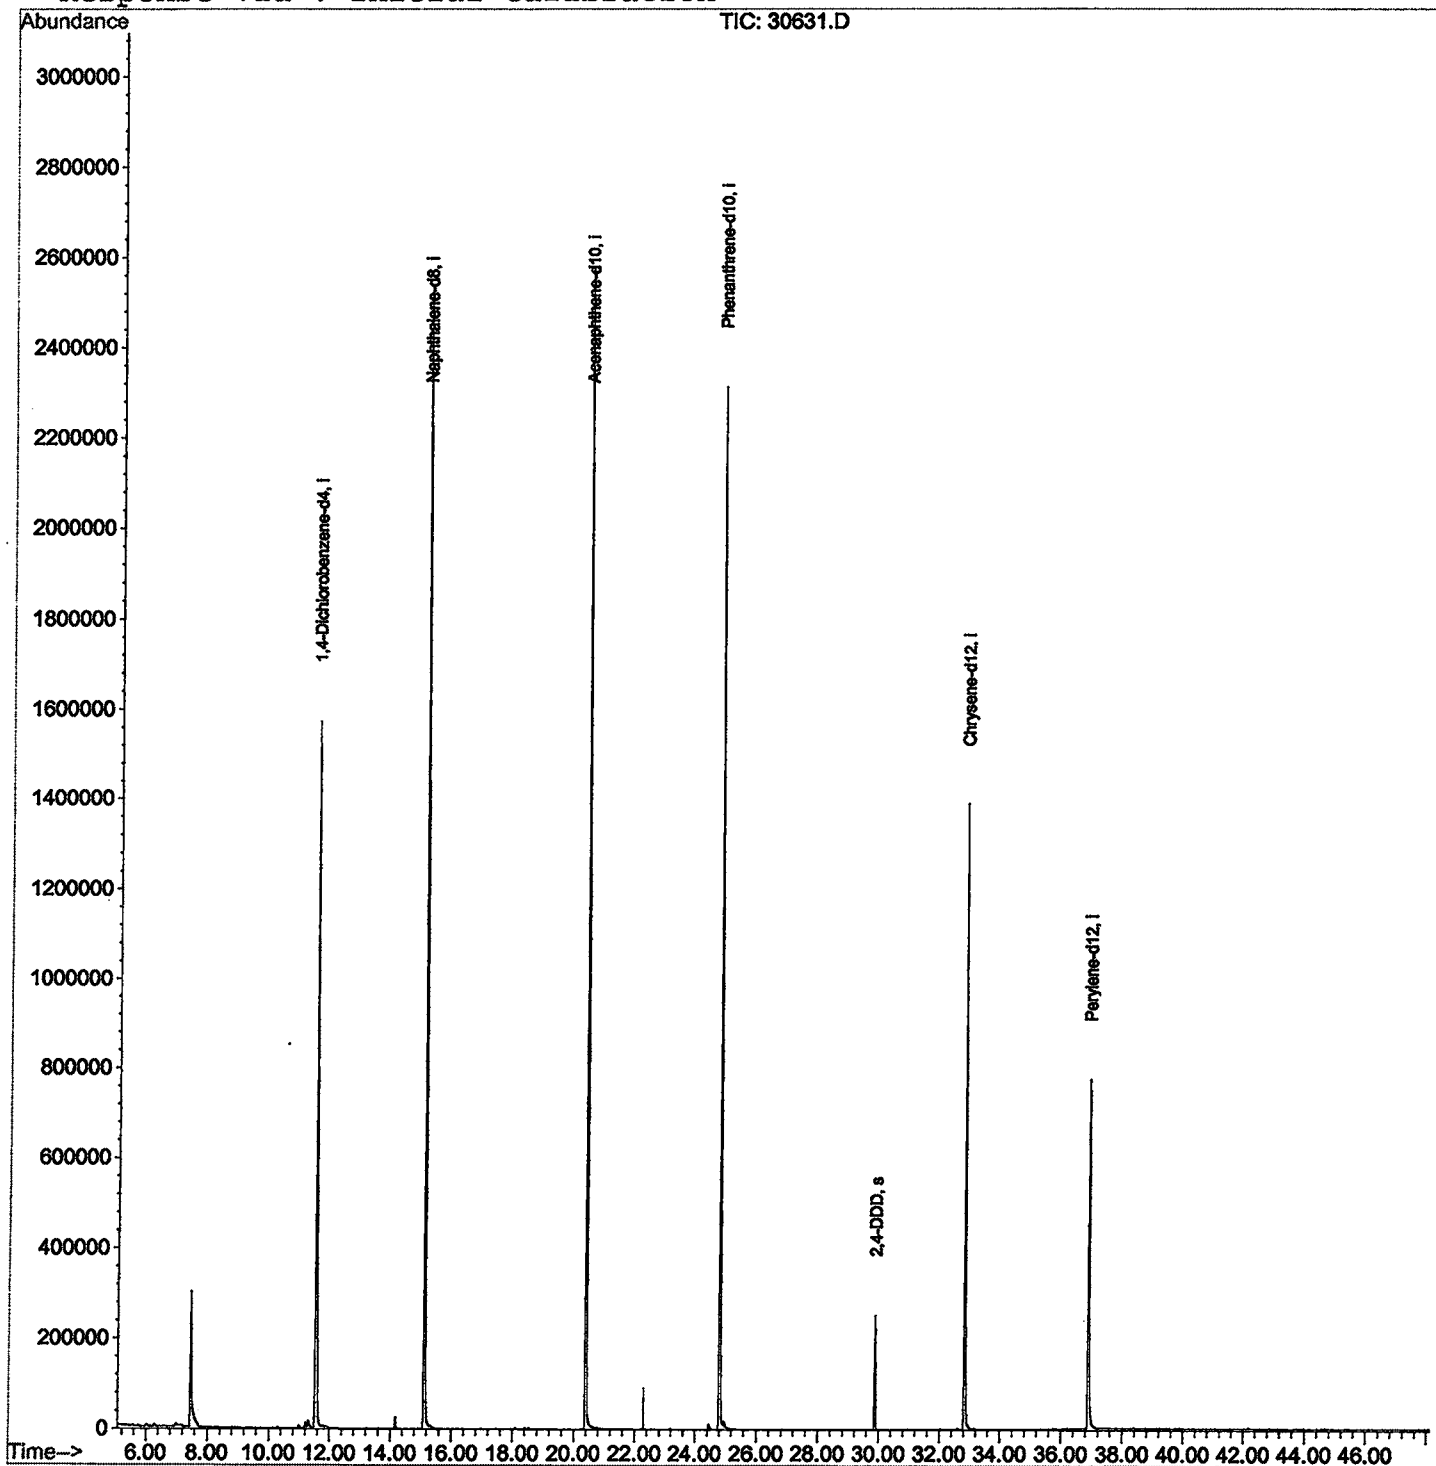

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\JAN0302\30631.D

Acq On : 4 Jan 2002 2:46 pm

Sample : gcms scan 1/2

Misc :

MS Integration Params: LSCINT.P

Vial: 30

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	7.465	260	264	300	rBV	299906	893248	16.59%	3.404%
2	11.523	701	706	726	rBV	1572646	4105621	76.24%	15.645%
3	15.121	1093	1098	1117	rBV	2516916	5200753	96.58%	19.818%
4	20.391	1666	1672	1693	rBV	2579966	5384881	100.00%	20.520%
5	24.806	2147	2153	2166	rBV2	2313525	4945670	91.84%	18.846%
6	29.883	2701	2706	2711	rBV	253760	483127	8.97%	1.841%
7	32.830	3021	3027	3045	rBV2	1389444	3149566	58.49%	12.002%
8	36.897	3464	3470	3488	rBV	773423	2079566	38.62%	7.924%


Sum of corrected areas: 26242432

30631.D GCMS1126.M

Thu Jan 10 10:50:44 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\JAN0302\30631.D
Operator : 209 GALOS
Acquired : 4 Jan 2002 2:46 pm using AcqMethod GCMS1126
Instrument : GC/MS 209
Sample Name: gcms scan 1/2
Misc Info :
Vial Number: 30
Quant File : GCMS1126.RES (RTE Integrator)

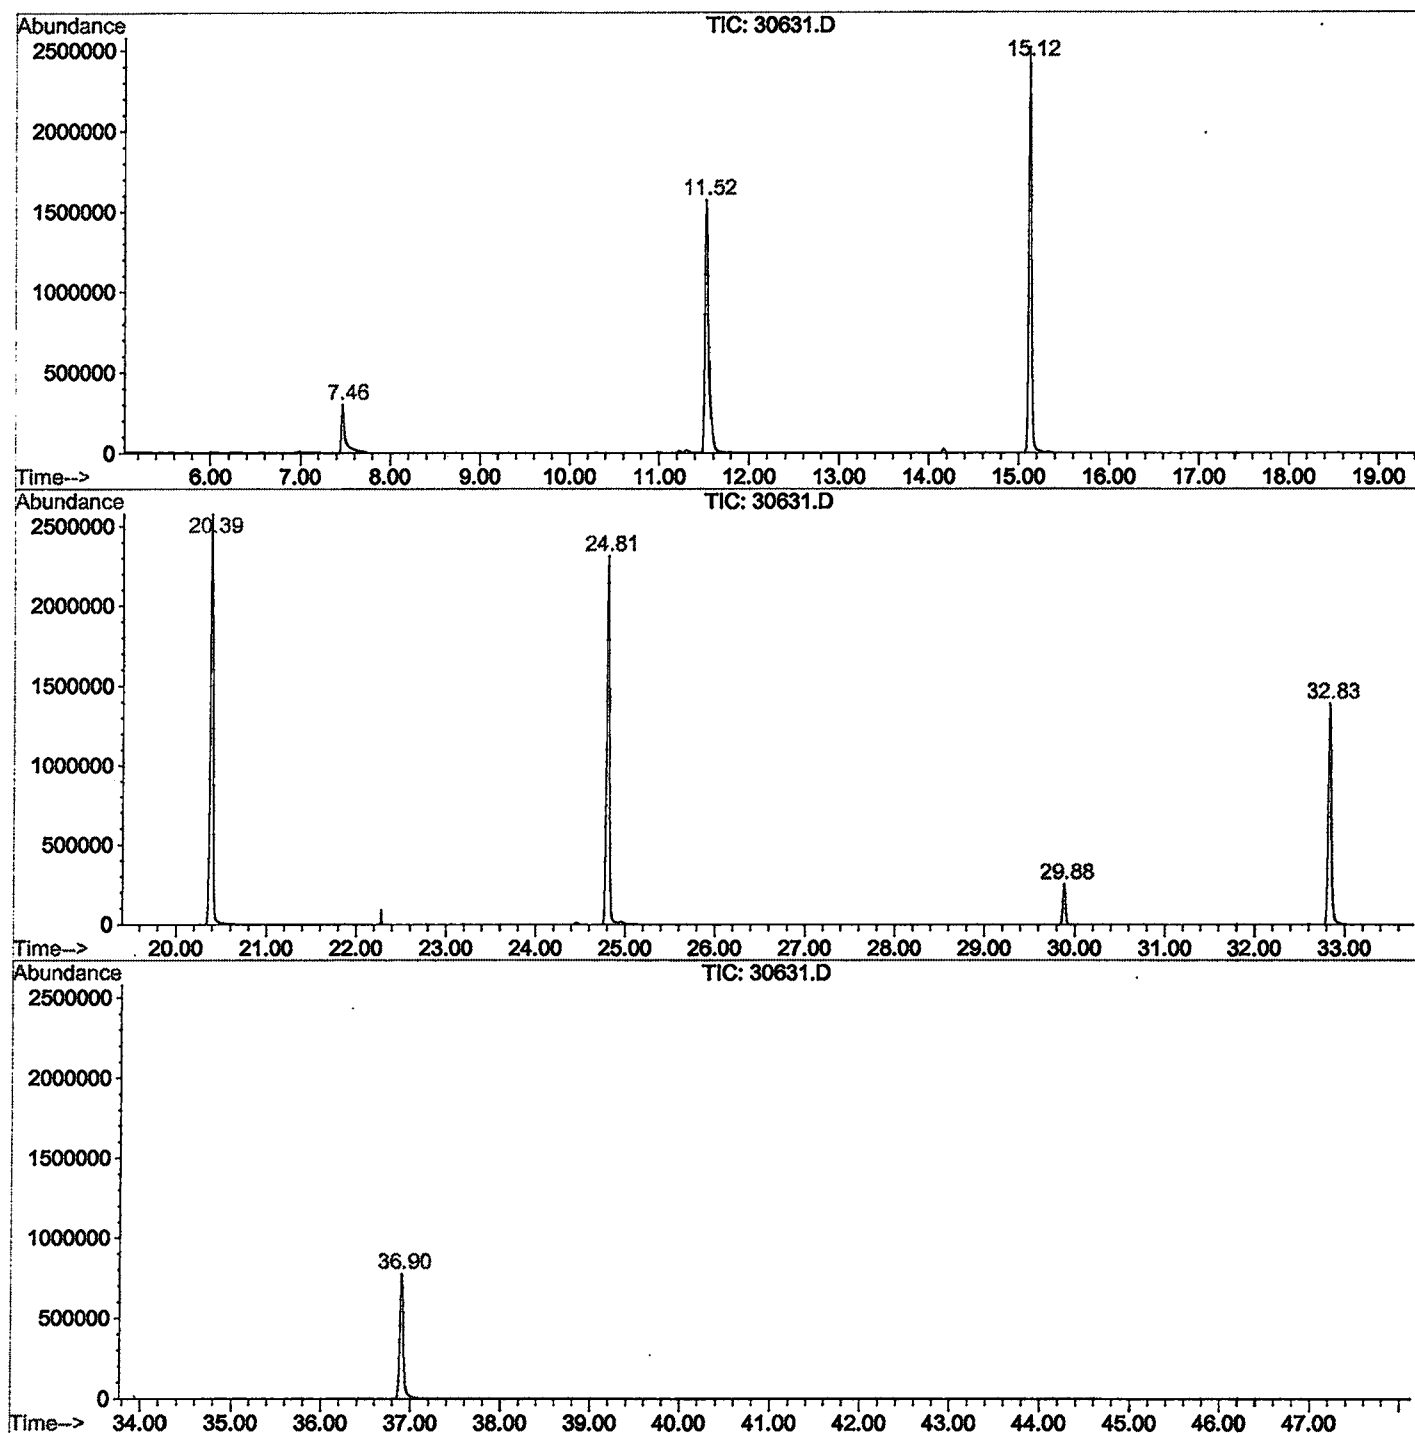

30631.D GCMS1126.M

Thu Jan 10 10:50:50 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\JAN0302\30631.D
 Acq On : 4 Jan 2002 2:46 pm
 Sample : gcms scan 1/2
 Misc :
 MS Integration Params: LSCINT.P










Vial: 30
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 3-Pentanol, 3-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.46	4.35 ug/l	893248	1,4-Dichlorobenzene-d4	11.53

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	33
2			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
3			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	9
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	9

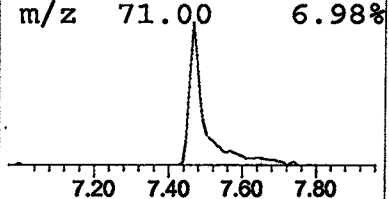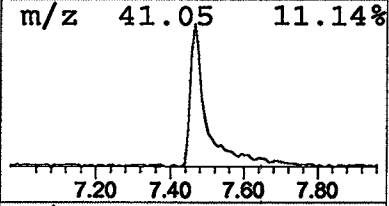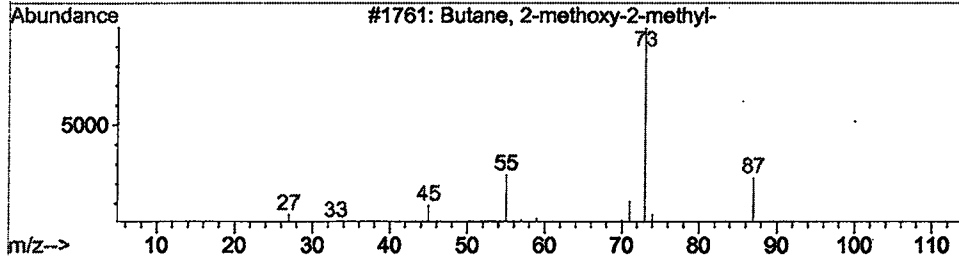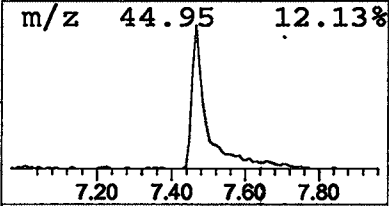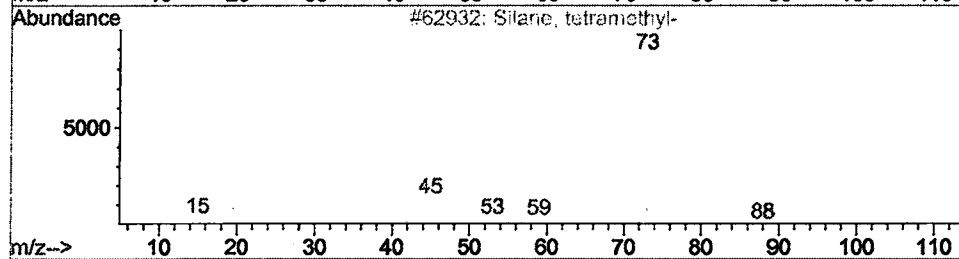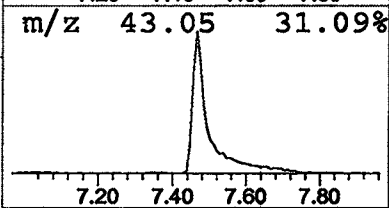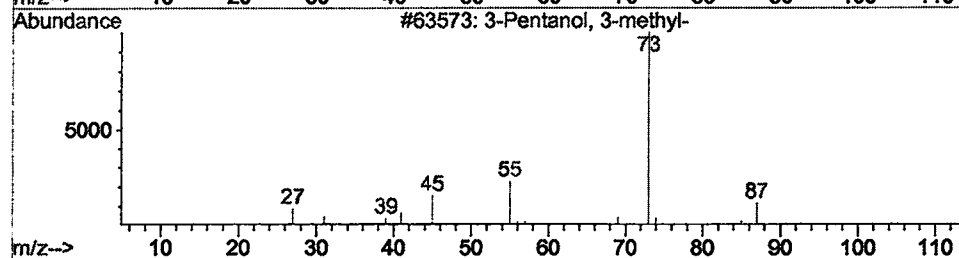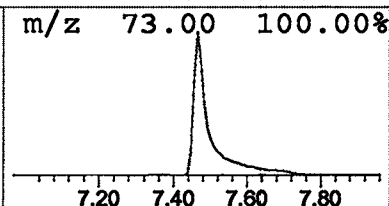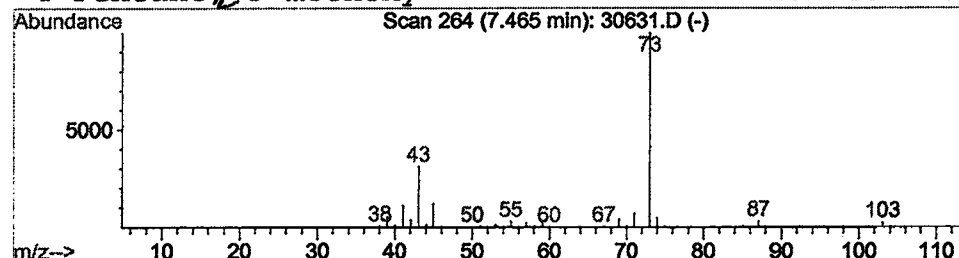

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 4 Jan 2002 2:46 pm
Data File: C:\HPCHEM\1\DATA\JAN0302\30631.D
Name: gcms scan 1/2
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
3-Pentanol , 3-methyl	7.46	4.4	ug/l	893248	ISTD01	11.53	4105620	20.0

30631.D GCMS1126.M Thu Jan 10 10:51:00 2002