

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 01/22/2002 Time: 12:15:42

Sample: AD30632
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 1/22/02 12:15 Ended: 1/22/02 12:15 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		90		5.0

Comments for Sample AD30632 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 01-22-2002 Time: 12:15:46

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Data File : C:\HPCHEM\1\DATA\JAN0302\30632.D

Acq On : 4 Jan 2002 11:51 am

Sample : gcms scan 1/2

Misc :

MS Integration Params: GOOFY.P

Quant Time: Jan 4 12:39 2002

Vial: 27

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 28 15:11:00 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	11.52	152	618530	20.00	ug/l	-0.18
10) Naphthalene-d8	15.12	136	2452798	20.00	ug/l	-0.18
17) Acenaphthene-d10	20.39	164	1236829	20.00	ug/l	-0.18
29) Phenanthrene-d10	24.81	188	1690288	20.00	ug/l	-0.18
38) Chrysene-d12	32.83	240	914518	20.00	ug/l	-0.20
44) Perylene-d12	36.90	264	518801	20.00	ug/l	-0.22

System Monitoring Compounds

37) 2,4-DDD	29.88	235	83616	4.50	ug/mL	-0.19
Spiked Amount	5.000		Recovery	=	90.00%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.18	128	4109	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	20.71	165	289	N.D.	
25) Diethylphthalate	21.92	149	664	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.	

(#) = qualifier out of range (m) = manual integration

30632.D GCMS1126.M

Tue Jan 15 09:46:44 2002

Page 1

Quantitation Report

(Not Reviewed)

Data File : C:\HPCHEM\1\DATA\JAN0302\30632.D

Acq On : 4 Jan 2002 11:51 am

Sample : gcms scan 1/2

Misc :

MS Integration Params: GOOFY.P

Quant Time: Jan 4 12:39 2002

Vial: 27

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 28 15:11:00 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Compound	R.T.	QIon	Response	Conc Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	
32) Hexachlorobenzene	0.00	284	0	N.D.	
33) Phenanthrene	24.87	178	1385	N.D.	
34) Anthracene	24.87	178	1385	N.D.	
35) Di-n-butylphthalate	26.83	149	2562	N.D.	
36) Fluoranthene	0.00	202	0	N.D.	
39) Pyrene	0.00	202	0	N.D.	
40) Butylbenzylphthalate	0.00	149	0	N.D.	
41) Benzo(a)anthracene	32.83	228	2304	N.D.	
42) Bis(2-ethylhexyl)phthalate	33.13	149	1182	N.D.	
43) Chrysene	32.83	228	2304	N.D.	
45) Di-n-Octylphthalate	0.00	149	0	N.D.	
46) Benzo(b)fluoranthene	0.00	252	0	N.D.	
47) Benzo(k)fluoranthene	0.00	252	0	N.D.	
48) Benzo(a)pyrene	36.90	252	2178	N.D.	
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.	
50) Dibenzo(a,h)anthracene	0.00	278	0	N.D.	
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.	

(#) = qualifier out of range (m) = manual integration

30632.D GCMS1126.M Tue Jan 15 09:46:47 2002

Page 2

Quantitation Report

Data File : C:\HPCHEM\1\DATA\JAN0302\30632.D

Vial: 27

Acq On : 4 Jan 2002 11:51 am

Operator: 209 GALOS

Sample : gcms scan 1/2

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Jan 4 12:39 2002


Quant Results File: GCMS1126.RES

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 28 15:11:00 2001

Response via : Initial Calibration

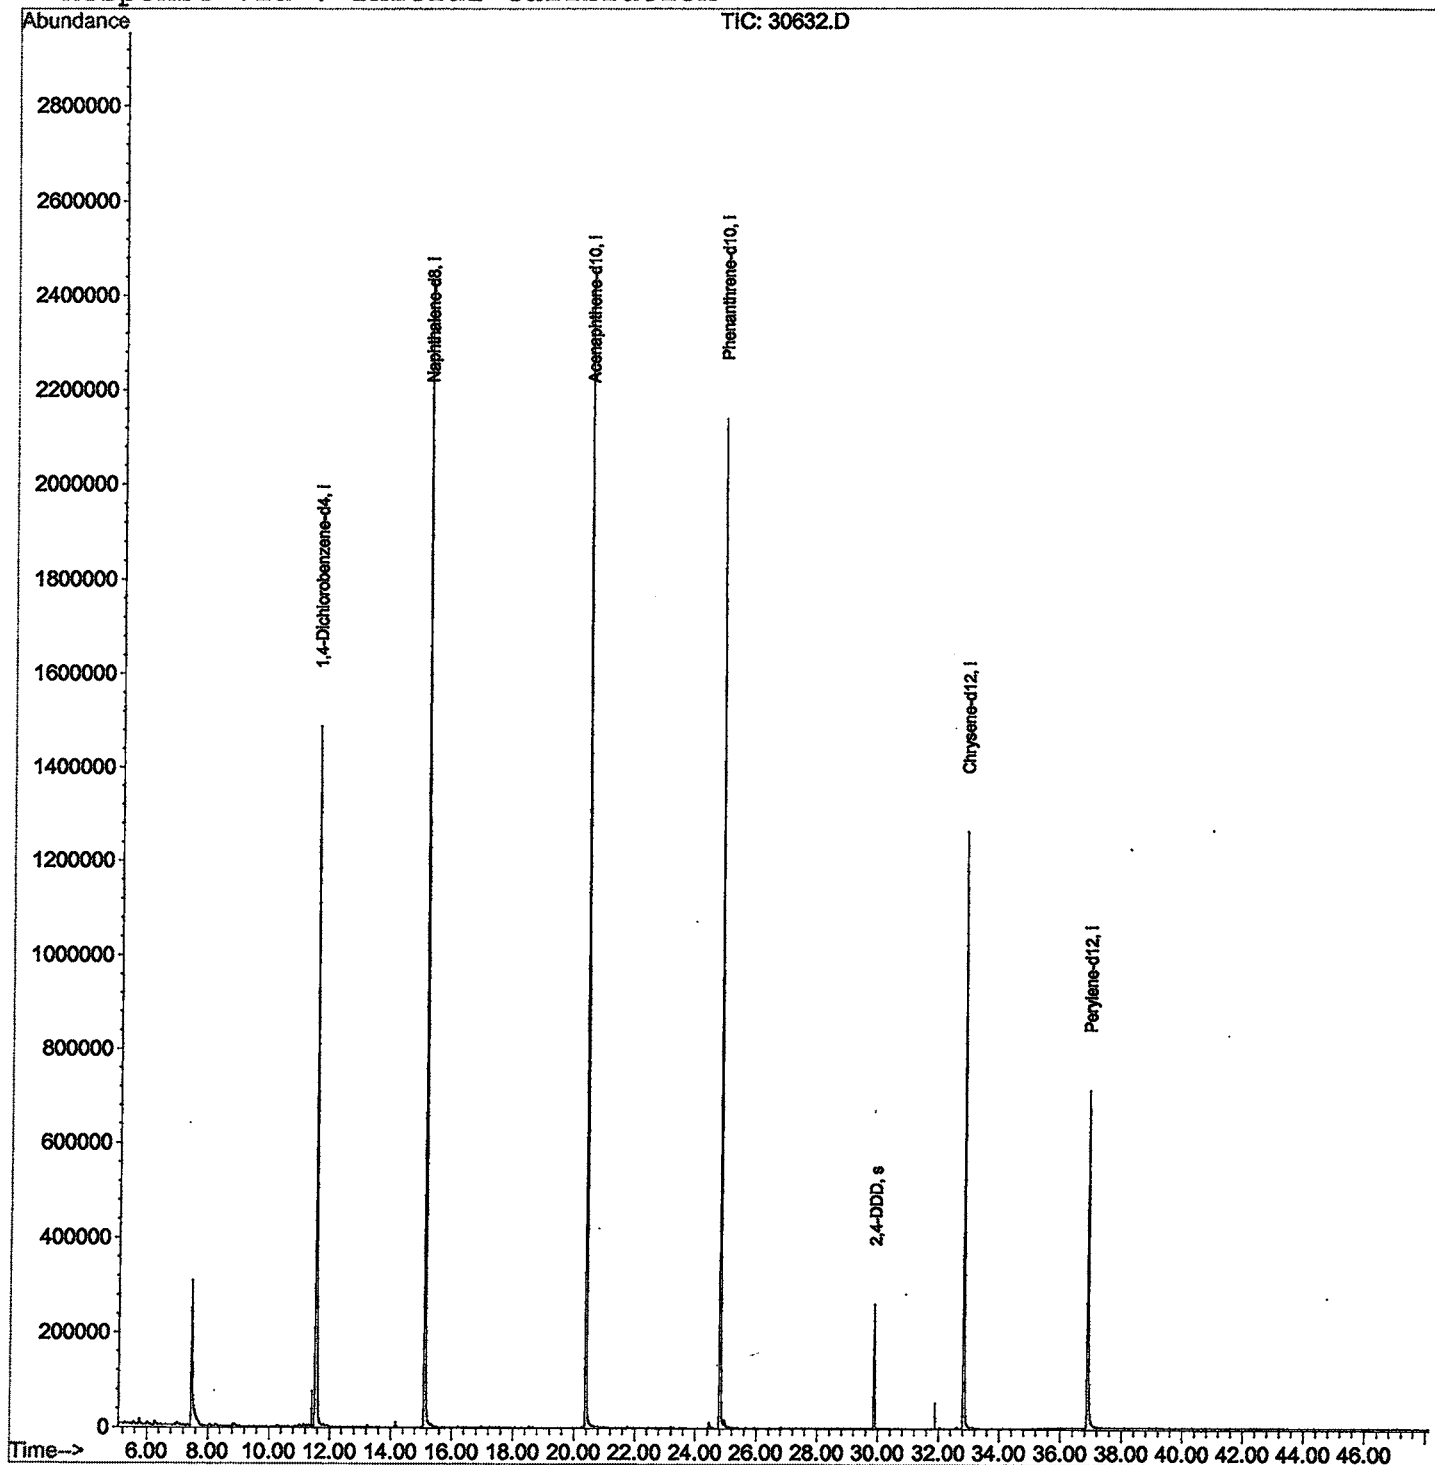

LSC Area Percent Report

, Data File : C:\HPCHEM\1\DATA\JAN0302\30632.D

Vial: 27

Acq On : 4 Jan 2002 11:51 am

Operator: 209 GALOS

Sample : gcms scan 1/2

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	7.465	260	264	288	rBV	306272	903361	17.43%	3.595%
2	11.523	701	706	727	rBV	1486534	3882066	74.91%	15.447%
3	15.122	1092	1098	1116	rBV	2427784	5022270	96.92%	19.984%
4	20.391	1666	1672	1693	rBV	2460743	5181996	100.00%	20.619%
5	24.807	2146	2153	2165	rBV2	2139406	4742627	91.52%	18.871%
6	29.884	2701	2706	2712	rBV	261499	519923	10.03%	2.069%
7	32.830	3021	3027	3044	rBV2	1263191	2941866	56.77%	11.706%
8	36.897	3463	3470	3489	rBV	711008	1937486	37.39%	7.709%


Sum of corrected areas: 25131595

30632.D GCMS1126.M

Tue Jan 15 09:48:15 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\JAN0302\30632.D
 Operator : 209 GALOS
 Acquired : 4 Jan 2002 11:51 am using AcqMethod GCMS1126
 Instrument : GC/MS 209
 Sample Name: gcms scan 1/2
 Misc Info :
 Vial Number: 27
 Quant File : GCMS1126.RES (RTE Integrator)

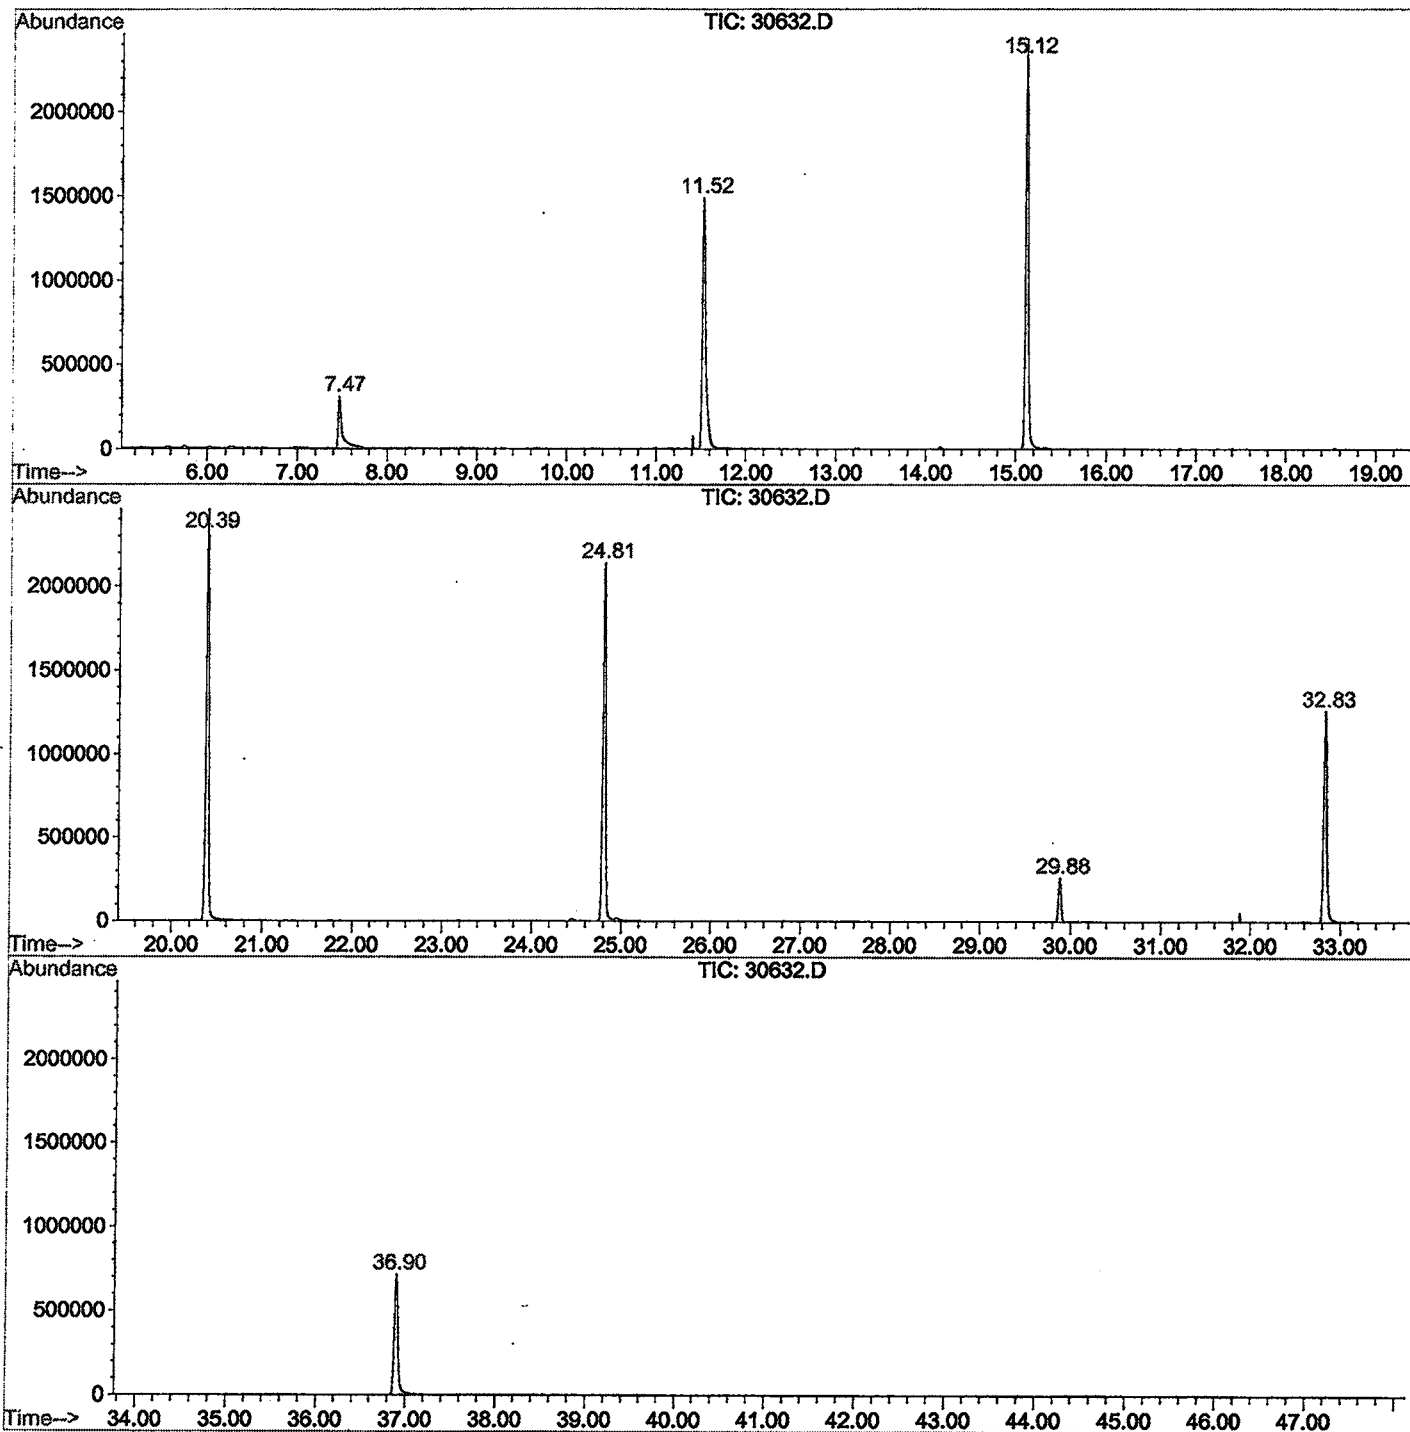

30632.D GCMS1126.M

Tue Jan 15 09:48:21 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\JAN0302\30632.D
 Acq On : 4 Jan 2002 11:51 am
 Sample : gcms scan 1/2
 Misc :
 MS Integration Params: LSCINT.P










Vial: 27
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 Silane, tetramethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.47	4.65 ug/l	903361	1,4-Dichlorobenzene-d4	11.52

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Silane, tetramethyl-	88	C4H12Si	000075-76-3	47
2	1,3-Dioxolane, 2-pentadecyl-	284	C18H36O2	004360-57-0	9
3	3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	9
4	Pentane, 3-methoxy-	102	C6H14O	036839-67-5	9

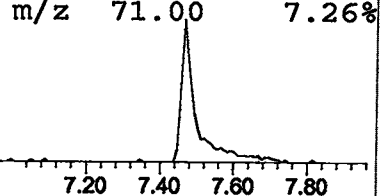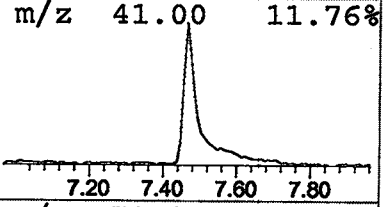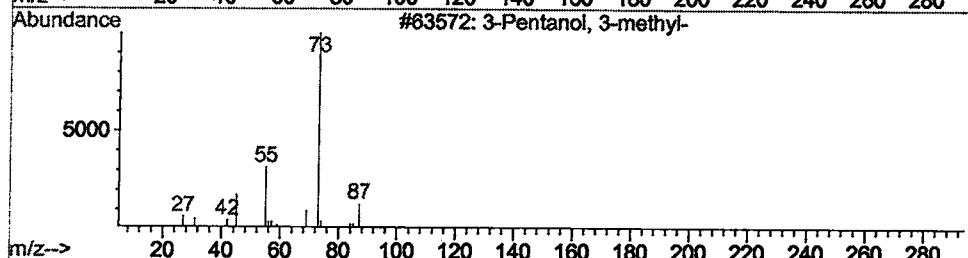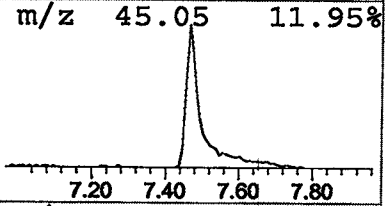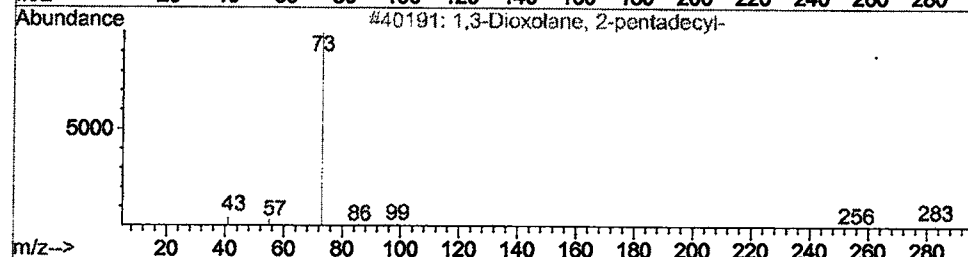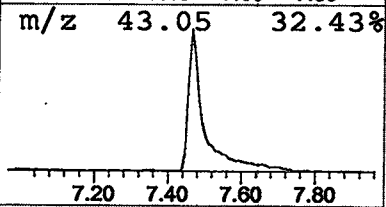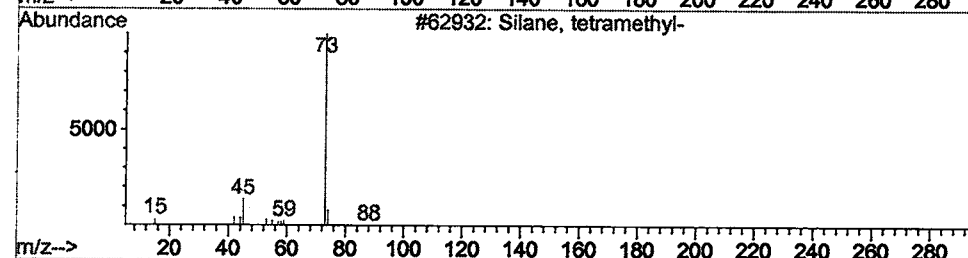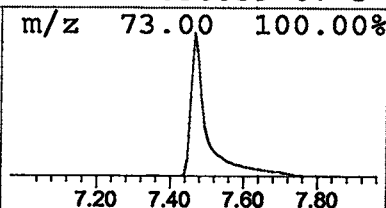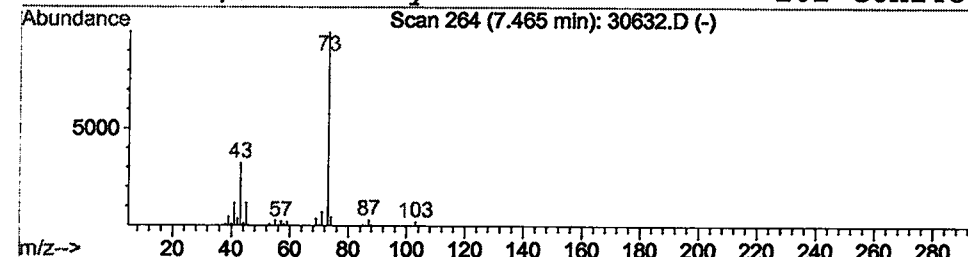

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 4 Jan 2002 11:51 am
 Data File: C:\HPCHEM\1\DATA\JAN0302\30632.D
 Name: gcms scan 1/2
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
Silane, tetramethyl-	7.47	4.7	ug/l	903361	ISTD01	11.52	3882070	20.0

30632.D GCMS1126.M Tue Jan 15 09:48:29 2002