


REF

11/10/2

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC2701\DFTPP3.D
 Acq On : 29 Dec 2001 5:42 pm
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

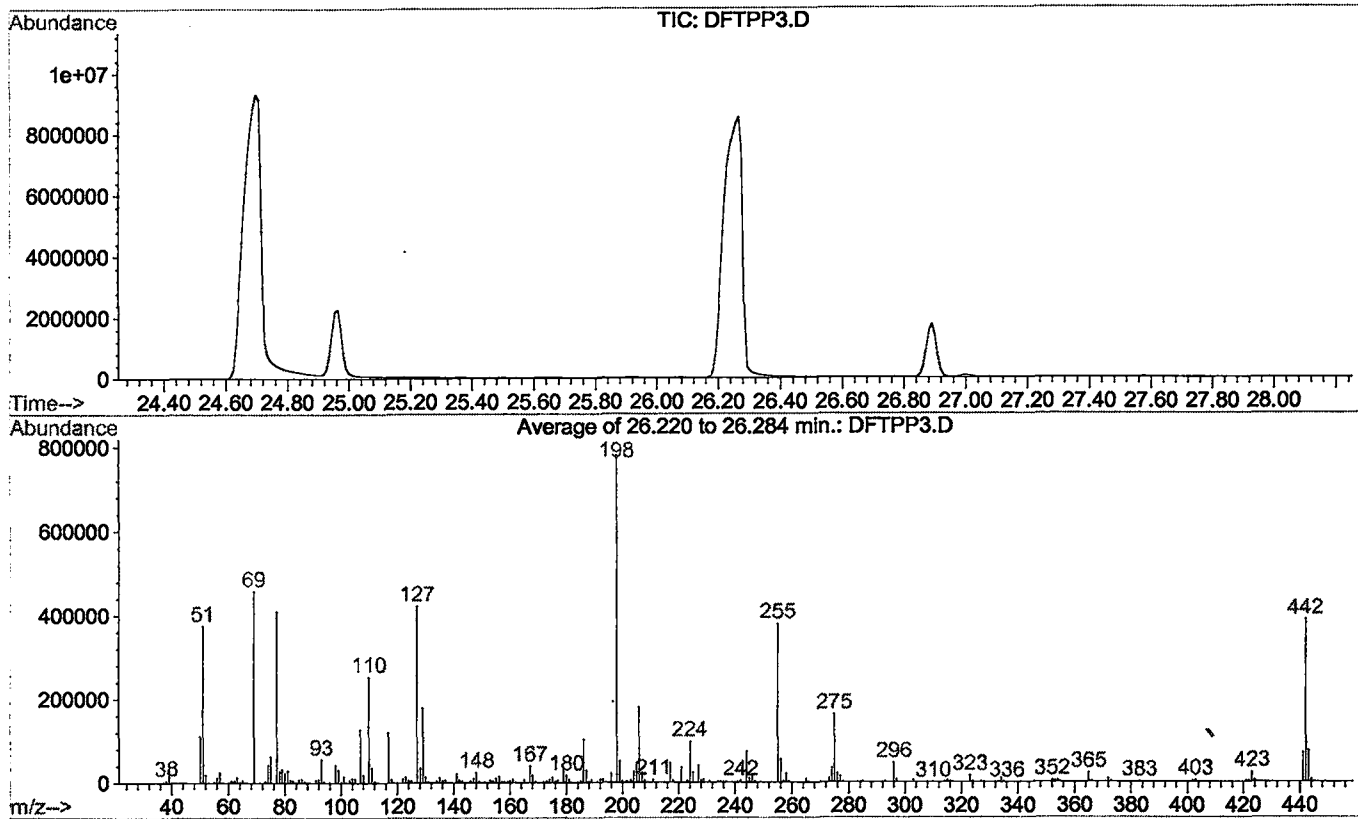

Spectrum Information: Average of 26.220 to 26.284 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	48.2	375534	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	58.8	458633	PASS
70	69	0.00	2	0.1	303	PASS
127	198	40	60	54.2	422724	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	779824	PASS
199	198	5	9	6.7	52272	PASS
275	198	10	30	20.9	163027	PASS
365	198	1	100	2.8	22213	PASS
441	443	0.01	100	93.7	70323	PASS
442	198	40	110	49.6	386776	PASS
443	442	17	23	19.4	75071	PASS

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC2701\DFTPP.D

Acq On : 27 Dec 2001 3:59 pm

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)


Title : 208 625/TCLP calibration table

Vial: 1

Operator: GALOS

Inst : GC/MS Ins

Multiplr: 1.00

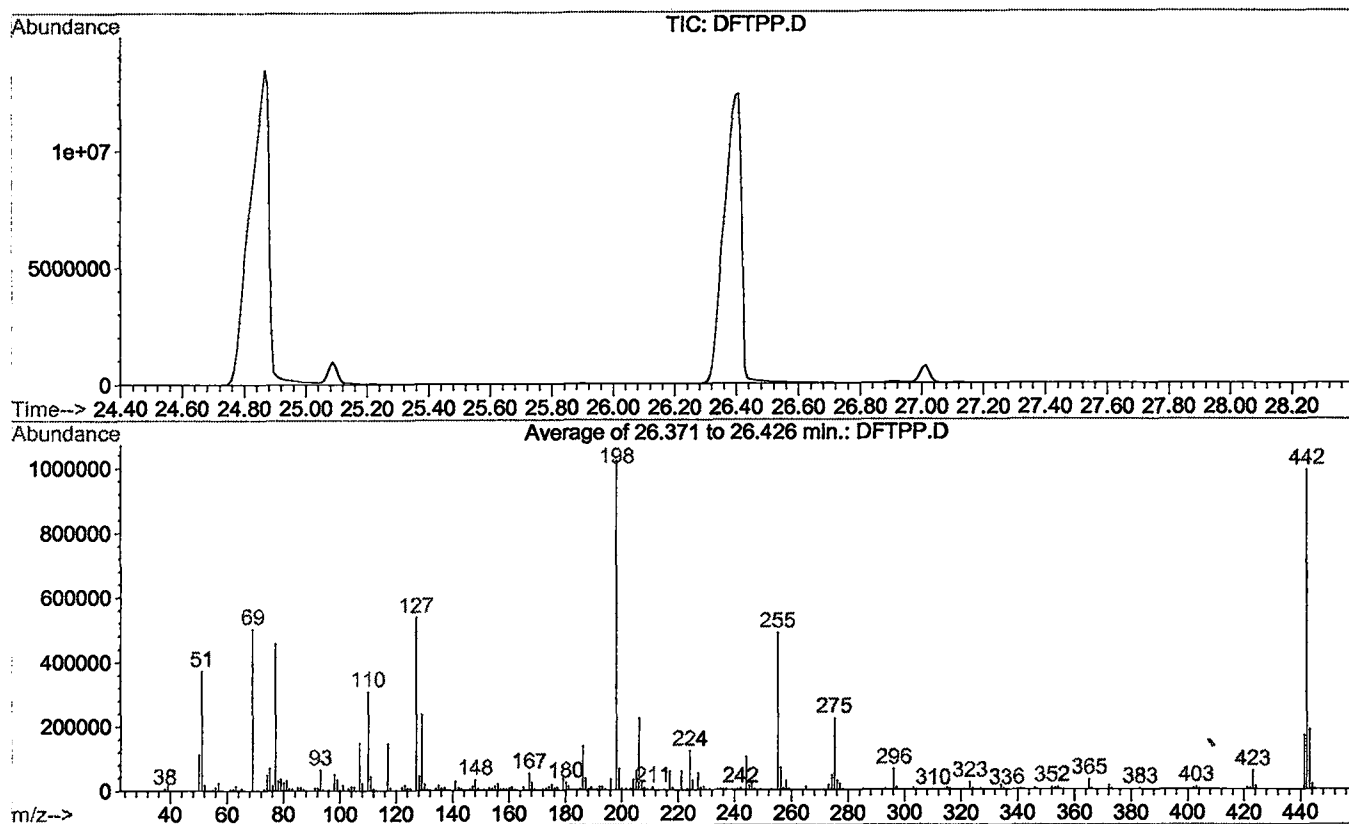

Spectrum Information: Average of 26.371 to 26.426 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	36.6	373589	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	49.3	502614	PASS
70	69	0.00	2	0.0	239	PASS
127	198	40	60	52.7	537166	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	1020144	PASS
199	198	5	9	6.5	66461	PASS
275	198	10	30	21.8	222737	PASS
365	198	1	99	3.0	30790	PASS
441	443	1	99	90.5	166606	PASS
442	198	40	110	97.0	989650	PASS
443	442	17	23	18.6	184048	PASS

DFTPP.D NP112701.M

Fri Dec 28 07:51:01 2001

Sequence Name: C:\HPCHEM\1\SEQUENCE\DEC2701.S

Comment: 208

Operator: GALOS

Data Path: C:\HPCHEM\1\DATA\dec2701\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch

☒ Full Method☒ Inject Anyway☐ Reprocessing Only☐ Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	NP112701	
2	Sample	2	LB	NP112701	gcms unknown 11/27
3	Sample	3	27828	NP112701	gcms unknown 11/27
4	Sample	4	27831	NP112701	gcms unknown 11/27
5	Sample	5	27778	NP112701	gcms unknown 11/27
6	Sample	6	27779	NP112701	gcms unknown 11/27
7	Sample	7	27778A	NP112701	gcms unknown 11/27
8	Sample	8	27779A	NP112701	gcms unknown 11/27
9	Sample	9	27775	NP112701	gcms unknown 11/27
10	Sample	10	27817	NP112701	gcms unknown 11/27
11	Sample	11	27793	NP112701	gcms unknown 11/27
12	Sample	12	27819	NP112701	gcms unknown 11/27
13	Sample	13	27774	NP112701	gcms unknown 11/27
14	Sample	14	27770	NP112701	gcms unknown 11/27