

Method 508 Mod.Date Extracted 12/14/01Page 66

REF

JGCM5-16497

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
L.B. ✓		500 ml		1 ml			1 M		7			
Ref ✓					0.5 ml							
30473 ✓	FB											
30490 ✓	FB											
30471 ✓												
30472 ✓												
30470 ✓												
30484 ✓												
30483 ✓												
30489 ✓												
Remarks												
Reviewed by <u>JS 5/15/02</u>												
drip rate must be between 5-15 ml/min for liq-liq extractors												
Extraction type -		Solv. lot# <u>V39466</u>		NaCl lot# <u>V4599</u>		Na2SO4 lot# <u>V39H00</u>						
STANDARD	INT STD LOG#											
CALIBRATION	<u>HP12601</u>											
REF/SPIKE	<u>91759</u>											
MDL/MDRF												
Q. CHECK												
INT. STD.												
SURROGATE	<u>GCM5 12/14/01</u>											
LPC												
ENDRIN/DDT												

Analyst A.D.
revision 4/12/01Verified by myReviewed by DN
Date 1/24/02

Sequence Name: C:\HPCHEM\1\SEQUENCE\DEC3101.S

Comment: INST 209; 30Mx0.25umX0.50

Operator: 209 GALOS

Data Path: C:\HPCHEM\1\data\dec3101\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run	On A Barcode Mismatch
(X) Full Method	(X) Inject Anyway
() Reprocessing Only	() Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	GCMS1126	
2	Sample	2	CAL40	GCMS1126	
3	Sample	3	SURR	GCMS1126	
4	Sample	4	REF	GCMS1126	gcms scan 12/13
5	Sample	5	LBA	GCMS1126	gcms scan 12/14
6	Sample	6	REFA	GCMS1126	gcms scan 12/14
7	Sample	7	30472	GCMS1126	gcms scan 12/14
8	Sample	8	30484	GCMS1126	gcms scan 12/14
9	Sample	9	30470	GCMS1126	gcms scan 12/14
10	Sample	10	30471	GCMS1126	gcms scan 12/14
11	Sample	11	30489	GCMS1126	gcms scan 12/14
12	Sample	12	30490	GCMS1126	gcms scan 12/14fb
13	Sample	13	30483	GCMS1126	gcms scan 12/14
14	Sample	14	30473	GCMS1126	gcms scan 12/14fb
15	Sample	15	LBC	GCMS1126	gcms scan 12/14a
16	Sample	16	REFC	GCMS1126	gcms scan 12/14a
17	Sample	17	29931	GCMS1126	gcms scan 12/14a
18	Sample	18	30350	GCMS1126	gcms scan 12/14a
19	Sample	19	25874	GCMS1126	gcms scan 12/14a
20	Sample	20	26011	GCMS1126	gcms scan 12/14a
21	Sample	21	30486	GCMS1126	gcms scan 12/14a
22	Sample	22	30487	GCMS1126	gcms scan 12/14a
23	Sample	23	30424	GCMS1126	gcms scan 12/14a
24	Sample	24	30423	GCMS1126	gcms scan 12/14a
25	Sample	25	25946	GCMS1126	gcms scan 12/14a
26	Sample	1	DFTPP1	GCMS1126	
27	Sample	2	CAL40A	GCMS1126	
28	Sample	26	LBD	GCMS1126	gcms scan 12/19
29	Sample	27	REFD	GCMS1126	gcms scan 12/19
30	Sample	28	30713	GCMS1126	gcms scan 12/19
31	Sample	29	30714	GCMS1126	gcms scan 12/19
32	Sample	30	30605	GCMS1126	gcms scan 12/19
33	Sample	31	30694	GCMS1126	gcms scan 12/19
34	Sample	32	30695	GCMS1126	gcms scan 12/19
35	Sample	33	30696	GCMS1126	gcms scan 12/19
36	Sample	34	30711	GCMS1126	gcms scan 12/19
37	Sample	35	30712	GCMS1126	gcms scan 12/19
38	Sample	36	30786	GCMS1126	gcms scan 12/19
39	Sample	37	30983	GCMS1126	gcms scan 12/19
40	Sample	38	30984	GCMS1126	gcms scan 12/19
41	Sample	39	30985	GCMS1126	gcms scan 12/19
42	Sample	40	LBE	GCMS1126	gcms scan 12/19a

Last Modified: Wed Jan 02 16:10:25 2002

Page: 1

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC3101\DFTPP.D

Acq On : 31 Dec 2001 10:52 am

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

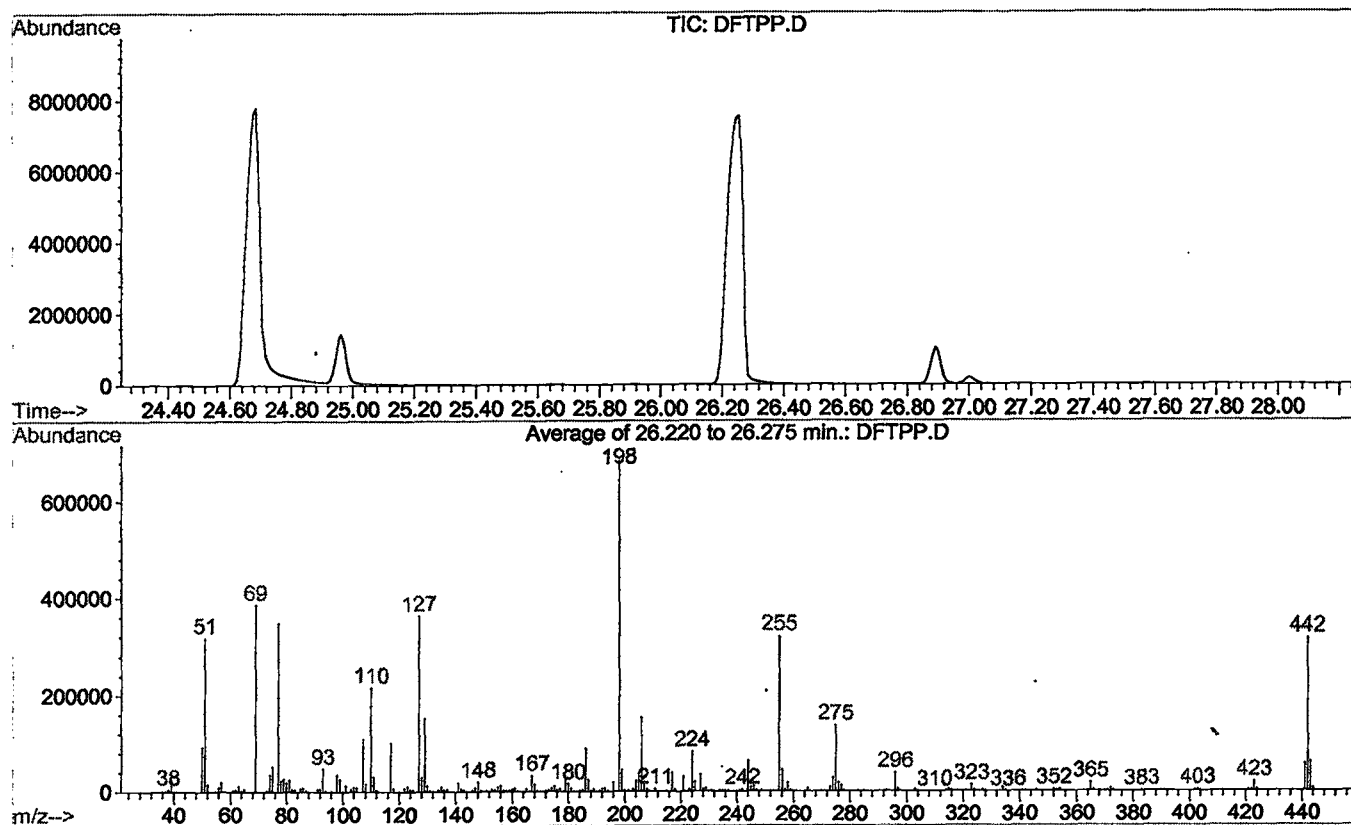

Spectrum Information: Average of 26.220 to 26.275 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	46.6	318011	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	56.6	386587	PASS
70	69	0.00	2	0.0	47	PASS
127	198	40	60	53.2	363176	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	682880	PASS
199	198	5	9	6.6	45188	PASS
275	198	10	30	20.2	137790	PASS
365	198	1	100	2.7	18201	PASS
441	443	0.01	100	93.4	57267	PASS
442	198	40	110	46.4	317102	PASS
443	442	17	23	19.3	61342	PASS

DFTPP.D GCMS1126.M

Mon Dec 31 16:03:21 2001