

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 01/24/2002 Time: 15:44:09

Sample: AD30490
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 1/24/02 15:43 Ended: 1/24/02 15:43 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		109		5.0

Comments for Sample AD30490 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 01-24-2002 Time: 15:44:15

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

The recoveries for 4 of the 43 compounds in the LCS Standard were above their acceptance ranges.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC3101\30490.D

Vial: 12

Acq On : 31 Dec 2001 9:40 pm

Operator: 209 GALOS

Sample : gcms scan 12/14fb

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Jan 15 11:22 2002

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 28 15:11:00 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	11.68	152	870120	20.00	ug/l	-0.02
10) Naphthalene-d8	15.28	136	3429358	20.00	ug/l	-0.03
17) Acenaphthene-d10	20.56	164	1777734	20.00	ug/l	-0.02
29) Phenanthrene-d10	24.98	188	2488434m	20.00	ug/l	-0.01
38) Chrysene-d12	33.02	240	1525729	20.00	ug/l	-0.01
44) Perylene-d12	37.12	264	819689	20.00	ug/l	0.00

System Monitoring Compounds

37) 2,4-DDD	30.07	235	149499	5.46	ug/mL	0.00
Spiked Amount	5.000		Recovery	=	109.20%	

Target Compounds

				Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.
9) Hexachloroethane	0.00	117	0	N.D.
11) Nitrobenzene	0.00	77	0	N.D.
12) Isophorone	0.00	82	0	N.D.
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.
15) Naphthalene	15.33	128	655	N.D.
16) Hexachlorobutadiene	0.00	225	0	N.D.
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.
19) 2-Chloronaphthalene	0.00	162	0	N.D.
20) Dimethylphthalate	0.00	163	0	N.D.
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.
22) Acenaphthylene	0.00	152	0	N.D.
23) Acenaphthene	0.00	153	0	N.D.
24) 2,4-Dinitrotoluene	21.25	165	173	N.D.
25) Diethylphthalate	22.24	149	100	N.D.
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.
27) Fluorene	0.00	166	0	N.D.
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.

(#)= qualifier out of range (m) = manual integration

30490.D GCMS1126.M

Tue Jan 15 11:22:50 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC3101\30490.D

Vial: 12

Acq On : 31 Dec 2001 9:40 pm

Operator: 209 GALOS

Sample : gcms scan 12/14fb

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Jan 15 11:22 2002

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 28 15:11:00 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	24.99	178	665	N.D.		
34) Anthracene	24.99	178	665	N.D.		
35) Di-n-butylphthalate	27.07	149	2387	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.02	228	3945	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.31	149	5180	N.D.		
43) Chrysene	33.02	228	3945	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	37.11	252	3095	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

30490.D GCMS1126.M

Tue Jan 15 11:22:54 2002

Page 2

Quantitation Report

Data File : C:\HPCHEM\1\DATA\DEC3101\30490.D

Vial: 12

Acq On : 31 Dec 2001 9:40 pm

Operator: 209 GALOS

Sample : gcms scan 12/14fb

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Jan 15 11:22 2002


Quant Results File: GCMS1126.RES

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 28 15:11:00 2001

Response via : Initial Calibration

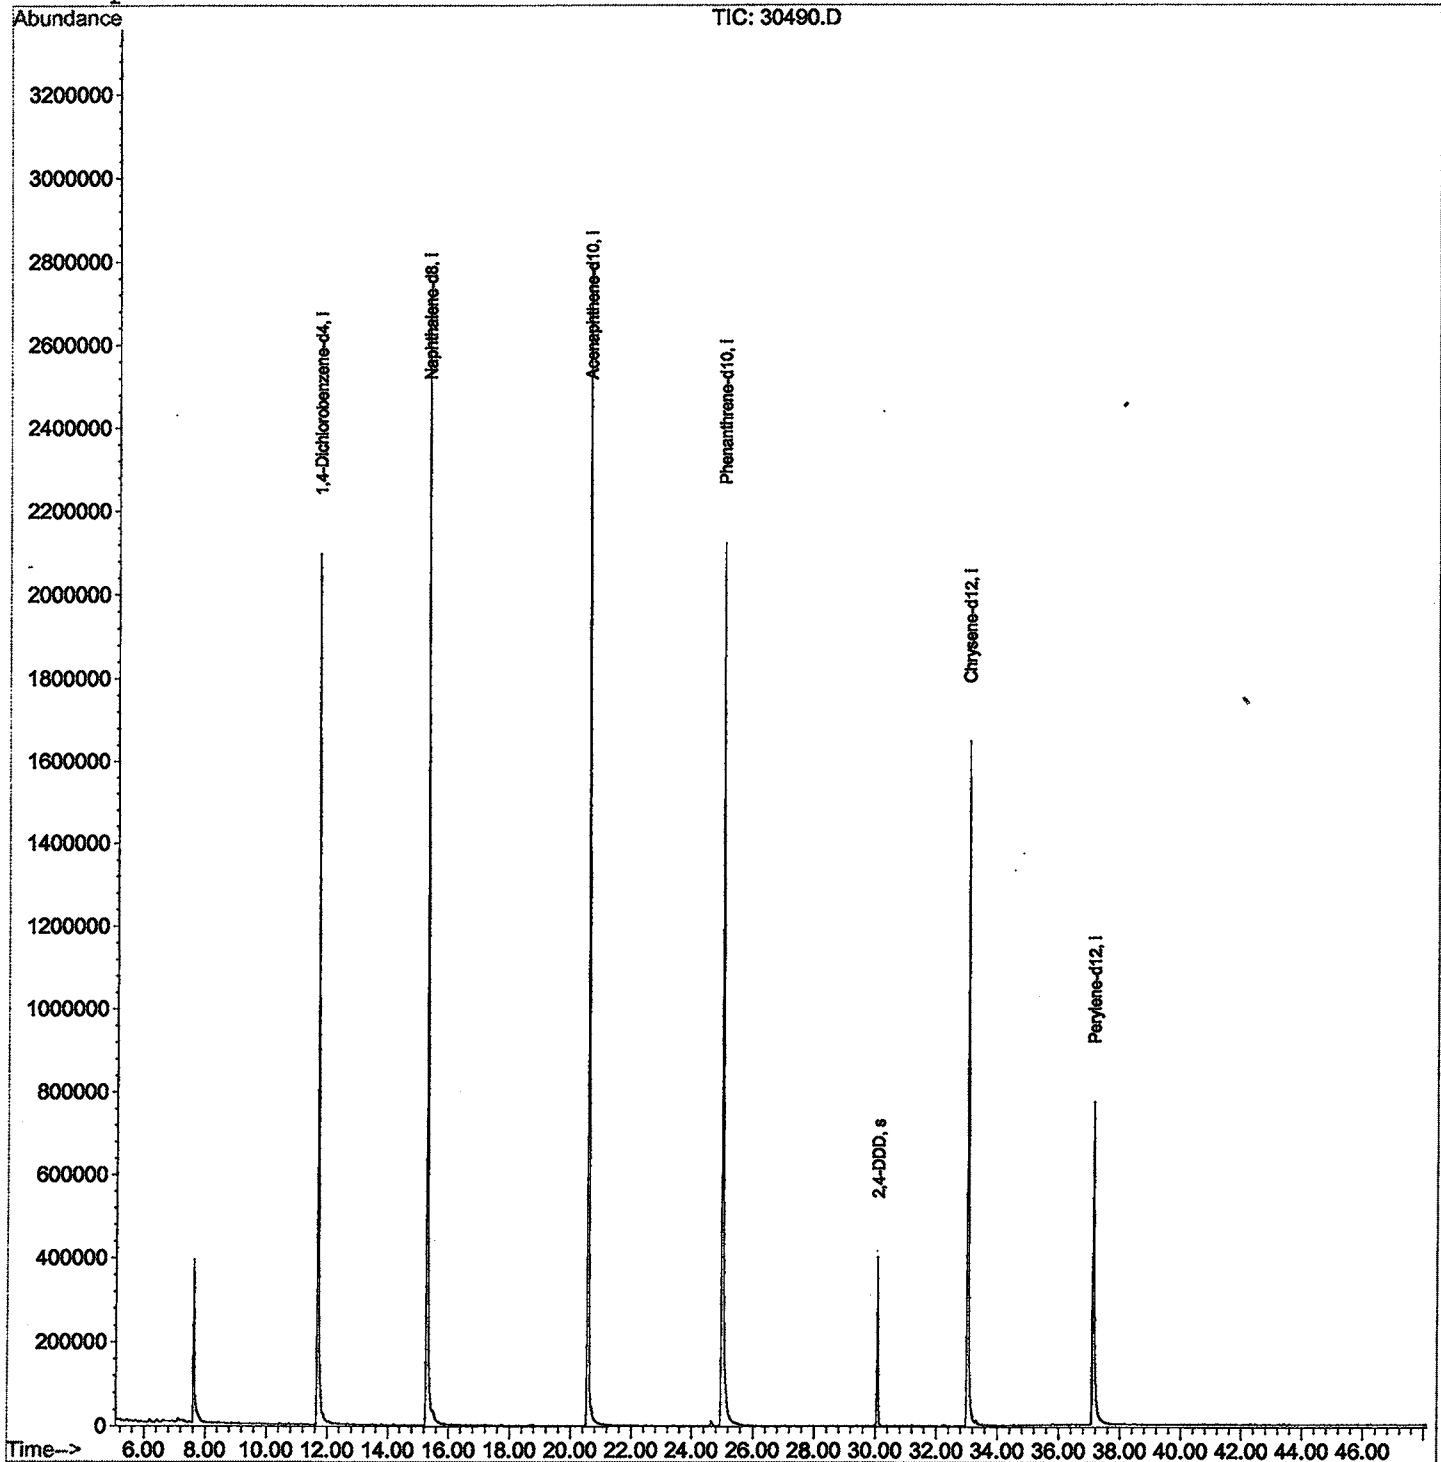

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\DEC3101\30490.D
 Acq On : 31 Dec 2001 9:40 pm
 Sample : gcms scan 12/14fb
 Misc :
 MS Integration Params: LSCINT.P

Vial: 12
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	7.612	276	280	309	rBV	386465	1122504	15.14%	3.073%
2	11.670	718	722	761	rBV	2094339	5415429	73.05%	14.827%
3	15.278	1110	1115	1135	rBV	2714210	6773510	91.37%	18.545%
4	20.557	1684	1690	1717	rBV	2796186	7412954	100.00%	20.296%
5	24.981	2166	2172	2217	rBV2	2122205	7025687	94.78%	19.235%
6	30.067	2720	2726	2737	rBV	402526	923621	12.46%	2.529%
7	33.023	3042	3048	3075	rBV2	1647326	4855006	65.49%	13.292%
8	37.118	3487	3494	3522	rBV2	771325	2996062	40.42%	8.203%

Sum of corrected areas: 36524773

30490.D GCMS1126.M Wed Jan 16 08:27:55 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\DEC3101\30490.D
 Operator : 209 GALOS
 Acquired : 31 Dec 2001 9:40 pm using AcqMethod GCMS1126
 Instrument : GC/MS 209
 Sample Name: gcms scan 12/14fb
 Misc Info :
 Vial Number: 12
 Quant File :GCMS1126.RES (RTE Integrator)

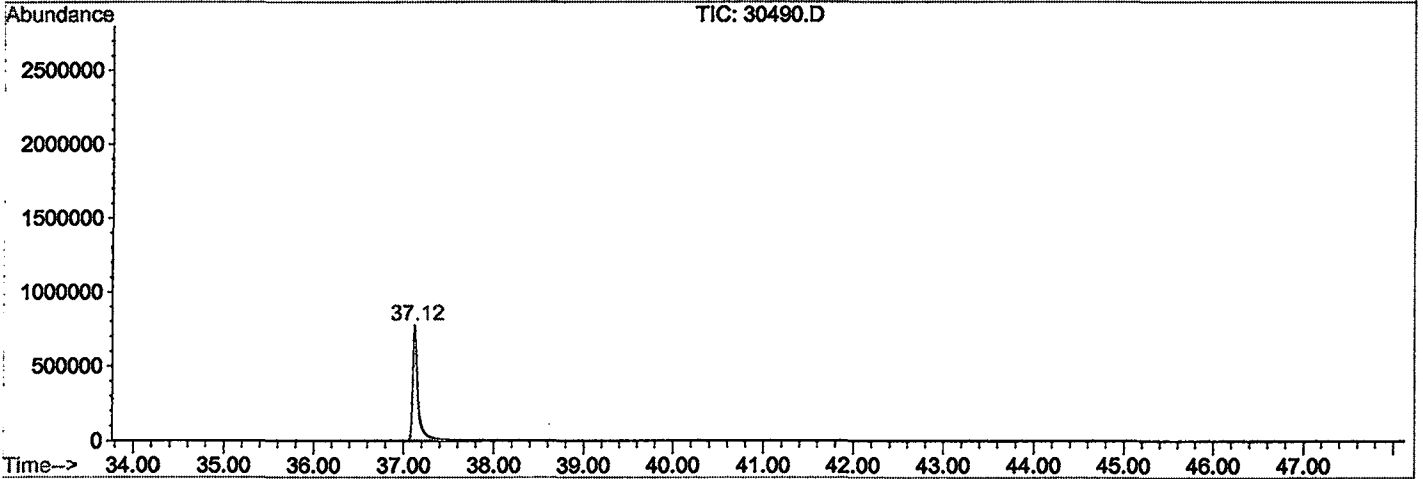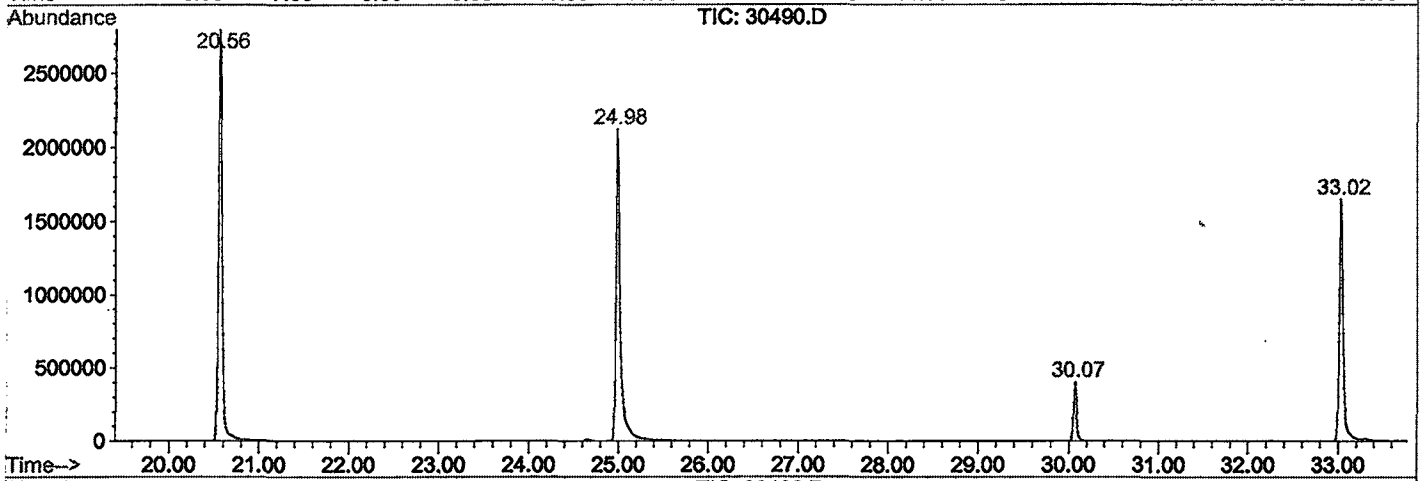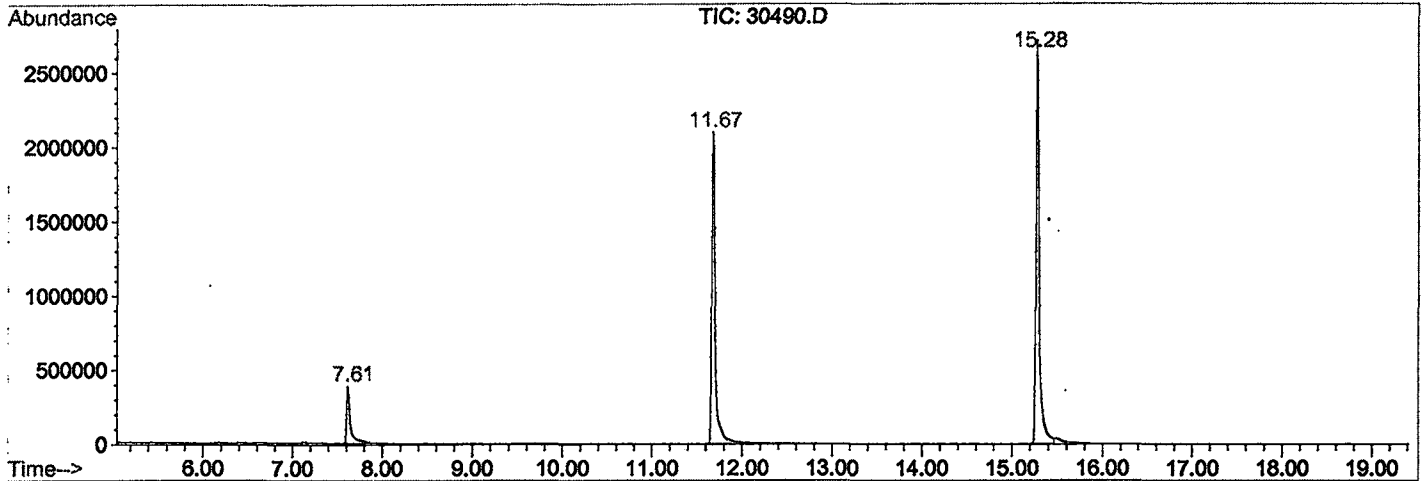

30490.D GCMS1126.M

Wed Jan 16 08:28:00 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\DEC3101\30490.D
Acq On : 31 Dec 2001 9:40 pm
Sample : gcms scan 12/14fb
Misc :
MS Integration Params: LSCINT.P










Vial: 12
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 Silane, tetramethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.61	4.15 ug/l	1122500	1,4-Dichlorobenzene-d4	11.68

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	9
3			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	9
4			N-Ethylformamide	73	C3H7NO	000627-45-2	5

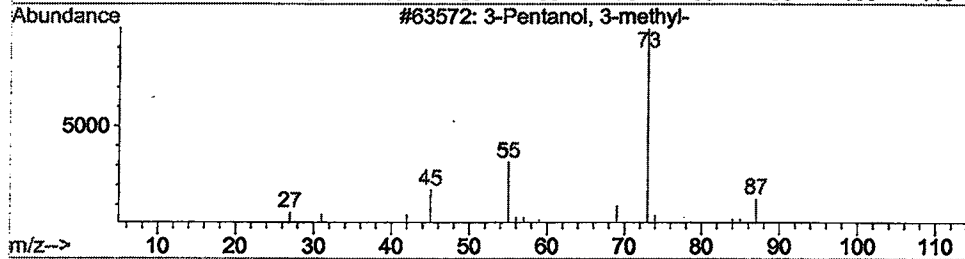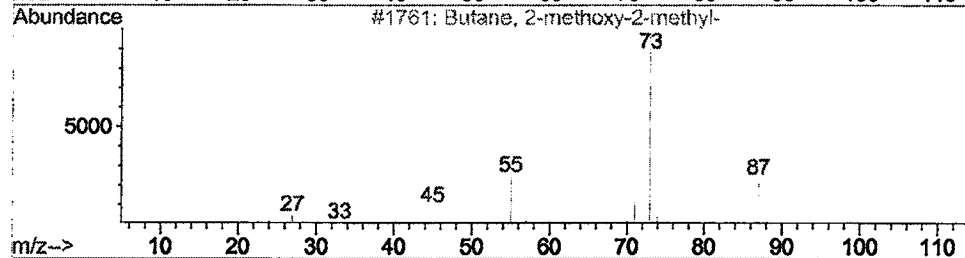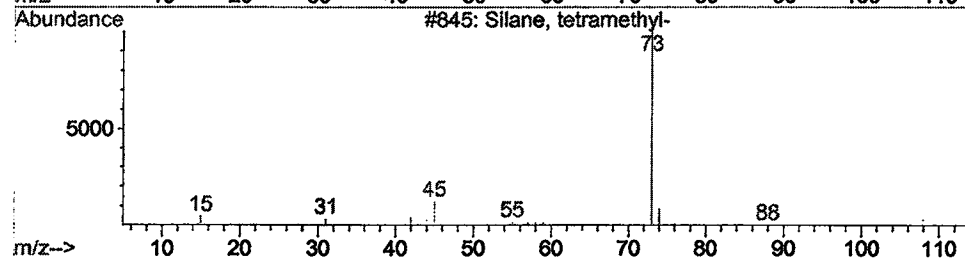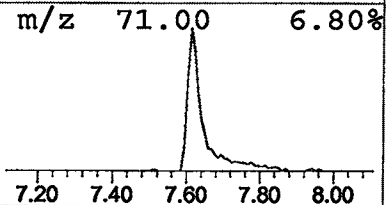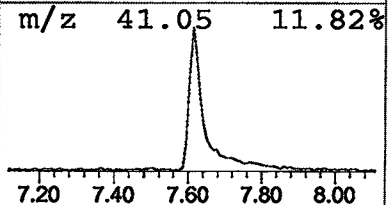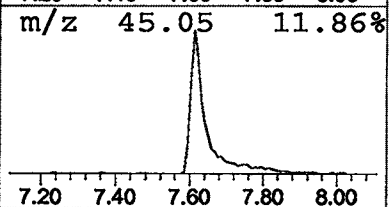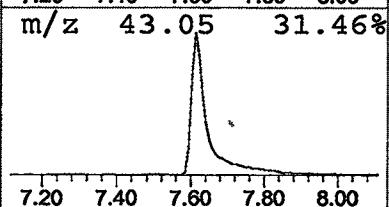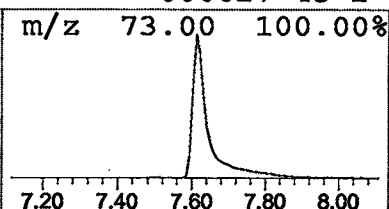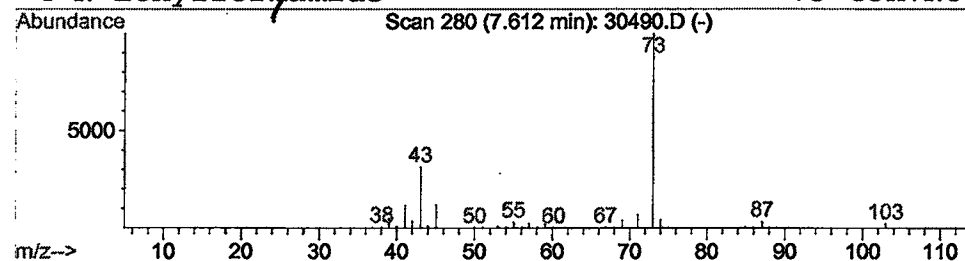

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 31 Dec 2001 9:40 pm
 Data File: C:\HPCHEM\1\DATA\DEC3101\30490.D
 Name: gcms scan 12/14fb
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
Silane, tetramethyl-	7.61	4.1	ug/l	1122500	ISTD01	11.68	5415430	20.0

30490.D GCMS1126.M Wed Jan 16 08:28:09 2002