

Comments for Sample AD26011 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 01-18-2002 Time: 17:50:46

A scan of the extract prepared for the 508 analysis, from 35 to 550 amu using a mass spectrometer, reveals the presence of 2-(2-ethoxyethoxy)ethanol at an estimated level of 4.7 ug/L and with a fit of 90 out of 100; and 2-ethoxybutane at an estimated level of 3.0 ug/L and with a fit of 49 out of 100. The Field Blank for this sample shows no contamination.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC3101\26011.D

Vial: 20

Acq On : 1 Jan 2002 5:25 am

Operator: 209 GALOS

Sample : gcms scan 12/14a

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Jan 15 14:03 2002

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 28 15:11:00 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.68	152	747055	20.00	ug/l	-0.02
10) Naphthalene-d8	15.28	136	2910065	20.00	ug/l	-0.02
17) Acenaphthene-d10	20.56	164	1473022	20.00	ug/l	-0.01
29) Phenanthrene-d10	24.99	188	1970751m	20.00	ug/l	0.00
38) Chrysene-d12	33.03	240	1186285	20.00	ug/l	0.00
44) Perylene-d12	37.12	264	665722	20.00	ug/l	0.00

System Monitoring Compounds

37) 2,4-DDD	30.07	235	116488	5.38	ug/mL	0.00
Spiked Amount	5.000		Recovery	=	107.60%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	5.28	74	189	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.34	128	632	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	21.00	165	564	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	

(#)=qualifier out of range (m)=manual integration

26011.D GCMS0103.M Tue Jan 15 14:03:30 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC3101\26011.D

Vial: 20

Acq On : 1 Jan 2002 5:25 am

Operator: 209 GALOS

Sample : gcms scan 12/14a

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Jan 15 14:03 2002

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 28 15:11:00 2001.

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	25.06	178	180	N.D.		
34) Anthracene	25.06	178	180	N.D.		
35) Di-n-butylphthalate	27.07	149	2461	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.02	228	2673	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.31	149	4268	N.D.		
43) Chrysene	33.02	228	2673	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	37.13	252	2371	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

26011.D GCMS0103.M

Tue Jan 15 14:03:34 2002

Page 2

Quantitation Report

Data File : C:\HPCHEM\1\DATA\DEC3101\26011.D

Vial: 20

Acq On : 1 Jan 2002 5:25 am

Operator: 209 GALOS

Sample : gcms scan 12/14a

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Jan 15 14:03 2002


Quant Results File: GCMS1126.RES

Method : C:\HPCHEM\1\METHODS\GCMS0103.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Mon Jan 07 10:31:02 2002

Response via : Initial Calibration

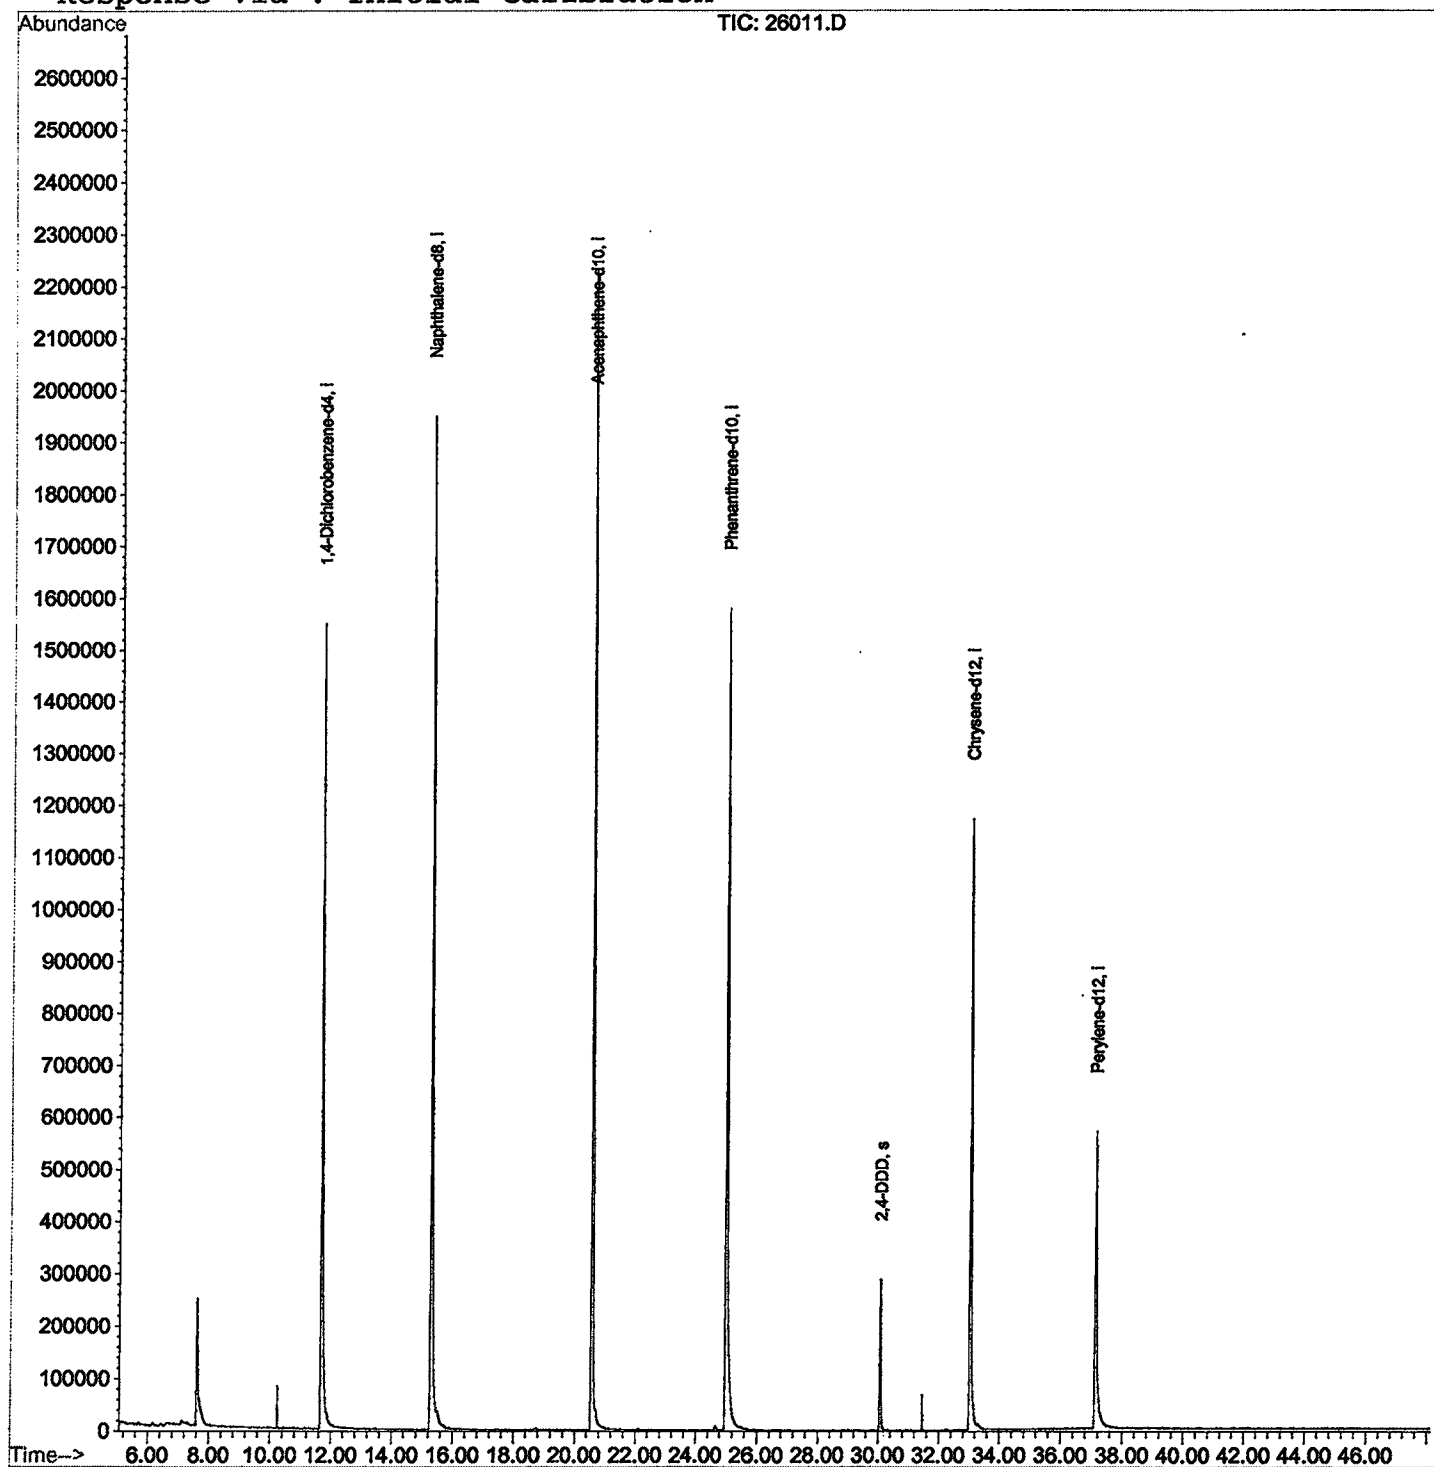

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\DEC3101\26011.D

Acq On : 1 Jan 2002 5:25 am

Sample : gcms scan 12/14a

Misc :

MS Integration Params: LSCINT.P

Vial: 20

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	7.617	275	280	314	rBV	241520	943075	15.32%	3.165%
2	11.675	717	722	740	rBV	1546355	4503519	73.15%	15.115%
3	15.283	1109	1115	1134	rBV	1947225	5681487	92.29%	19.069%
4	20.562	1684	1690	1718	rBV	2232439	6156176	100.00%	20.662%
5	24.987	2166	2172	2214	rBV2	1579298	5620375	91.30%	18.864%
6	30.072	2720	2726	2741	rBV	288124	720736	11.71%	2.419%
7	33.029	3041	3048	3069	rBV2	1171731	3743720	60.81%	12.565%
8	37.123	3487	3494	3525	rBV2	567908	2425494	39.40%	8.141%


Sum of corrected areas: 29794582

26011.D GCMS1126.M

Tue Jan 15 14:47:10 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\DEC3101\26011.D
Operator : 209 GALOS
Acquired : 1 Jan 2002 5:25 am using AcqMethod GCMS1126
Instrument : GC/MS 209
Sample Name: gcms scan 12/14a
Misc Info :
Vial Number: 20
Quant File :GCMS1126.RES (RTE Integrator)

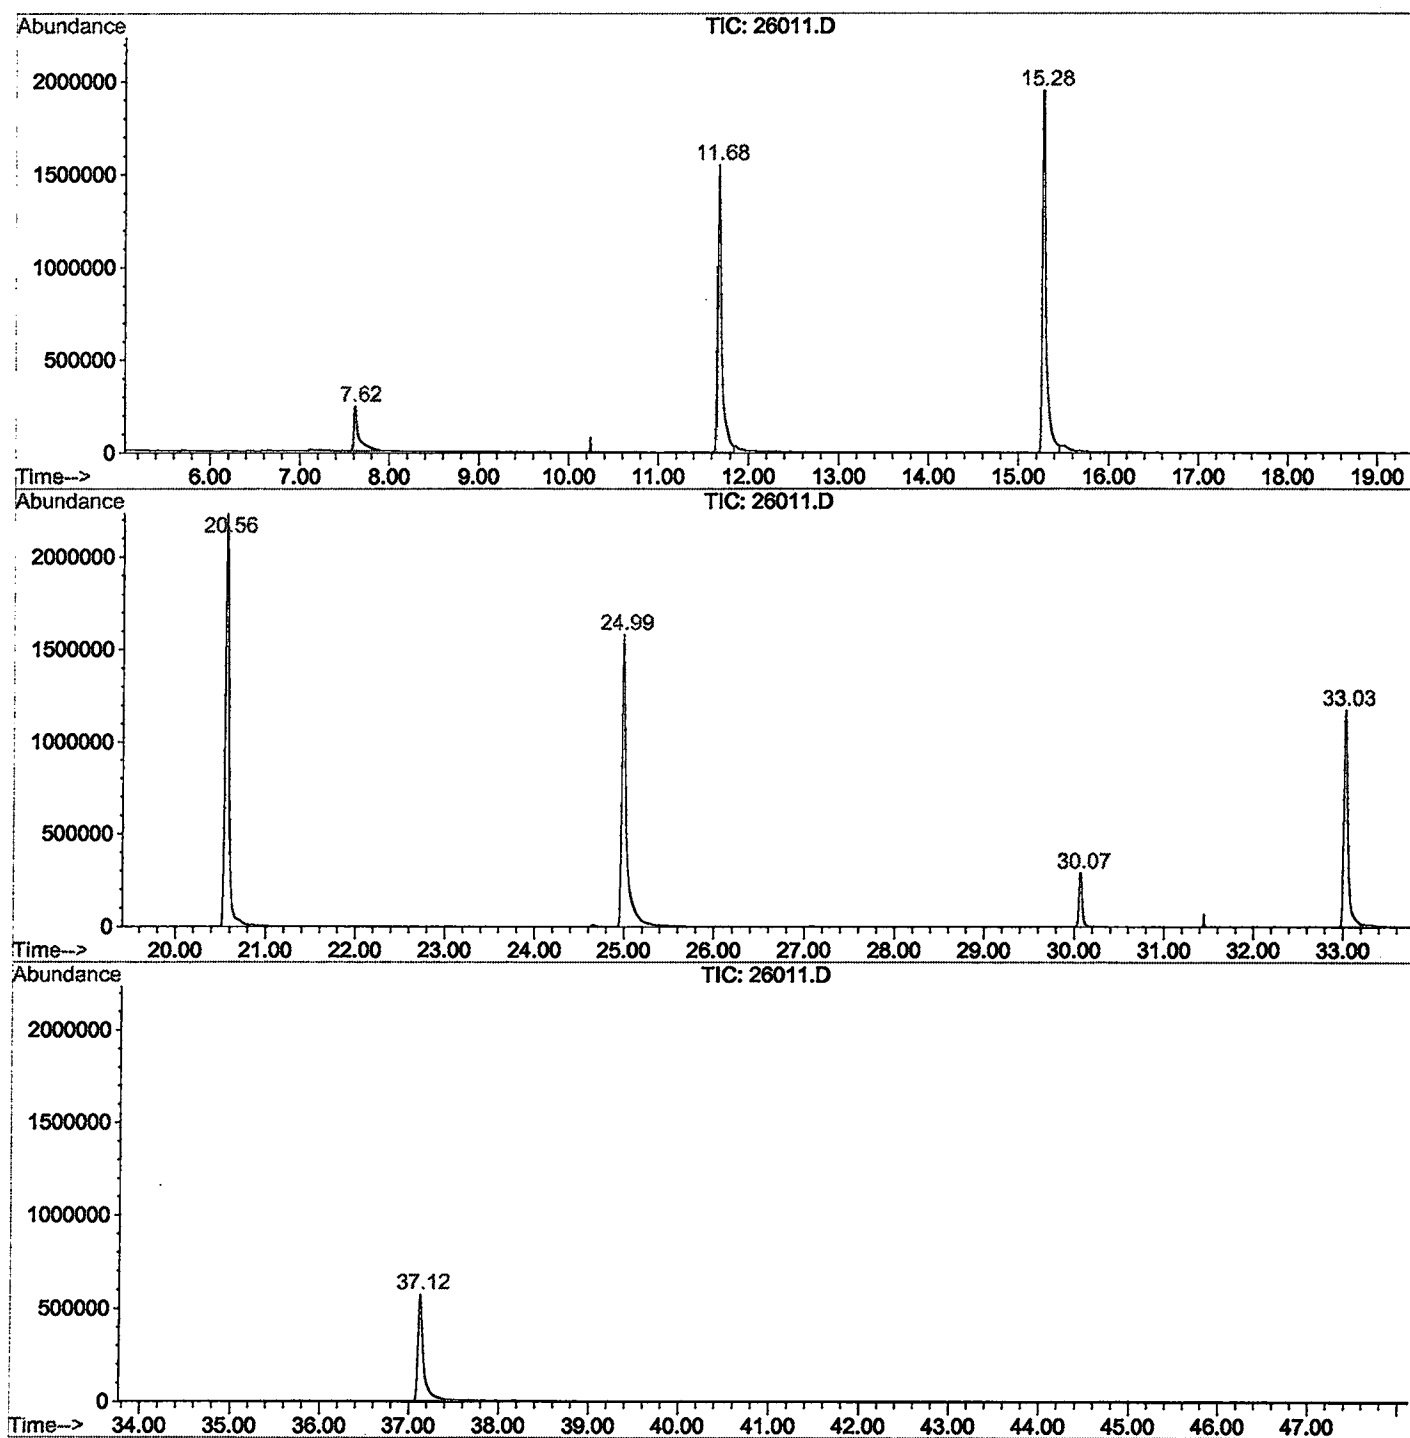

26011.D GCMS1126.M

Tue Jan 15 14:47:17 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\DEC3101\26011.D
Acq On : 1 Jan 2002 5:25 am
Sample : gcms scan 12/14a
Misc :
MS Integration Params: LSCINT.P









Vial: 20
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 3-Pentanol, 3-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.62	4.19 ug/l	943075	1,4-Dichlorobenzene-d4	11.68

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	28
2			1-Butanamine, 3-methyl-	87	C5H13N	000107-85-7	9
3			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	9

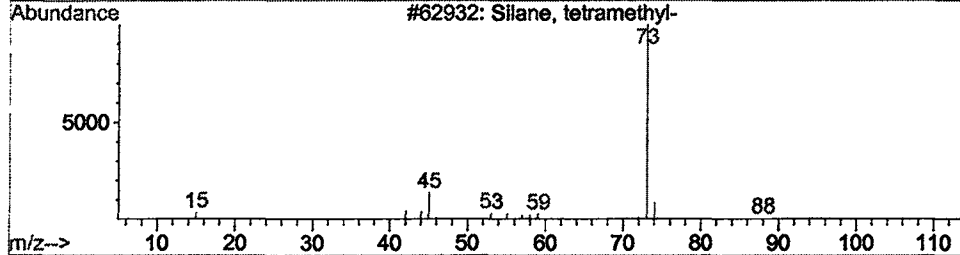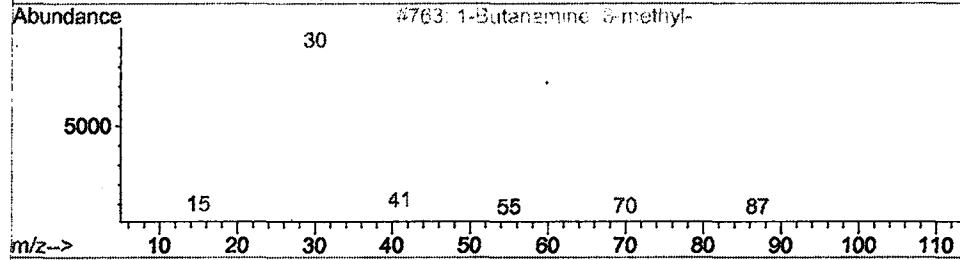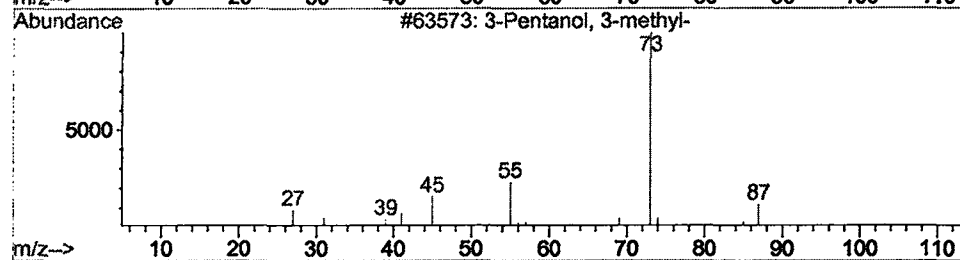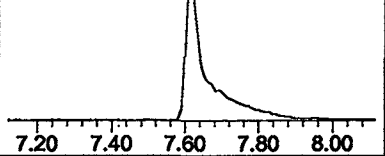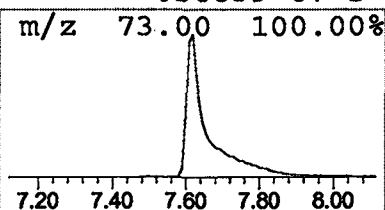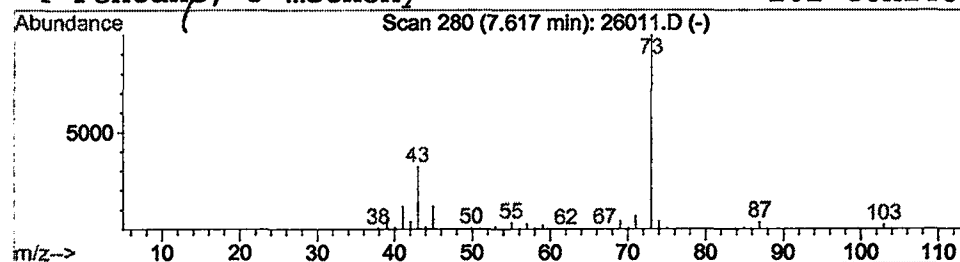

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 1 Jan 2002 5:25 am
 Data File: C:\HPCHEM\1\DATA\DEC3101\26011.D
 Name: gcms scan 12/14a
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
3-Pentanol, 3-methyl	7.62	4.2	ug/l	943075	ISTD01	11.68	4503520	20.0

26011.D GCMS1126.M Tue Jan 15 14:47:26 2002