


DFTPP

Data File : C:\HPCHEM\1\DATA\DEC3101\DFTPP1.D
 Acq On : 1 Jan 2002 11:13 am
 Sample :
 Misc :
 MS Integration Params: RTEINT.P
 Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

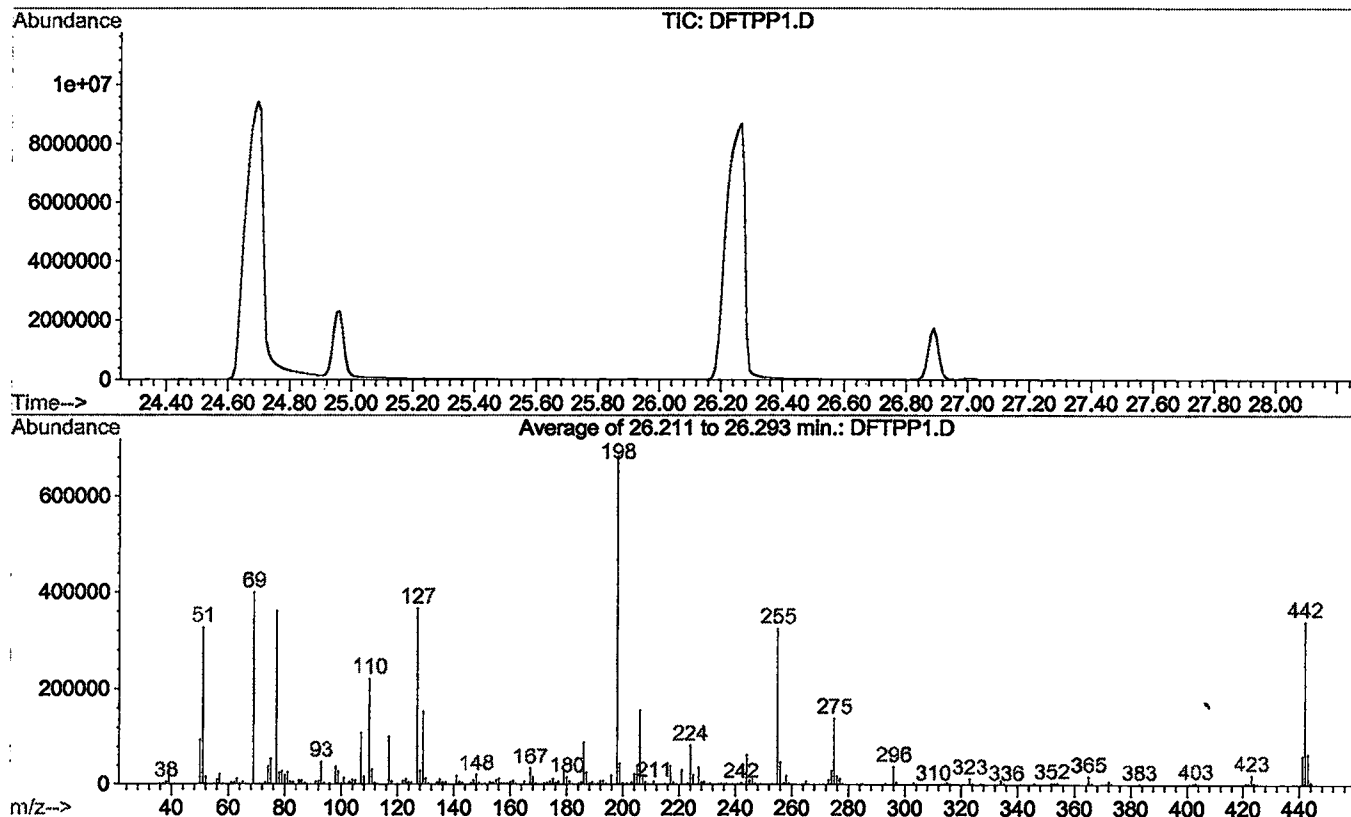

Spectrum Information: Average of 26.211 to 26.293 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	47.9	327188	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	58.5	399652	PASS
70	69	0.00	2	0.0	65	PASS
127	198	40	60	53.7	366996	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	683025	PASS
199	198	5	9	6.7	46057	PASS
275	198	10	30	20.5	140101	PASS
365	198	1	100	2.7	18430	PASS
441	443	0.01	100	94.1	62255	PASS
442	198	40	110	49.8	340466	PASS
443	442	17	23	19.4	66137	PASS