User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 02/13/2002 Time: 07:55:59

Sample: AD31364
Analysis: $GCMS GCMS Scan For Unknowns
Units: ug
Started: 2/13/02 07:54 Ended: 2/13/02 07:54 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		128		5.0

Comments for Sample AD31364 - Analysis $GCMS

Westchester Dept. of Labs & Research
User: Vinci, David L
Date: 02-13-2002 Time: 07:56:11

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.
The recoveries for 3 of the 43 compounds in the LCS Standard were above their acceptance ranges.

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\JAN1602\31364.D Vial: 16
Acq On : 17 Jan 2002 2:18 am Operator: 209 GALOS
Sample : gc/ms scan 12/27 Inst : GC/MS 209
Misc : Multiplr: 1.00
MS Integration Params: GOOFY.P
Quant Time: Feb 7 9:01 2002 Quant Results File: GCMS0103.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0103.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Mon Jan 07 10:31:02 2002
Response via : Initial Calibration
DataAcq Meth : GCMS0103

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.50	152	801206	20.00	ug/l	-0.03
10) Naphthalene-d8	15.09	136	3124549	20.00	ug/l	-0.03
17) Acenaphthene-d10	20.36	164	1573488	20.00	ug/l	-0.03
29) Phenanthrene-d10	24.77	188	2183107	20.00	ug/l	-0.04
38) Chrysene-d12	32.80	240	1408251	20.00	ug/l	-0.04
44) Perylene-d12	36.87	264	944522	20.00	ug/l	-0.03
System Monitoring Compounds						
37) 2,4-DDD	29.85	235	160898	6.42	ug/mL	-0.22
Spiked Amount 5.000			Recovery = 128.40%			
Target Compounds						Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.		
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.		
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.		
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.		
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.		
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.		
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.		
9) Hexachloroethane	0.00	117	0	N.D.		
11) Nitrobenzene	0.00	77	0	N.D.		
12) Isophorone	0.00	82	0	N.D.		
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.		
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
15) Naphthalene	15.15	128	670	N.D.		
16) Hexachlorobutadiene	0.00	225	0	N.D.		
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
19) 2-Chloronaphthalene	0.00	162	0	N.D.		
20) Dimethylphthalate	0.00	163	0	N.D.		
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d	
22) Acenaphthylene	0.00	152	0	N.D.		
23) Acenaphthene	0.00	153	0	N.D.		
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.		
25) Diethylphthalate	21.88	149	991	N.D.		
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.		
27) Fluorene	0.00	166	0	N.D.		
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.		

(#) = qualifier out of range (m) = manual integration

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\JAN1602\31364.D Vial: 16
Acq On : 17 Jan 2002 2:18 am Operator: 209 GALOS
Sample : gc/ms scan 12/27 Inst : GC/MS 209
Misc : Multiplr: 1.00
MS Integration Params: GOOFY.P
Quant Time: Feb 7 9:01 2002 Quant Results File: GCMS0103.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0103.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Mon Jan 07 10:31:02 2002
Response via : Initial Calibration
DataAcq Meth : GCMS0103

	Compound	R.T.	QIon	Response	Conc Unit	Qvalue
30)	N-Nitrosodiphenylamine	0.00	168	0	N.D.	
31)	4-Bromophenyl-phenylether	0.00	248	0	N.D.	
32)	Hexachlorobenzene	0.00	284	0	N.D.	
33)	Phenanthrene	24.78	178	763	N.D.	
34)	Anthracene	24.78	178	763	N.D.	
35)	Di-n-butylphthalate	26.80	149	33807	N.D.	
36)	Fluoranthene	0.00	202	0	N.D.	
39)	Pyrene	0.00	202	0	N.D.	
40)	Butylbenzylphthalate	0.00	149	0	N.D.	
41)	Benzo(a)anthracene	32.80	228	3397	N.D.	
42)	Bis(2-ethylhexyl)phthalate	33.11	149	4229	N.D.	
43)	Chrysene	32.80	228	3397	N.D.	
45)	Di-n-Octylphthalate	35.32	149	100	N.D.	
46)	Benzo(b)fluoranthene	0.00	252	0	N.D.	
47)	Benzo(k)fluoranthene	0.00	252	0	N.D.	
48)	Benzo(a)pyrene	36.87	252	3626	N.D.	
49)	Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.	
50)	Dibenz(a,h)anthracene	0.00	278	0	N.D.	
51)	Benzo(g,h,i)perylene	0.00	276	0	N.D.	

(#) = qualifier out of range (m) = manual integration

Quantitation Report

Data File : C:\HPCHEM\1\DATA\JAN1602\31364.D
Acq On : 17 Jan 2002 2:18 am
Sample : gc/ms scan 12/27
Misc :
MS Integration Params: GOOFY.P
Quant Time: Feb 7 9:01 2002

Vial: 16
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00
Quant Results File: GCMS0103.RES

Method : C:\HPCHEM\1\METHODS\GCMS0103.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Mon Jan 07 10:31:02 2002
Response via : Initial Calibration

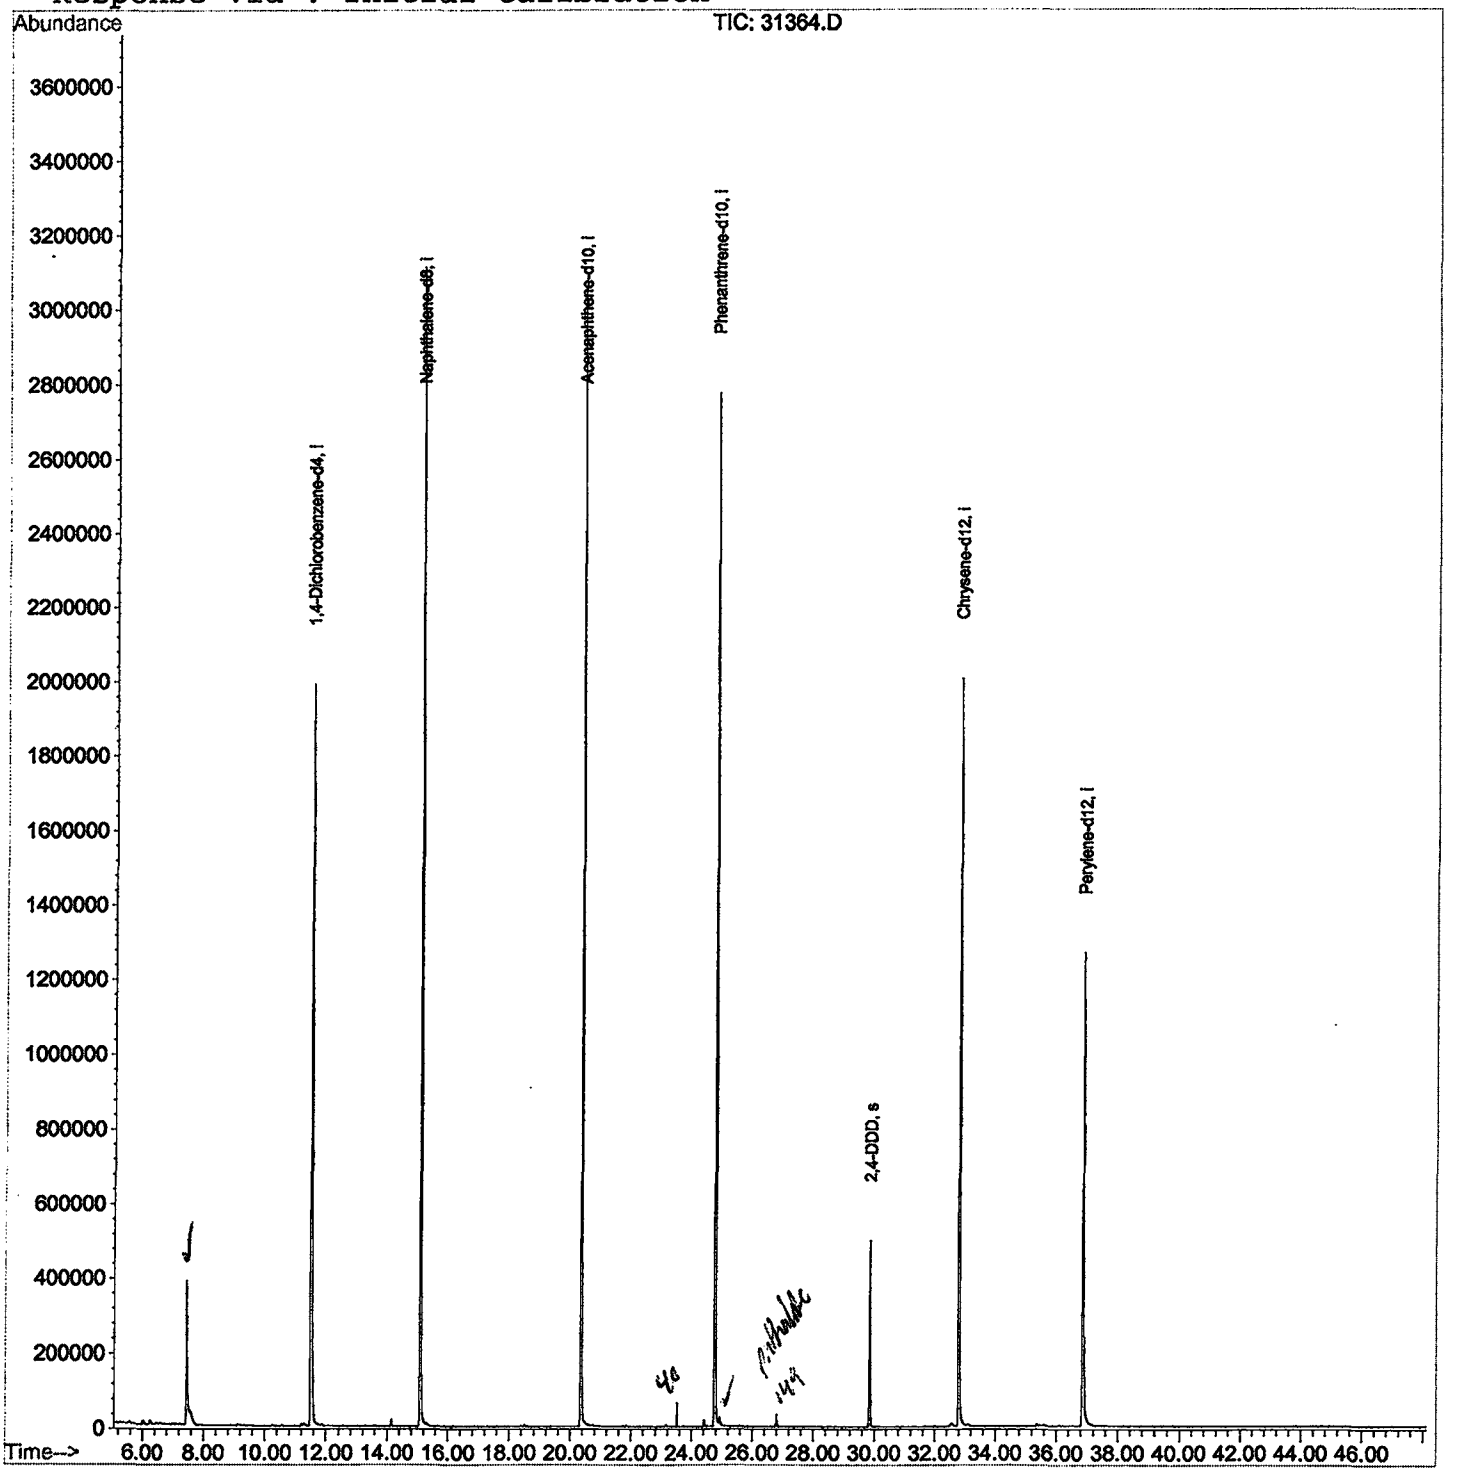

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\JAN1602\31364.D Vial: 16
Acq On : 17 Jan 2002 2:18 am Operator: 209 GALOS
Sample : gc/ms scan 12/27 Inst : GC/MS 209
Misc : Multiplr: 1.00
MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS0103.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	7.443	257	261	275	rBV	382949	1019890	15.49%	2.955%
2	11.501	698	703	721	rBV	1986880	5112547	77.67%	14.813%
3	15.091	1089	1094	1114	rBV	3107133	6429862	97.68%	18.630%
4	20.360	1661	1668	1682	rBV	3054428	6582351	100.00%	19.072%
5	24.767	2142	2148	2161	rBV2	2772545	6171240	93.75%	17.881%
6	24.923	2161	2165	2181	rVB	22456	75934	1.15%	0.220%
7	29.853	2696	2702	2711	rBV	495121	1015631	15.43%	2.943%
8	32.799	3017	3023	3045	rBV2	2000966	4553388	69.18%	13.193%
9	36.866	3457	3466	3497	rBV2	1263002	3552171	53.97%	10.292%

Sum of corrected areas: 34513014

31364.D GCMS0103.M Thu Feb 07 09:12:04 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\JAN1602\31364.D
Operator : 209 GALOS
Acquired : 17 Jan 2002 2:18 am using AcqMethod GCMS0103
Instrument : GC/MS 209
Sample Name: gc/ms scan 12/27
Misc Info :
Vial Number: 16
Quant File :GCMS0103.RES (RTE Integrator)

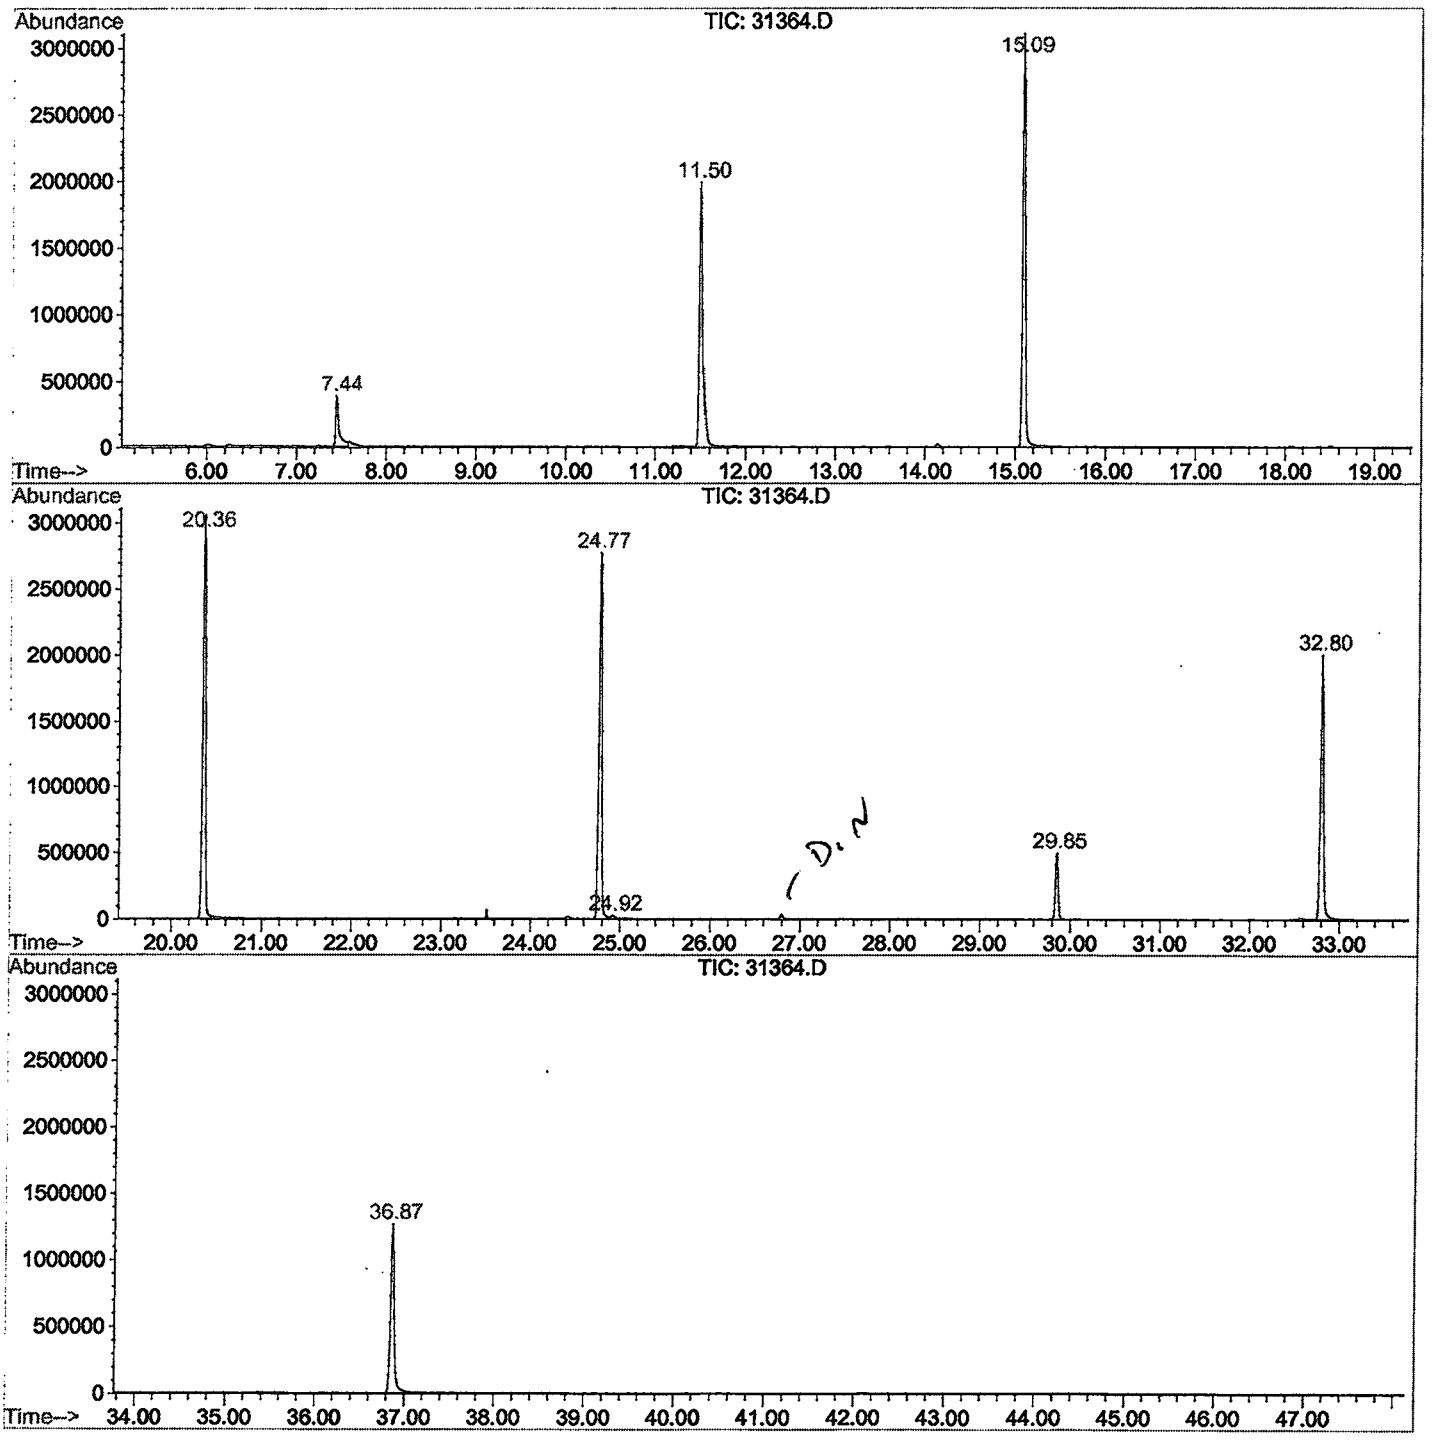

31364.D GCMS0103.M Thu Feb 07 09:12:10 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\JAN1602\31364.D
Acq On : 17 Jan 2002 2:18 am
Sample : gc/ms scan 12/27
Misc :
MS Integration Params: LSCINT.P

Vial: 16
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0103.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

****

Peak Number 1 3-Pentanol, 3-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.44	3.99 ug/l	1019890	1,4-Dichlorobenzene-d4	11.50

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	33
2	1-Butanamine, 3-methyl-	87	C5H13N	000107-85-7	9
3	Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
4	Pentane, 3-methoxy-	102	C6H14O	036839-67-5	9

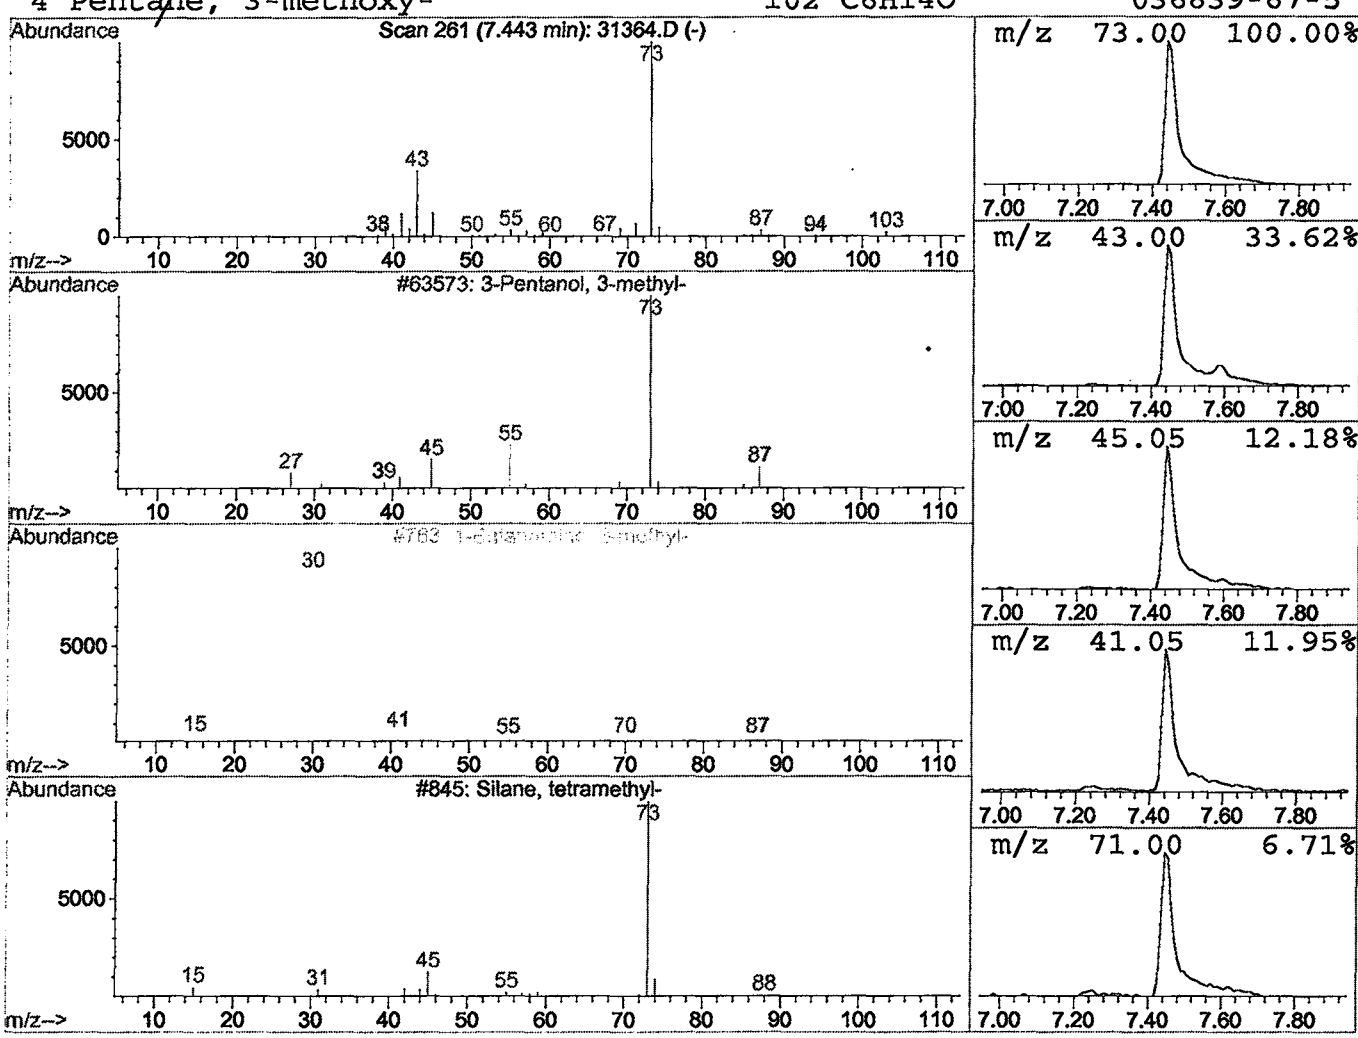

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\JAN1602\31364.D
Acq On : 17 Jan 2002 2:18 am
Sample : gc/ms scan 12/27
Misc :
MS Integration Params: LSCINT.P

Vial: 16
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0103.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

****

Peak Number 2 Anthracene-d10- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
24.92	0.25 ug/l	75934	Phenanthrene-d10	24.77

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Anthracene-d10-	188	C14D10	001719-06-8	78
2	2-Quinolinecarboxaldehyde, 8-hydrox	188	C10H8N2O2	005603-22-5	40
3	3-Quinolinecarbonitrile, 1,2,3,4-te	188	C10H8N2O2	022384-05-0	40
4	5-Oxazolecarboxamide, 2-phenyl-	188	C10H8N2O2	039819-42-6	40

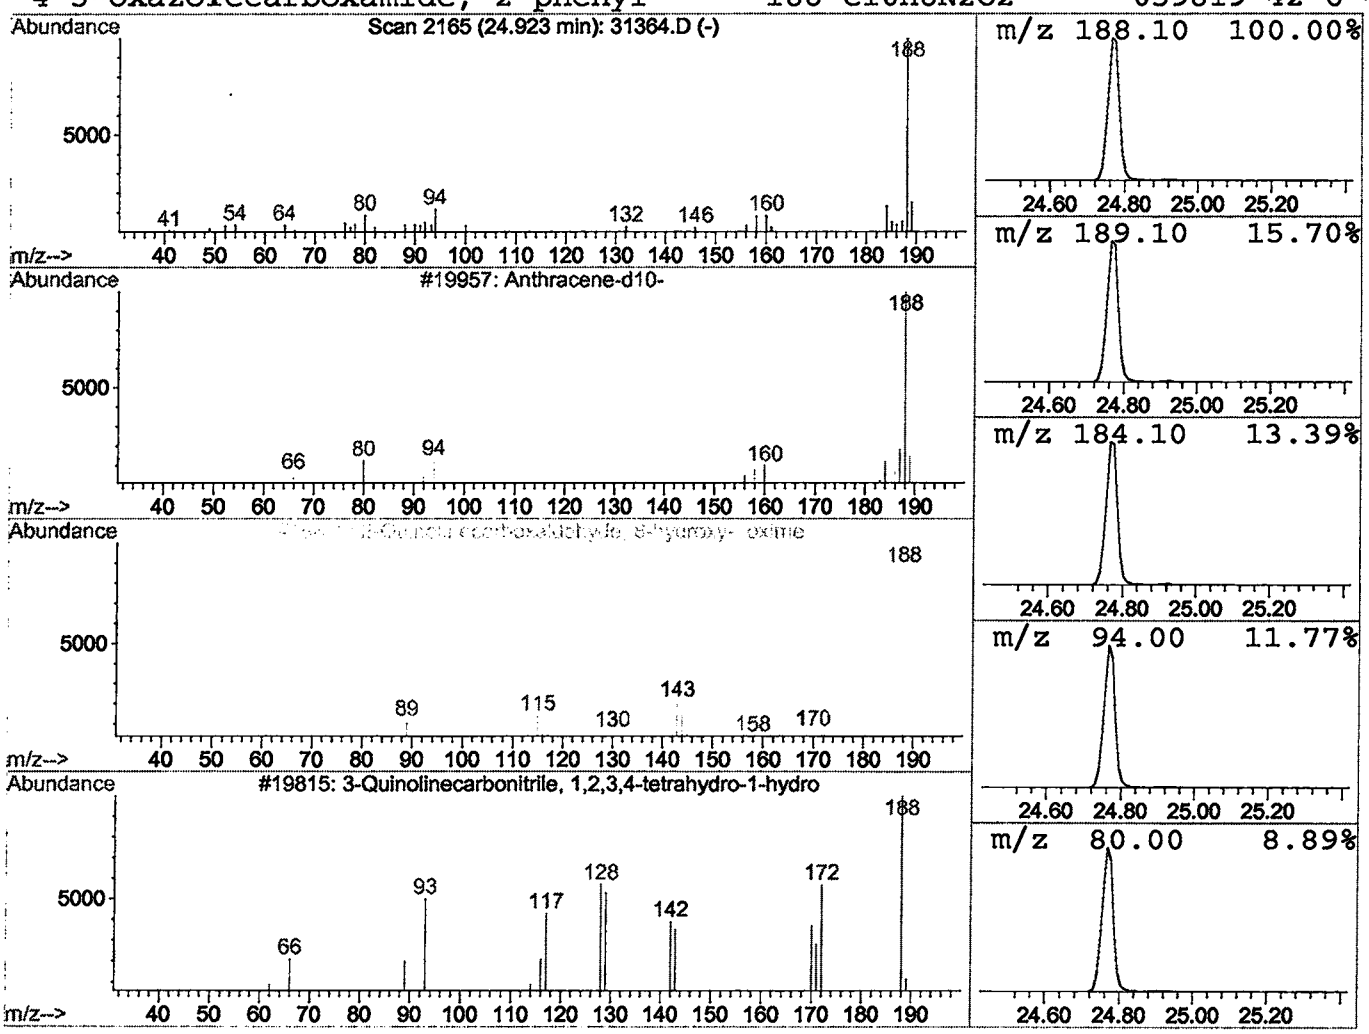

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 17 Jan 2002 2:18 am
Data File: C:\HPCHEM\1\DATA\JAN1602\31364.D
Name: gc/ms scan 12/27
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0103.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
3-Pentanol, 3-methyl	7.44	4.0	ug/l	1019890	ISTD01	11.50	5112550	20.0
Anthracene-d10	24.92	0.2	ug/l	75934	ISTD04	24.77	6171240	20.0

31364.D GCMS0103.M Thu Feb 07 09:12:24 2002