

Method 508 mod

Date Extracted 12/19/01

Page 78

ref

#GCMS - 16592

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
LB ✓		500mL		1mL			1mL	8B	7			
Ref ✓					0.5mL			6B				
30705 ✓								6A				
30904 ✓								8A				
30905 ✓								6A				
30906 ✓								7A				
30907 ✓								7B				
30908 ✓								9B				
30909 ✓								7B				
30933 ✓								6B				
30934 ✓								8A				
30935 ✓								7A				
30936 ✓								8B				
Remarks												
Reviewed by, <u>JB 5/15/02</u>												
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate -												
Extraction type <u>sep fun</u>		Solv. lot# <u>V39466</u>		NaCl lot# <u>V11599</u>		Na2SO4 lot# <u>V39H00</u>						
STANDARD	INT STD LOG#											
CALIBRATION	<u>HP 112601</u>											
REF/SPIKE	<u>9/17/59</u>											
MDL/MDRF												
Q. CHECK												
INT. STD.												
SURROGATE	<u>GCMS 12/1/01</u>											
LPC												
ENDRIN/DDT												

Analyst LF
revision 4/12/01


Verified by My

Reviewed by DN
Date 1/28/02

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC3101\DFTPP1.D
 Acq On : 1 Jan 2002 11:13 am
 Sample :
 Misc :
 MS Integration Params: RTEINT.P
 Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

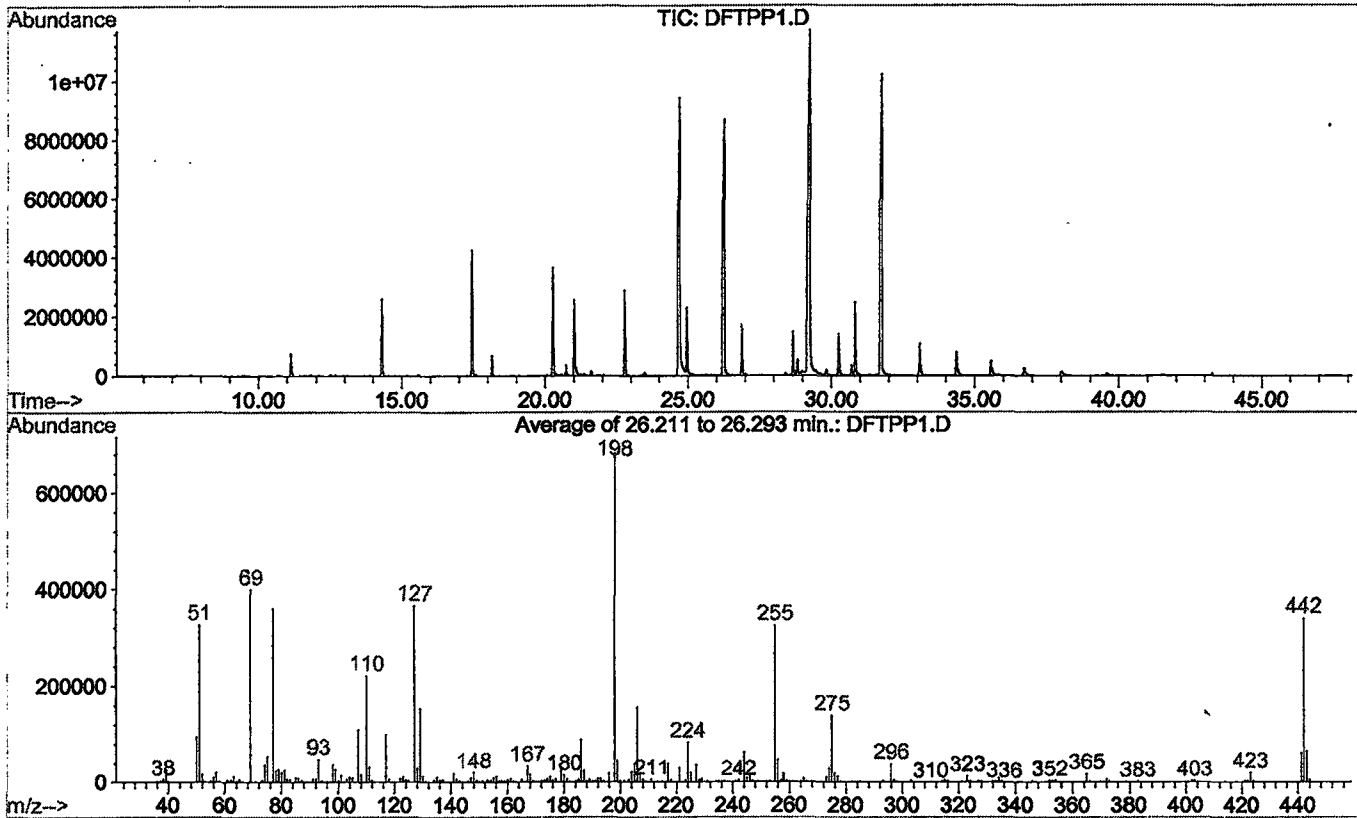

Spectrum Information: Average of 26.211 to 26.293 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	47.9	327188	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	58.5	399652	PASS
70	69	0.00	2	0.0	65	PASS
127	198	40	60	53.7	366996	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	683025	PASS
199	198	5	9	6.7	46057	PASS
275	198	10	30	20.5	140101	PASS
365	198	1	100	2.7	18430	PASS
441	443	0.01	100	94.1	62255	PASS
442	198	40	110	49.8	340466	PASS
443	442	17	23	19.4	66137	PASS