


Sequence Name: C:\HPCHEM\1\SEQUENCE\Dec2101.S

Line	Type	Vial	DataFile	Method	Sample Name
44	Sample	19	30606	GCMS1126	gc/ms scan 12/17
45	Sample	20	30488	GCMS1126	gc/ms scan 12/17
46	Sample	21	29735	GCMS1126	gc/ms scan 12/17
47	Sample	22	26830	GCMS1126	gc/ms scan 12/17
48	Sample	23	30485	GCMS1126	gc/ms scan 12/17
49	Sample	24	LBF	GCMS1126	gc/ms scan 12/17a
50	Sample	25	REFF	GCMS1126	gc/ms scan 12/17a
51	Sample	26	30631	GCMS1126	gc/ms scan 12/17a
52	Sample	27	30632	GCMS1126	gc/ms scan 12/17a
53	Sample	28	30633	GCMS1126	gc/ms scan 12/17a
54	Sample	29	30634	GCMS1126	gc/ms scan 12/17a
55	Sample	30	30601	GCMS1126	gc/ms scan 12/17a
56	Sample	31	30602	GCMS1126	gc/ms scan 12/17a
57	Sample	32	30603	GCMS1126	gc/ms scan 12/17a
58	Sample	33	30608	GCMS1126	gc/ms scan 12/17a
59	Sample	34	30607	GCMS1126	gc/ms scan 12/17a
60	Sample	35	30604	GCMS1126	gc/ms scan 12/17a
61	Sample	1	DFTPP3	GCMS1126	
62	Sample	81	CAL25A	GCMS1126	
63	Sample	54	LBG	GCMS1126	gc/ms scan 12/18
64	Sample	55	REFG	GCMS1126	gc/ms scan 12/18
65	Sample	56	28323	GCMS1126	gc/ms scan 12/18
66	Sample	57	28322	GCMS1126	gc/ms scan 12/18
67	Sample	58	30645	GCMS1126	gc/ms scan 12/18
68	Sample	59	30706	GCMS1126	gc/ms scan 12/18
69	Sample	60	30648	GCMS1126	gc/ms scan 12/18
70	Sample	61	30643	GCMS1126	gc/ms scan 12/18
71	Sample	62	28324	GCMS1126	gc/ms scan 12/18
72	Sample	63	29231	GCMS1126	gc/ms scan 12/18
73	Sample	64	30647	GCMS1126	gc/ms scan 12/18
74	Sample	65	30646	GCMS1126	gc/ms scan 12/18
75	Sample	66	29232	GCMS1126	gc/ms scan 12/18
76	Sample	67	30644	GCMS1126	gc/ms scan 12/18
77	Sample	68	LBH	GCMS1126	gc/ms scan 12/18a
78	Sample	69	REFH	GCMS1126	gc/ms scan 12/18a
79	Sample	70	30641	GCMS1126	gc/ms scan 12/18a
80	Sample	71	30649	GCMS1126	gc/ms scan 12/18a
81	Sample	72	30642	GCMS1126	gc/ms scan 12/18a
82	Sample	73	30704	GCMS1126	gc/ms scan 12/18a
83	Sample	74	30707	GCMS1126	gc/ms scan 12/18a
84	Sample	75	30703	GCMS1126	gc/ms scan 12/18a
85	Sample	76	30709	GCMS1126	gc/ms scan 12/18a
86	Sample	77	30650	GCMS1126	gc/ms scan 12/18a
87	Sample	78	30710	GCMS1126	gc/ms scan 12/18a
88	Sample	79	30651	GCMS1126	gc/ms scan 12/18a
89	Sample	80	30708	GCMS1126	gc/ms scan 12/18a
90	Sample	1	DFTPP	GCMS1126	
91	Sample	2	CAL40	GCMS1126	
92	Sample	3	LB	GCMS1126	gc/ms scan 12/19
93	Sample	4	REF	GCMS1126	gc/ms scan 12/19
94	Sample	5	26532FB	GCMS1126	30984
95	Sample	6	26533FB	GCMS1126	30985

DFTPP

Data File : M:\INSTRU~1\209\DATA\DEC2101\DFTPP2.D
 Acq On : 22 Dec 2001 8:29 pm
 Sample :
 Misc :
 MS Integration Params: RTEINT.P
 Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

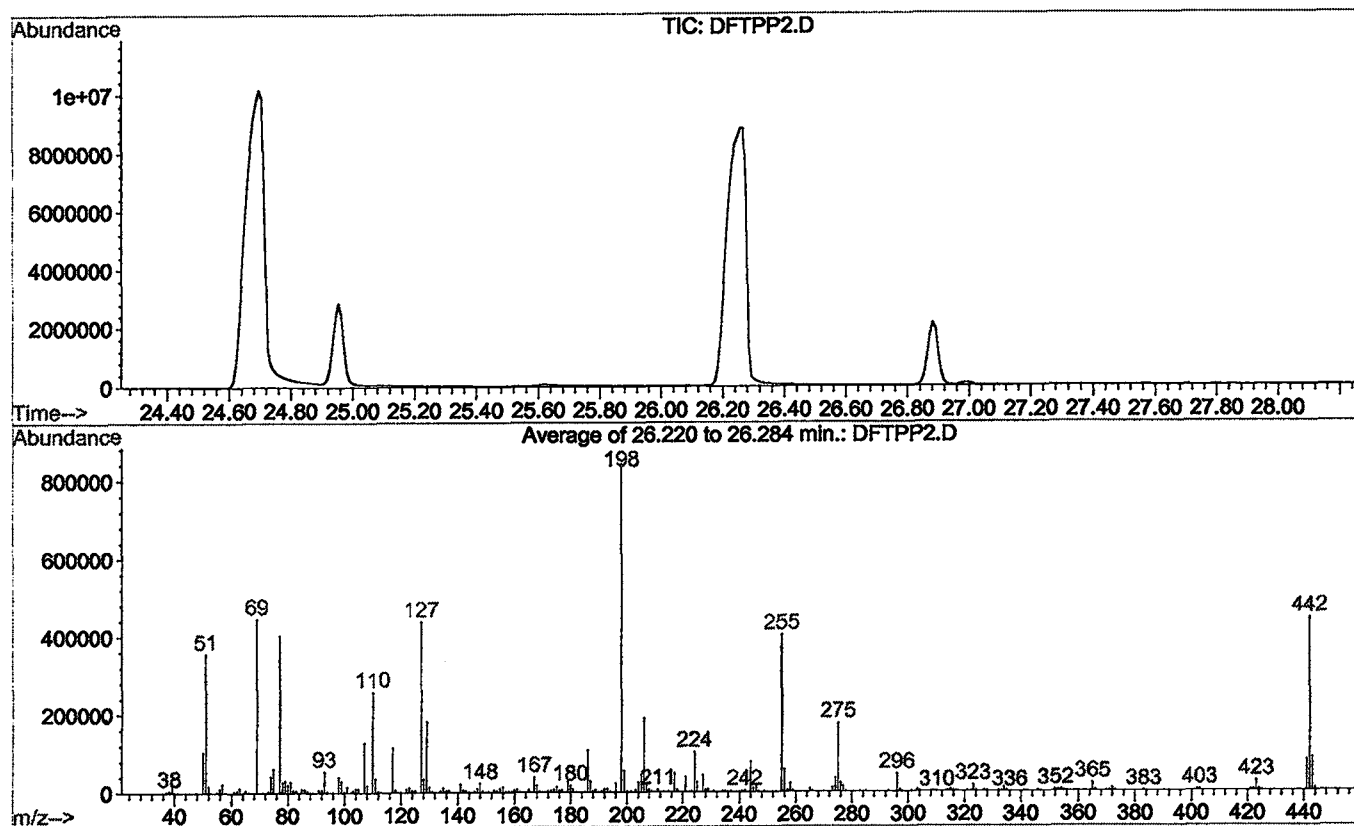

Spectrum Information: Average of 26.220 to 26.284 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	42.4	356724	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	53.0	446059	PASS
70	69	0.00	2	0.0	49	PASS
127	198	40	60	52.1	438444	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	841745	PASS
199	198	5	9	6.7	56197	PASS
275	198	10	30	21.0	176475	PASS
365	198	1	100	2.7	22348	PASS
441	443	0.01	100	93.8	81086	PASS
442	198	40	110	52.6	442760	PASS
443	442	17	23	19.5	86464	PASS