

Method 508 modDate Extracted 12/13/01Page 63

ref

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
LB	✓	500mL		1mL			1mL	1A	7			
Ref	✓				0.5mL			B				
30085	✓							2A				
30115	✓							2B				
30204	✓							3A				
30250	✓							3B				
30255	✓							4A				
30256	✓							4B				
30319	✓							1B				
30315	✓							2A				
30313	✓							5A				
30312	✓							5B				
Remarks												
Reviewed by												
drip rate must be between 5-15 ml/min for liq-liq extractors												
drip rate -												
Extraction type <u>sephun</u>		Solv. lot# <u>V39466</u>		NaCl lot# <u>V11599</u>		Na2SO4 lot# <u>V39400</u>						
STANDARD	INT STD LOG#											
CALIBRATION												
REF/SPIKE	<u>91759</u>											
MDL/MDRF												
Q. CHECK												
INT. STD.												
SURROGATE	<u>6015 12/10/01</u>											
LPC												
ENDRIN/DDT												

Analyst LF
revision 4/12/01

Verified by _____

Reviewed by 1/9/12
Date _____

Sequence Name: C:\HPCHEM\1\SEQUENCE\Dec2101.S

Comment: INST 209; 30Mx0.25umX0.50

Operator: 209 GALOS

Data Path: C:\HPCHEM\1\data\dec2101\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run	On A Barcode Mismatch
(X) Full Method	(X) Inject Anyway
() Reprocessing Only	() Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	NP091101	
2	Sample	2	CAL40	NP091101	
3	Sample	21	30107	GCMS1126	gc/ms scan 12/12 a
4	Sample	22	30111	GCMS1126	gc/ms scan 12/12 a
5	Sample	23	30110	GCMS1126	gc/ms scan 12/12 a
6	Sample	24	30010	GCMS1126	gc/ms scan 12/12 a
7	Sample	25	30009	GCMS1126	gc/ms scan 12/12 a
8	Sample	54	26477	GCMS1126	gc/ms scan
9	Sample	55	26827	GCMS1126	gc/ms scan
10	Sample	26	30023	GCMS1126	gc/ms scan 12/12 a
11	Sample	41	LBC	GCMS1126	gc/ms scan 12/13
12	Sample	53	REFC	GCMS1126	gc/ms scan 12/13
13	Sample	42	30251	GCMS1126	gc/ms scan 12/13
14	Sample	43	30354	GCMS1126	gc/ms scan 12/13
15	Sample	44	30425	GCMS1126	gc/ms scan 12/13
16	Sample	45	30355	GCMS1126	gc/ms scan 12/13
17	Sample	46	30252	GCMS1126	gc/ms scan 12/13
18	Sample	47	30357	GCMS1126	gc/ms scan 12/13
19	Sample	48	30352	GCMS1126	gc/ms scan 12/13
20	Sample	49	30353	GCMS1126	gc/ms scan 12/13
21	Sample	50	30351	GCMS1126	gc/ms scan 12/13
22	Sample	51	30356	GCMS1126	gc/ms scan 12/13
23	Sample	52	30426	GCMS1126	gc/ms scan 12/13
24	Sample	1	DFTPP1	GCMS1126	
25	Sample	2	CAL40A	GCMS1126	
26	Sample	3	LBD	GCMS1126	gc/ms scan 12/13a
27	Sample	4	REFD	GCMS1126	gc/ms scan 12/13a
28	Sample	5	30314	GCMS1126	gc/ms scan 12/13a
29	Sample	6	30315	GCMS1126	gc/ms scan 12/13a
30	Sample	7	30085	GCMS1126	gc/ms scan 12/13a
31	Sample	8	30115	GCMS1126	gc/ms scan 12/13a
32	Sample	9	30250	GCMS1126	gc/ms scan 12/13a
33	Sample	10	30255	GCMS1126	gc/ms scan 12/13a
34	Sample	11	30256	GCMS1126	gc/ms scan 12/13a
35	Sample	12	30254	GCMS1126	gc/ms scan 12/13a
36	Sample	13	30312	GCMS1126	gc/ms scan 12/13a
37	Sample	14	30313	GCMS1126	gc/ms scan 12/13a
38	Sample	1	DFTPP2	GCMS1126	
39	Sample	81	CAL25	GCMS1126	
40	Sample	15	LBE	GCMS1126	gc/ms scan 12/17
41	Sample	16	REFE	GCMS1126	gc/ms scan 12/17
42	Sample	17	28860	GCMS1126	gc/ms scan 12/17

Last Modified: Mon Dec 24 13:53:24 2001

Page: 1

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC2101\DFTPP2.D

Acq On : 22 Dec 2001 8:29 pm

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

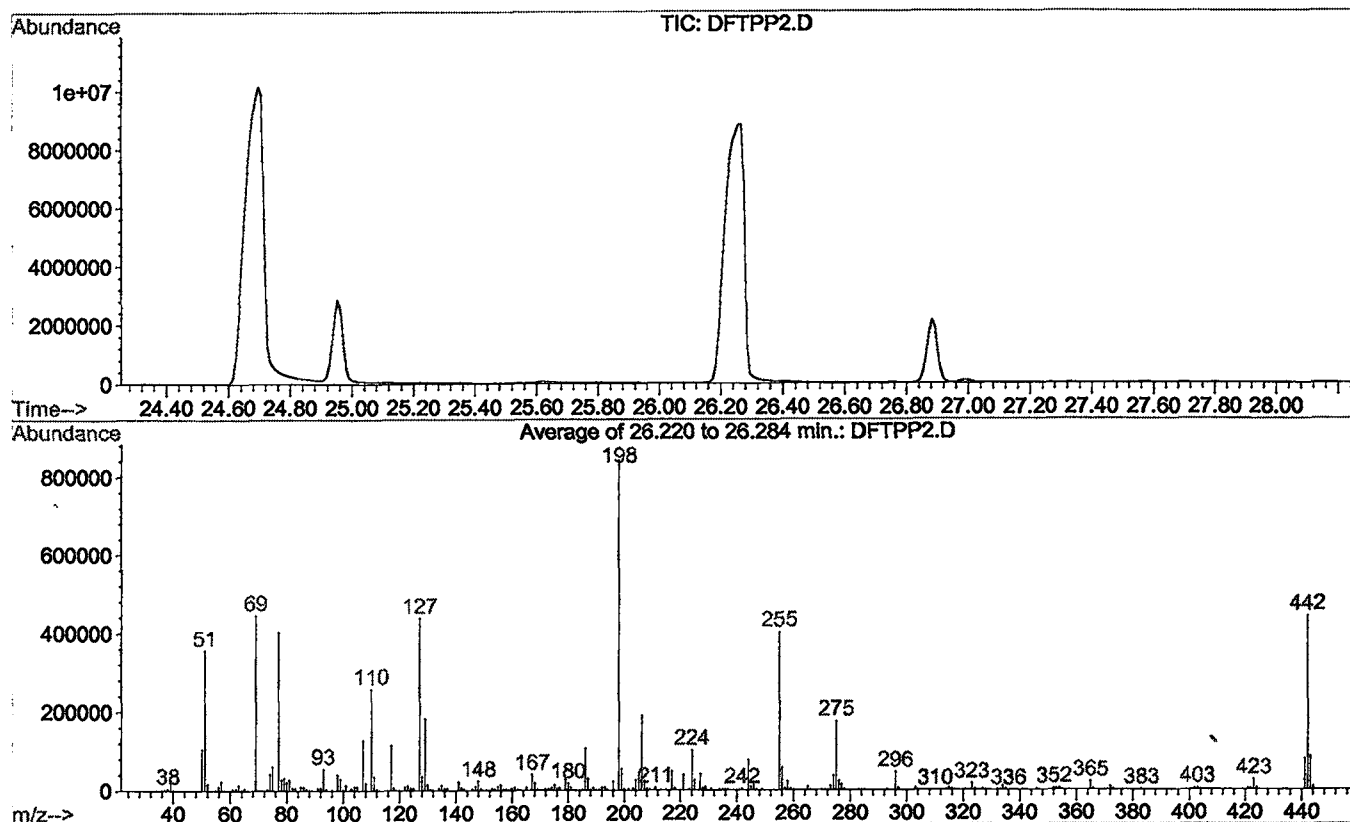

Spectrum Information: Average of 26.220 to 26.284 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	42.4	356724	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	53.0	446059	PASS
70	69	0.00	2	0.0	49	PASS
127	198	40	60	52.1	438444	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	841745	PASS
199	198	5	9	6.7	56197	PASS
275	198	10	30	21.0	176475	PASS
365	198	1	100	2.7	22348	PASS
441	443	0.01	100	93.8	81086	PASS
442	198	40	110	52.6	442760	PASS
443	442	17	23	19.5	86464	PASS

DFTPP2.D GCMS1126.M

Thu Dec 27 09:51:01 2001

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC2701\DFTPP3.D

Acq On : 29 Dec 2001 5:42 pm

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

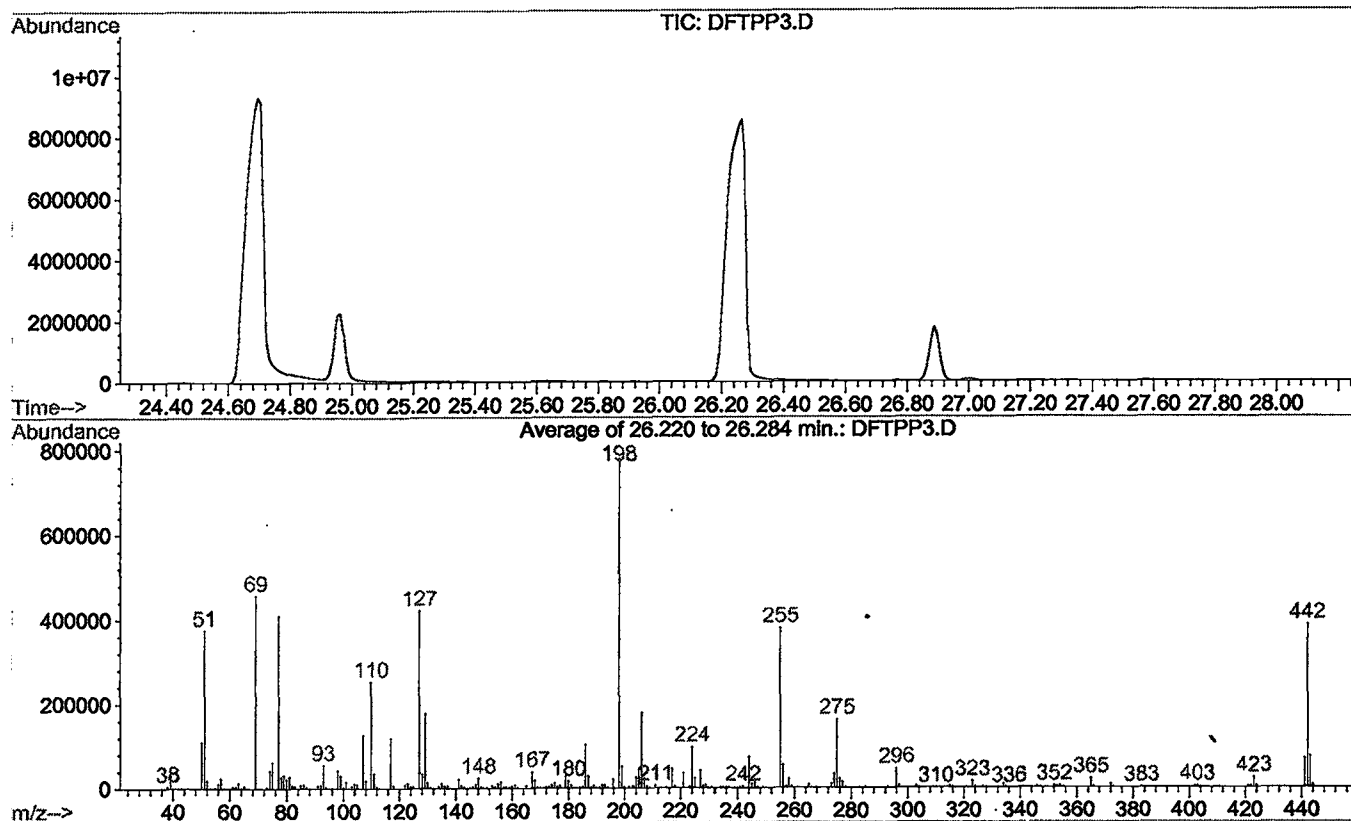

Spectrum Information: Average of 26.220 to 26.284 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	48.2	375534	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	58.8	458633	PASS
70	69	0.00	2	0.1	303	PASS
127	198	40	60	54.2	422724	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	779824	PASS
199	198	5	9	6.7	52272	PASS
275	198	10	30	20.9	163027	PASS
365	198	1	100	2.8	22213	PASS
441	443	0.01	100	93.7	70323	PASS
442	198	40	110	49.6	386776	PASS
443	442	17	23	19.4	75071	PASS