

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 01/09/2002 Time: 13:16:59

Sample: AD30312
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 1/9/02 13:16 Ended: 1/9/02 13:16 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		73		5.0

Comments for Sample AD30312 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 01-09-2002 Time: 13:17:08

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recovery for 8 of the 43 compounds in the LCS Standard were above their acceptance range.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC2101\30312.D

Vial: 13

Acq On : 22 Dec 2001 6:33 pm

Operator: 209 GALOS

Sample : gc/ms scan 12/13a

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Dec 22 19:21 2001

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 14 12:19:30 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.68	152	975677	20.00	ug/l	-0.02
10) Naphthalene-d8	15.27	136	3696045	20.00	ug/l	-0.03
17) Acenaphthene-d10	20.55	164	1842341	20.00	ug/l	-0.02
29) Phenanthrene-d10	24.98	188	2643007	20.00	ug/l	-0.01
38) Chrysene-d12	33.01	240	1440769	20.00	ug/l	-0.02
44) Perylene-d12	37.10	264	969428	20.00	ug/l	-0.01

System Monitoring Compounds

37) 2,4-DDD	30.05	235	139835	3.66	ug/mL	-0.02
Spiked Amount	5.000		Recovery	=	73.20%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.33	128	1232	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	21.21	165	167	N.D.	
25) Diethylphthalate	22.10	149	1280	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	

(#)=qualifier out of range (m)=manual integration

30312.D GCMS1126.M Thu Dec 27 10:01:23 2001

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC2101\30312.D

Vial: 13

Acq On : 22 Dec 2001 6:33 pm

Operator: 209 GALOS

Sample : gc/ms scan 12/13a

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Dec 22 19:21 2001

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 14 12:19:30 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	24.98	178	1022	N.D.		
34) Anthracene	24.98	178	1022	N.D.		
35) Di-n-butylphthalate	27.01	149	10421	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	31.50	149	171	N.D.		
41) Benzo(a)anthracene	33.01	228	3399	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.29	149	6598	N.D.		
43) Chrysene	33.01	228	3399	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	37.10	252	3860	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

 (#) = qualifier out of range (m) = manual integration

30312.D GCMS1126.M

Thu Dec 27 10:01:26 2001

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\DEC2101\30312.D
Acq On : 22 Dec 2001 6:33 pm
Sample : gc/ms scan 12/13a
Misc :
MS Integration Params: GOOFY.P
Quant Time: Dec 22 19:21 2001

Vial: 13
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS1126.RES

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri Dec 14 12:19:30 2001
Response via : Initial Calibration

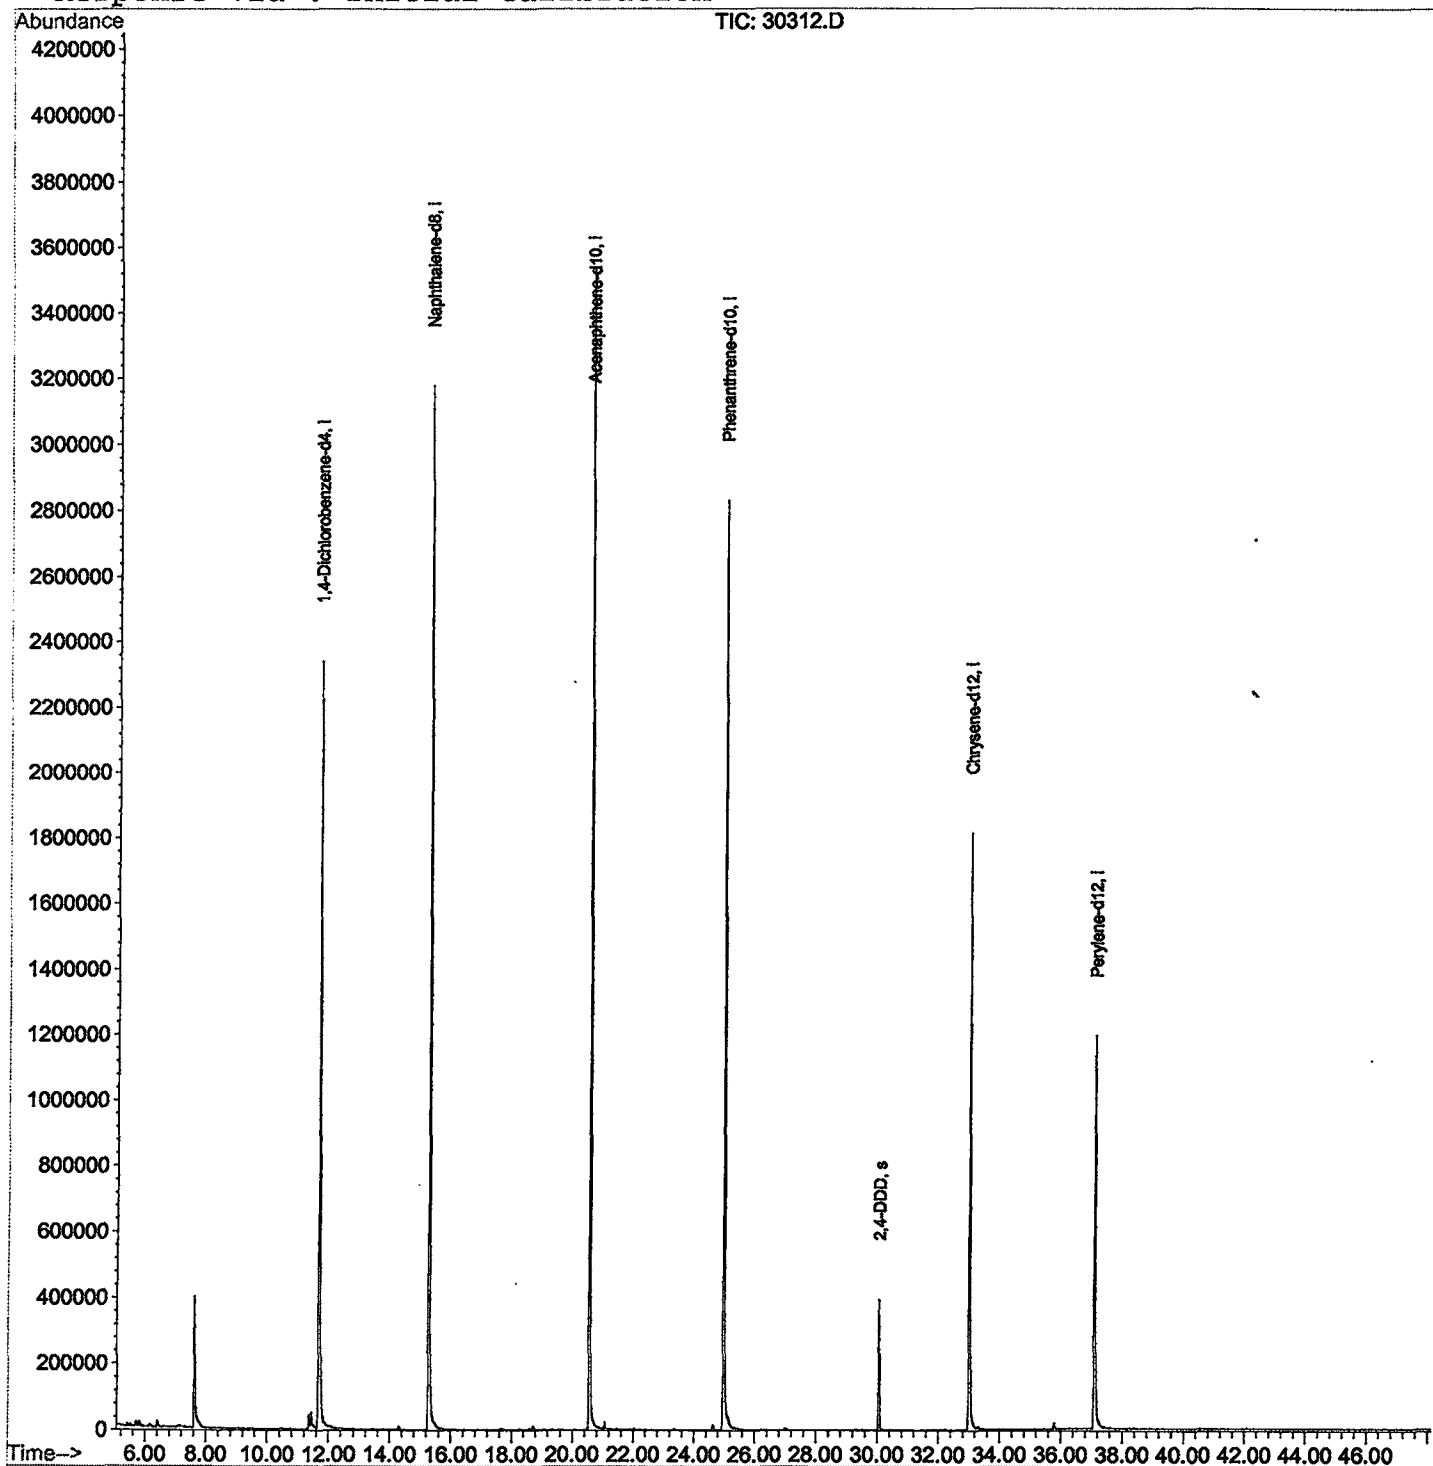

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\DEC2101\30312.D
Acq On : 22 Dec 2001 6:33 pm
Sample : gc/ms scan 12/13a
Misc :
MS Integration Params: LSCINT.P

Vial: 13
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Signal : TIC


peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	7.608	275	279	311	rBV	397680	1129196	14.28%	2.930%
2	11.354	683	687	692	rBV	42996	102944	1.30%	0.267%
3	11.437	692	696	716	rVB	49852	175937	2.22%	0.457%
4	11.675	717	722	747	rBV	2333436	5987534	75.71%	15.537%
5	15.274	1109	1114	1134	rBV	3178000	7279505	92.04%	18.890%
6	20.553	1683	1689	1713	rBV	3538032	7908805	100.00%	20.523%
7	24.977	2164	2171	2185	rBV2	2831608	6986925	88.34%	18.131%
8	30.054	2718	2724	2735	rBV2	394214	822117	10.39%	2.133%
9	33.010	3039	3046	3071	rBV2	1814372	4596092	58.11%	11.927%
10	37.105	3484	3492	3512	rBV2	1190576	3547744	44.86%	9.206%

Sum of corrected areas: 38536799

30312.D GCMS1126.M Wed Jan 02 10:15:54 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\DEC2101\30312.D
Operator : 209 GALOS
Acquired : 22 Dec 2001 6:33 pm using AcqMethod GCMS1126
Instrument : GC/MS 209
Sample Name: gc/ms scan 12/13a
Misc Info :
Vial Number: 13
Quant File : GCMS1126.RES (RTE Integrator)

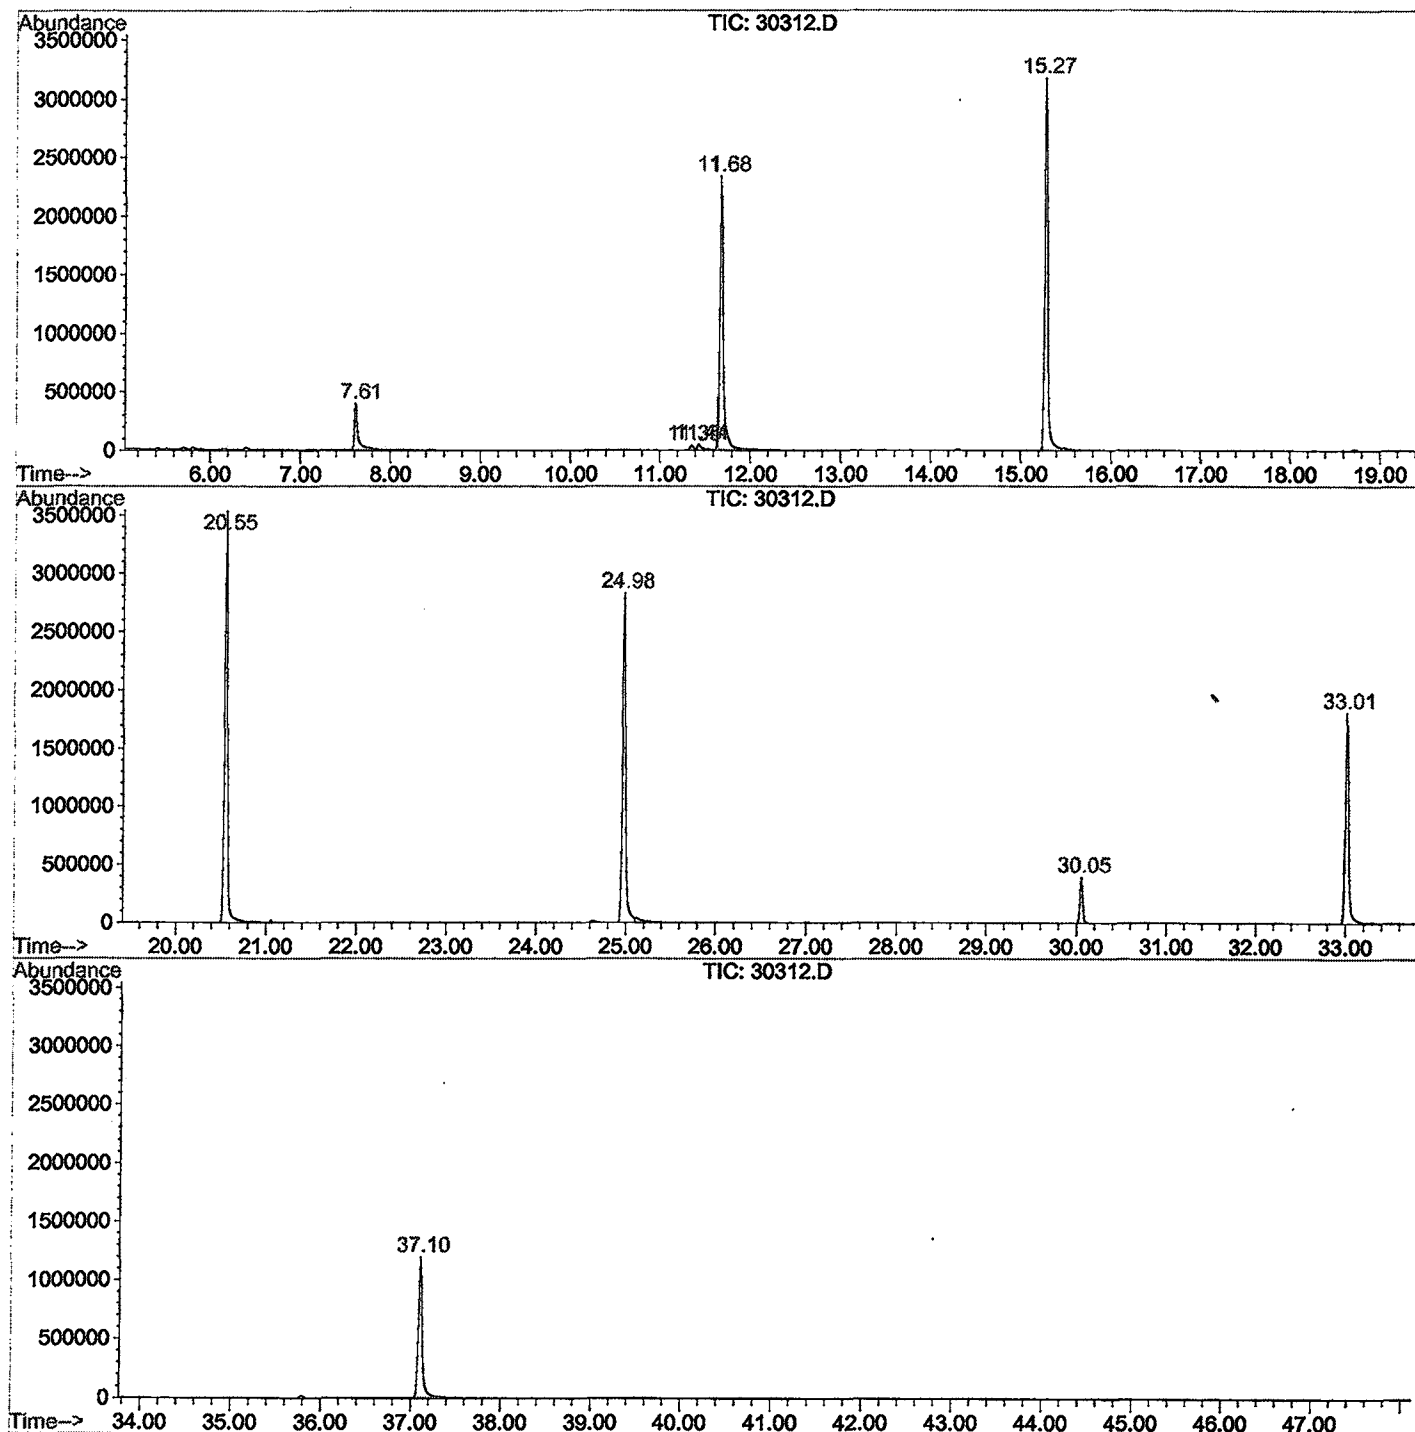

30312.D GCMS1126.M Wed Jan 02 10:16:00 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\DEC2101\30312.D
Acq On : 22 Dec 2001 6:33 pm
Sample : gc/ms scan 12/13a
Misc :
MS Integration Params: LSCINT.P









Vial: 13
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 Silane, tetramethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.61	3.77 ug/l	1129200	1,4-Dichlorobenzene-d4	11.68

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
2			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	9
3			N-Ethylformamide	73	C3H7NO	000627-45-2	9
4			1-Butanamine, 3-methyl-	87	C5H13N	000107-85-7	9

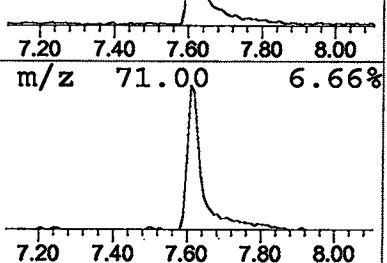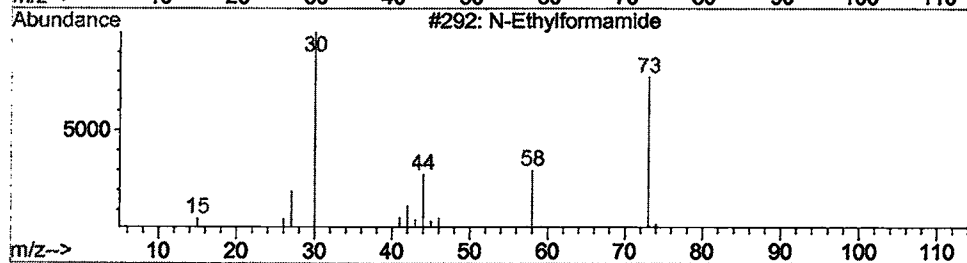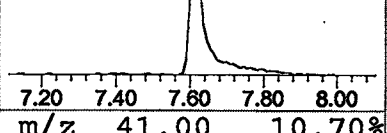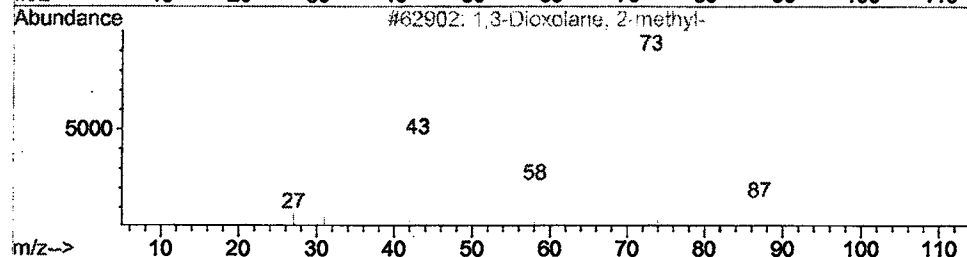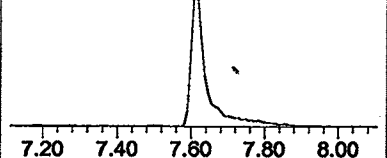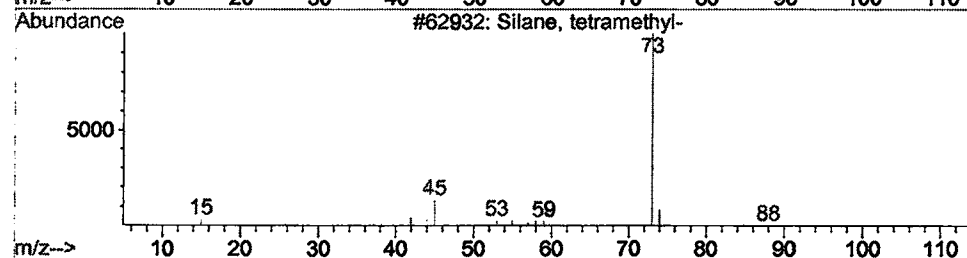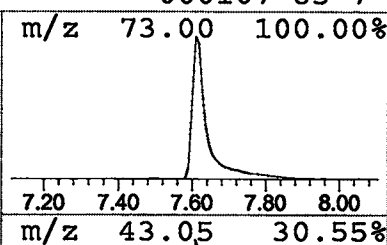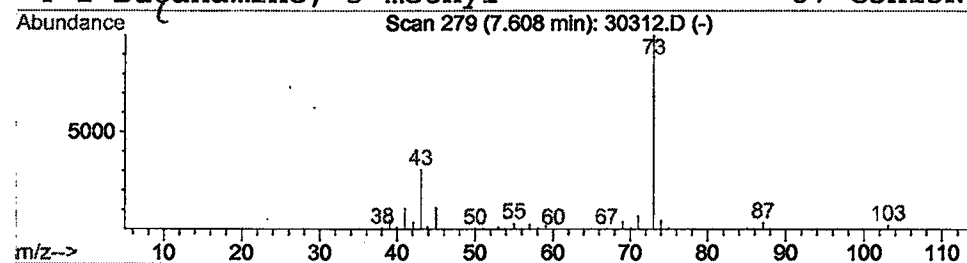

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\DEC2101\30312.D
 Acq On : 22 Dec 2001 6:33 pm
 Sample : gc/ms scan 12/13a
 Misc :
 MS Integration Params: LSCINT.P









Vial: 13
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 2 2-Propanol, 1-(2-methoxy-1-met Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.44	0.59 ug/l	175937	1,4-Dichlorobenzene-d4	11.68

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Propanol, 1-(2-methoxy-1-methylet	148	C7H16O3	020324-32-7	78
2			1-Propanol, 2-(2-hydroxypropoxy)-	134	C6H14O3	000106-62-7	53
3			2-Propanol, 1,1'-oxybis-	134	C6H14O3	000110-98-5	39
4			Propane, 1,2-dimethoxy-	104	C5H12O2	007778-85-0	38

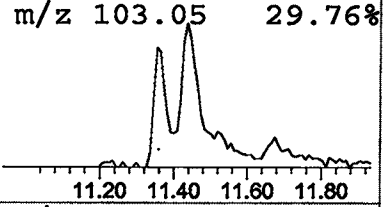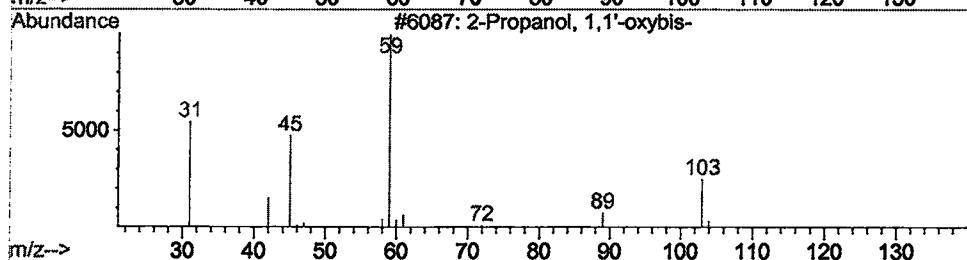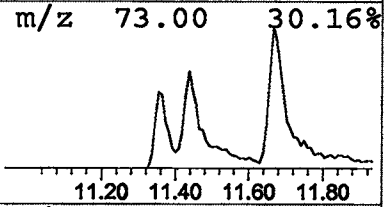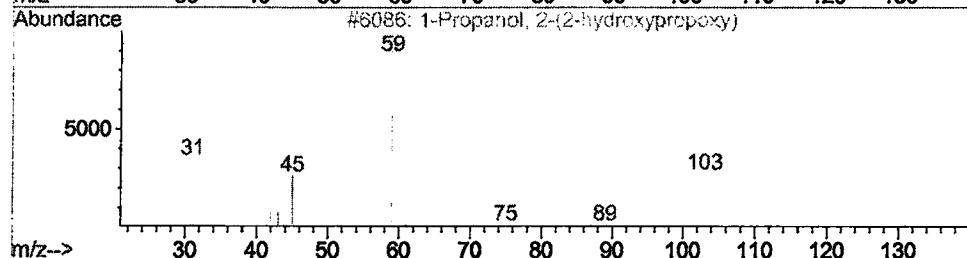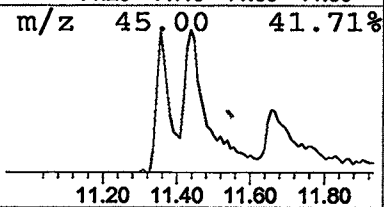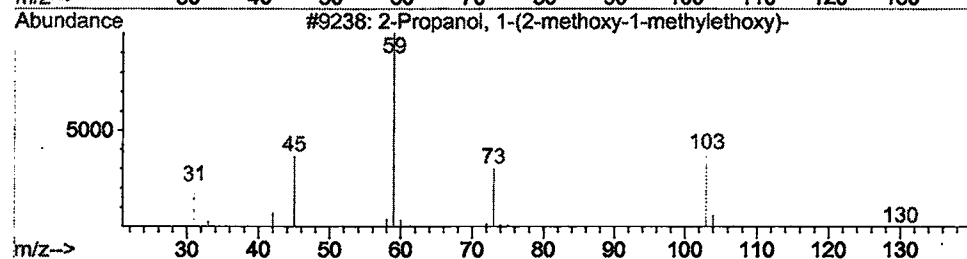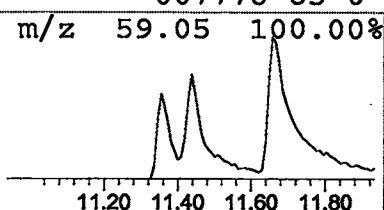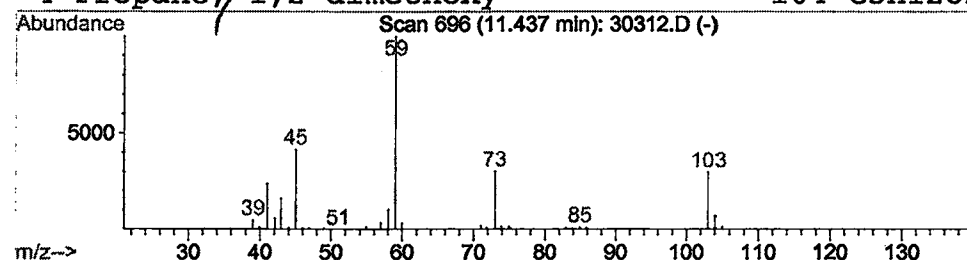

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 22 Dec 2001 6:33 pm
 Data File: C:\HPCHEM\1\DATA\DEC2101\30312.D
 Name: gc/ms scan 12/13a
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
-----	-----	-----	-----	-----	-----	-----	-----	-----
Silane, tetramethyl-	7.61	3.8	ug/l	1129200	ISTD01	11.68	5987530	20.0
2-Propanol, 1-(2-met	11.44	0.6	ug/l	175937	ISTD01	11.68	5987530	20.0

30312.D GCMS1126.M Wed Jan 02 10:16:13 2002