

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR2502\9332.D
 Acq On : 25 Apr 2002 8:30 pm
 Sample : gc/ms scan 4/18
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Apr 26 7:44 2002

Vial: 9
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0412.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Thu Apr 25 15:21:43 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0412

*lan les
lan sum*

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	12.21	152	554199	20.00	ug/l	-0.03
10) Naphthalene-d8	15.84	136	2012798	20.00	ug/l	-0.03
17) Acenaphthene-d10	21.15	164	1133937	20.00	ug/l	-0.02
30) Phenanthrene-d10	25.58	188	1667616	20.00	ug/l	-0.03
39) Chrysene-d12	33.64	240	1069869	20.00	ug/l	-0.03
45) Perylene-d12	37.87	264	652594	20.00	ug/l	-0.05

System Monitoring Compounds

28) TCMX	23.28	209	38548	6.72 ^{6.87} ug/L	-0.05
Spiked Amount	10.000		Recovery	= 67.20% ^{69%}	
38) 2,4-DDD	0.00	235	0	0.00 ug/mL	
Spiked Amount	5.000		Recovery	= 0.00%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.90	128	201	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.62	149	793	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	

(#) = qualifier out of range (m) = manual integration

9332.D GCMS0412.M Fri Apr 26 07:45:47 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR2502\9332.D
 Acq On : 25 Apr 2002 8:30 pm
 Sample : gc/ms scan 4/18
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Apr 26 7:44 2002

Vial: 9
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0412.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Thu Apr 25 15:21:43 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0412

Compound	R.T.	QIon	Response	Conc Unit	Qvalue
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	25.65	178	395	N.D.	
35) Anthracene	25.65	178	395	N.D.	
36) Di-n-butylphthalate	27.55	149	2484	N.D.	
37) Fluoranthene	29.28	202	284	N.D.	
40) Pyrene	0.00	202	0	N.D.	
41) Butylbenzylphthalate	0.00	149	0	N.D.	
42) Benzo(a)anthracene	33.64	228	2062	N.D.	
43) Bis(2-ethylhexyl)phthalate	33.86	149	38869	1.45 ug/l #	94
44) Chrysene	33.64	228	2489	N.D.	
46) Di-n-Octylphthalate	35.60	149	274	N.D.	
47) Benzo(b)fluoranthene	0.00	252	0	N.D.	
48) Benzo(k)fluoranthene	0.00	252	0	N.D.	
49) Benzo(a)pyrene	37.88	252	2571	N.D.	
50) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.	
51) Dibenz(a,h)anthracene	0.00	278	0	N.D.	
52) Benzo(g,h,i)perylene	0.00	276	0	N.D.	

 (#) = qualifier out of range (m) = manual integration
 9332.D GCMS0412.M Fri Apr 26 07:45:48 2002


Quantitation Report

Data File : C:\HPCHEM\1\DATA\APR2502\9332.D
Acq On : 25 Apr 2002 8:30 pm
Sample : gc/ms scan 4/18
Misc :
MS Integration Params: GOOFY.P
Quant Time: Apr 26 7:44 2002

Vial: 9
Operator:
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0412.RES

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Thu Apr 25 15:21:43 2002
Response via : Initial Calibration

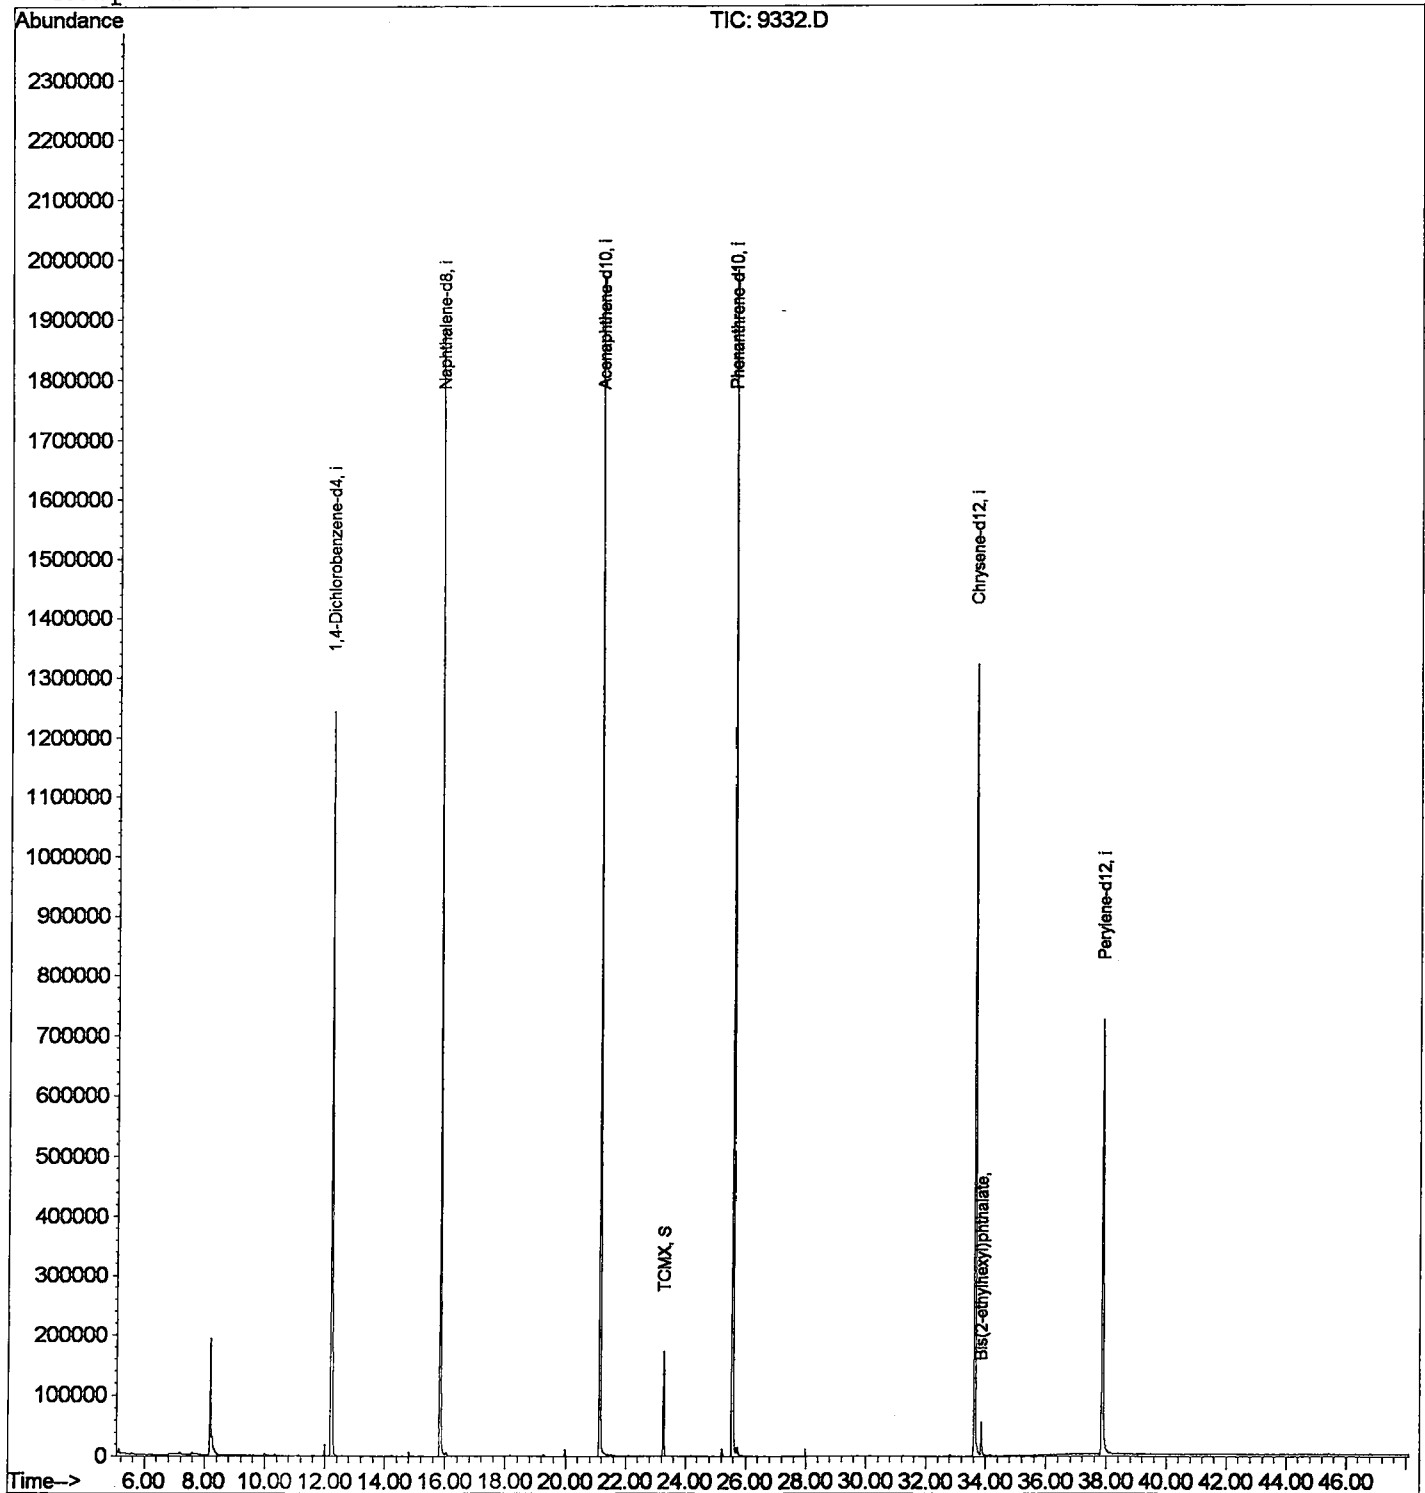

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\APR2502\9332.D
 Acq On : 25 Apr 2002 8:30 pm
 Sample : gc/ms scan 4/18
 Misc :
 MS Integration Params: LSCINT.P

Vial: 9
 Operator:
 Inst : 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.188	338	342	347	rBV	192527	391622	9.15%	1.837%
2	12.209	775	780	791	rBV	1242934	2966947	69.29%	13.914%
3	15.844	1170	1176	1193	rBV	1885615	3796839	88.67%	17.806%
4	21.151	1747	1754	1768	rBV	1972407	4282030	100.00%	20.082%
5	23.280	1979	1986	1994	rVB	172984	339882	7.94%	1.594%
6	25.585	2231	2237	2249	rBV2	1980523	4175247	97.51%	19.581%
7	33.645	3108	3115	3134	rBV	1321756	3059174	71.44%	14.347%
8	33.856	3134	3138	3145	rVV	53364	118870	2.78%	0.557%
9	37.868	3567	3575	3593	rBV2	723236	2192260	51.20%	10.281%

Sum of corrected areas: 21322871

9332.D GCMS0412.M Fri Apr 26 08:18:45 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\APR2502\9332.D
 Operator :
 Acquired : 25 Apr 2002 8:30 pm using AcqMethod GCMS0412
 Instrument : 209
 Sample Name: gc/ms scan 4/18
 Misc Info :
 Vial Number: 9
 Quant File :GCMS0412.RES (RTE Integrator)

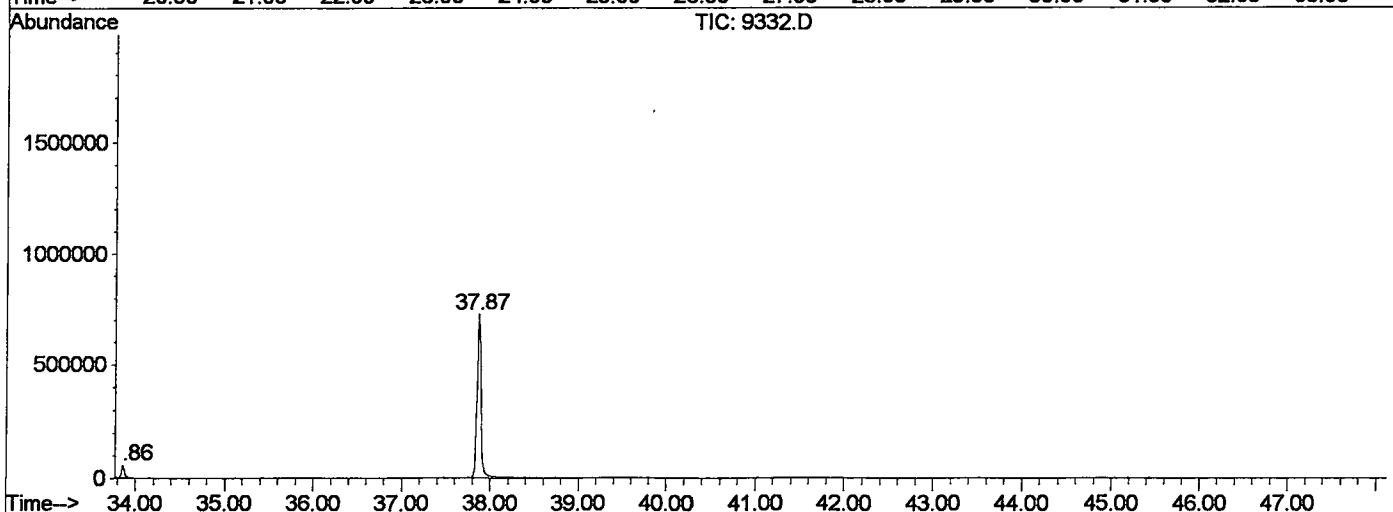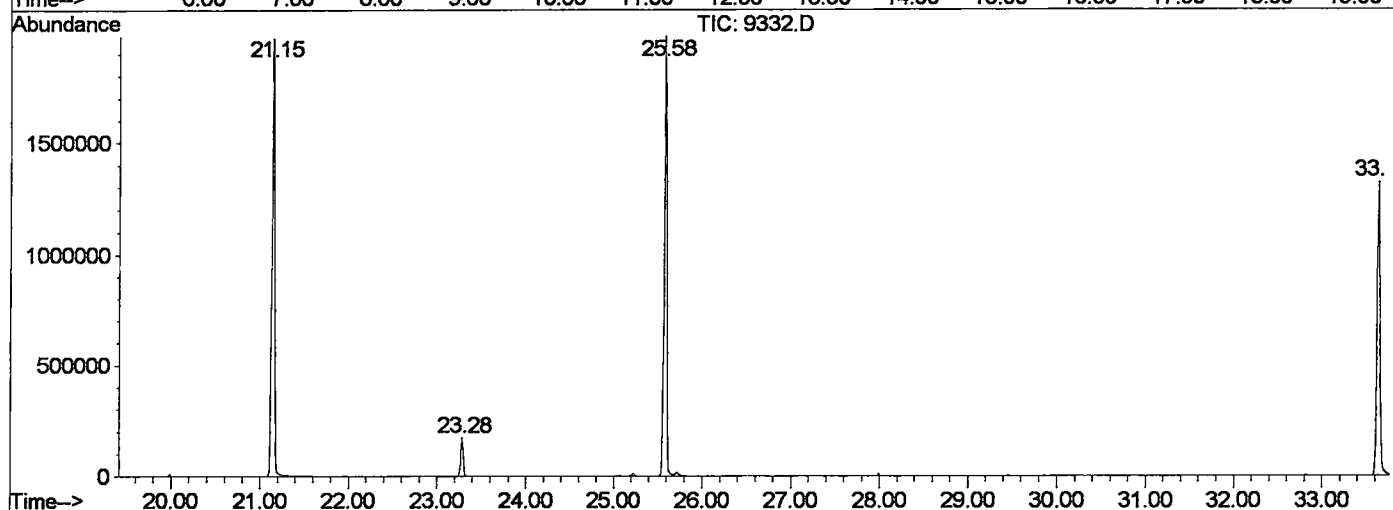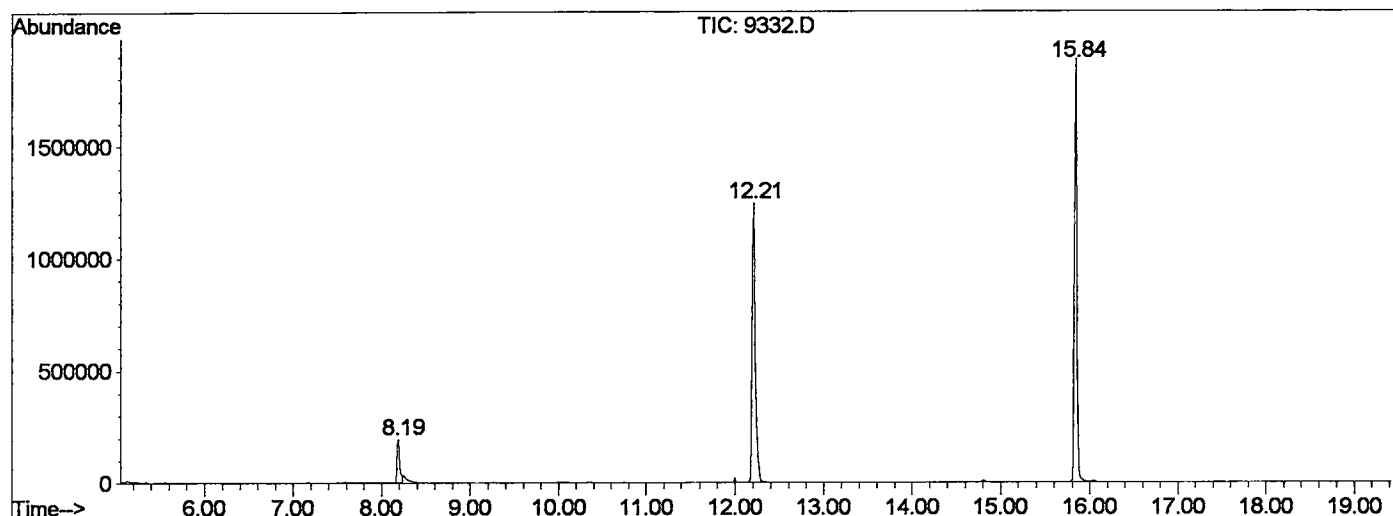

9332.D GCMS0412.M Fri Apr 26 08:18:46 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\APR2502\9332.D
 Acq On : 25 Apr 2002 8:30 pm
 Sample : gc/ms scan 4/18
 Misc :
 MS Integration Params: LSCINT.P


Vial: 9
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.19	2.64 ug/l	391622	1,4-Dichlorobenzene-d4	12.21

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2		Acetic acid, 1,1-dimethylethyl este	116	C6H12O2	000540-88-5	33
3		5-Hexen-2-one	98	C6H10O	000109-49-9	9
4		3-Hydroxy-2-pentanone	102	C5H10O2	003142-66-3	9

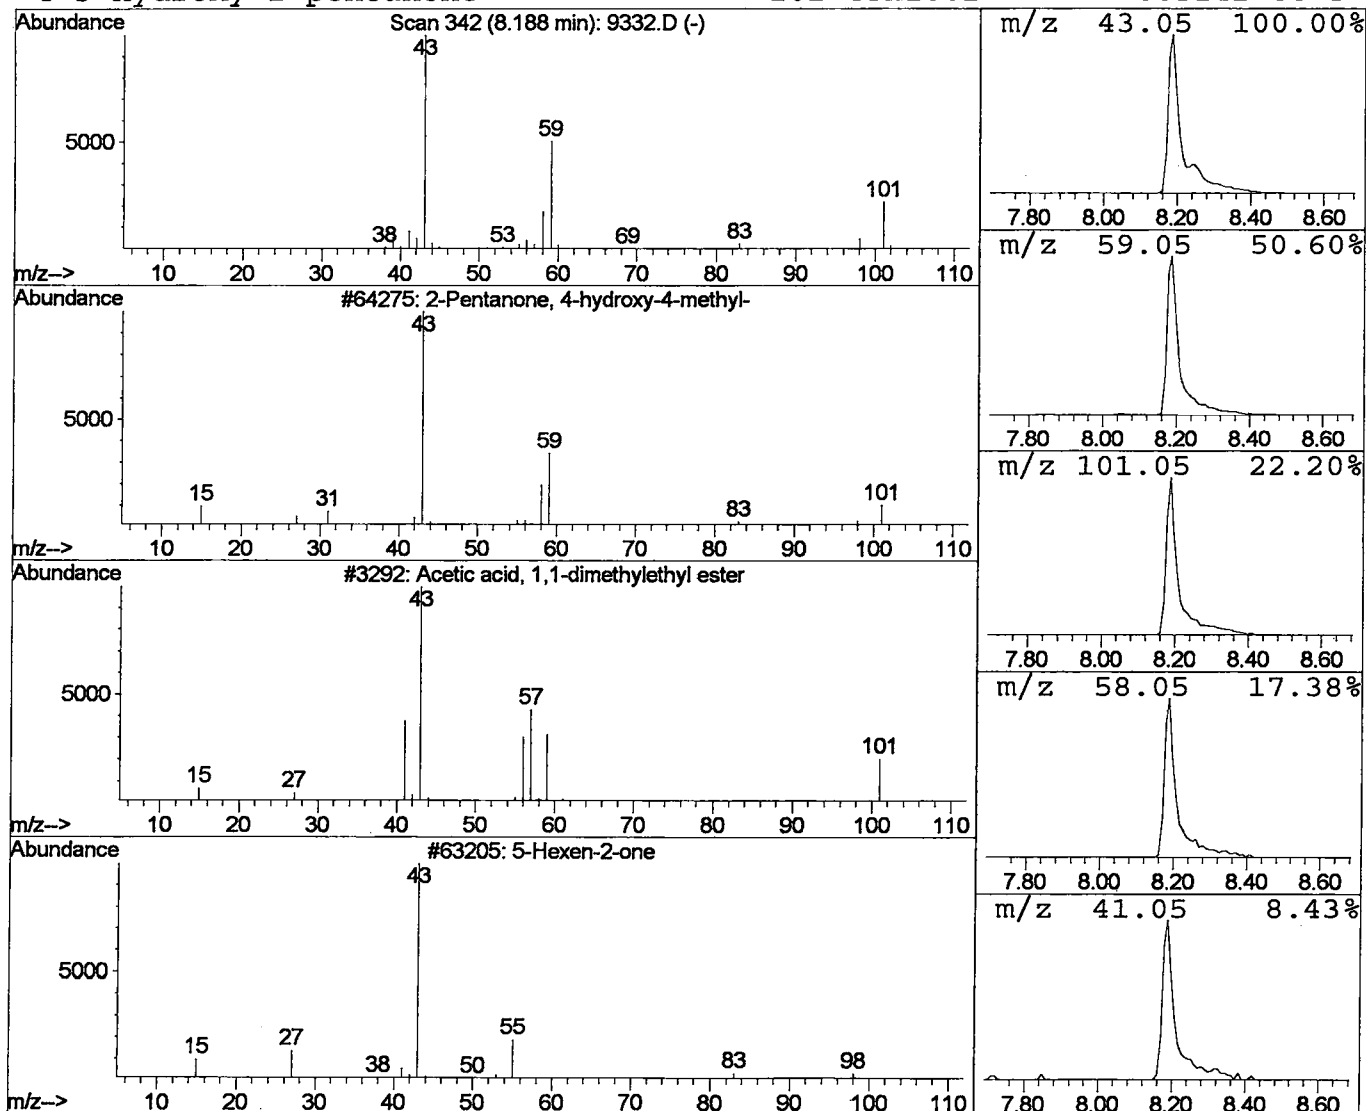

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 25 Apr 2002 8:30 pm
 Data File: C:\HPCHEM\1\DATA\APR2502\9332.D
 Name: gc/ms scan 4/18
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.19	2.6	ug/l	391622	ISTD01	12.21	2966950	20.0

9332.D GCMS0412.M Fri Apr 26 08:18:47 2002