

Data File : C:\HPCHEM\1\DATA\MAY0302\LBC.D

Vial: 39

Acq On : 5 May 2002 5:15 am

Operator:

Sample : GC/MS SCAN 4/23

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: May 7 14:27 2002

Quant Results File: GCMS0501.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed May 01 10:40:31 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0501

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	12.19	152	501040	40.00	ug/l	-0.02
10) Naphthalene-d8	15.82	136	1840686	40.00	ug/l	-0.03
17) Acenaphthene-d10	21.14	164	990142	40.00	ug/l	-0.01
30) Phenanthrene-d10	25.57	188	1368264	40.00	ug/l	-0.02
38) Chrysene-d12	33.64	240	861455	40.00	ug/l	-0.03
44) Perylene-d12	37.86	264	572501	40.00	ug/l	-0.02

System Monitoring Compounds

28) TCMX	23.27	209	22400	4.65	ug/L	-0.02
Spiked Amount	10.000		Recovery	=	46.50%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.61	149	621	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	25.58	178	249	N.D.	

(#)= qualifier out of range (m) = manual integration

LBC.D GCMS0501.M Tue May 07 14:27:53 2002

Page 1

Data File : C:\HPCHEM\1\DATA\MAY0302\LBC.D
 Acq On : 5 May 2002 5:15 am
 Sample : GC/MS SCAN 4/23
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 7 14:27 2002

Vial: 39
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0501.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed May 01 10:40:31 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0501

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
35) Anthracene	25.58	178	249	N.D.		
36) Di-n-butylphthalate	27.55	149	2004	N.D.		
37) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.64	228	1892	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.86	149	1871	N.D.		
43) Chrysene	33.64	228	1892	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	37.86	252	2133	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration
 LBC.D GCMS0501.M Tue May 07 14:27:54 2002


Page 2

Data File : C:\HPCHEM\1\DATA\MAY0302\LBC.D
 Acq On : 5 May 2002 5:15 am
 Sample : GC/MS SCAN 4/23
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 7 14:27 2002

Vial: 39
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0501.RES

Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed May 01 10:40:31 2002
 Response via : Initial Calibration

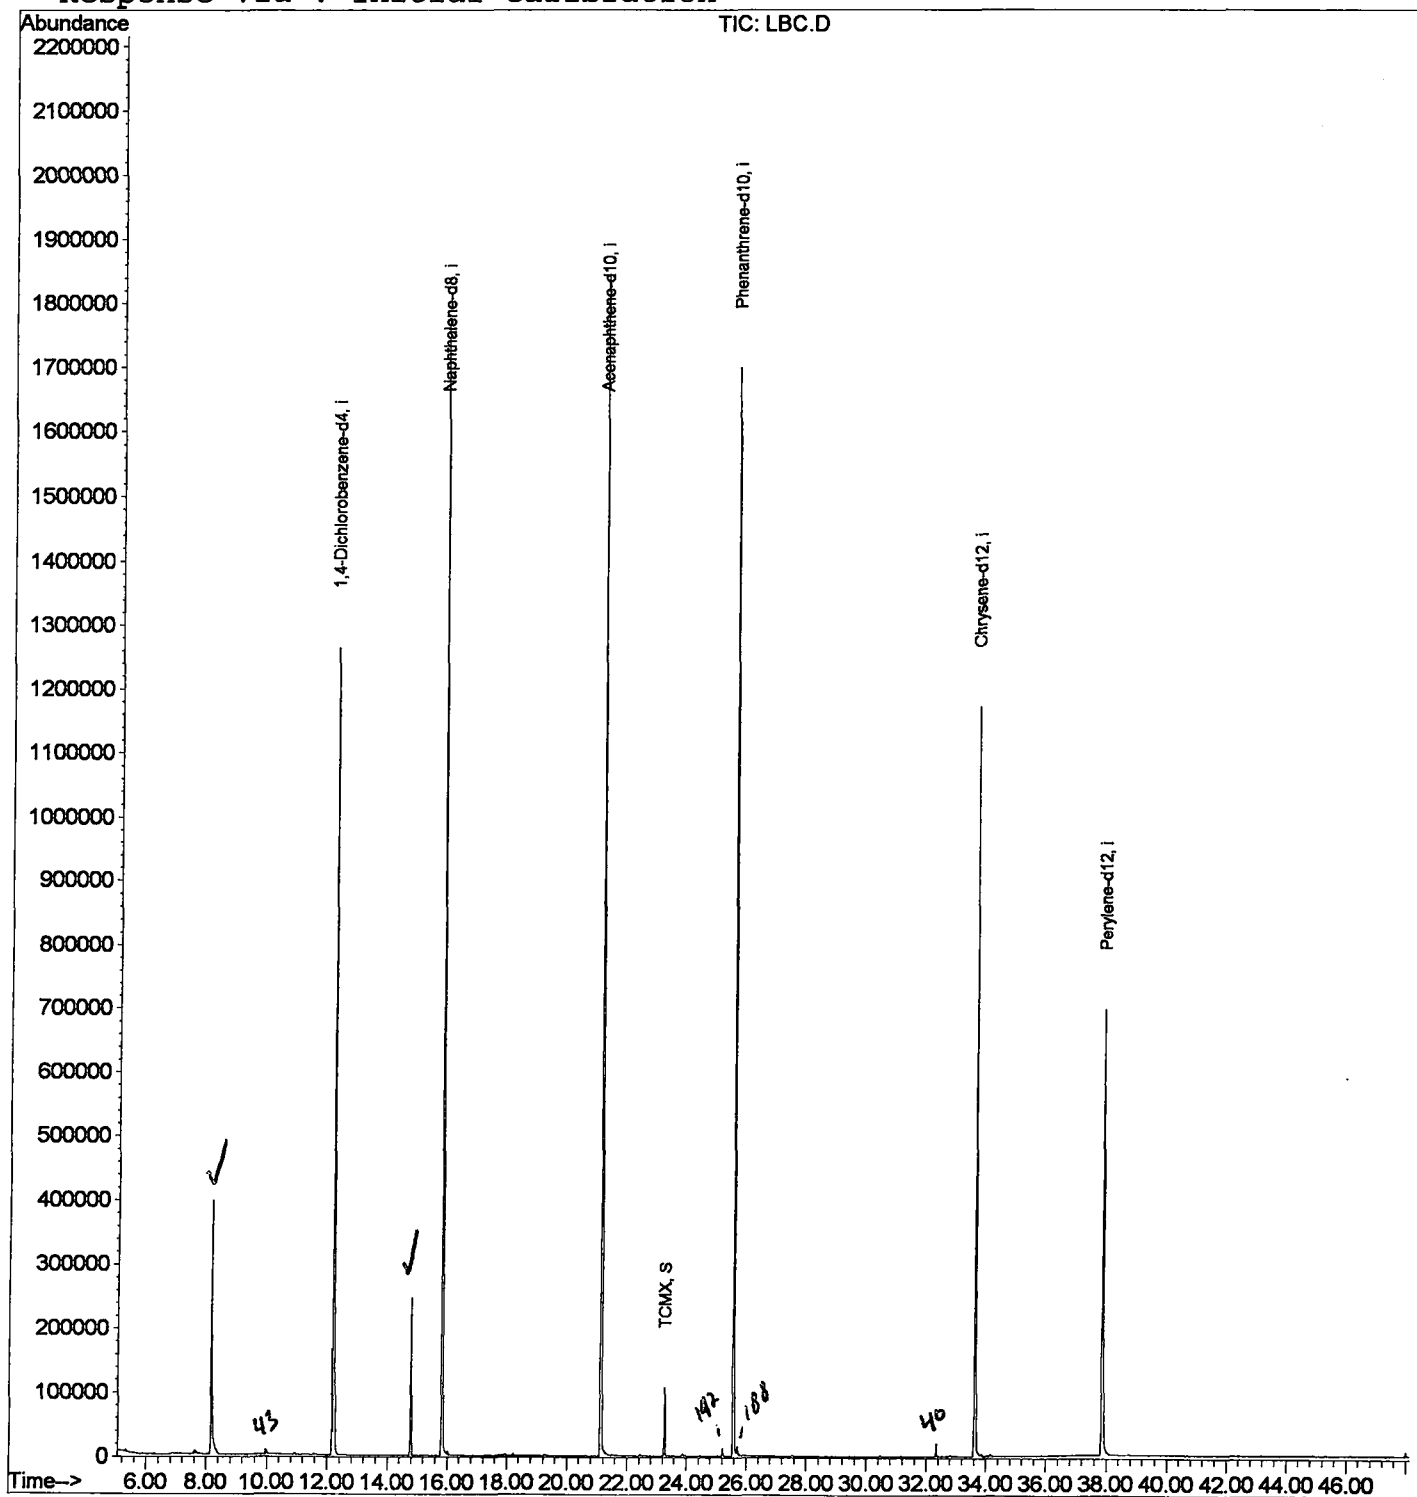

Data File : C:\HPCHEM\1\DATA\MAY0302\LBC.D
 Acq On : 5 May 2002 5:15 am
 Sample : GC/MS SCAN 4/23
 Misc :
 MS Integration Params: LSCINT.P

Vial: 39
 Operator:
 Inst : 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC


peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.153	337	340	367	rBV	395490	936898	23.22%	4.558%
2	12.194	775	781	797	rBV	1261561	2899124	71.85%	14.104%
3	14.796	1059	1065	1071	rBV	245463	478104	11.85%	2.326%
4	15.823	1171	1177	1191	rBV	1775492	3664664	90.83%	17.829%
5	21.138	1750	1757	1771	rBV	1844432	4034727	100.00%	19.629%
6	23.273	1980	1990	1996	rVB	106688	219729	5.45%	1.069%
7	25.573	2235	2241	2253	rBV2	1697289	3697916	91.65%	17.990%
8	33.637	3114	3121	3136	rBV	1172093	2607780	64.63%	12.687%
9	37.861	3574	3582	3598	rBV2	696032	2015991	49.97%	9.808%

Sum of corrected areas: 20554933

LBC.D GCMS0501.M Tue May 07 15:03:29 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAY0302\LBC.D
 Operator :
 Acquired : 5 May 2002 5:15 am using AcqMethod GCMS0501
 Instrument : 209
 Sample Name: GC/MS SCAN 4/23
 Misc Info :
 Vial Number: 39
 Quant File :GCMS0501.RES (RTE Integrator)

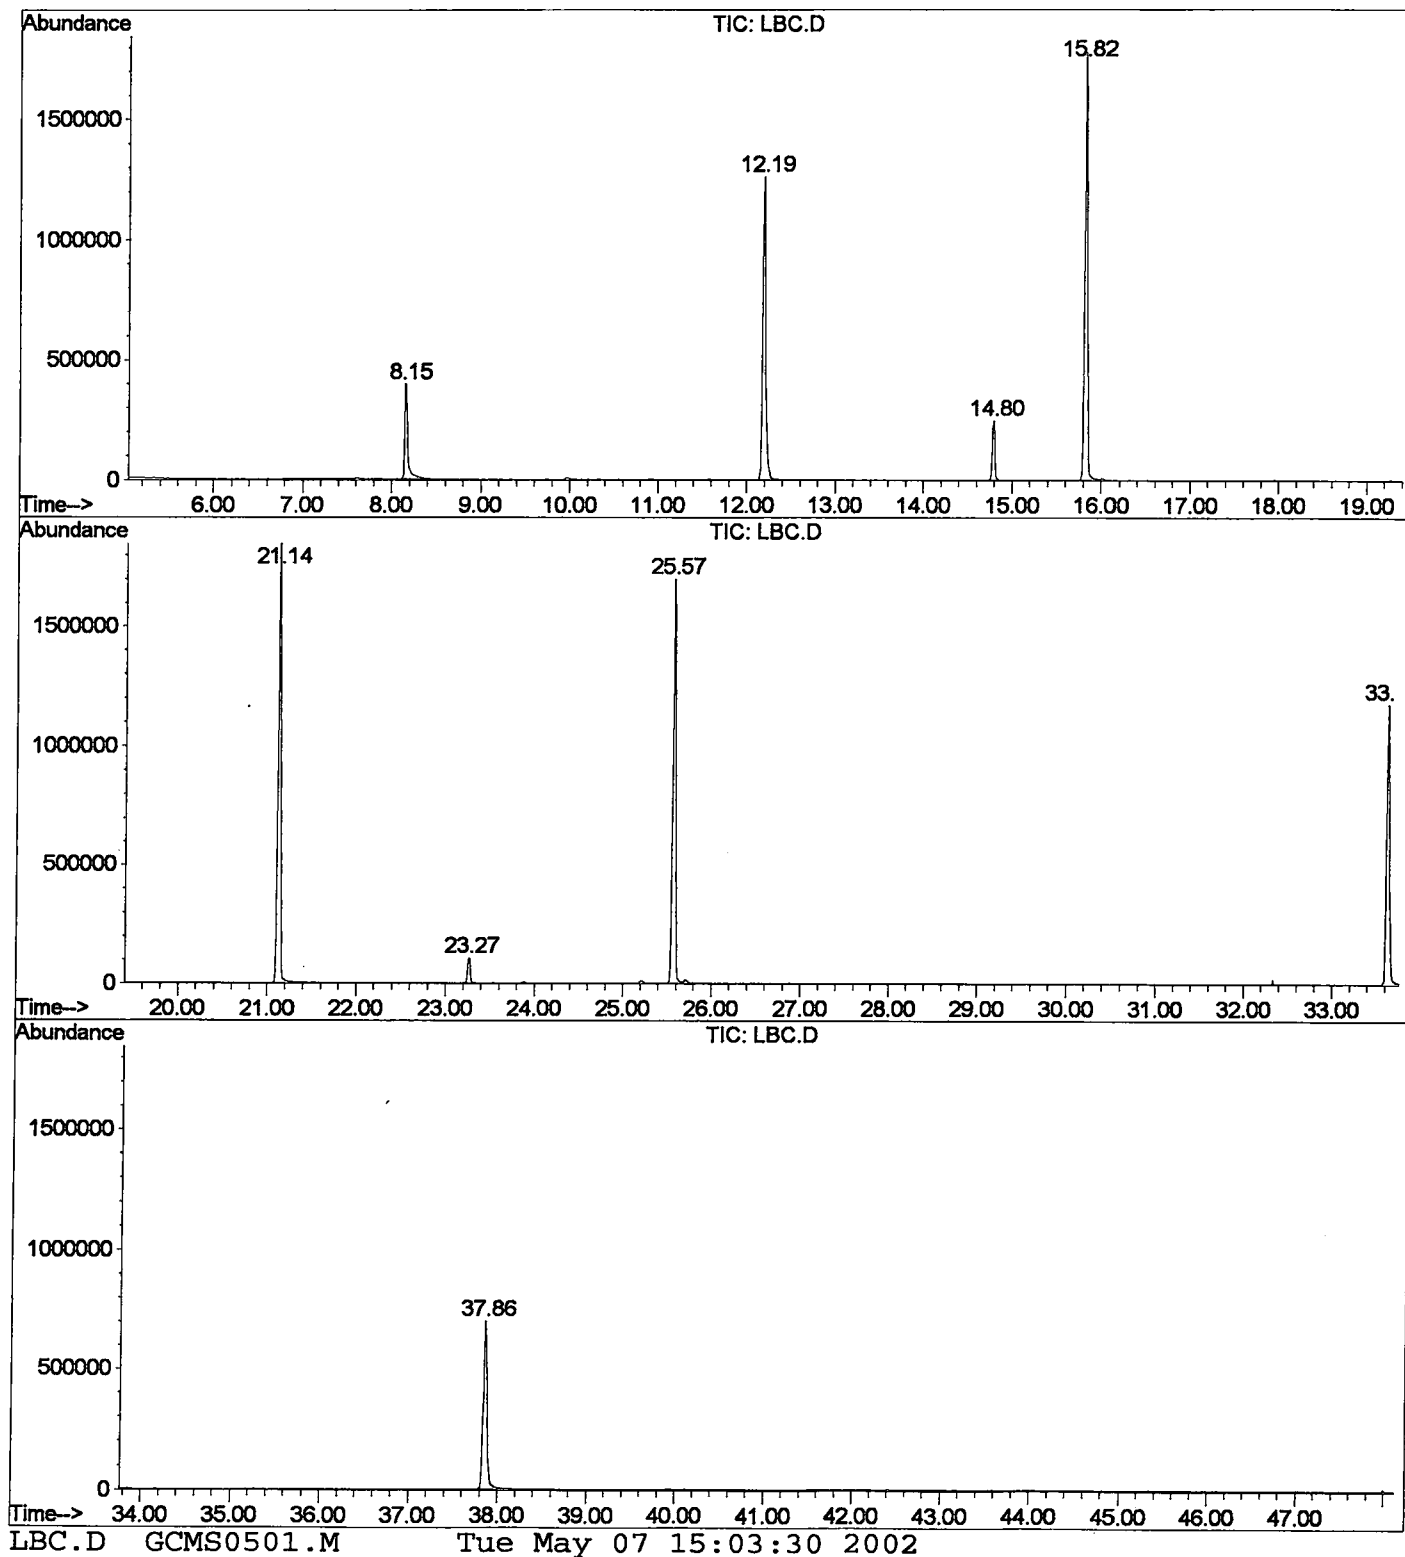

Data File : C:\HPCHEM\1\DATA\MAY0302\LBC.D
 Acq On : 5 May 2002 5:15 am
 Sample : GC/MS SCAN 4/23
 Misc :
 MS Integration Params: LSCINT.P


Vial: 39
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.15	12.93 ug/l	936898	1,4-Dichlorobenzene-d4	12.19

Hit# of	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	78
2	3-Hydroxy-2-pentanone	102	C5H10O2	003142-66-3	9
3	CH2=CHCH2C(O)OCH3	100	C5H8O2	003724-55-8	9
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	7

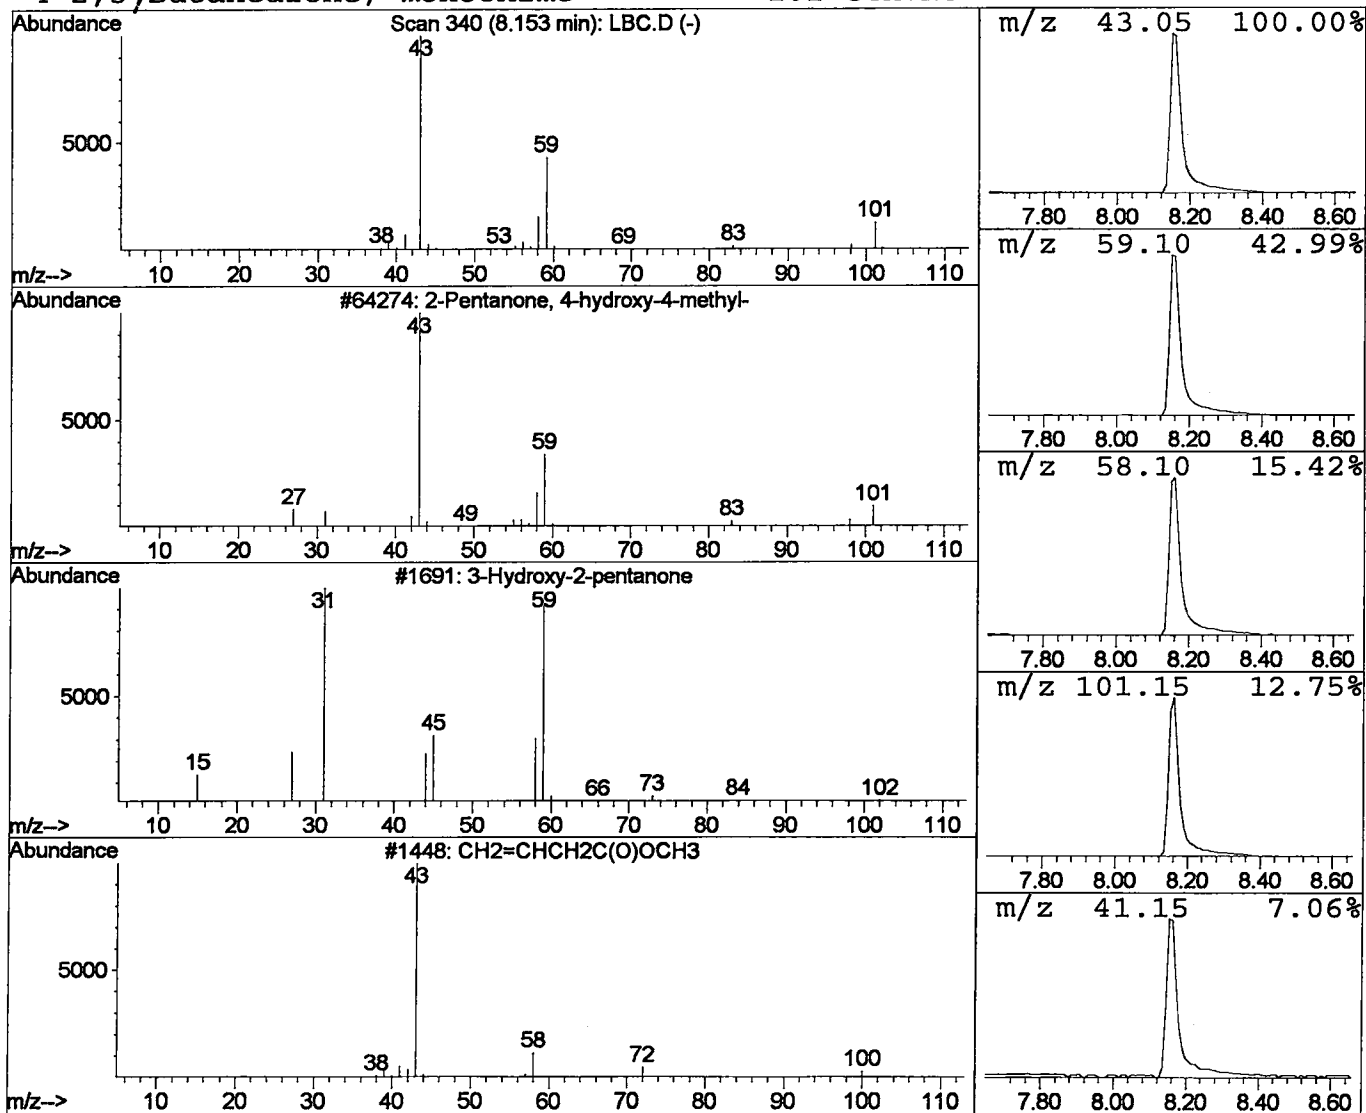

Data File : C:\HPCHEM\1\DATA\MAY0302\LBC.D
 Acq On : 5 May 2002 5:15 am
 Sample : GC/MS SCAN 4/23
 Misc :
 MS Integration Params: LSCINT.P


Vial: 39
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 2 Cyclopentasiloxane, decamethyl Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.80	5.22 ug/l	478104	Naphthalene-d8	15.82

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	72
2		Benzeneethanamine, N-[(pentafluorop	563	C24H34F5NO3Si3	055429-13-5	37
3		Benzoic acid, 2,4-bis[(trimethylsil	370	C16H30O4Si3	010586-16-0	37
4		Benzoic acid, 2,6-bis[(trimethylsil	370	C16H30O4Si3	003782-85-2	33

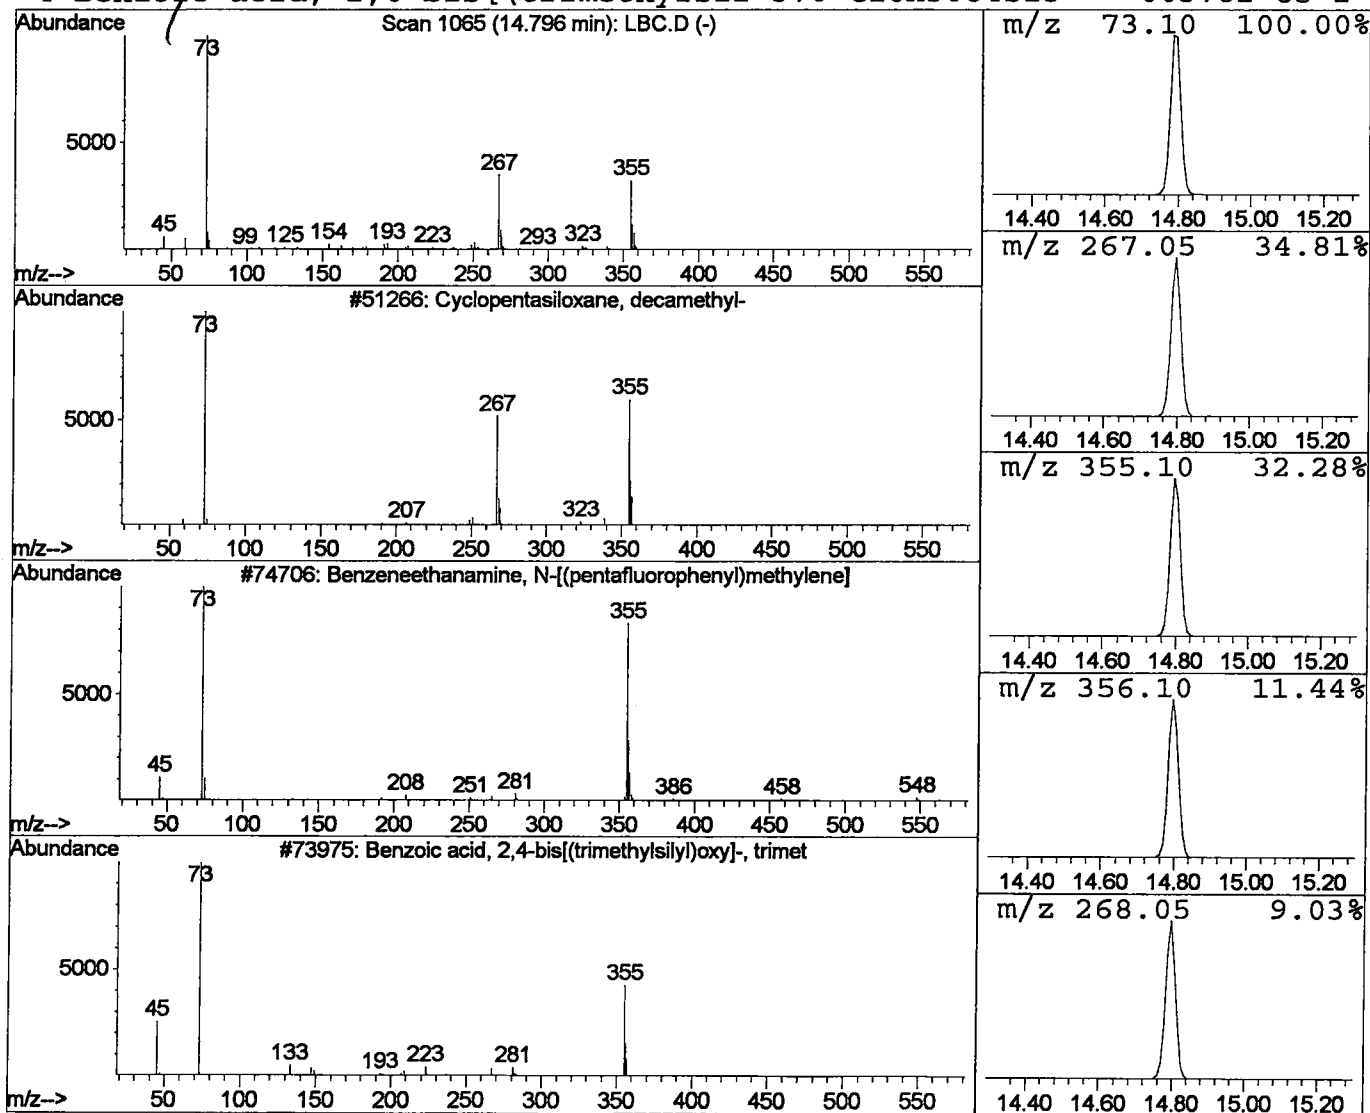

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 5 May 2002 5:15 am
Data File: C:\HPCHEM\1\DATA\MAY0302\LBC.D
Name: GC/MS SCAN 4/23
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.15	12.9	ug/l	936898	ISTD01	12.19	2899120	40.0
Cyclopentasiloxane,	14.80	5.2	ug/l	478104	ISTD02	15.82	3664660	40.0

LBC.D GCMS0501.M Tue May 07 15:03:32 2002