

Data File : C:\HPCHEM\1\DATA\MAY0302\9574.D
 Acq On : 5 May 2002 1:05 pm
 Sample : GC/MS SCAN 4/23
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 7 14:54 2002

Vial: 47
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0501.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed May 01 10:40:31 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0501

Original

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	12.19	152	498088	40.00	ug/l	-0.02
10) Naphthalene-d8	15.82	136	1824353m	40.00	ug/l	-0.03
17) Acenaphthene-d10	21.14	164	980717	40.00	ug/l	-0.01
30) Phenanthrene-d10	25.58	188	1368589	40.00	ug/l	-0.01
38) Chrysene-d12	33.64	240	909568	40.00	ug/l	-0.03
44) Perylene-d12	37.87	264	616979	40.00	ug/l	-0.01

System Monitoring Compounds

28) TCMX	23.27	209	31294	6.55	ug/L	-0.02
Spiked Amount	10.000		Recovery	=	65.50%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.89	128	212	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.61	149	904	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	25.58	178	453	N.D.	

(#) = qualifier out of range (m) = manual integration
 9574.D GCMS0501.M Tue May 07 14:54:37 2002

Data File : C:\HPCHEM\1\DATA\MAY0302\9574.D
Acq On : 5 May 2002 1:05 pm
Sample : GC/MS SCAN 4/23
Misc :
MS Integration Params: GOOFY.P
Quant Time: May 7 14:54 2002

Vial: 47
Operator:
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0501.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed May 01 10:40:31 2002
Response via : Initial Calibration
DataAcq Meth : GCMS0501

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
35) Anthracene	25.58	178	453	N.D.		
36) Di-n-butylphthalate	27.55	149	2979	N.D.		
37) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.64	228	2172	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.87	149	4752	N.D.		
43) Chrysene	33.64	228	2172	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	37.87	252	2142	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

9574.D GCMS0501.M Tue May 07 14:54:38 2002


Page 2

Data File : C:\HPCHEM\1\DATA\MAY0302\9574.D
 Acq On : 5 May 2002 1:05 pm
 Sample : GC/MS SCAN 4/23
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 7 14:54 2002

Vial: 47
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0501.RES

Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed May 01 10:40:31 2002
 Response via : Initial Calibration

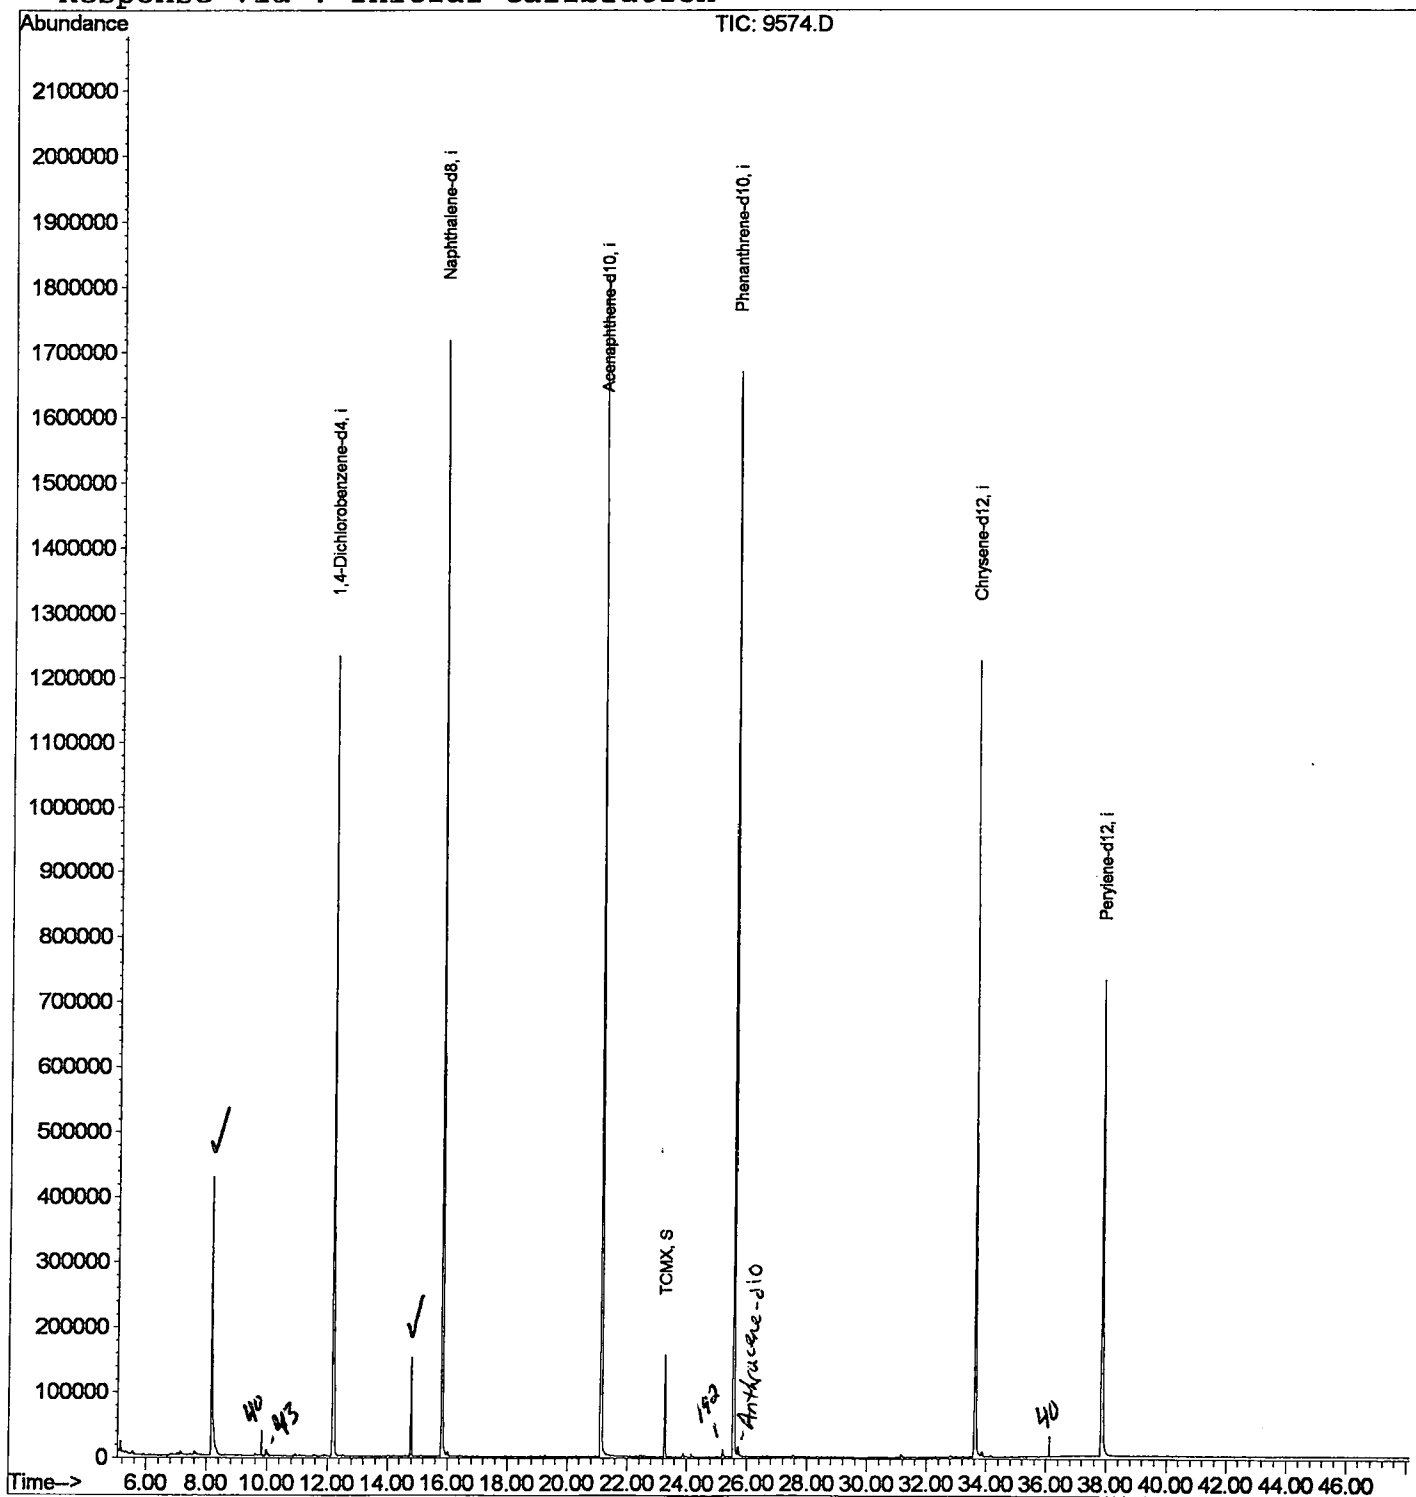

Data File : C:\HPCHEM\1\DATA\MAY0302\9574.D
 Acq On : 5 May 2002 1:05 pm
 Sample : GC/MS SCAN 4/23
 Misc :
 MS Integration Params: LSCINT.P

Vial: 47
 Operator:
 Inst : 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC


peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.163	337	341	346	rBV	427014	843905	21.27%	4.114%
2	12.195	775	781	799	rVB	1231973	2869629	72.33%	13.989%
3	14.797	1059	1065	1071	rBV	152417	290840	7.33%	1.418%
4	15.824	1171	1177	1195	rBV	1717600	3643980	91.85%	17.764%
5	21.129	1750	1756	1772	rBV	1818525	3967341	100.00%	19.341%
6	23.274	1982	1990	1997	rBV	156277	308062	7.76%	1.502%
7	25.583	2234	2242	2252	rBV2	1668237	3682947	92.83%	17.954%
8	33.638	3114	3121	3140	rBV2	1225943	2727169	68.74%	13.295%
9	37.871	3574	3583	3604	rBV2	730117	2179205	54.93%	10.623%

Sum of corrected areas: 20513078

9574.D GCMS0501.M Tue May 07 15:01:04 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAY0302\9574.D
Operator :
Acquired : 5 May 2002 1:05 pm using AcqMethod GCMS0501
Instrument : 209
Sample Name: GC/MS SCAN 4/23
Misc Info :
Vial Number: 47
Quant File :GCMS0501.RES (RTE Integrator)

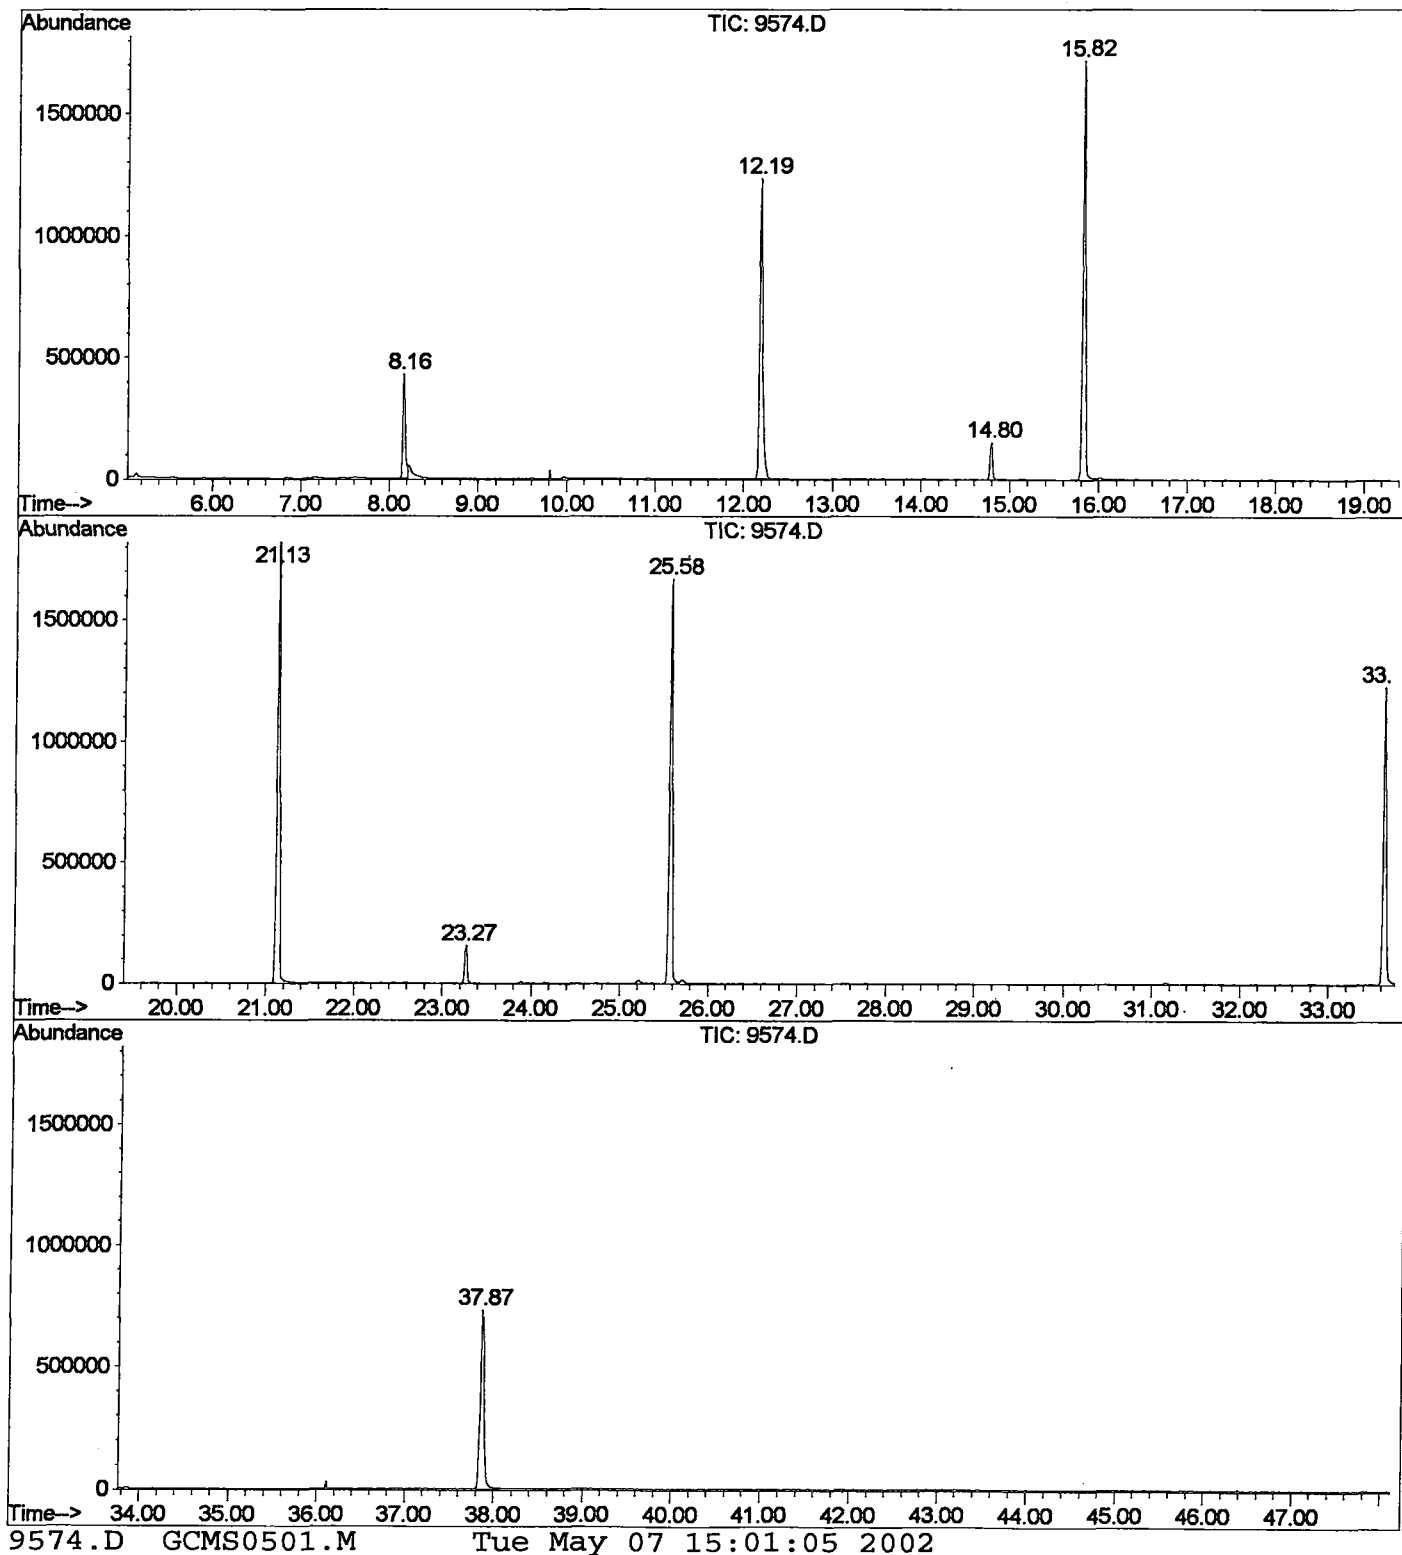

Data File : C:\HPCHEM\1\DATA\MAY0302\9574.D
 Acq On : 5 May 2002 1:05 pm
 Sample : GC/MS SCAN 4/23
 Misc :
 MS Integration Params: LSCINT.P


Vial: 47
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.16	11.76 ug/l	843905	1,4-Dichlorobenzene-d4	12.19

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64		
2	Acetone	58	C3H6O	000067-64-1	9		
3	CH2=CHCH2C(O)OCH3	100	C5H8O2	003724-55-8	9		
4	N,N'-Bis(2-methyl-2-nitrosopentan-4	258	C12H22N2O4	094514-30-4	9		

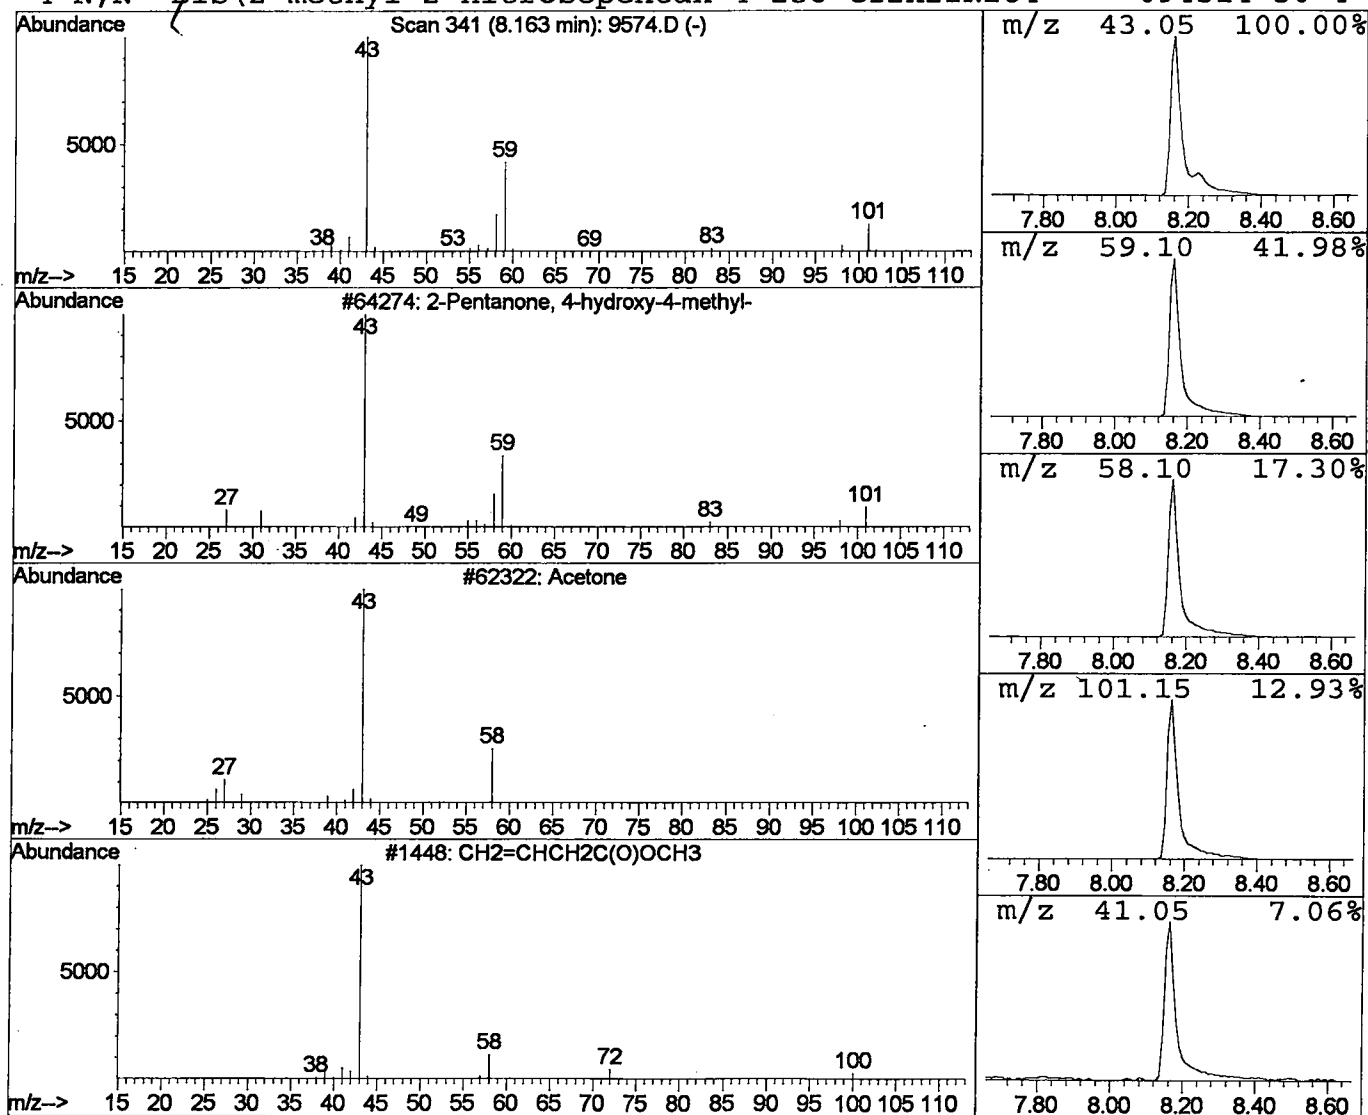

Data File : C:\HPCHEM\1\DATA\MAY0302\9574.D
 Acq On : 5 May 2002 1:05 pm
 Sample : GC/MS SCAN 4/23
 Misc :
 MS Integration Params: LSCINT.P


Vial: 47
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 2 Cyclopentasiloxane, decamethyl Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.80	3.19 ug/l	290840	Naphthalene-d8	15.82

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	53
2		Benzoic acid, 2,4-bis[(trimethylsil	370	C16H30O4Si3	010586-16-0	38
3		Benzeneethanamine, N-[(pentafluorop	563	C24H34F5NO3Si3	055429-13-5	38
4		3,4-Dihydroxybenzyl alcohol, tris(tr	356	C16H32O3Si3	068595-79-9	37

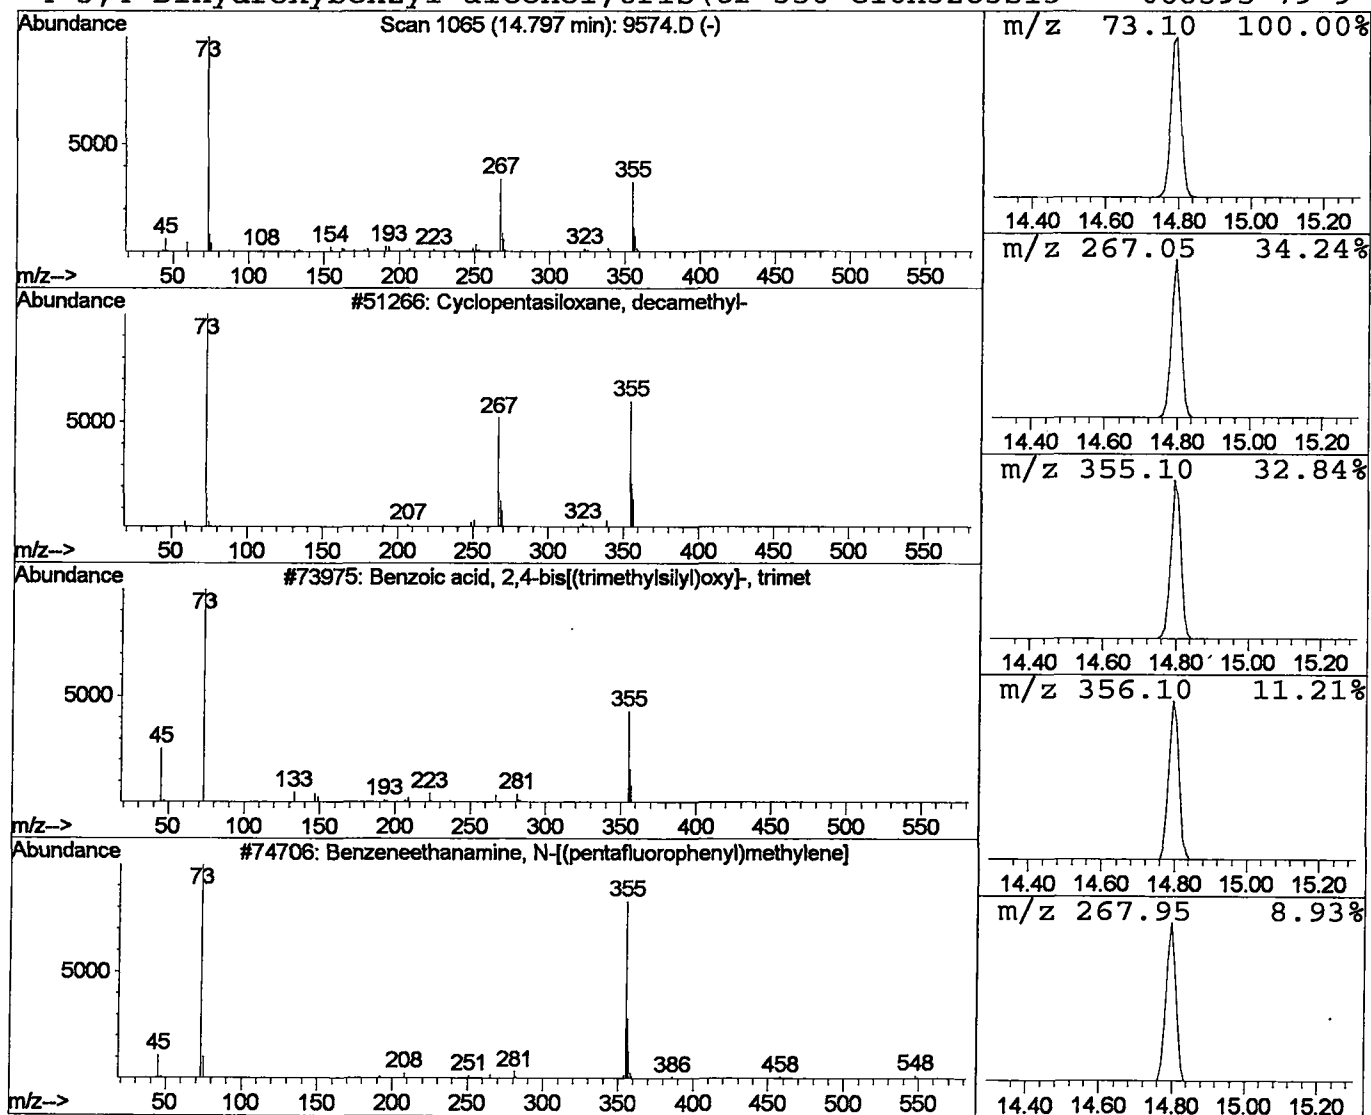

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 5 May 2002 1:05 pm
Data File: C:\HPCHEM\1\DATA\MAY0302\9574.D
Name: GC/MS SCAN 4/23
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.16	11.8	ug/l	843905	ISTD01	12.19	2869630	40.0
Cyclopentasiloxane,	14.80	3.2	ug/l	290840	ISTD02	15.82	3643980	40.0

9574.D GCMS0501.M Tue May 07 15:01:07 2002