

Method

Date Extracted

Page

#GCM5-18435

[illegible]

Analyst A.D.
Revision 4/12/01

Verified by

Reviewed by _____
Date _____

Sequence Name: C:\HPCHEM\1\SEQUENCE\MAY0902.S
 Comment:
 Operator:
 Data Path: C:\HPCHEM\1\DATA\MAY0902\
 Pre-Seq Cmd:
 Post-Seq Cmd:


Method Sections To Run On A Barcode Mismatch
 (X) Full Method (X) Inject Anyway
 () Reprocessing Only () Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name		
1	Sample	1	DFTPP	GCMS0507			
2	Sample	2	CAL80	GCMS0507			
3	Sample	3	LB	GCMS0507	GC/MS	SCAN	5/8
4	Sample	4	REF1	GCMS0507	GC/MS	SCAN	5/8
5	Sample	5	REF2	GCMS0507	GC/MS	SCAN	5/8
6	Sample	6	9578	GCMS0507	GC/MS	SCAN	5/8
7	Sample	7	9518	GCMS0507	GC/MS	SCAN	5/8
8	Sample	8	9520	GCMS0507	GC/MS	SCAN	5/8
9	Sample	9	8271	GCMS0507	GC/MS	SCAN	5/8 FB
10	Sample	10	8430	GCMS0507	GC/MS	SCAN	5/8
11	Sample	11	8485	GCMS0507	GC/MS	SCAN	5/8
12	Sample	12	8487	GCMS0507	GC/MS	SCAN	5/8
13	Sample	13	9446	GCMS0507	GC/MS	SCAN	5/8

DFTPP

Data File : C:\HPCHEM\1\DATA\MAY0902\DFTPP.D
 Acq On : 9 May 2002 2:17 pm
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : 209
 Multiplr: 1.00

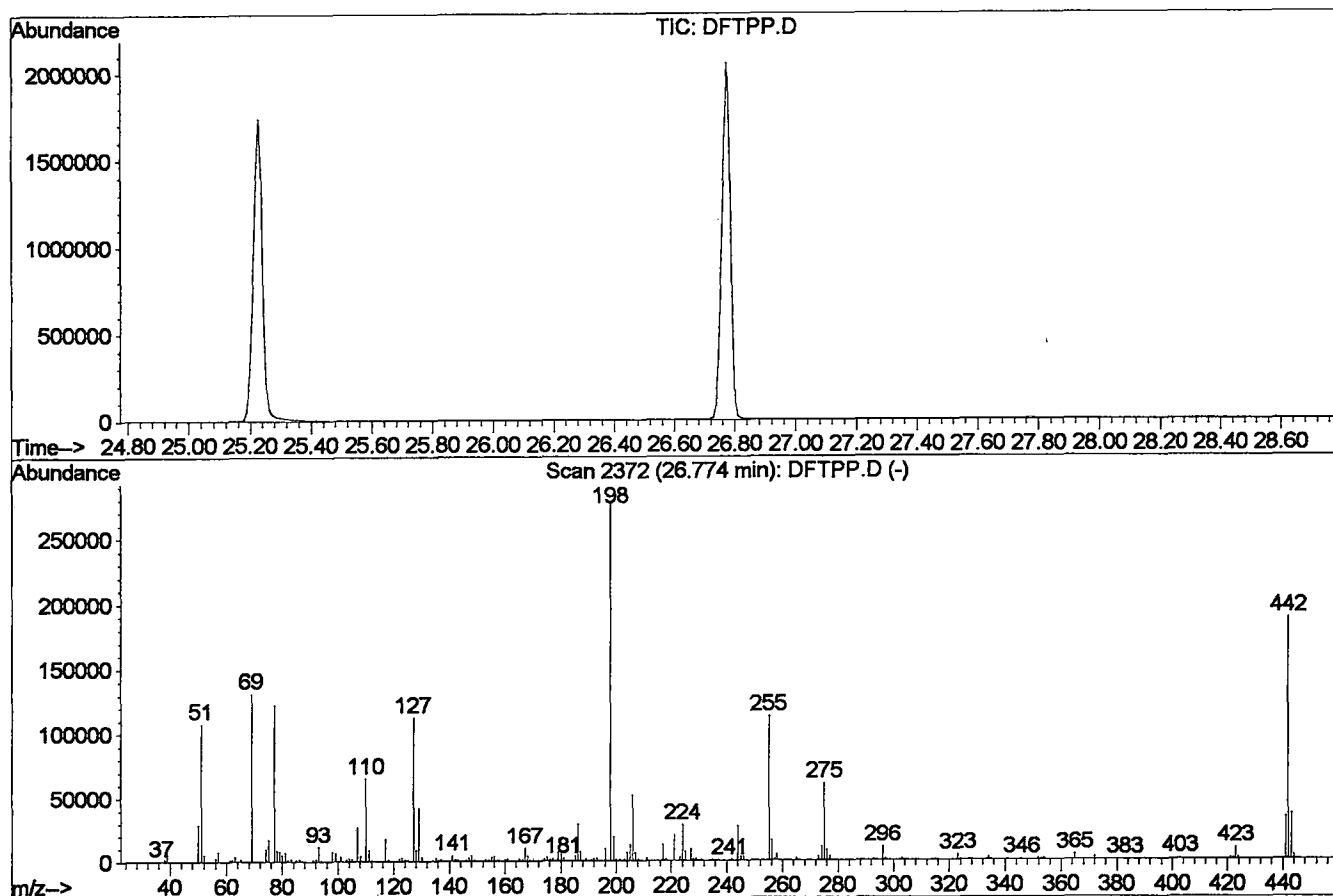

Spectrum Information: Scan 2372

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	38.7	107944	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	47.1	131328	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	40.4	112568	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	278720	PASS
199	198	5	9	6.8	18832	PASS
275	198	10	30	21.8	60816	PASS
365	198	1	100	1.5	4301	PASS
441	443	0.01	100	92.9	33624	PASS
442	198	40	110	67.5	188096	PASS
443	442	17	23	19.2	36200	PASS