

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 05/16/2002 Time: 15:02:24

Sample: AE08485
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 5/16/02 14:59 Ended: 5/16/02 14:59 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		81		10.0

Comments for Sample AE08485 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 05-16-2002 Time: 15:11:56

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY0902\8485.D
 Acq On : 10 May 2002 12:12 am
 Sample : GC/MS SCAN 5/8
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 10 13:53 2002

Vial: 11
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0510.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri May 10 09:59:40 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0507

Re-analysis

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.20	152	498688	40.00	ug/l	0.00
10) Naphthalene-d8	15.82	136	1836158	40.00	ug/l	0.00
17) Acenaphthene-d10	21.14	164	1007620	40.00	ug/l	0.00
30) Phenanthrene-d10	25.57	188	1394642	40.00	ug/l	0.00
38) Chrysene-d12	33.64	240	836890	40.00	ug/l	0.00
44) Perylene-d12	37.86	264	515008	40.00	ug/l	0.00

System Monitoring Compounds

28) TCMX	23.27	209	162079	32.34	ug/L	0.00
Spiked Amount	40.000		Recovery	=	80.85%	

Target Compounds

					Qvalue
2) N-nitrosodimethylamine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitrosodi-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.61	149	522	N.D.	
26) 4-Chlorophenylphenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzene	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	23.27	168	354	N.D.	
32) 4-Bromophenylphenylether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	25.57	178	232	N.D.	

(#) = qualifier out of range (m) = manual integration

8485.D GCMS0510.M Fri May 10 13:54:02 2002

Page 1

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY0902\8485.D
Acq On : 10 May 2002 12:12 am
Sample : GC/MS SCAN 5/8
Misc :
MS Integration Params: GOOFY.P
Quant Time: May 10 13:53 2002

Vial: 11
Operator:
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0510.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri May 10 09:59:40 2002
Response via : Initial Calibration
DataAcq Meth : GCMS0507

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
35) Anthracene	25.57	178	232	N.D.		
36) Di-n-butylphthalate	27.55	149	2777	N.D.		
37) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.64	228	1849	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.86	149	964	N.D.		
43) Chrysene	33.64	228	1849	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	37.87	252	1929	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenzo(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

8485.D GCMS0510.M Fri May 10 13:54:03 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\MAY0902\8485.D
 Acq On : 10 May 2002 12:12 am
 Sample : GC/MS SCAN 5/8
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 10 13:53 2002

Vial: 11
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0510.RES

Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri May 10 09:59:40 2002
 Response via : Initial Calibration

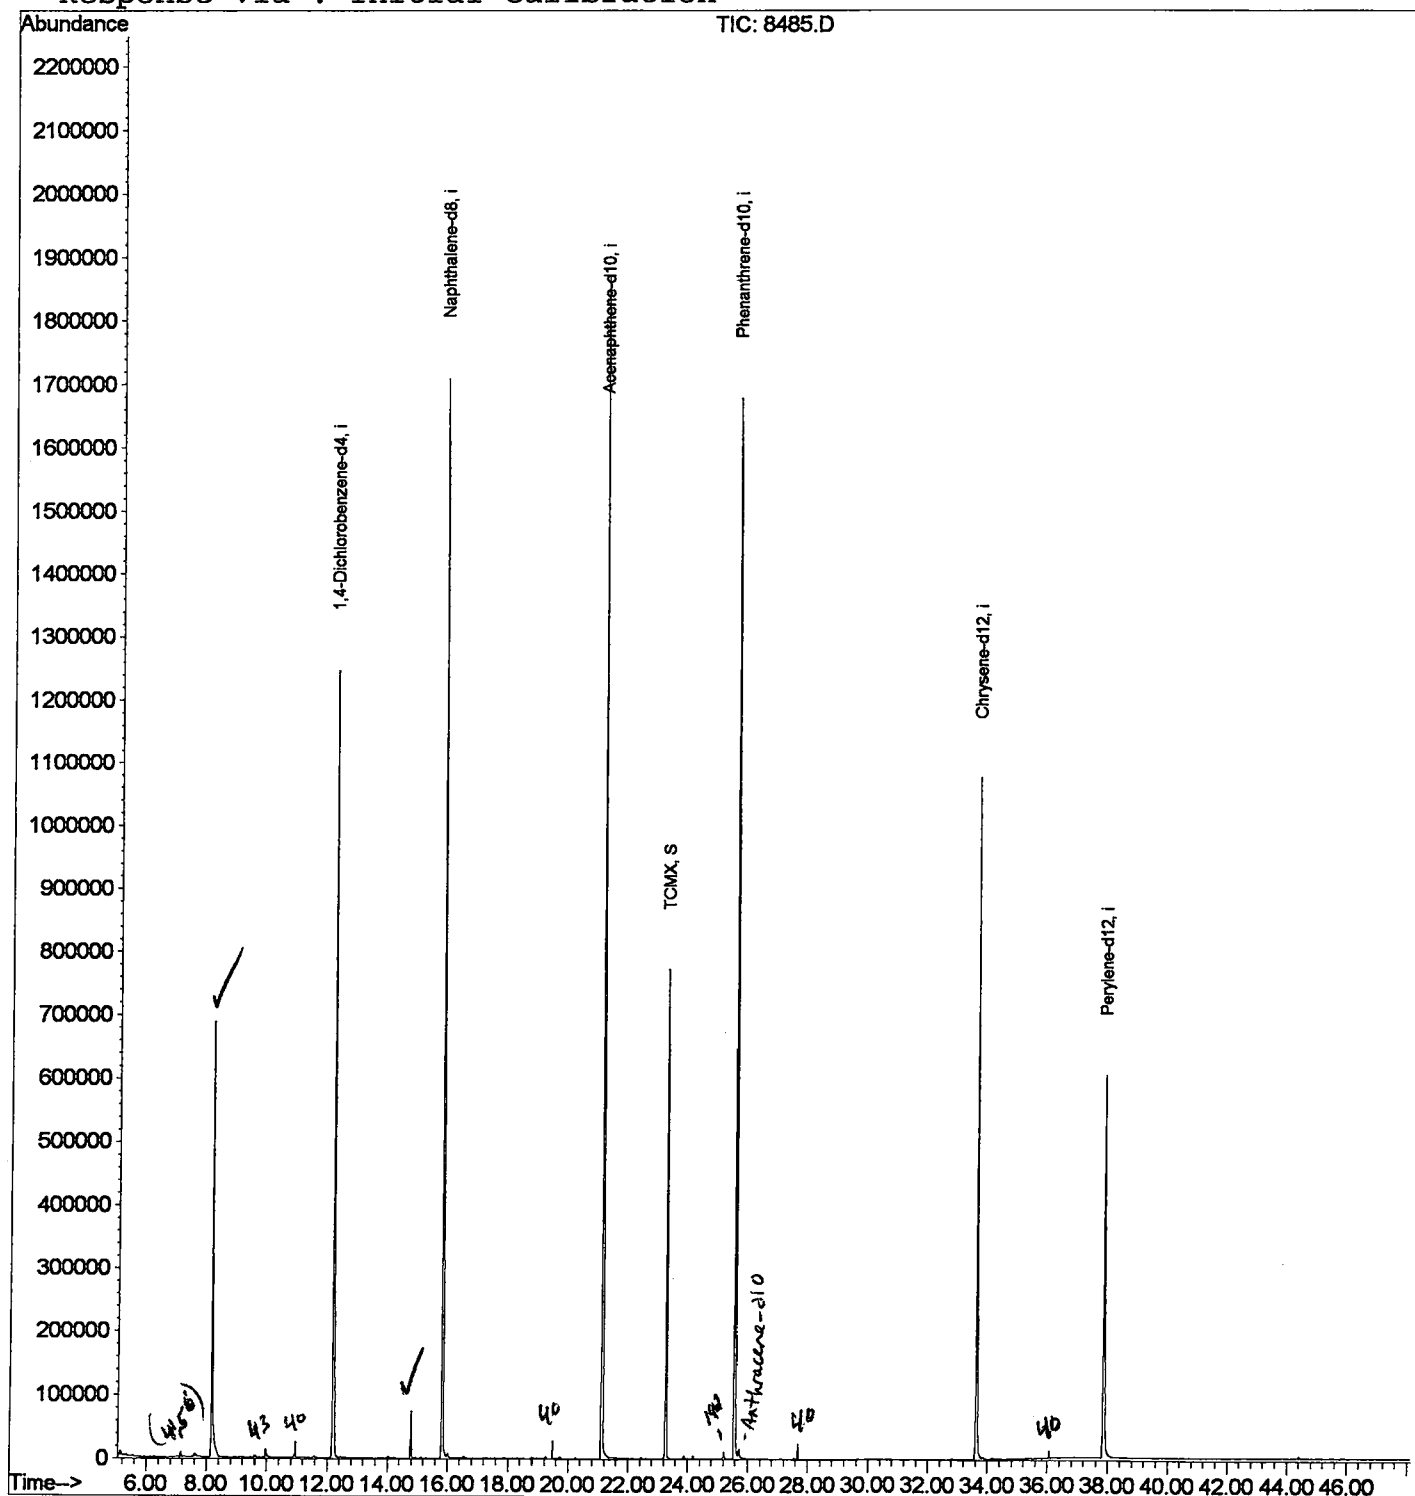

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\MAY0902\8485.D
 Acq On : 10 May 2002 12:12 am
 Sample : GC/MS SCAN 5/8
 Misc :
 MS Integration Params: LSCINT.P

Vial: 11
 Operator:
 Inst : 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.163	337	341	372	rVB	686835	1534276	37.91%	7.070%
2	12.195	775	781	796	rBV	1245811	2836065	70.08%	13.069%
3	14.798	1060	1065	1072	rVB	73646	137181	3.39%	0.632%
4	15.824	1171	1177	1194	rBV	1708499	3603541	89.04%	16.605%
5	21.139	1750	1757	1775	rBV	1871623	4046934	100.00%	18.648%
6	23.274	1981	1990	1999	rBV	771003	1565516	38.68%	7.214%
7	25.574	2234	2241	2252	rBV2	1677858	3688396	91.14%	16.996%
8	33.638	3114	3121	3140	rBV2	1075995	2503136	61.85%	11.534%
9	37.862	3573	3582	3605	rBV2	601369	1786441	44.14%	8.232%

Sum of corrected areas: 21701486

8485.D GCMS0510.M Fri May 10 13:57:43 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAY0902\8485.D
 Operator :
 Acquired : 10 May 2002 12:12 am using AcqMethod GCMS0507
 Instrument : 209
 Sample Name: GC/MS SCAN 5/8
 Misc Info :
 Vial Number: 11
 Quant File :GCMS0510.RES (RTE Integrator)

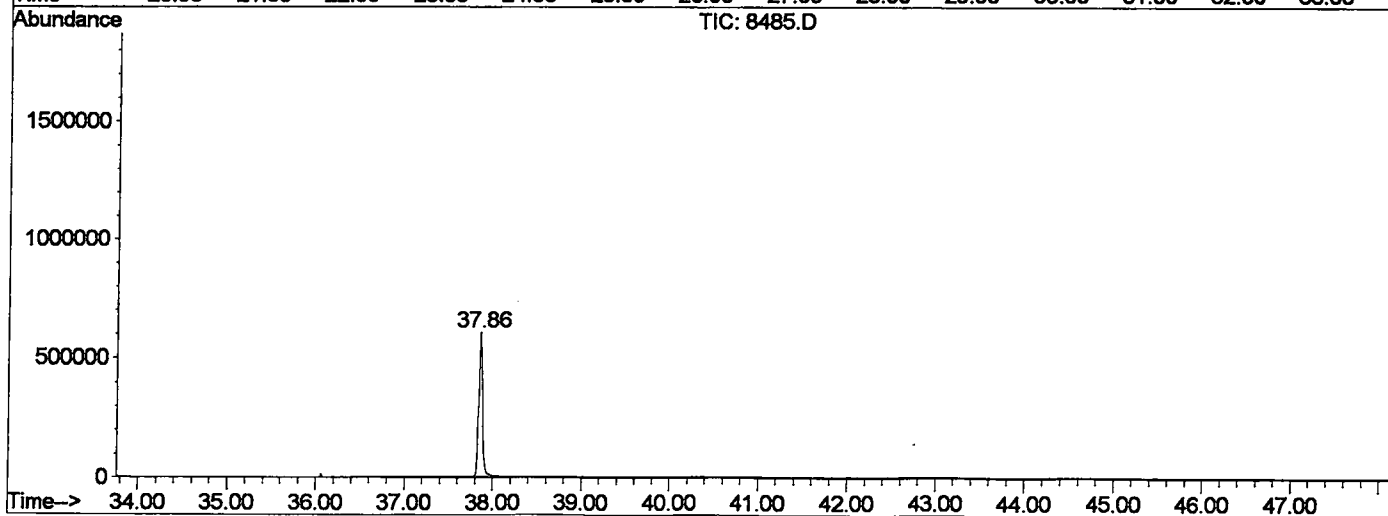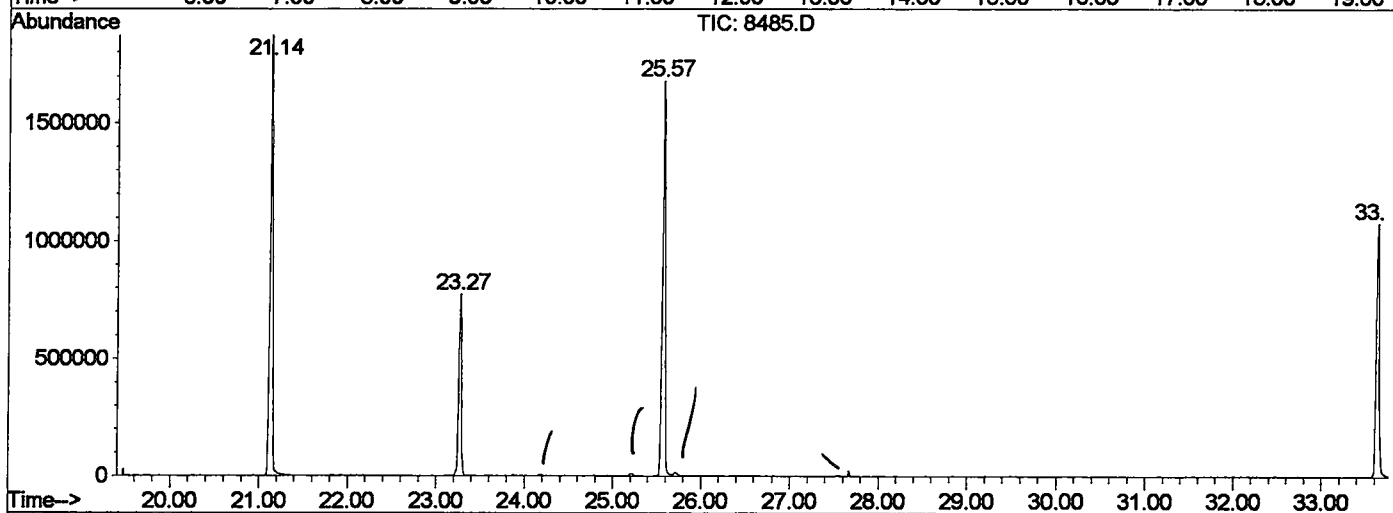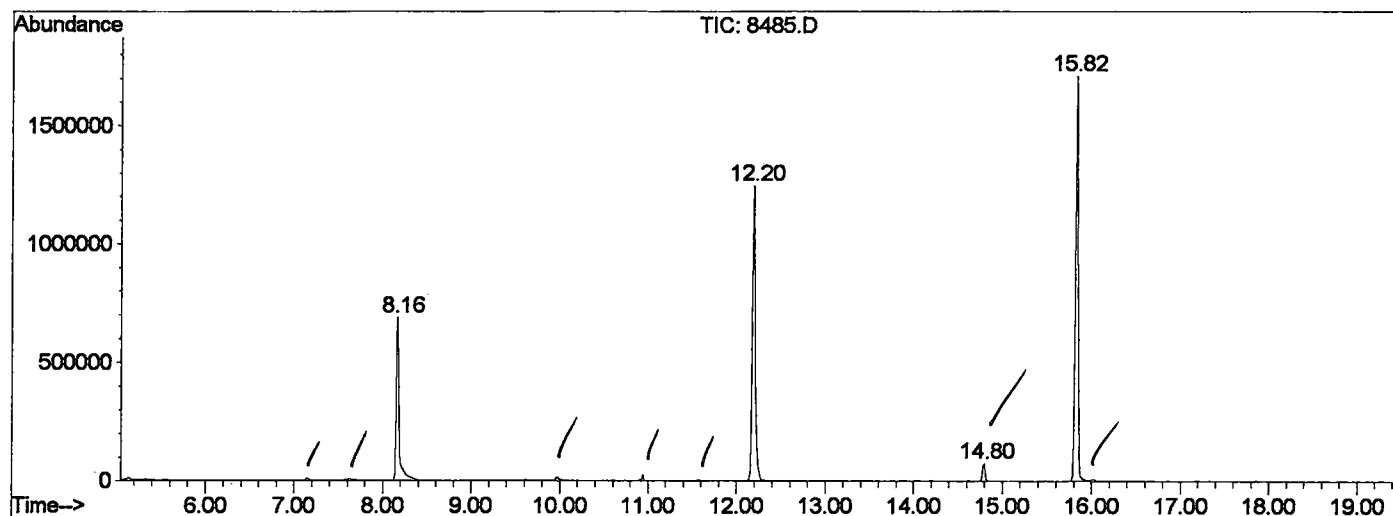

8485.D GCMS0510.M Fri May 10 13:57:44 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAY0902\8485.D
 Acq On : 10 May 2002 12:12 am
 Sample : GC/MS SCAN 5/8
 Misc :
 MS Integration Params: LSCINT.P


Vial: 11
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.16	21.64 ug/l	1534280	1,4-Dichlorobenzene-d4	12.20

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2		3-Hydroxy-2-pentanone	102	C5H10O2	003142-66-3	9
3		CH2=CHCH2C(O)OCH3	100	C5H8O2	003724-55-8	9
4		Acetic acid, 1,1-dimethylethyl este	116	C6H12O2	000540-88-5	9

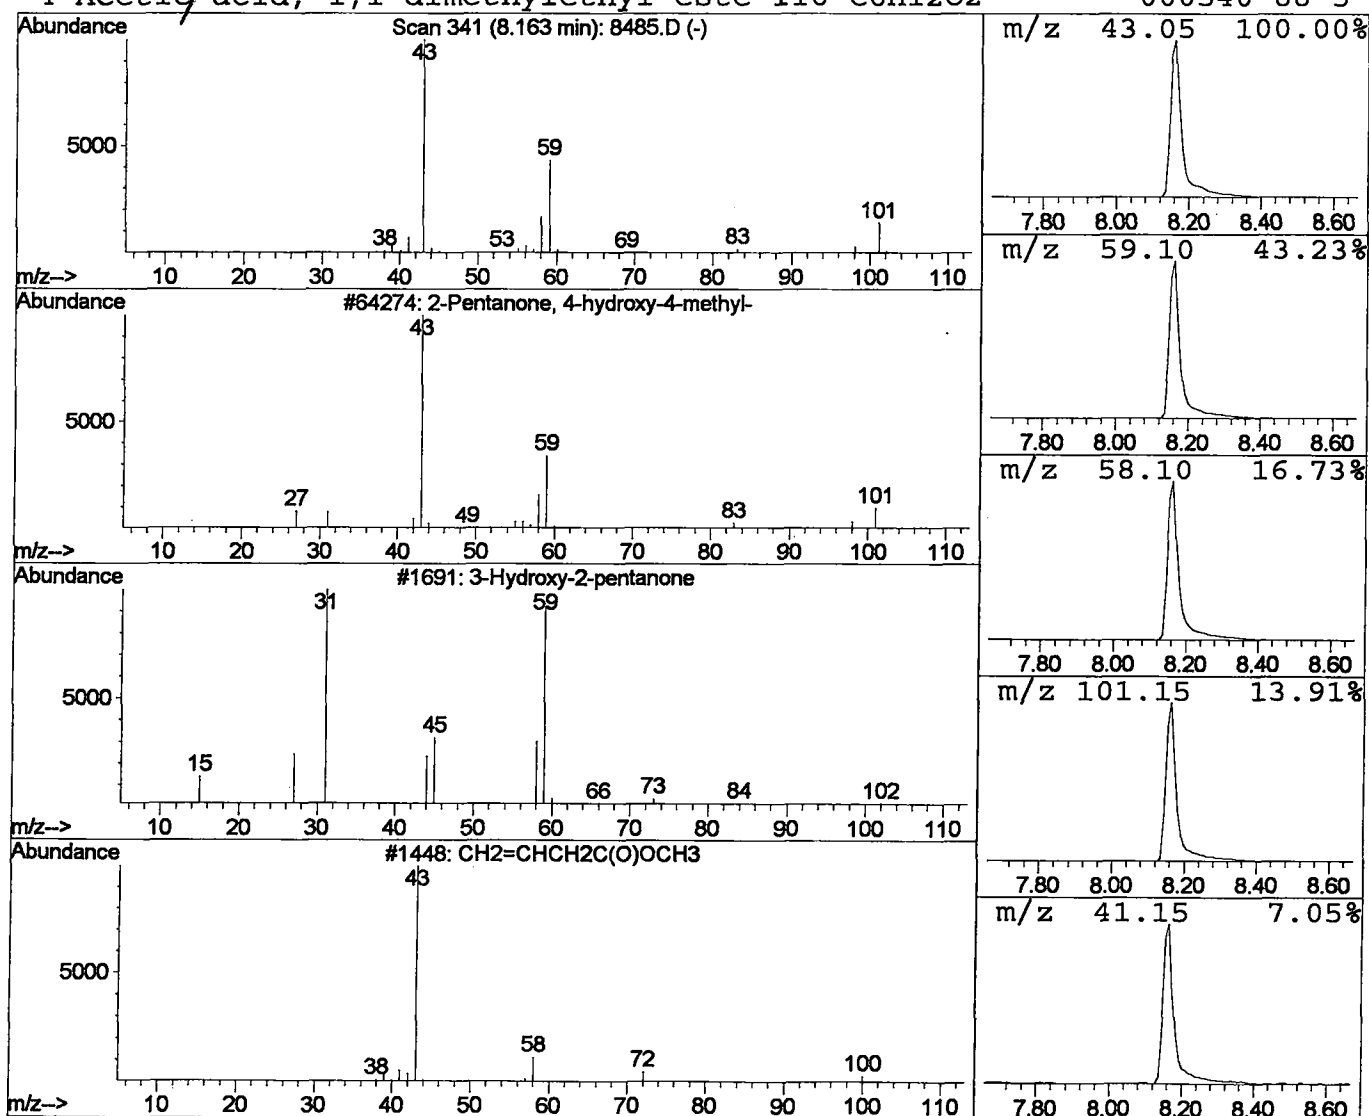

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAY0902\8485.D
 Acq On : 10 May 2002 12:12 am
 Sample : GC/MS SCAN 5/8
 Misc :
 MS Integration Params: LSCINT.P









Vial: 11
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 2 Cyclopentasiloxane, decamethyl Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.80	1.52 ug/l	137181	Naphthalene-d8	15.82

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	80
2		3,4-Dihydroxybenzyl alcohol, tris(tr	356	C16H32O3Si3	068595-79-9	38
3		Noradrenaline, tetra-TMS	457	C20H43NO3Si4	000000-00-0	37
4		Benzeneethanamine, N-[(pentafluorop	563	C24H34F5NO3Si3	055429-13-5	37

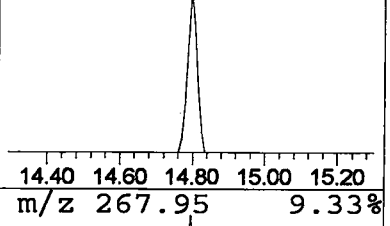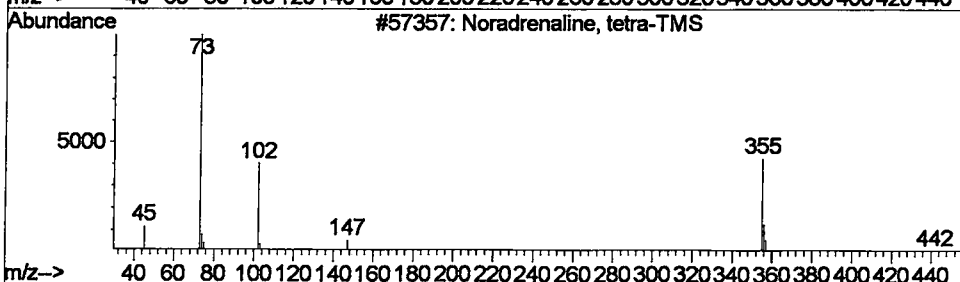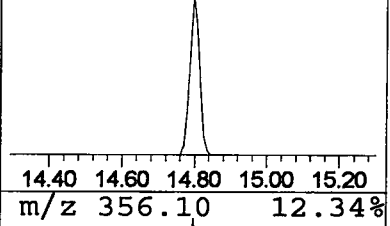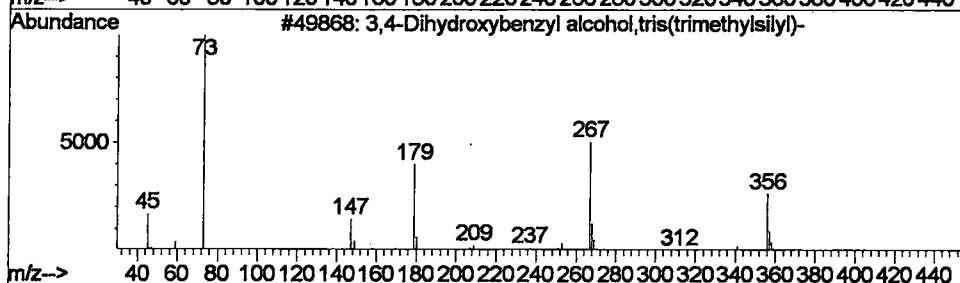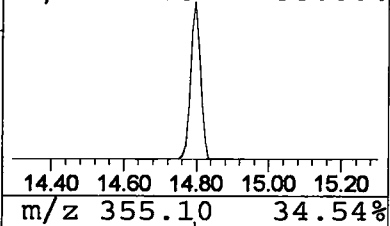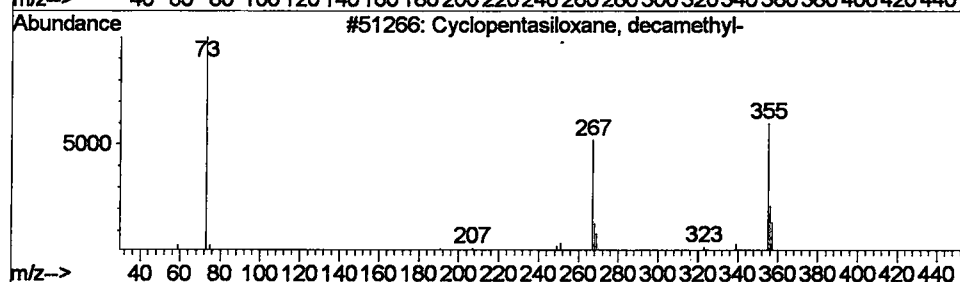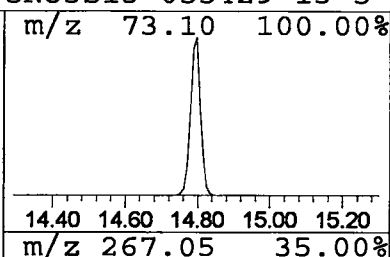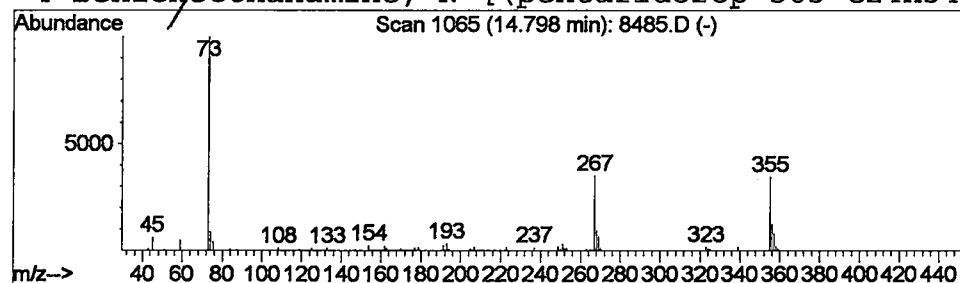

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 10 May 2002 12:12 am
Data File: C:\HPCHEM\1\DATA\MAY0902\8485.D
Name: GC/MS SCAN 5/8
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.16	21.6	ug/l	1534280	ISTD01	12.20	2836070	40.0
Cyclopentasiloxane,	14.80	1.5	ug/l	137181	ISTD02	15.82	3603540	40.0

8485.D GCMS0510.M Fri May 10 13:57:47 2002