

User: Vinci, David L.
Westchester Dept. of Labs & Research
Date: 05/16/2002 Time: 15:30:11

Sample: AE09518
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 5/16/02 15:29 Ended: 5/16/02 15:29 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		83		10.0

Comments for Sample AE09518 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 05-16-2002 Time: 15:30:33

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Data File : C:\HPCHEM\1\DATA\MAY0902\9518.D
 Acq On : 9 May 2002 8:14 pm
 Sample : GC/MS SCAN 5/8
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 10 13:50 2002

Vial: 7
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0510.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri May 10 09:59:40 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0507

Reanalysis

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	12.19	152	481646	40.00	ug/l	0.00
10) Naphthalene-d8	15.83	136	1762537	40.00	ug/l	0.00
17) Acenaphthene-d10	21.13	164	959315	40.00	ug/l	0.00
30) Phenanthrene-d10	25.58	188	1338912	40.00	ug/l	0.00
38) Chrysene-d12	33.63	240	824364	40.00	ug/l	0.00
44) Perylene-d12	37.87	264	496527	40.00	ug/l	0.00

System Monitoring Compounds

28) TCMX	23.28	209	157662	33.04	ug/L	0.00
Spiked Amount	40.000		Recovery	=	82.60%	

Target Compounds

					Qvalue
2) N-nitrosodimethylamine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitrosodi-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.88	128	303	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.62	149	593	N.D.	
26) 4-Chlorophenylphenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzene	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	23.28	168	497	N.D.	
32) 4-Bromophenylphenylether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	25.58	178	299	N.D.	

(#) = qualifier out of range (m) = manual integration

9518.D GCMS0510.M Fri May 10 13:50:39 2002

Page 1

Data File : C:\HPCHEM\1\DATA\MAY0902\9518.D
Acq On : 9 May 2002 8:14 pm
Sample : GC/MS SCAN 5/8
Misc :
MS Integration Params: GOOFY.P
Quant Time: May 10 13:50 2002

Vial: 7
Operator:
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0510.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri May 10 09:59:40 2002
Response via : Initial Calibration
DataAcq Meth : GCMS0507

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
35) Anthracene	25.58	178	299		N.D.	
36) Di-n-butylphthalate	27.55	149	3538		N.D.	
37) Fluoranthene	0.00	202	0		N.D.	
39) Pyrene	0.00	202	0		N.D.	
40) Butylbenzylphthalate	0.00	149	0		N.D.	
41) Benzo(a)anthracene	33.63	228	2113		N.D.	
42) Bis(2-ethylhexyl)phthalate	33.85	149	1148		N.D.	
43) Chrysene	33.63	228	2113		N.D.	
45) Di-n-Octylphthalate	0.00	149	0		N.D.	
46) Benzo(b)fluoranthene	0.00	252	0		N.D.	
47) Benzo(k)fluoranthene	36.76	252	200		N.D.	
48) Benzo(a)pyrene	37.86	252	2071		N.D.	
49) Indeno(1,2,3-cd)pyrene	0.00	276	0		N.D.	
50) Dibenz(a,h)anthracene	0.00	278	0		N.D.	
51) Benzo(g,h,i)perylene	0.00	276	0		N.D.	

(#) = qualifier out of range (m) = manual integration

9518.D GCMS0510.M Fri May 10 13:50:40 2002


Page 2

Data File : C:\HPCHEM\1\DATA\MAY0902\9518.D
 Acq On : 9 May 2002 8:14 pm
 Sample : GC/MS SCAN 5/8
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 10 13:50 2002

Vial: 7
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0510.RES

Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri May 10 09:59:40 2002
 Response via : Initial Calibration

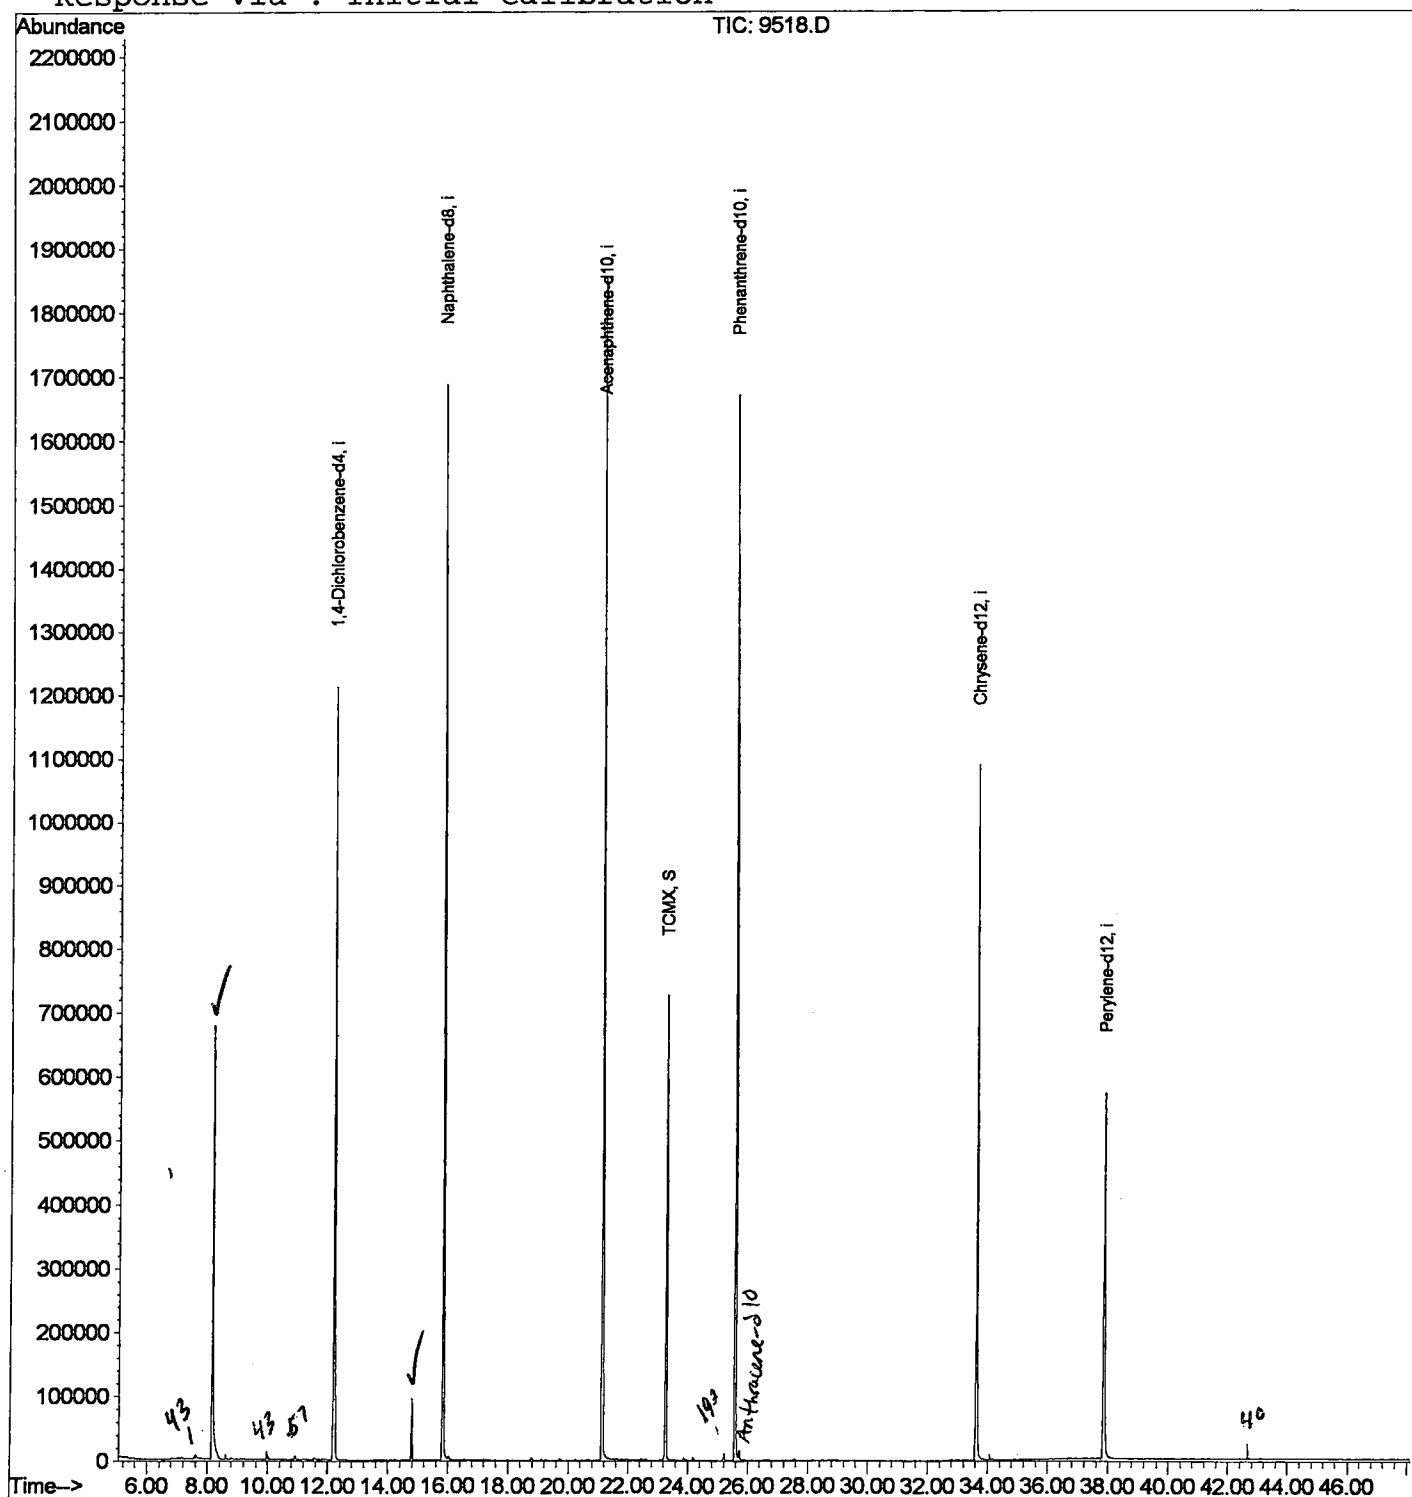

Data File : C:\HPCHEM\1\DATA\MAY0902\9518.D
Acq On : 9 May 2002 8:14 pm
Sample : GC/MS SCAN 5/8
Misc :
MS Integration Params: LSCINT.P

Vial: 7
Operator:
Inst : 209
Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.159	336	340	370	rBV	677099	1481035	38.38%	7.064%
2	12.191	772	780	795	rBV	1211846	2741119	71.04%	13.074%
3	14.793	1059	1064	1070	rVB	94940	182336	4.73%	0.870%
4	15.828	1171	1177	1194	rBV	1686536	3459155	89.65%	16.499%
5	21.134	1749	1756	1778	rBV	1855556	3858651	100.00%	18.404%
6	23.278	1981	1990	1995	rBV	726430	1524229	39.50%	7.270%
7	25.579	2234	2241	2252	rBV2	1669015	3555762	92.15%	16.959%
8	33.633	3113	3120	3141	rBV2	1089474	2442505	63.30%	11.650%
9	37.867	3573	3582	3597	rBV2	571571	1721673	44.62%	8.212%




Sum of corrected areas: 20966465

9518.D
GCMS0510.M

Fri May 10 13:58:41 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAY0902\9518.D
 Operator :
 Acquired : 9 May 2002 8:14 pm using AcqMethod GCMS0507
 Instrument : 209
 Sample Name: GC/MS SCAN 5/8
 Misc Info :
 Vial Number: 7
 Quant File :GCMS0510.RES (RTE Integrator)

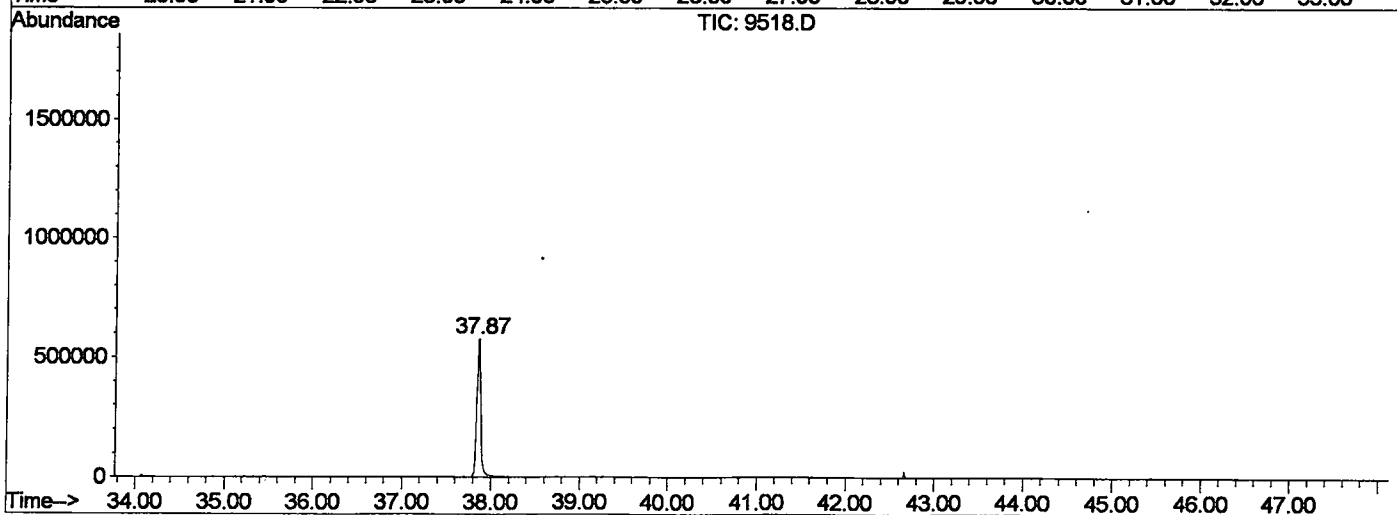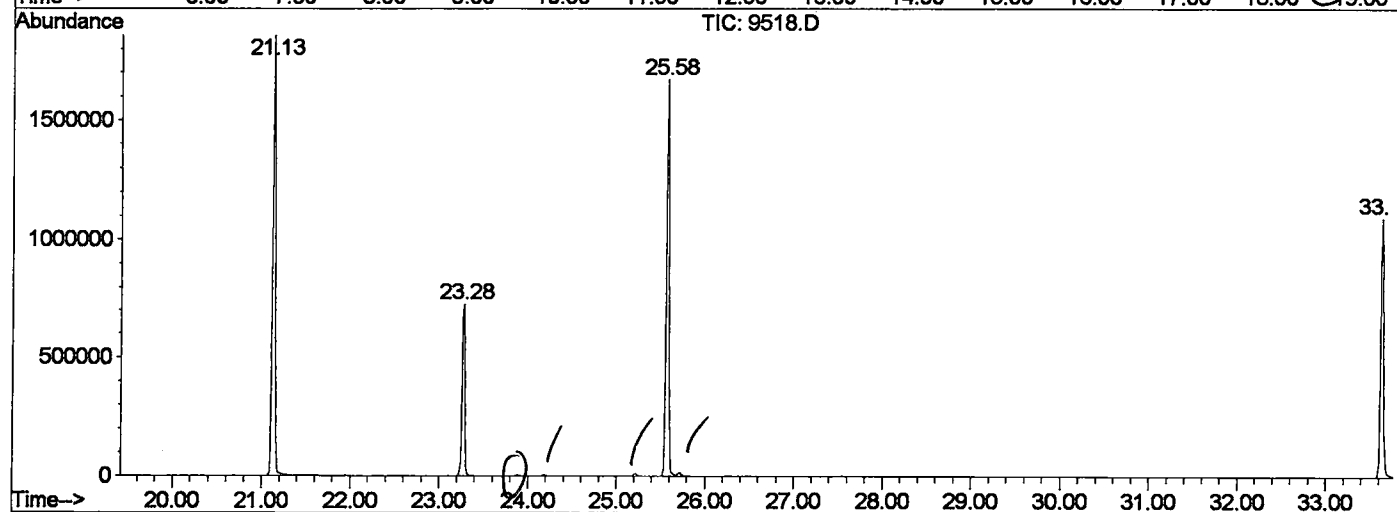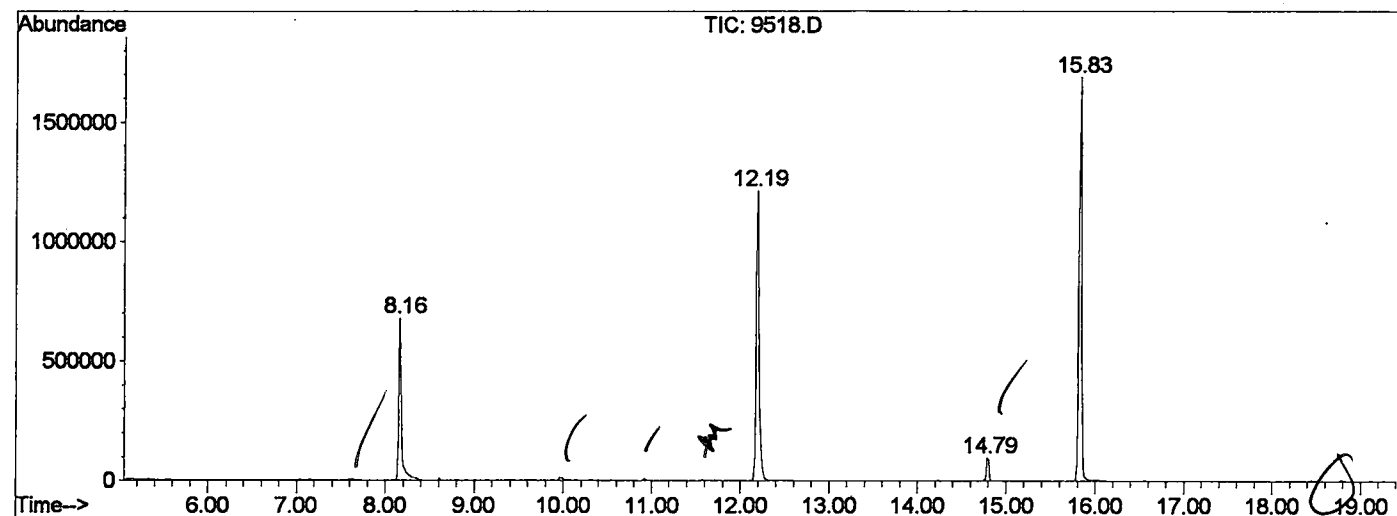

9518.D GCMS0510.M Fri May 10 13:58:41 2002

Data File : C:\HPCHEM\1\DATA\MAY0902\9518.D
 Acq On : 9 May 2002 8:14 pm
 Sample : GC/MS SCAN 5/8
 Misc :
 MS Integration Params: LSCINT.P


Vial: 7
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 2-Pentanone, 4-hydroxy-4-methyl Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.16	21.61 ug/l	1481040	1,4-Dichlorobenzene-d4	12.19

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2			3-Hydroxy-2-pentanone	102	C5H10O2	003142-66-3	9
3			CH2=CHCH2C(O)OCH3	100	C5H8O2	003724-55-8	9
4			5-Hexen-2-one	98	C6H10O	000109-49-9	7

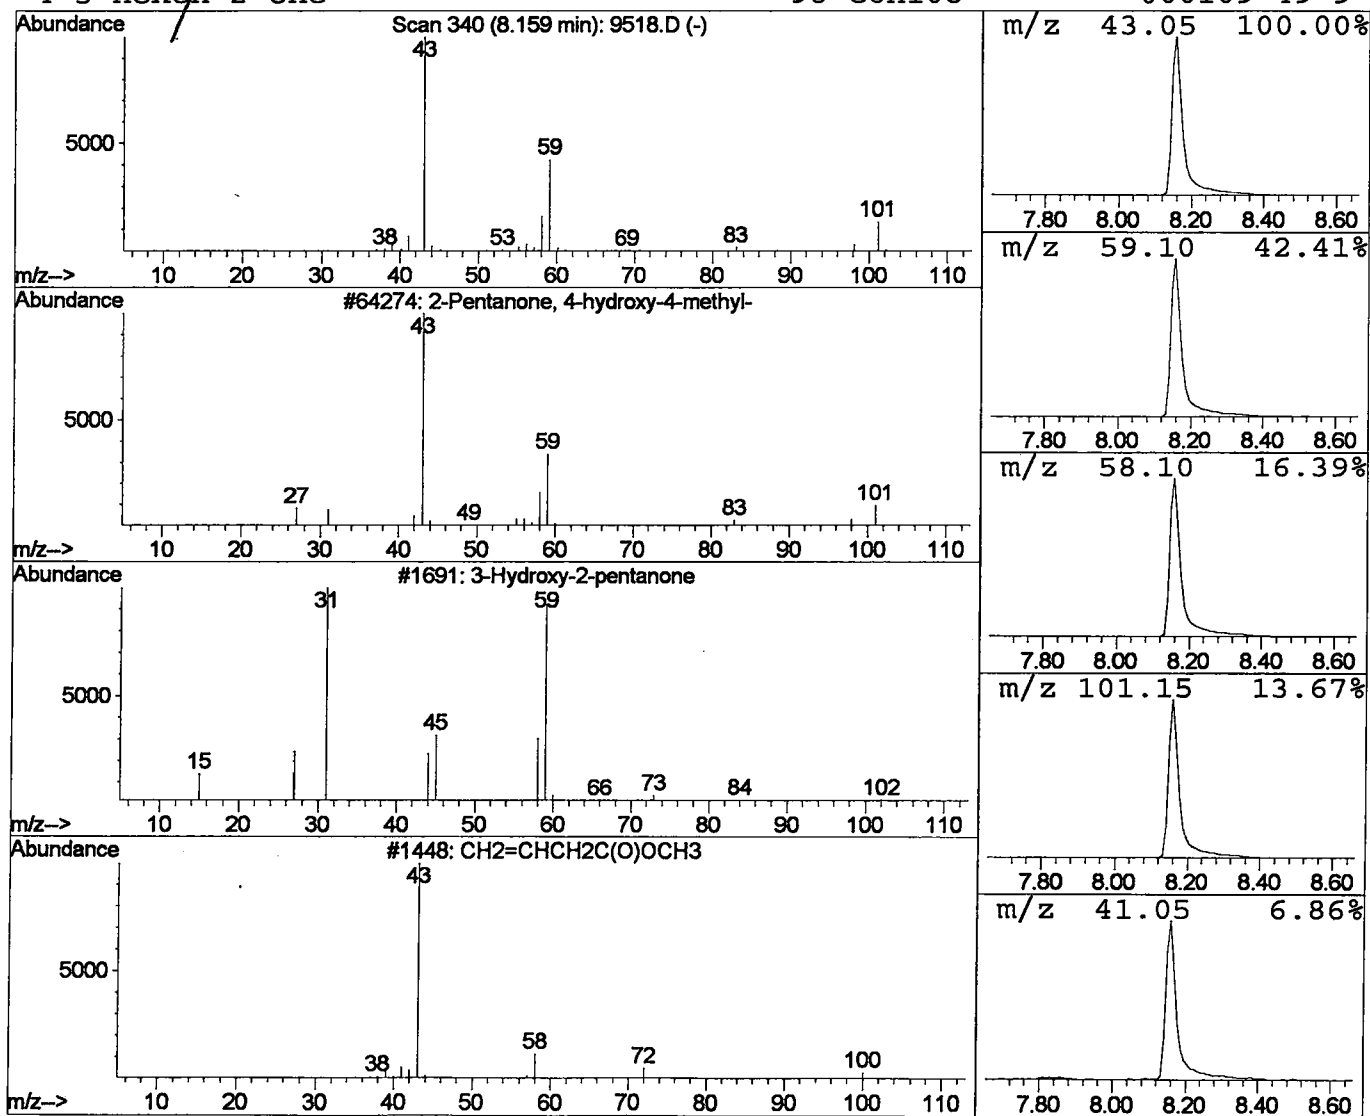

Data File : C:\HPCHEM\1\DATA\MAY0902\9518.D
 Acq On : 9 May 2002 8:14 pm
 Sample : GC/MS SCAN 5/8
 Misc :
 MS Integration Params: LSCINT.P


Vial: 7
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 2 Cyclopentasiloxane, decamethyl Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.79	2.11 ug/l	182336	Naphthalene-d8	15.83

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	80
2		3,4-Dihydroxybenzyl alcohol, tris(tr	356	C16H32O3Si3	068595-79-9	46
3		Benzeneethanamine, N-[(pentafluorop	563	C24H34F5NO3Si3	055429-13-5	38
4		Benzoic acid, 2,4-bis[(trimethylsil	370	C16H30O4Si3	010586-16-0	38

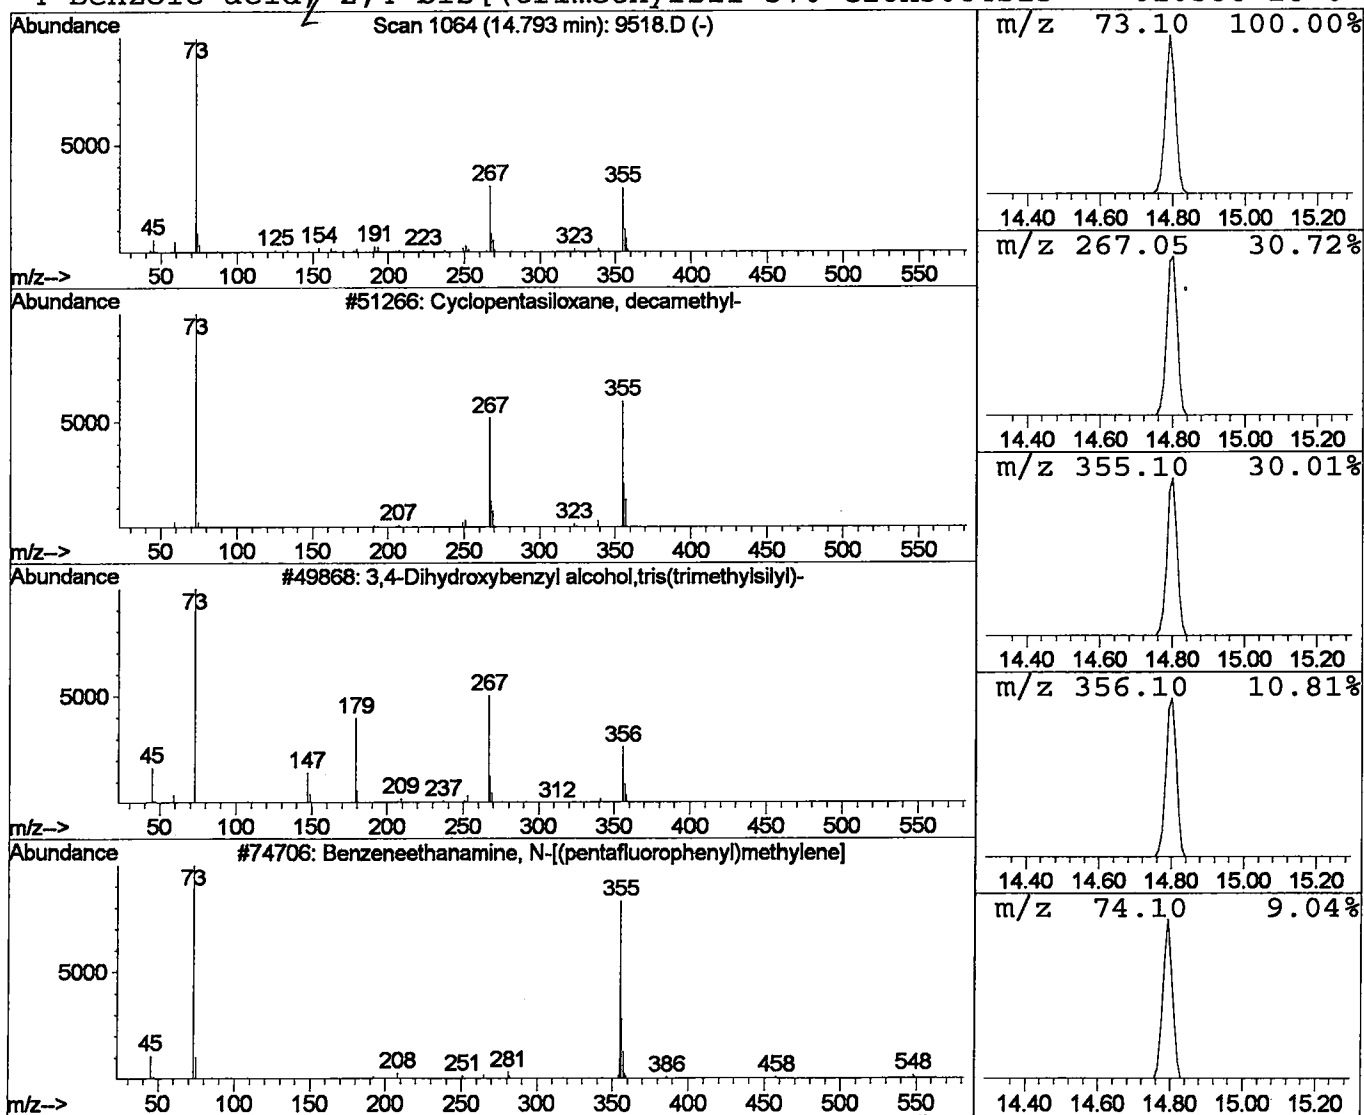

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 9 May 2002 8:14 pm
Data File: C:\HPCHEM\1\DATA\MAY0902\9518.D
Name: GC/MS SCAN 5/8
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.16	21.6	ug/l	1481040	ISTD01	12.19	2741120	40.0
Cyclopentasiloxane,	14.79	2.1	ug/l	182336	ISTD02	15.83	3459160	40.0

9518.D GCMS0510.M Fri May 10 13:58:44 2002