

Date Extracted 5/7/04

Ref

\$GCMs - 18610

[illegible]

Analyst GA
revision 4/12/01


Verified by

Reviewed by _____
Date _____

DFTPP

Data File : C:\HPCHEM\1\DATA\MAY2002\DFTPP.D
 Acq On : 20 May 2002 9:03 am
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : 209
 Multiplr: 1.00

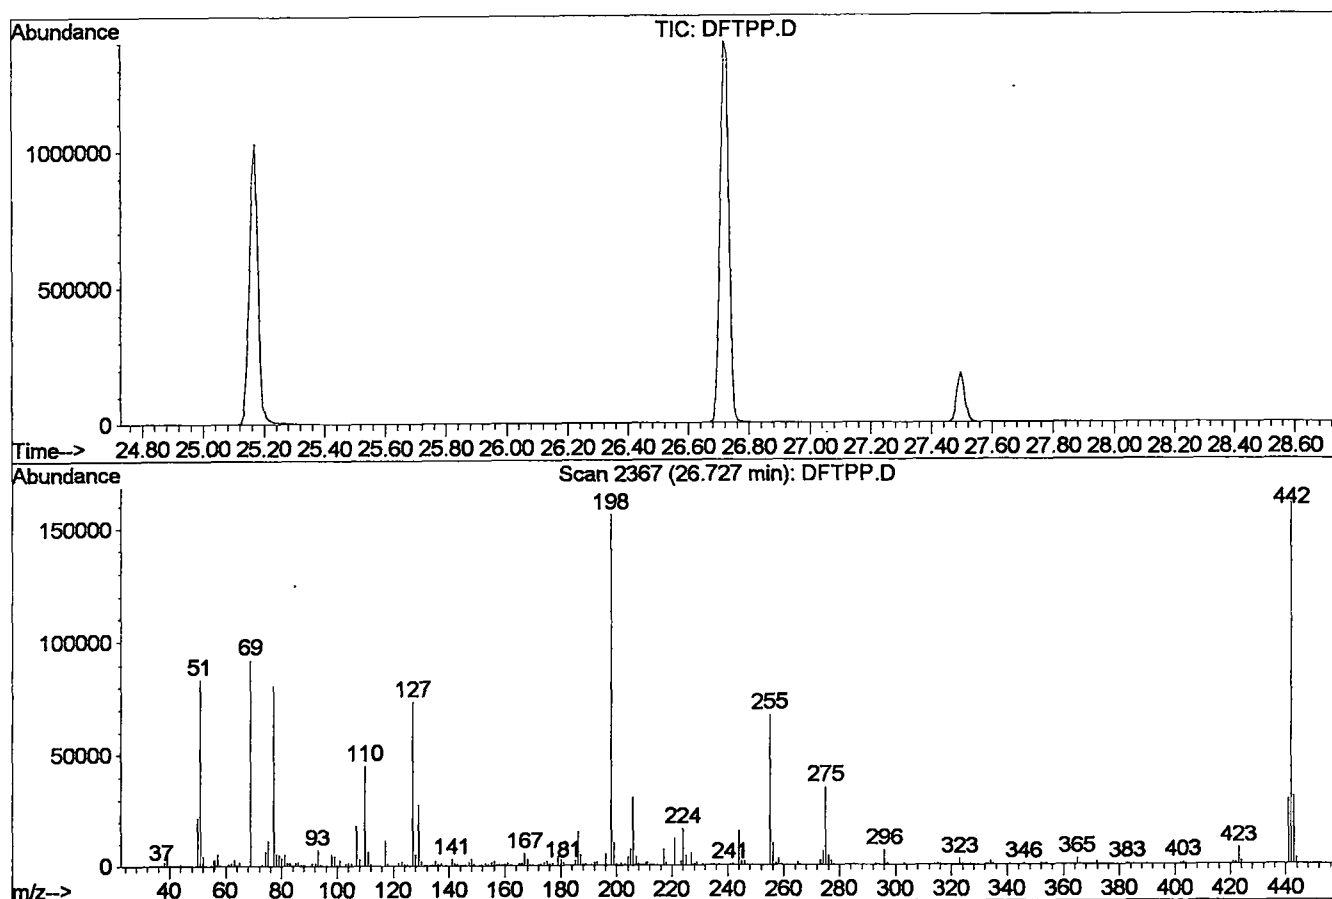

Spectrum Information: Scan 2367

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	53.5	83416	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	59.1	92224	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	47.2	73584	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	156032	PASS
199	198	5	9	6.5	10210	PASS
275	198	10	30	22.5	35088	PASS
365	198	1	100	1.7	2720	PASS
441	443	0.01	100	95.0	29336	PASS
442	198	40	110	102.8	160384	PASS
443	442	17	23	19.2	30872	PASS