

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 05/23/2002 Time: 15:29:19

Sample: AE10065
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 5/23/02 15:28 Ended: 5/23/02 15:28 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		103		10.0

Comments for Sample AE10065 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 05-23-2002 Time: 15:29:53

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY2002\10065.D
 Acq On : 20 May 2002 9:55 pm
 Sample : EXTRACTED 5/9
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 21 11:33 2002

Vial: 16
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0520.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Mon May 20 15:10:30 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0520

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	12.15	152	346579	40.00	ug/l	0.00
10) Naphthalene-d8	15.77	136	1382686	40.00	ug/l	-0.02
17) Acenaphthene-d10	21.08	164	654304	40.00	ug/l	0.00
30) Phenanthrene-d10	25.52	188	878899	40.00	ug/l	-0.02
38) Chrysene-d12	33.58	240	476264	40.00	ug/l	-0.03
44) Perylene-d12	37.79	264	289352	40.00	ug/l	-0.02

System Monitoring Compounds

28) TCMX	23.22	209	136100	41.39	ug/L	0.00
Spiked Amount	40.000		Recovery	=	103.48%	

Target Compounds

					Qvalue
2) N-nitrosodimethylamine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitrosodi-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.84	128	195	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenylphenylether	23.22	204	521	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzene	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	23.21	168	198	N.D.	
32) 4-Bromophenylphenylether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	0.00	178	0	N.D.	

(#) = qualifier out of range (m) = manual integration

10065.D GCMS0520.M Tue May 21 11:34:10 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY2002\10065.D

Vial: 16

Acq On : 20 May 2002 9:55 pm

Operator:

Sample : EXTRACTED 5/9

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: May 21 11:33 2002

Quant Results File: GCMS0520.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Mon May 20 15:10:30 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0520

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
35) Anthracene	0.00	178	0	N.D.		
36) Di-n-butylphthalate	27.49	149	6152	N.D.		
37) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.57	228	1053	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.81	149	2189	N.D.		
43) Chrysene	33.57	228	1053	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	37.79	252	1173	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

10065.D GCMS0520.M

Tue May 21 11:34:11 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\MAY2002\10065.D
 Acq On : 20 May 2002 9:55 pm
 Sample : EXTRACTED 5/9
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 21 11:33 2002

Vial: 16
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0520.RES

Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Mon May 20 15:10:30 2002
 Response via : Initial Calibration

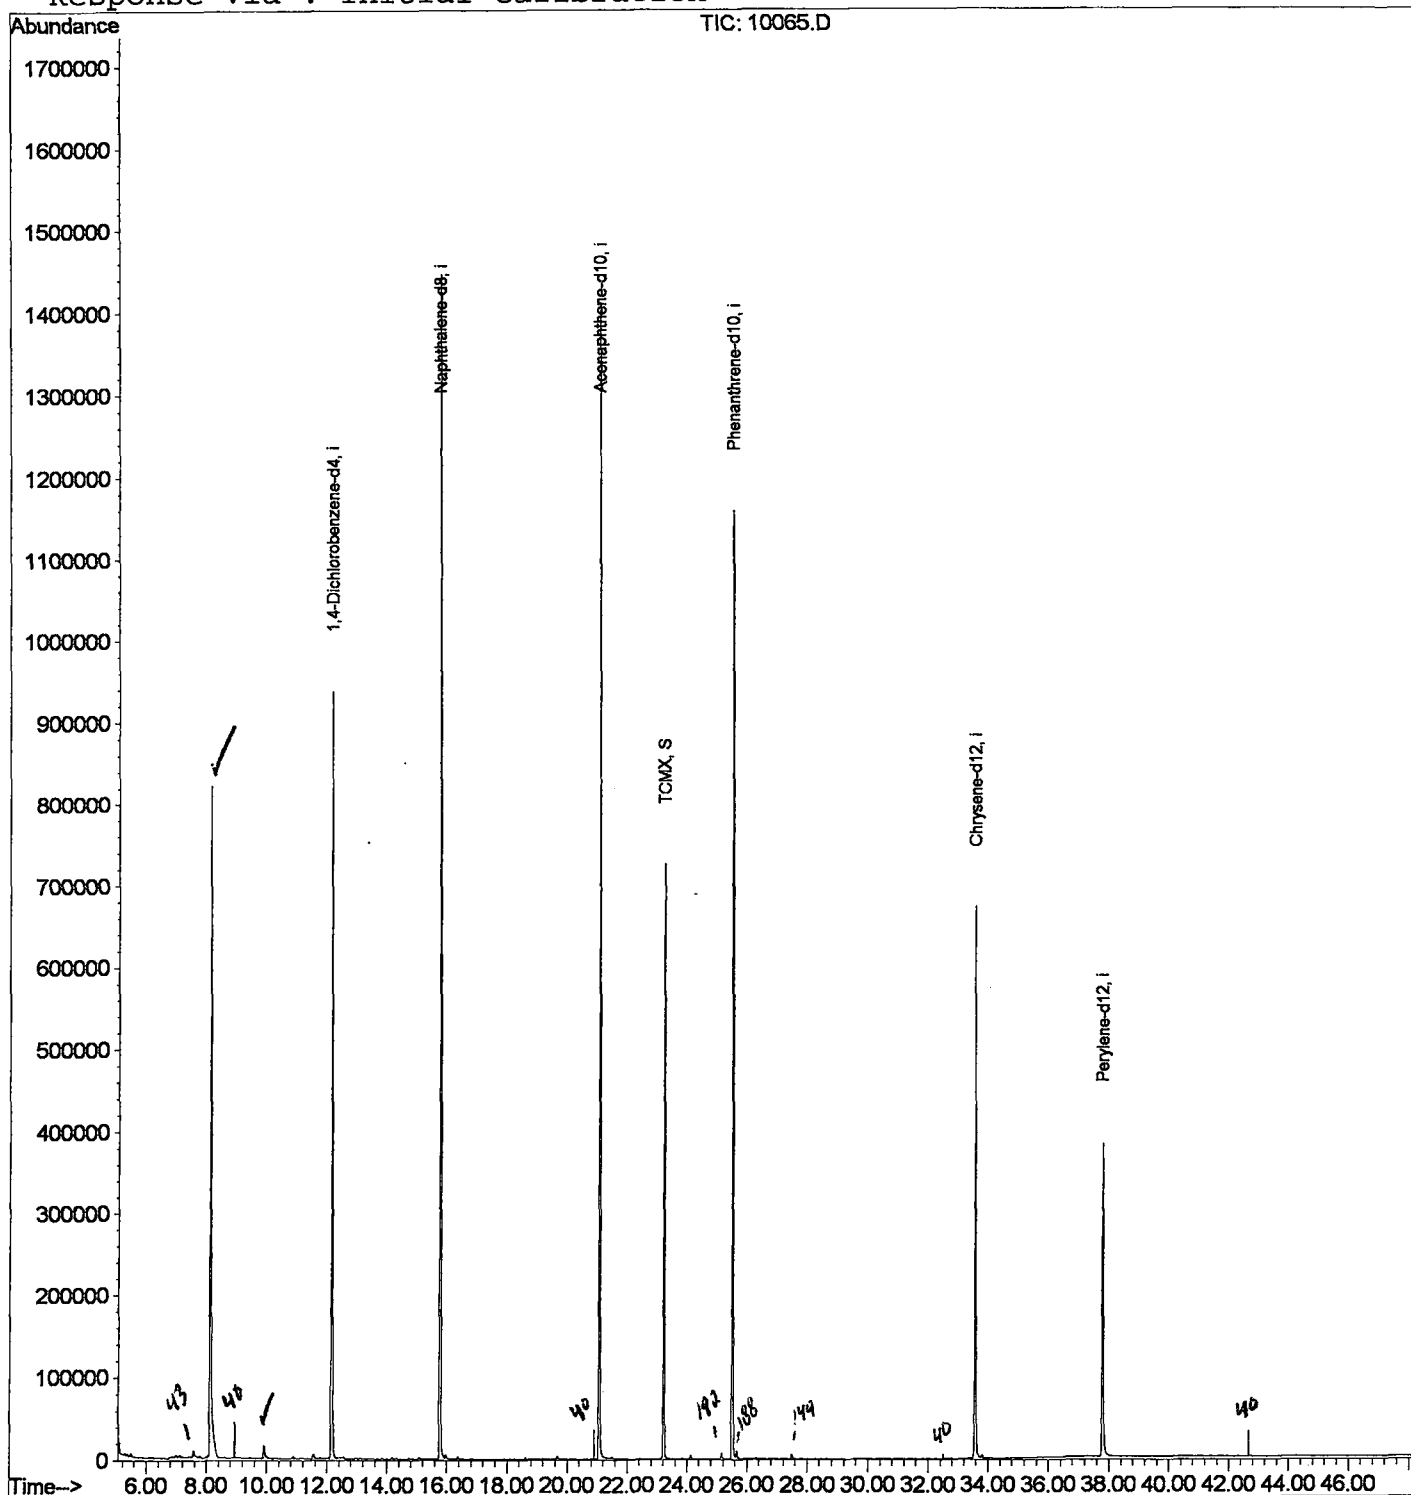

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\MAY2002\10065.D

Vial: 16

Acq On : 20 May 2002 9:55 pm

Operator:

Sample : EXTRACTED 5/9

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.113	331	335	366	rVB	819746	1867343	64.63%	11.354%
2	9.919	528	532	545	rVB	15010	40608	1.41%	0.247%
3	12.145	769	775	793	rVB	935641	2239112	77.50%	13.615%
4	15.774	1165	1171	1189	rBV	1445049	2889206	100.00%	17.568%
5	21.080	1744	1750	1770	rBV	1410733	2831923	98.02%	17.219%
6	23.224	1975	1984	1994	rBV	724437	1453061	50.29%	8.835%
7	25.515	2228	2234	2244	rBV2	1157440	2490858	86.21%	15.145%
8	33.579	3107	3114	3130	rBV2	671300	1534717	53.12%	9.332%
9	37.785	3564	3573	3589	rBV2	381287	1099450	38.05%	6.685%




Sum of corrected areas: 16446278

10065.D GCMS0520.M

Tue May 21 11:38:05 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAY2002\10065.D
 Operator :
 Acquired : 20 May 2002 9:55 pm using AcqMethod GCMS0520
 Instrument : 209
 Sample Name: EXTRACTED 5/9
 Misc Info :
 Vial Number: 16
 Quant File :GCMS0520.RES (RTE Integrator)

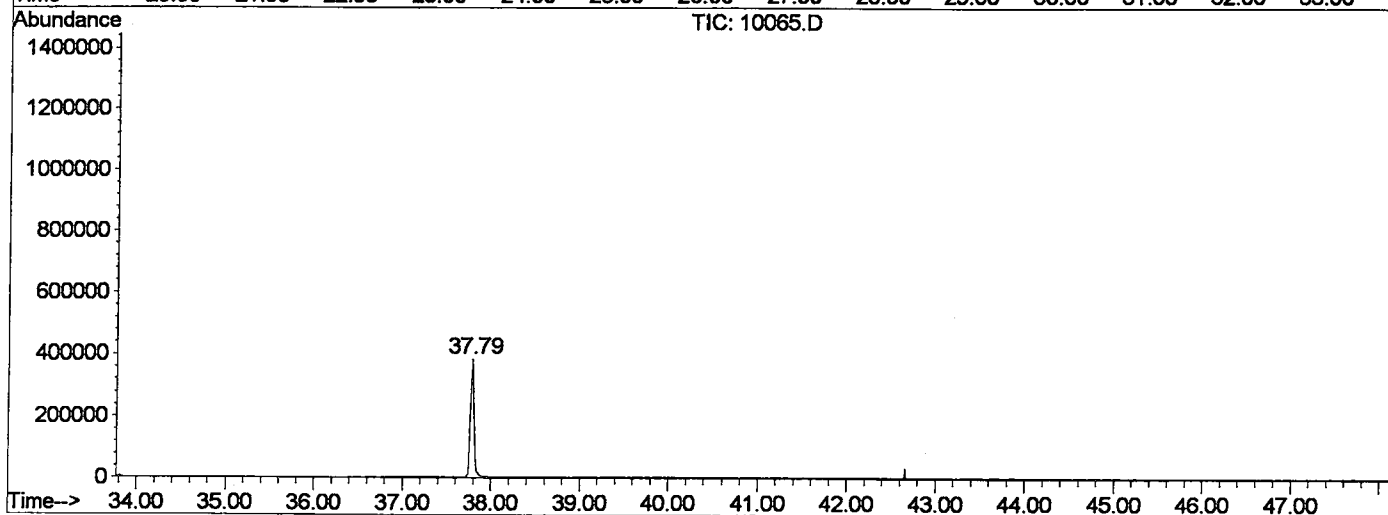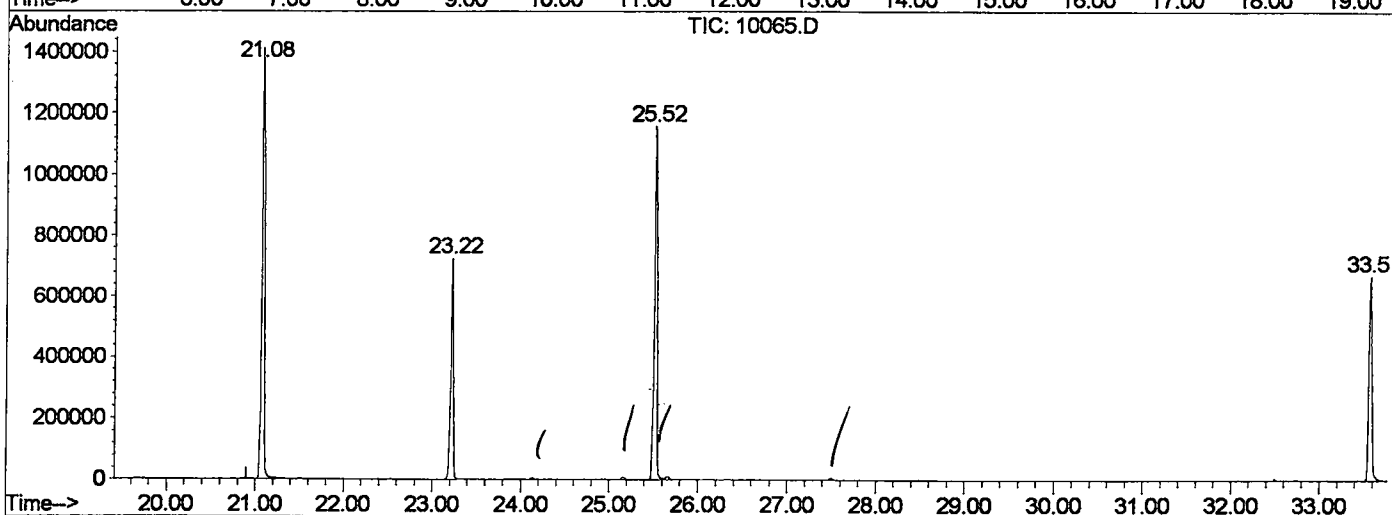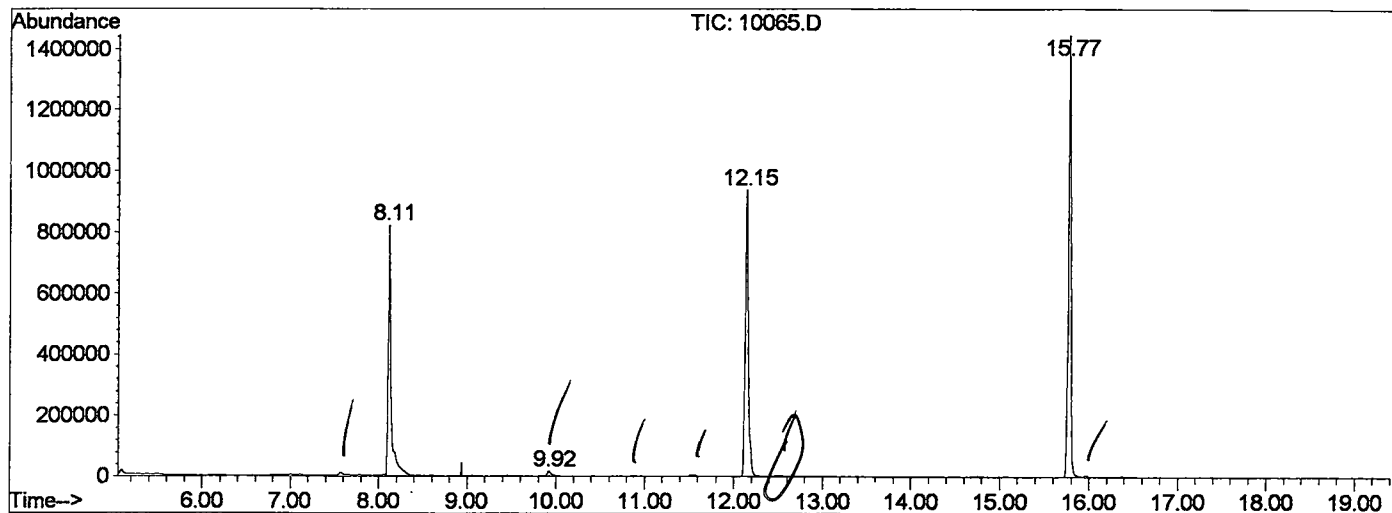

10065.D GCMS0520.M Tue May 21 11:38:06 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAY2002\10065.D
 Acq On : 20 May 2002 9:55 pm
 Sample : EXTRACTED 5/9
 Misc :
 MS Integration Params: LSCINT.P


Vial: 16
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.11	33.36 ug/l	1867340	1,4-Dichlorobenzene-d4	12.15

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2		CH2=CHCH2C(O)OCH3	100	C5H8O2	003724-55-8	9
3		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	7
4		Acetone	58	C3H6O	000067-64-1	7

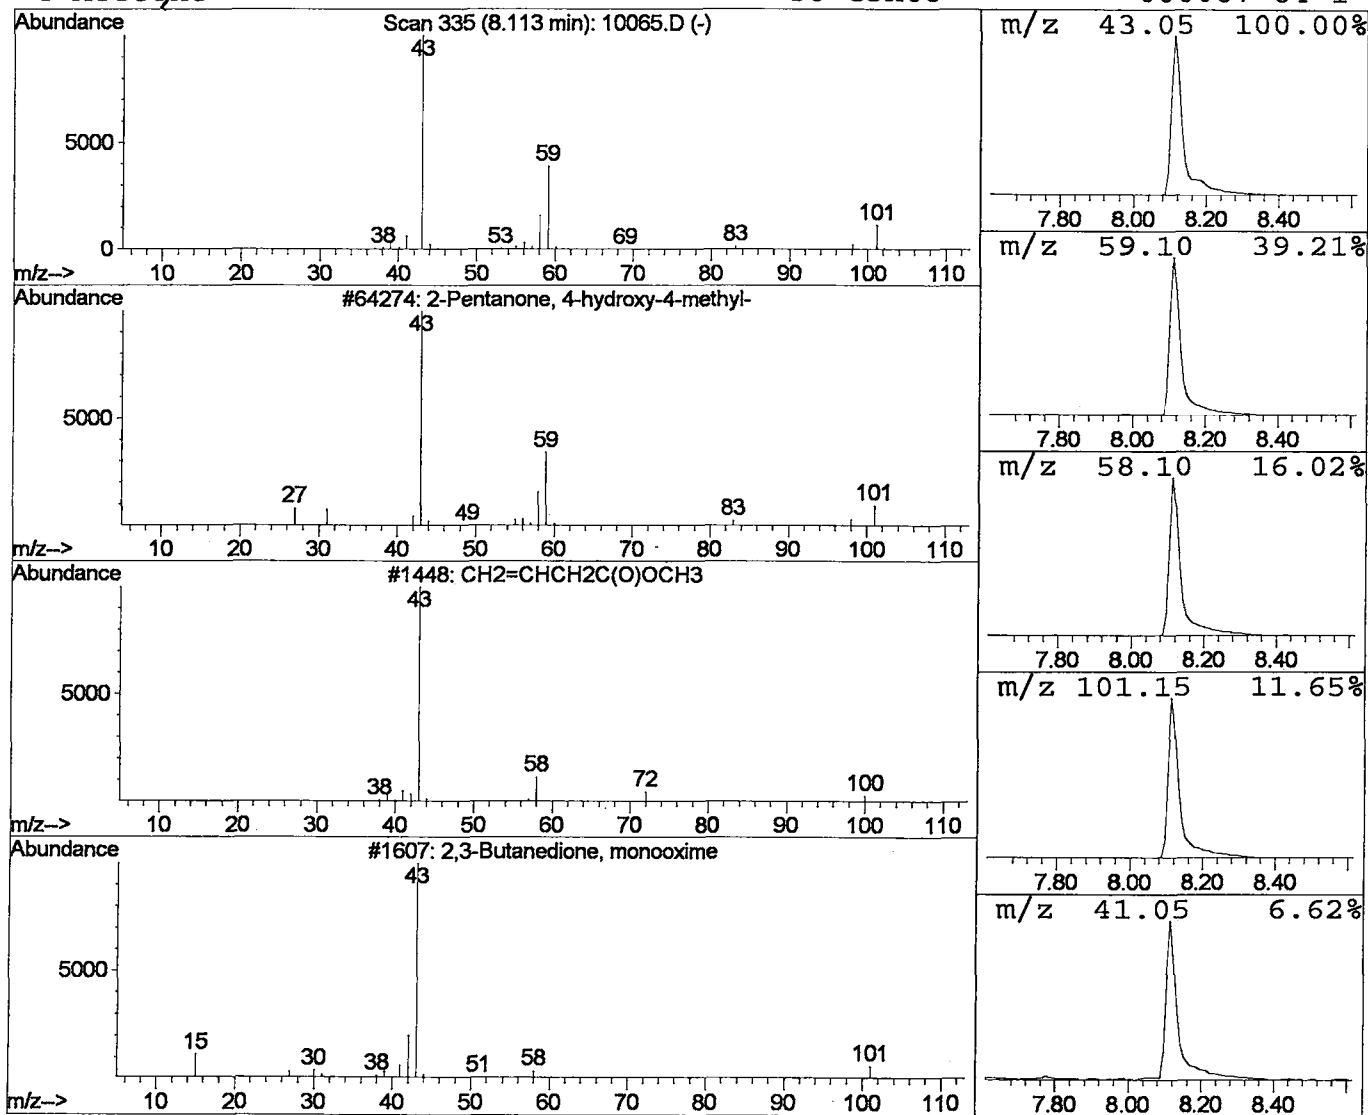

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAY2002\10065.D
 Acq On : 20 May 2002 9:55 pm
 Sample : EXTRACTED 5/9
 Misc :
 MS Integration Params: LSCINT.P


Vial: 16
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 2 Acetic acid, 1-methylpropyl es Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.92	0.73 ug/l	40608	1,4-Dichlorobenzene-d4	12.15

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Acetic acid, 1-methylpropyl ester	116	C6H12O2	000105-46-4	25	
2	Acetone	58	C3H6O	000067-64-1	9	
3	5-Hexen-2-one	98	C6H10O	000109-49-9	7	
4	2-Propanone, 1-cyclopropyl-	98	C6H10O	004160-75-2	5	

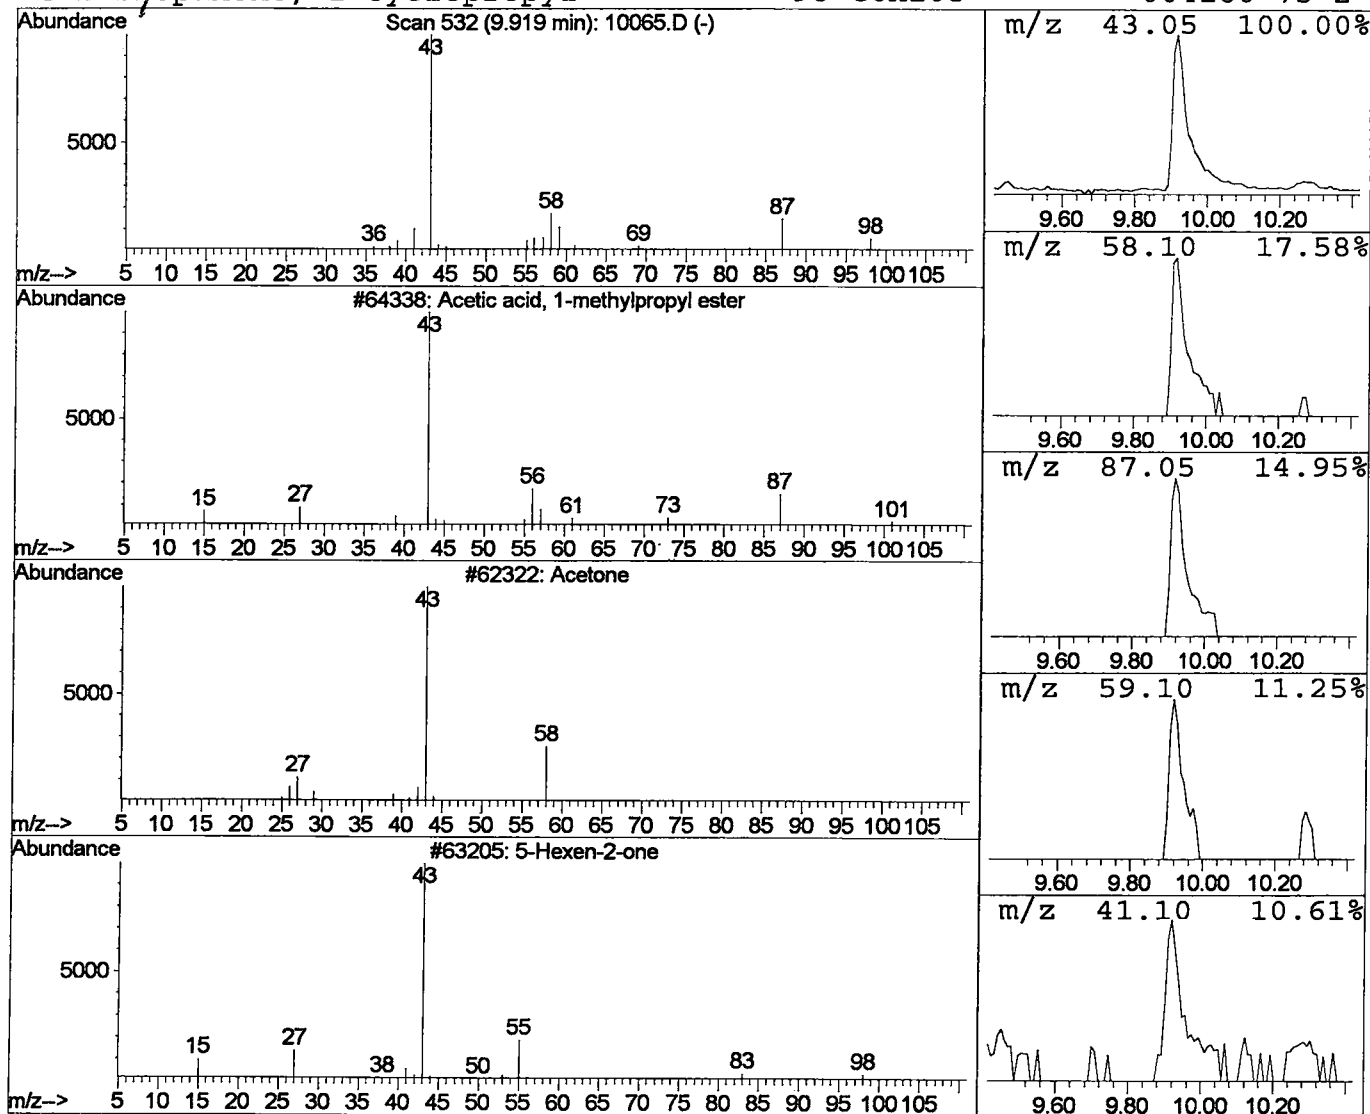

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 20 May 2002 9:55 pm
Data File: C:\HPCHEM\1\DATA\MAY2002\10065.D
Name: EXTRACTED 5/9
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.11	33.4	ug/l	1867340	ISTD01	12.15	2239110	40.0
Acetic acid, 1-methy	9.92	0.7	ug/l	40608	ISTD01	12.15	2239110	40.0

10065.D GCMS0520.M Tue May 21 11:38:08 2002