

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY0302\10065.D

Vial: 38

Acq On : 5 May 2002 4:16 am

Operator:

Sample : GC/MS SCAN 4/26

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: May 7 11:58 2002

Quant Results File: GCMS0501.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed May 01 10:40:31 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0501

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.20	152	496023	40.00	ug/l	-0.02
10) Naphthalene-d8	15.82	136	1825538	40.00	ug/l	-0.03
17) Acenaphthene-d10	21.13	164	981599	40.00	ug/l	-0.02
30) Phenanthrene-d10	25.57	188	1367289	40.00	ug/l	-0.02
38) Chrysene-d12	33.64	240	888351	40.00	ug/l	-0.03
44) Perylene-d12	37.86	264	581358	40.00	ug/l	-0.02

System Monitoring Compounds

28) TCMX	23.27	209	23605	4.94	ug/L	-0.02
Spiked Amount	10.000		Recovery	=	49.40%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.62	149	936	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	25.57	178	366	N.D.	

(#)=qualifier out of range (m)=manual integration

10065.D GCMS0501.M

Tue May 07 11:58:57 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY0302\10065.D

Vial: 38

Acq On : 5 May 2002 4:16 am

Operator:

Sample : GC/MS SCAN 4/26

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: May 7 11:58 2002

Quant Results File: GCMS0501.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed May 01 10:40:31 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0501

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
35) Anthracene	25.57	178	366		N.D.	
36) Di-n-butylphthalate	27.55	149	4556		N.D.	
37) Fluoranthene	0.00	202	0		N.D.	
39) Pyrene	0.00	202	0		N.D.	
40) Butylbenzylphthalate	32.08	149	1107		N.D.	
41) Benzo(a)anthracene	33.64	228	1936		N.D.	
42) Bis(2-ethylhexyl)phthalate	33.86	149	108869	5.14	ug/l	100
43) Chrysene	33.64	228	1936		N.D.	
45) Di-n-Octylphthalate	0.00	149	0		N.D.	
46) Benzo(b)fluoranthene	0.00	252	0		N.D.	
47) Benzo(k)fluoranthene	0.00	252	0		N.D.	
48) Benzo(a)pyrene	37.87	252	2280		N.D.	
49) Indeno(1,2,3-cd)pyrene	0.00	276	0		N.D.	
50) Dibenz(a,h)anthracene	0.00	278	0		N.D.	
51) Benzo(g,h,i)perylene	0.00	276	0		N.D.	

 (#) = qualifier out of range (m) = manual integration

10065.D GCMS0501.M

Tue May 07 11:58:58 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\MAY0302\10065.D
Acq On : 5 May 2002 4:16 am
Sample : GC/MS SCAN 4/26
Misc :
MS Integration Params: GOOFY.P
Quant Time: May 7 11:58 2002

Vial: 38
Operator:
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0501.RES

Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed May 01 10:40:31 2002
Response via : Initial Calibration

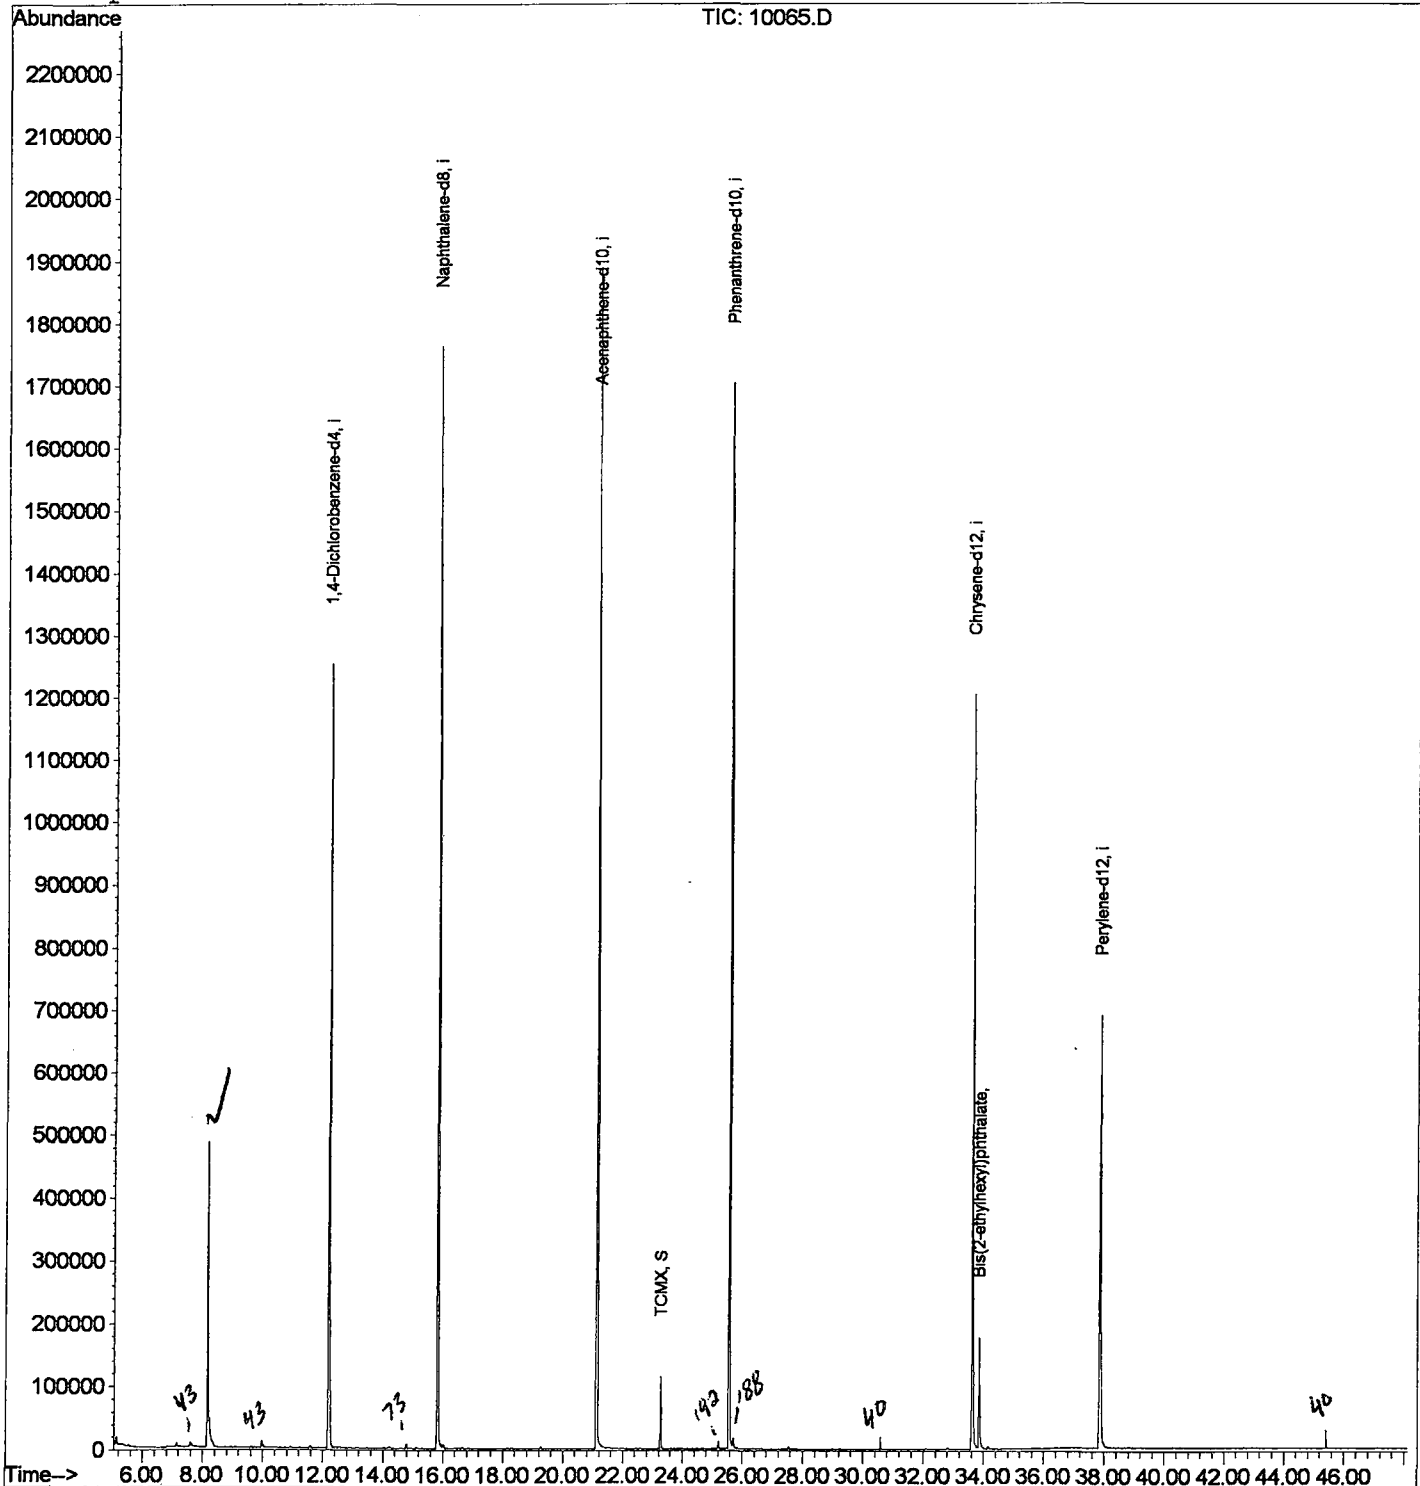

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\MAY0302\10065.D

Vial: 38

Acq On : 5 May 2002 4:16 am

Operator:

Sample : GC/MS SCAN 4/26

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.155	337	340	346	rBV	483522	945970	23.55%	4.603%
2	12.196	775	781	797	rBV	1251150	2873587	71.54%	13.981%
3	15.825	1171	1177	1195	rBV	1761288	3651334	90.91%	17.765%
4	21.131	1750	1756	1771	rBV	1887924	4016555	100.00%	19.542%
5	23.275	1984	1990	1996	rBV	113947	228955	5.70%	1.114%
6	25.575	2234	2241	2252	rBV2	1701547	3701844	92.16%	18.011%
7	33.639	3114	3121	3132	rBV	1204646	2671943	66.52%	13.000%
8	33.859	3139	3145	3161	rVB	175453	400530	9.97%	1.949%
9	37.863	3573	3582	3603	rBV2	689180	2062523	51.35%	10.035%




Sum of corrected areas: 20553241

10065.D GCMS0501.M

Tue May 07 12:00:58 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAY0302\10065.D
 Operator :
 Acquired : 5 May 2002 4:16 am using AcqMethod GCMS0501
 Instrument : 209
 Sample Name: GC/MS SCAN 4/26
 Misc Info :
 Vial Number: 38
 Quant File :GCMS0501.RES (RTE Integrator)

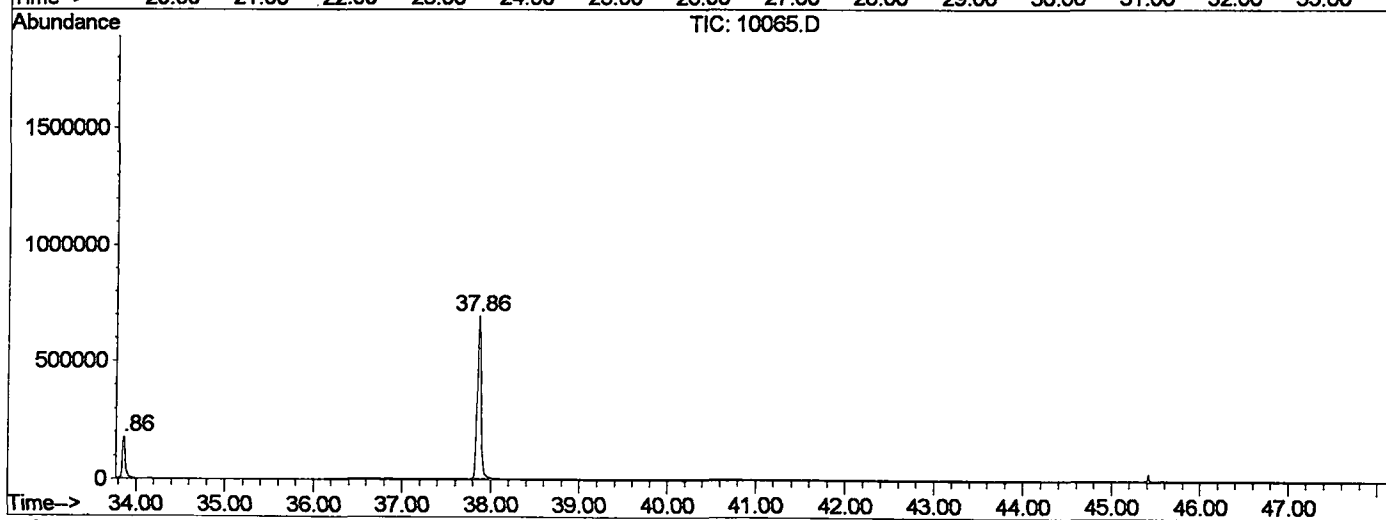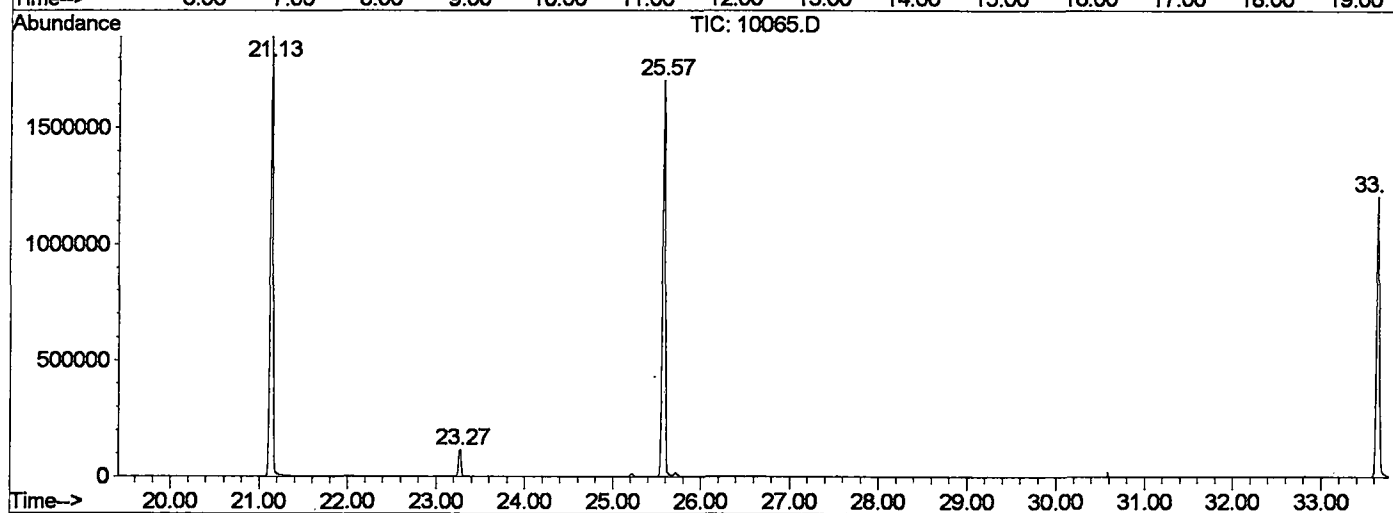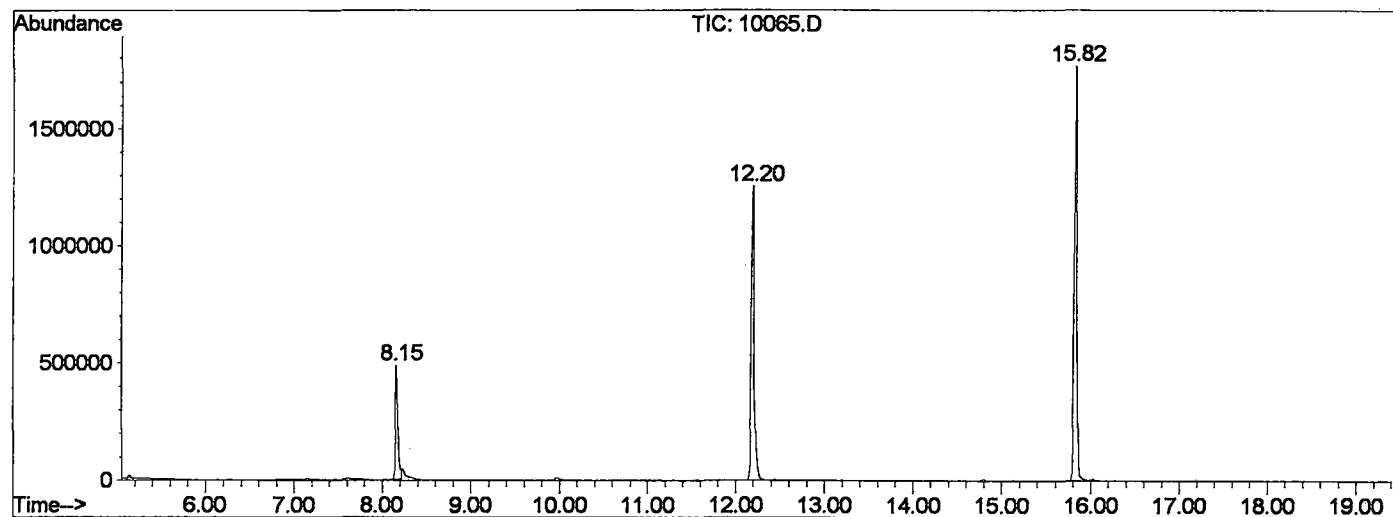

10065.D GCMS0501.M Tue May 07 12:00:59 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAY0302\10065.D
Acq On : 5 May 2002 4:16 am
Sample : GC/MS SCAN 4/26
Misc :
MS Integration Params: LSCINT.P


Vial: 38
Operator:
Inst : 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-methyl Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.15	13.17 ug/l	945970	1,4-Dichlorobenzene-d4	12.20

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	78		
2	3-Hydroxy-2-pentanone	102	C5H10O2	003142-66-3	9		
3	CH2=CHCH2C(O)OCH3	100	C5H8O2	003724-55-8	9		
4	Acetone	58	C3H6O	000067-64-1	7		

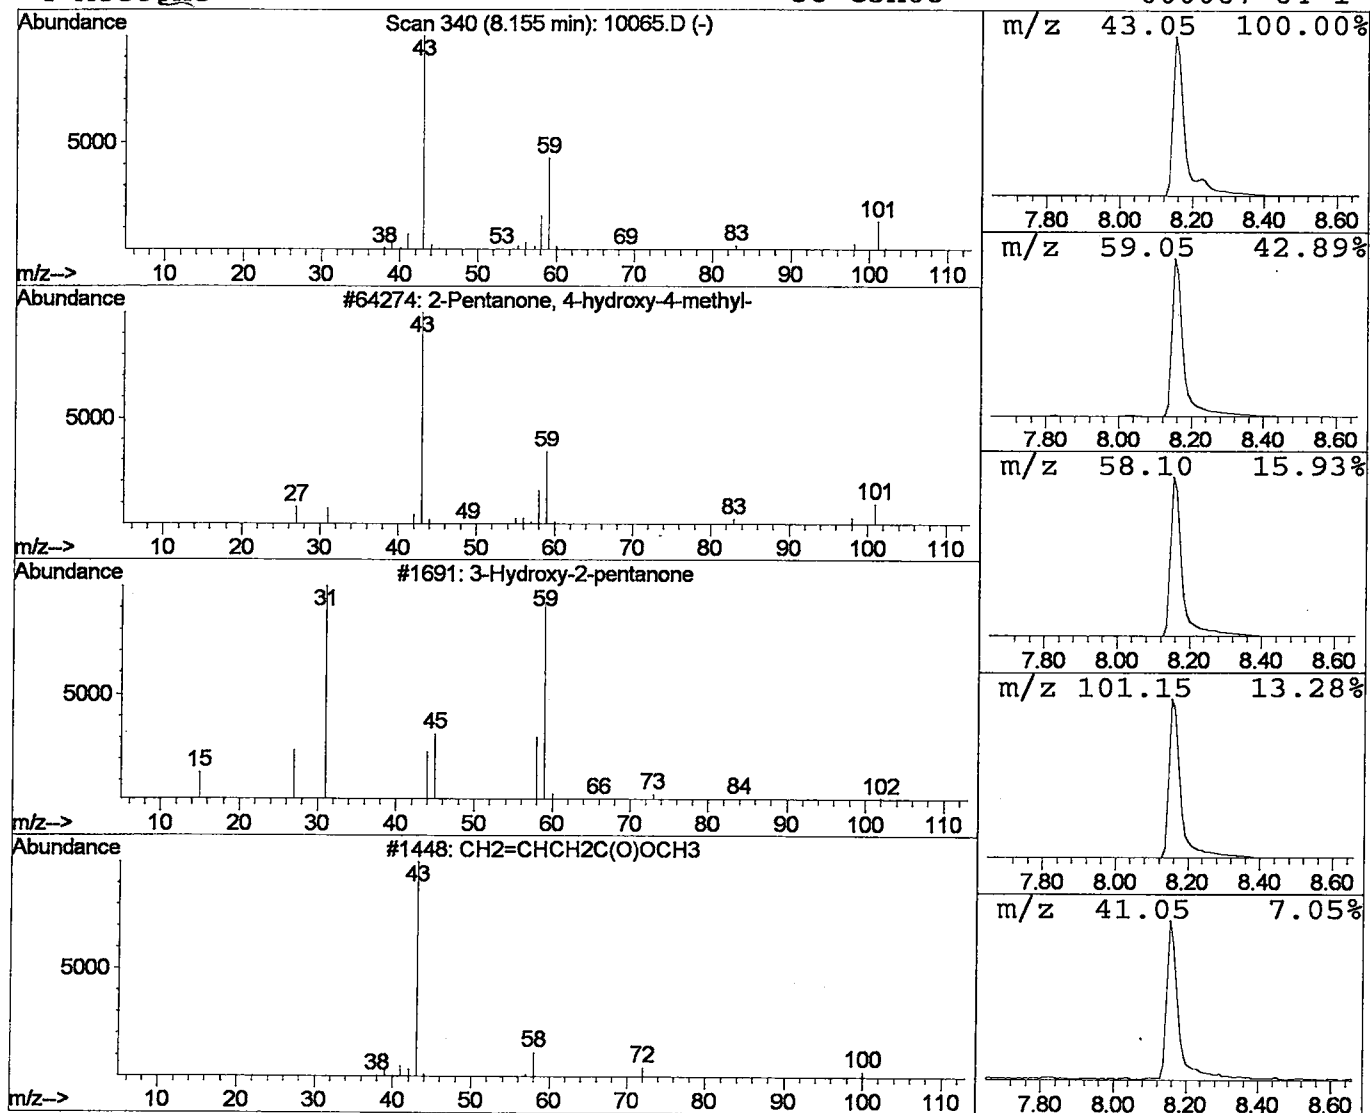

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 5 May 2002 4:16 am
Data File: C:\HPCHEM\1\DATA\MAY0302\10065.D
Name: GC/MS SCAN 4/26
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.15	13.2	ug/l	945970	ISTD01	12.20	2873590	40.0
10065.D GCMS0501.M								

10065.D GCMS0501.M Tue May 07 12:01:00 2002