

Quantitation Report


(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY0602\9680.D
 Acq On : 7 May 2002 1:51 pm
 Sample : GC/MS SCAN 4/25 FB
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 9 9:22 2002

Vial: 23
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0501.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed May 01 10:40:31 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0501



Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.19	152	537724	40.00	ug/l	-0.02
10) Naphthalene-d8	15.83	136	1977949	40.00	ug/l	-0.02
17) Acenaphthene-d10	21.14	164	1072668	40.00	ug/l	-0.01
30) Phenanthrene-d10	25.58	188	1500514	40.00	ug/l	-0.01
38) Chrysene-d12	33.64	240	885489	40.00	ug/l	-0.03
44) Perylene-d12	37.86	264	558173	40.00	ug/l	-0.02

System Monitoring Compounds

28) TCMX	23.27	209	33985	6.51	ug/L	-0.02
Spiked Amount	10.000		Recovery	=	65.10%	

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.		
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.		
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.		
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.		
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.		
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.		
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.		
9) Hexachloroethane	0.00	117	0	N.D.		
11) Nitrobenzene	0.00	77	0	N.D.		
12) Isophorone	0.00	82	0	N.D.		
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.		
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
15) Naphthalene	0.00	128	0	N.D.		
16) Hexachlorobutadiene	0.00	225	0	N.D.		
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
19) 2-Chloronaphthalene	0.00	162	0	N.D.		
20) Dimethylphthalate	0.00	163	0	N.D.		
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d	
22) Acenaphthylene	0.00	152	0	N.D.		
23) Acenaphthene	0.00	153	0	N.D.		
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.		
25) Diethylphthalate	22.62	149	250	N.D.		
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.		
27) Fluorene	0.00	166	0	N.D.		
29) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
33) Hexachlorobenzene	0.00	284	0	N.D.		
34) Phenanthrene	25.57	178	297	N.D.		

(#) = qualifier out of range (m) = manual integration

9680.D GCMS0501.M Thu May 09 09:23:12 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY0602\9680.D

Vial: 23

Acq On : 7 May 2002 1:51 pm

Operator:

Sample : GC/MS SCAN 4/25 FB

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: May 9 9:22 2002

Quant Results File: GCMS0501.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed May 01 10:40:31 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0501

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
35) Anthracene	25.57	178	297	N.D.		
36) Di-n-butylphthalate	27.54	149	1493	N.D.		
37) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.64	228	1984	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.86	149	5212	N.D.		
43) Chrysene	33.64	228	1984	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	37.87	252	2075	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

9680.D GCMS0501.M Thu May 09 09:23:13 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\MAY0602\9680.D
Acq On : 7 May 2002 1:51 pm
Sample : GC/MS SCAN 4/25 FB
Misc :
MS Integration Params: GOOFY.P
Quant Time: May 9 9:22 2002

Vial: 23
Operator:
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0501.RES

Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed May 01 10:40:31 2002
Response via : Initial Calibration

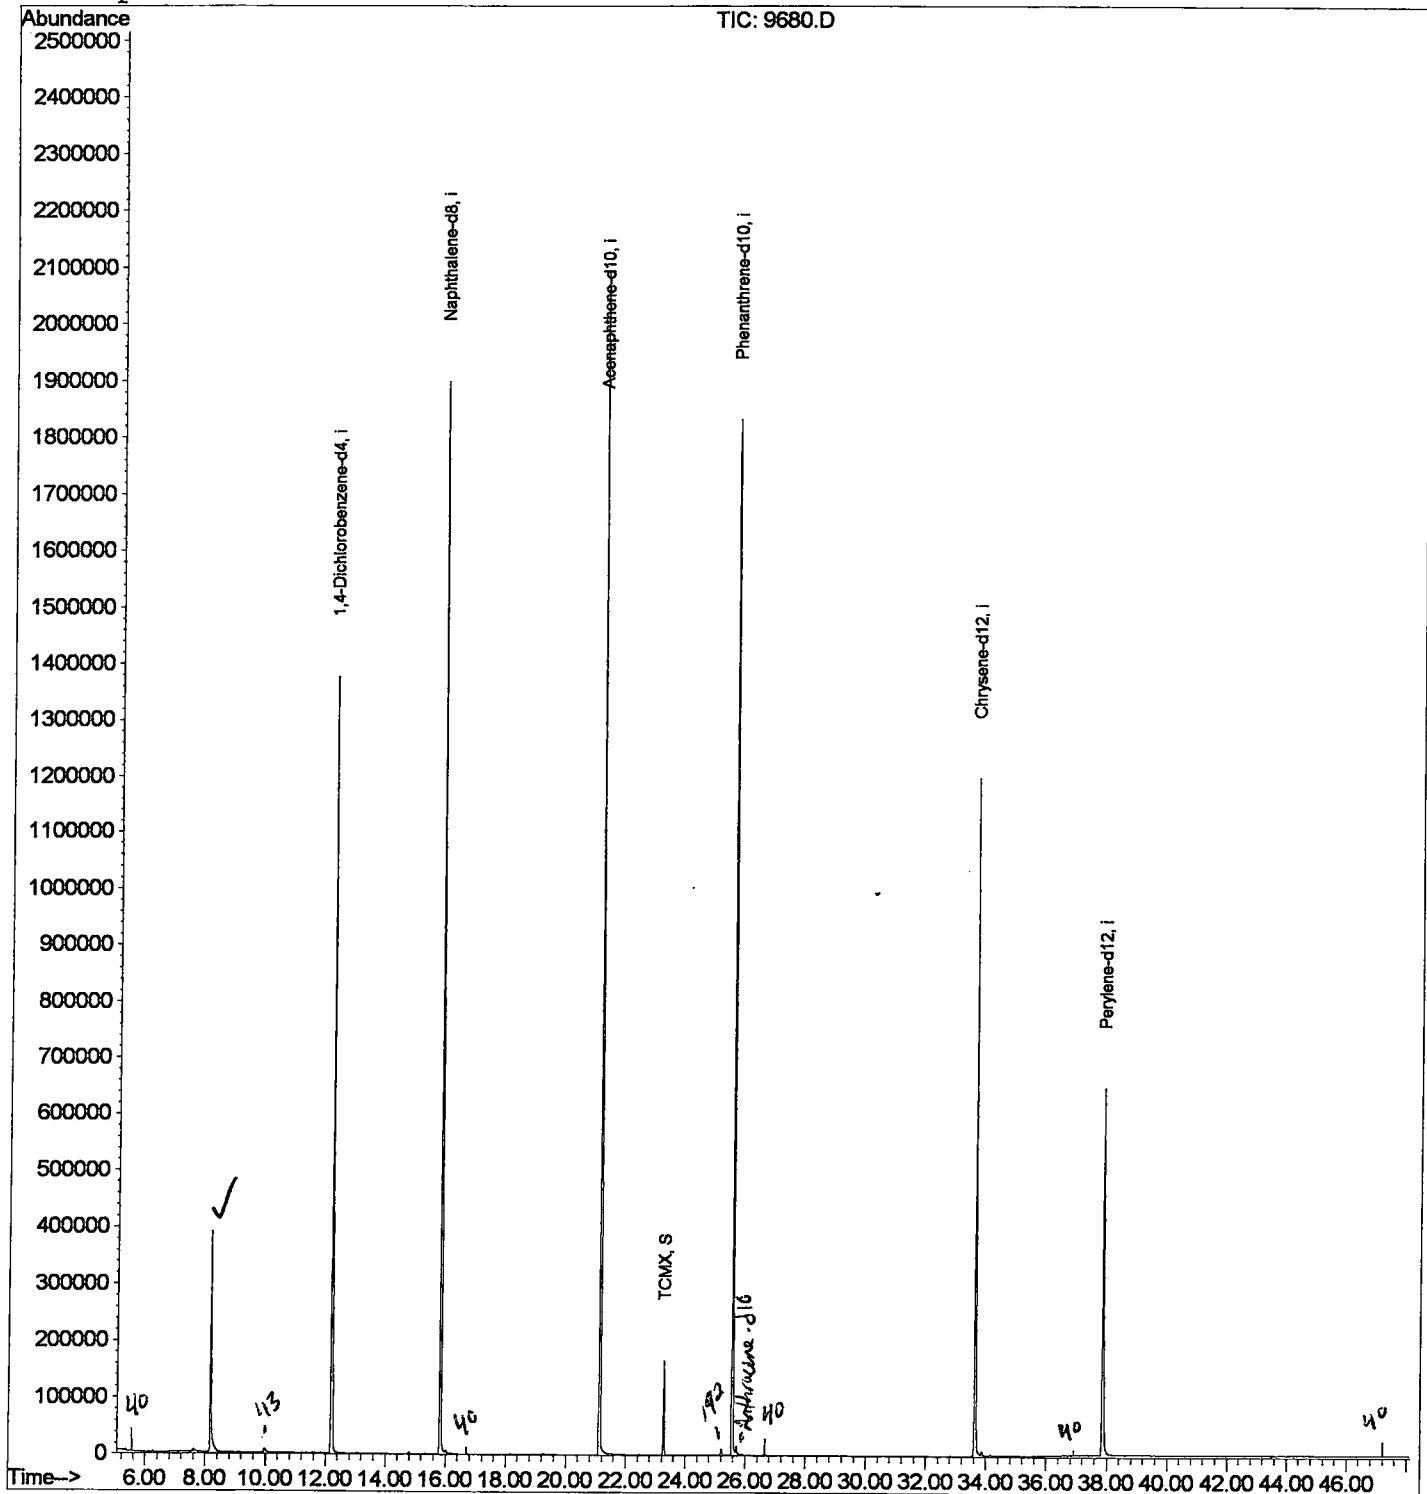

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\MAY0602\9680.D

Acq On : 7 May 2002 1:51 pm

Sample : GC/MS SCAN 4/25 FB

Misc :

MS Integration Params: LSCINT.P

Vial: 23

Operator:

Inst : 209

Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.162	337	341	367	rBV	389470	855555	19.70%	4.060%
2	12.194	775	781	796	rBV	1375743	3064109	70.55%	14.542%
3	15.832	1171	1178	1195	rBV	1898604	3903098	89.87%	18.524%
4	21.137	1750	1757	1779	rBV	2094884	4342886	100.00%	20.611%
5	23.272	1983	1990	1996	rBV	165361	319658	7.36%	1.517%
6	25.582	2235	2242	2253	rBV2	1832160	3995100	91.99%	18.960%
7	33.636	3114	3121	3138	rBV2	1199766	2637411	60.73%	12.517%
8	37.861	3574	3582	3604	rBV2	646252	1953135	44.97%	9.269%




Sum of corrected areas: 21070952

9680.D GCMS0501.M

Thu May 09 11:25:47 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAY0602\9680.D
 Operator :
 Acquired : 7 May 2002 1:51 pm using AcqMethod GCMS0501
 Instrument : 209
 Sample Name: GC/MS SCAN 4/25 FB
 Misc Info :
 Vial Number: 23
 Quant File : GCMS0501.RES (RTE Integrator)

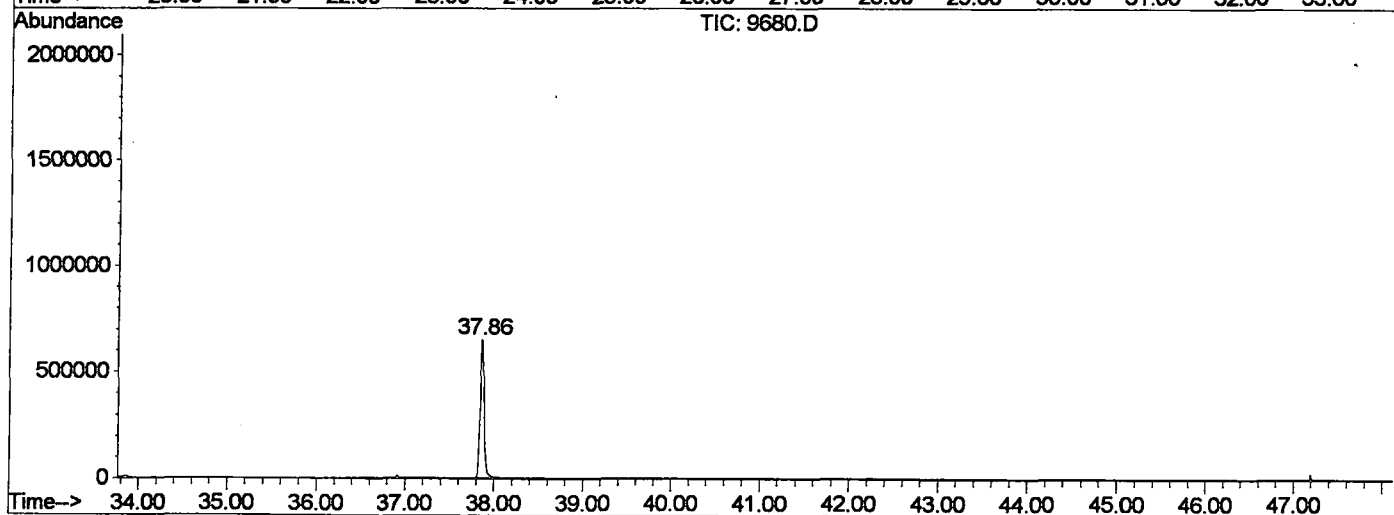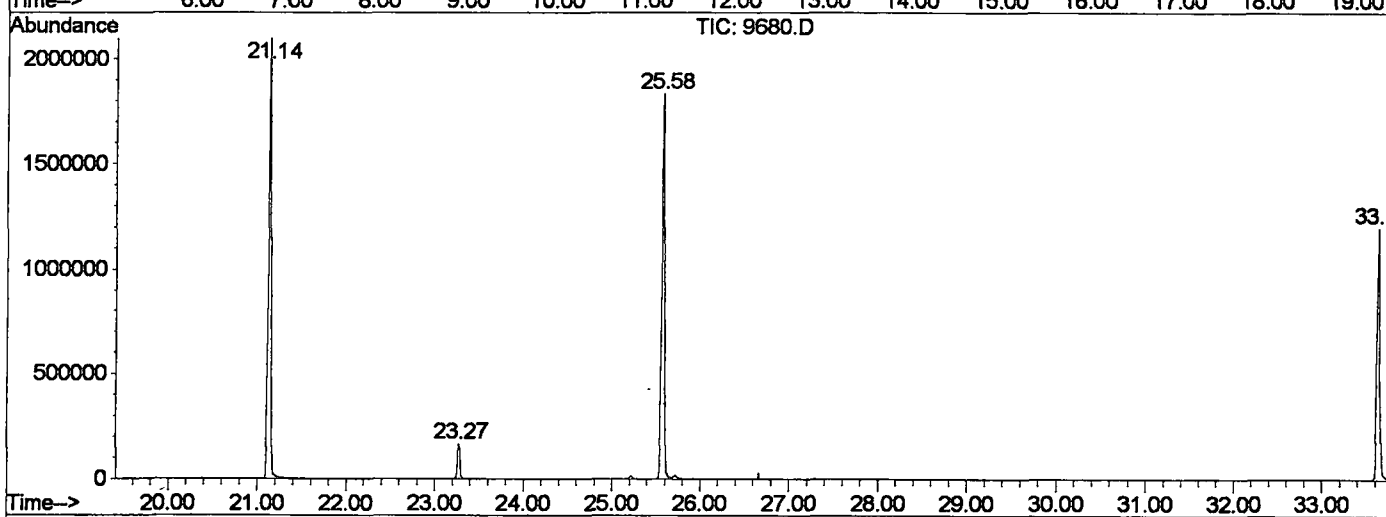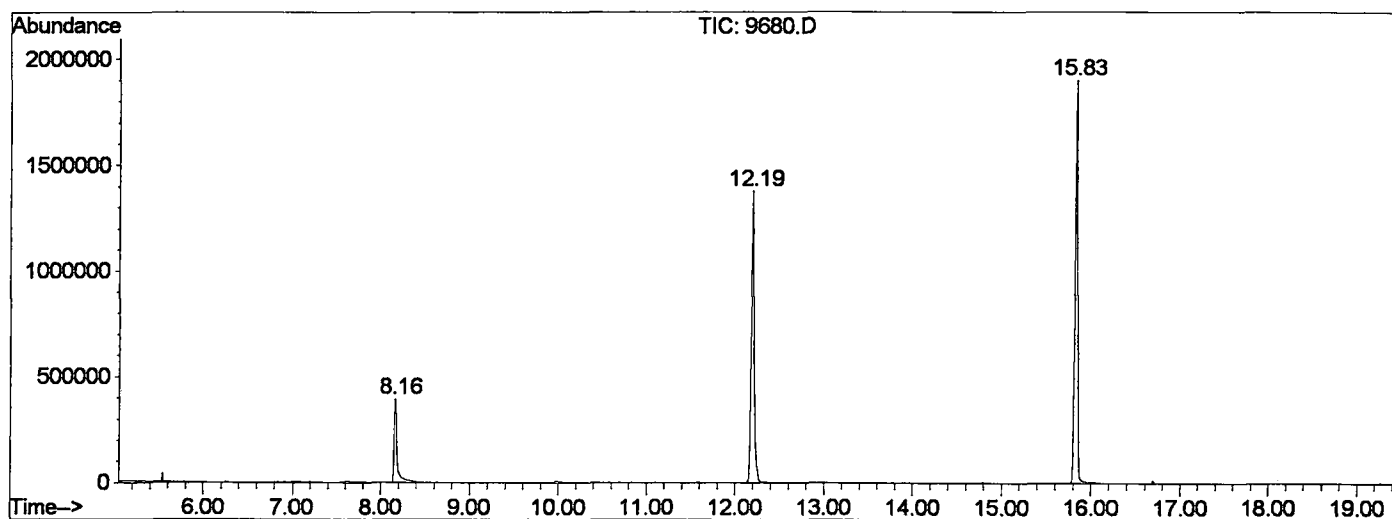

9680.D GCMS0501.M Thu May 09 11:25:48 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAY0602\9680.D
Acq On : 7 May 2002 1:51 pm
Sample : GC/MS SCAN 4/25 FB
Misc :
MS Integration Params: LSCINT.P


Vial: 23
Operator:
Inst : 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.16	11.17 ug/l	855555	1,4-Dichlorobenzene-d4	12.19

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	78
2		CH2=CHCH2C(O)OCH3	100	C5H8O2	003724-55-8	9
3		Acetone	58	C3H6O	000067-64-1	7
4		5-Hexen-2-one	98	C6H10O	000109-49-9	5

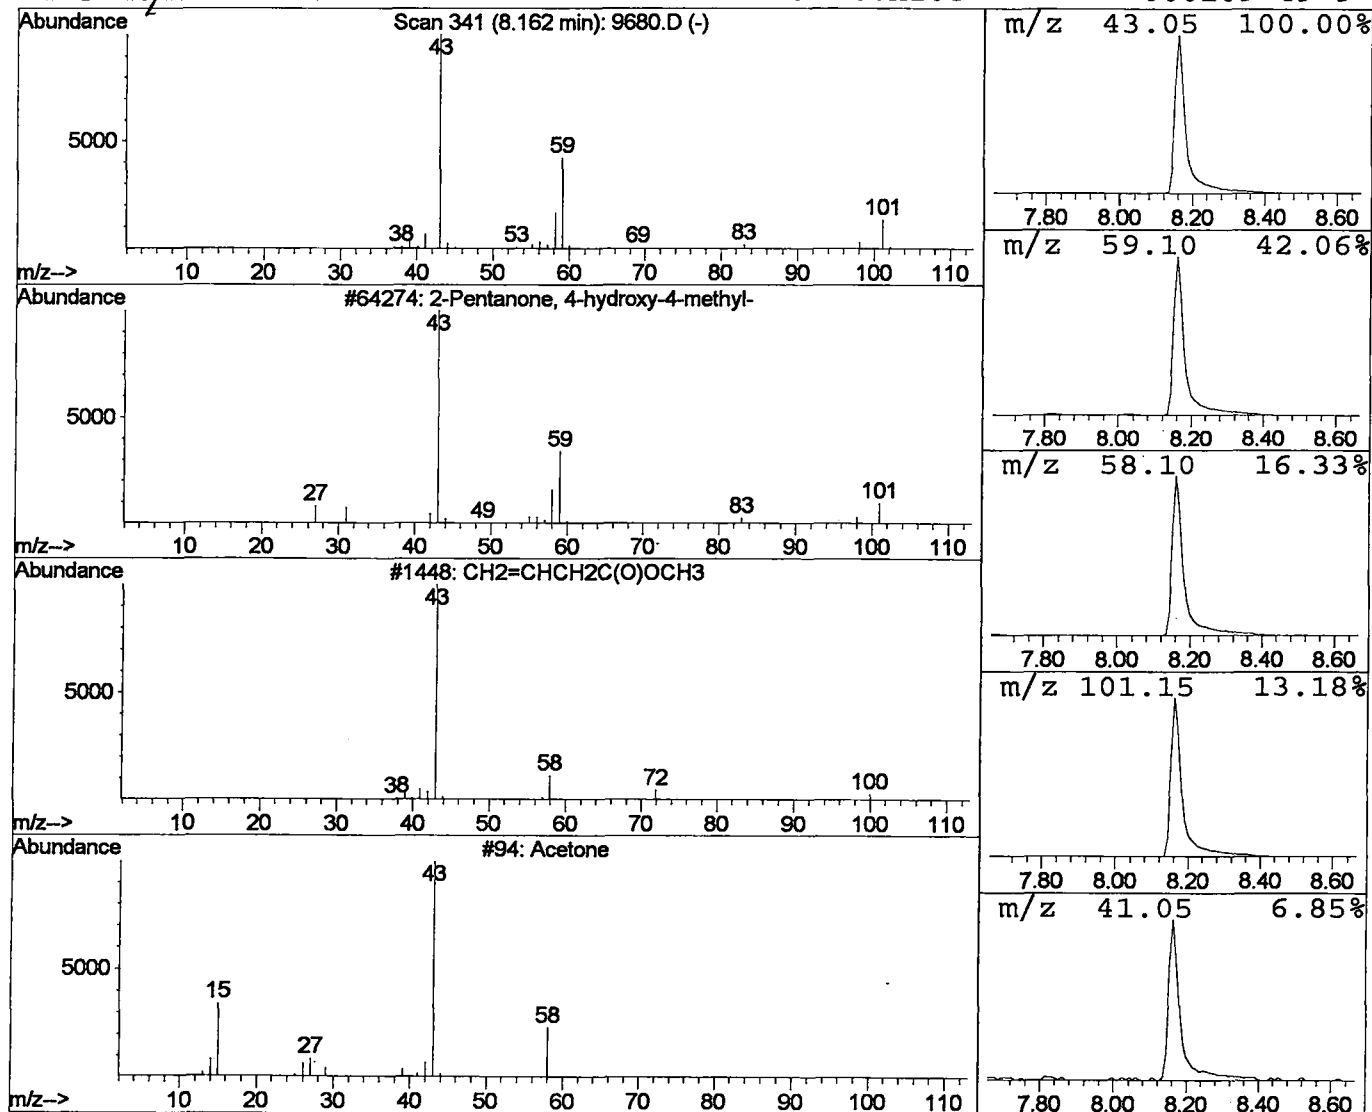

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 7 May 2002 1:51 pm
 Data File: C:\HPCHEM\1\DATA\MAY0602\9680.D
 Name: GC/MS SCAN 4/25 FB
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.16	11.2	ug/l	855555	ISTD01	12.19	3064110	40.0
9680.D GCMS0501.M	Thu May 09 11:25:49 2002							