


DFTPP

Data File : C:\HPCHEM\1\DATA\MAY1602\DFTPP.D
 Acq On : 16 May 2002 9:56 am
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : 209
 Multiplr: 1.00

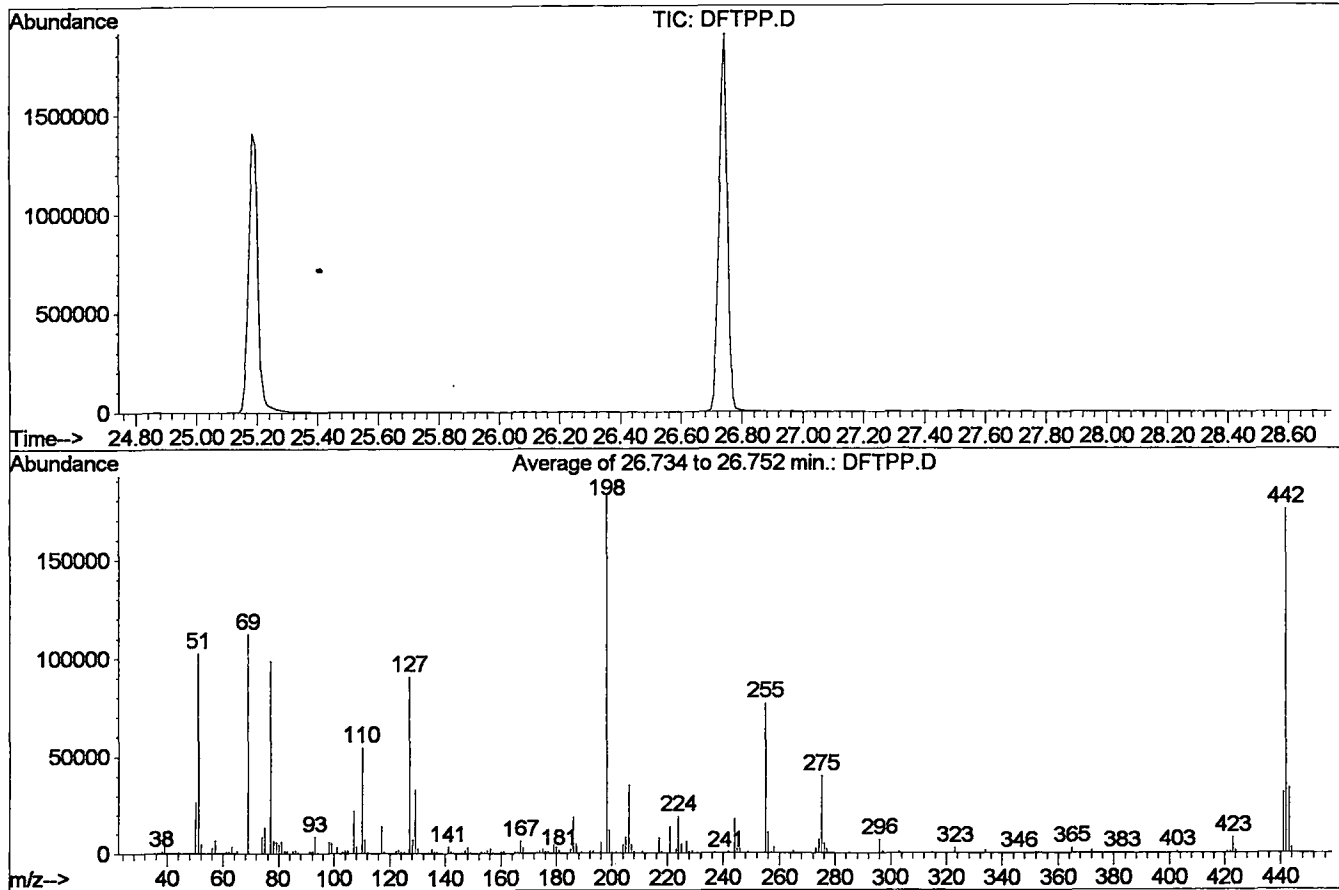

Spectrum Information: Average of 26.734 to 26.752 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	55.9	102517	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	61.2	112320	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	49.4	90624	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	183488	PASS
199	198	5	9	6.7	12244	PASS
275	198	10	30	21.9	40128	PASS
365	198	1	100	1.7	3127	PASS
441	443	0.01	100	93.4	31600	PASS
442	198	40	110	95.6	175349	PASS
443	442	17	23	19.3	33832	PASS

Sequence Name: C:\HPCHEM\1\SEQUENCE\MAY1602.S

Comment:

Operator:

Data Path: C:\HPCHEM\1\DATA\MAY1602\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch

☒ Full Method☒ Inject Anyway☐ Reprocessing Only☐ Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
------	------	------	----------	--------	-------------

1	Sample	1	DFTPP	GCMS0510	
2	Sample	2	CAL20	GCMS0510	
3	Sample	3	LB	GCMS0510	GC/MS SCAN 5/9
4	Sample	4	REF1	GCMS0510	GC/MS SCAN 5/9
5	Sample	5	REF2	GCMS0510	GC/MS SCAN 5/9
6	Sample	6	9680	GCMS0510	GC/MS SCAN 5/9 FB/Q
7	Sample	7	9676	GCMS0510	GC/MS SCAN 5/9 FB/Q
8	Sample	8	9673	GCMS0510	GC/MS SCAN 5/9
9	Sample	9	9654	GCMS0510	GC/MS SCAN 5/9 FB/Q
10	Sample	10	10062	GCMS0510	GC/MS SCAN 5/9
11	Sample	11	10063	GCMS0510	GC/MS SCAN 5/9
12	Sample	12	10064	GCMS0510	GC/MS SCAN 5/9
13	Sample	13	10065	GCMS0510	GC/MS SCAN 5/9

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY1602\LB.D
 Acq On : 16 May 2002 11:53 am
 Sample : GC/MS SCAN 5/9
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 17 11:41 2002

Vial: 3
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0510.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri May 17 11:28:42 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0510

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.16	152	370293	40.00	ug/l	-0.04
10) Naphthalene-d8	15.79	136	1479225	40.00	ug/l	-0.05
17) Acenaphthene-d10	21.09	164	701951	40.00	ug/l	-0.05
30) Phenanthrene-d10	25.54	188	1004677	40.00	ug/l	-0.04
38) Chrysene-d12	33.60	240	648747	40.00	ug/l	-0.04
44) Perylene-d12	37.83	264	399608	40.00	ug/l	-0.03

System Monitoring Compounds

28) TCMX	23.24	209	130170	37.28	ug/L	-0.04
Spiked Amount	10.000		Recovery	=	372.80%	

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) N-nitrosodimethylamine	0.00	74	0	N.D.		
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.		
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.		
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.		
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.		
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.		
8) N-Nitrosodi-n-propylamine	0.00	70	0	N.D.		
9) Hexachloroethane	0.00	117	0	N.D.		
11) Nitrobenzene	0.00	77	0	N.D.		
12) Isophorone	0.00	82	0	N.D.		
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.		
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
15) Naphthalene	15.84	128	607	N.D.		
16) Hexachlorobutadiene	0.00	225	0	N.D.		
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
19) 2-Chloronaphthalene	0.00	162	0	N.D.		
20) Dimethylphthalate	0.00	163	0	N.D.		
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.		
22) Acenaphthylene	0.00	152	0	N.D.		
23) Acenaphthene	0.00	153	0	N.D.		
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.		
25) Diethylphthalate	22.59	149	191	N.D.		
26) 4-Chlorophenylphenylether	0.00	204	0	N.D.		
27) Fluorene	0.00	166	0	N.D.		
29) Azobenzene	0.00	77	0	N.D.		
31) N-Nitrosodiphenylamine	23.24	168	317	N.D.		
32) 4-Bromophenylphenylether	0.00	248	0	N.D.		
33) Hexachlorobenzene	0.00	284	0	N.D.		
34) Phenanthrene	25.61	178	295	N.D.		

(#) = qualifier out of range (m) = manual integration

LB.D GCMS0510.M Fri May 17 11:42:11 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY1602\LB.D

Vial: 3

Acq On : 16 May 2002 11:53 am

Operator:

Sample : GC/MS SCAN 5/9

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: May 17 11:41 2002

Quant Results File: GCMS0510.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri May 17 11:28:42 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0510

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
35) Anthracene	25.61	178	295		N.D.	
36) Di-n-butylphthalate	27.52	149	961		N.D.	
37) Fluoranthene	29.25	202	429		N.D.	
39) Pyrene	29.92	202	569		N.D.	
40) Butylbenzylphthalate	0.00	149	0		N.D.	
41) Benzo(a)anthracene	33.60	228	2776		N.D.	
42) Bis(2-ethylhexyl)phthalate	33.83	149	1567		N.D.	
43) Chrysene	33.67	228	1316		N.D.	
45) Di-n-Octylphthalate	0.00	149	0		N.D.	
46) Benzo(b)fluoranthene	36.74	252	291		N.D.	
47) Benzo(k)fluoranthene	36.74	252	291		N.D.	
48) Benzo(a)pyrene	37.83	252	1677		N.D.	
49) Indeno(1,2,3-cd)pyrene	0.00	276	0		N.D.	
50) Dibenz(a,h)anthracene	0.00	278	0		N.D.	
51) Benzo(g,h,i)perylene	0.00	276	0		N.D.	

(#) = qualifier out of range (m) = manual integration

LB.D GCMS0510.M Fri May 17 11:42:12 2002

Page 2

Quantitation Report

Data File : C:\HPCHEM\1\DATA\MAY1602\LB.D
Acq On : 16 May 2002 11:53 am
Sample : GC/MS SCAN 5/9
Misc :
MS Integration Params: GOOFY.P
Quant Time: May 17 11:41 2002

Vial: 3
Operator:
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0510.RES

Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri May 17 11:28:42 2002
Response via : Initial Calibration

