

mod SUB MOD

Date Extracted 5/11/02
5/1/02

Page 11

GCMS-18476 / 05714/02

ab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count	
207		500ml		1ml			1ml	9B	7		
208	FB				1ml			9A			
209					1ml			10A			
210								10B			
211	FB							1A			
2236								1B			
2237								4B			
2238								2B			
2239	FB							2A			
2240								5A			
								4A			
								9A			
								10A			
marks											
rate must be between 5-15 ml/min for liq-liq extractors drip rate - traction type - <u>SEP. FW</u> Solv. lot# <u>X05E10</u> NaCl lot# <u>V39614</u> Na2SO4 lot# <u>V46648</u> TANDARD INT STD LOG# ALIBRATION REF SPIKE <u>2279E</u> MDL/MDRF Q. CHECK INT. STD. SURROGATE <u>TCMX / 4/25</u> LPC MDRIN/DDT											

Reviewed by,
6/15/02

Analyst WLS
vision 4/12/01

Verified by _____

Reviewed by (Signature)
Date 5/2/02

Comment: GUMS scan
Operator: Nefliu
Data Path: C:\MSDchem\1\DATA\020509\
Pre-Seq Cmd:
Post-Seq Cmd:

Method Sections To Run On A Barcode Mismatch
(X) Full Method (X) Inject Anyway
() Reprocessing Only () Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	508FAST	
2	Sample	2	0509C3	508SCAN1	ccv
3	Sample	3	0501LB1	508SCAN1	05/01 lab blk kb
4	Sample	4	0501LB2	508SCAN1	05/01 lab blk bn
5	Sample	5	0501REF1	508SCAN1	05/01 ref kb
6	Sample	6	0501REF2	508SCAN1	05/01 ref kb
7	Sample	7	0501REF3	508SCAN1	05/01 ref bn
8	Sample	8	0501REF4	508SCAN1	05/01 ref bn
9	Sample	9	10207	508SCAN1	sample
10	Sample	10	10208	508SCAN1	sample
11	Sample	11	10209	508SCAN1	sample
12	Sample	12	10210	508SCAN1	sample
13	Sample	13	10211	508SCAN1	sample
14	Sample	14	10236	508SCAN1	sample
15	Sample	15	10237	508SCAN1	sample
16	Sample	16	10238	508SCAN1	sample
17	Sample	17	10239	508SCAN1	sample
18	Sample	18	10240	508SCAN1	sample
19	Sample	19	10241	508SCAN1	sample
20	Sample	20	10242	508SCAN1	sample
21	Sample	21	10243	508SCAN1	sample
22	Sample	22	10244	508SCAN1	sample
23	Sample	23	10245	508SCAN1	sample
24	Sample	24	10246	508SCAN1	sample
25	Sample	25	10247	508SCAN1	sample
26	Sample	26	10301	508SCAN1	sample
27	Sample	27	10302	508SCAN1	sample
28	Sample	28	SURR	508SCAN1	05/10 surr unextracted

Lab #	Filename	Description	Vial #		Inj.	Standards used - Lot #				Remarks	Initials
			front	rear	ul	Calibration	Reference	Surrogate	Int. Std.		
	dftpp	dftpp	1		1						MN
	0509C3	car	2			22876/22874/2286e					
	0501LB1	lab lks	3					2285	2286		
	2		4								
	0501Ref1	ref	5				2279e				
	2		6								
	3		7								
	4		8								
	10207	sample	9								
	10208		10								
	10209		11								
	10210		12								
	10211		13								
	10236		14								
	10232		15								
	10238		16								
	10239		17								
	10240		18								
	10241		19								
	10242		20								
	10243		21								
	10244		22								
	10245		23								
	10246		24								
	10247		25								
	10301		26								
	10302		27								
	fwyr		28								

Date 05/09/02


Extraction date 05/01/02

Page 7

DFTPP

Data File : C:\MSDCHEM\1\DATA\020509\DFTPP.D
 Acq On : 9 May 2002 10:42 am
 Sample :
 Misc :
 MS Integration Params: rteint.e
 Method : C:\MSDCHEM\1\METHODS\SCAN020507.M (RTE Integrator)
 Title : Method 508 GC/MS Scan

Vial: 1
 Operator: Nefliu
 Inst : Instrume
 Multiplr: 1.00

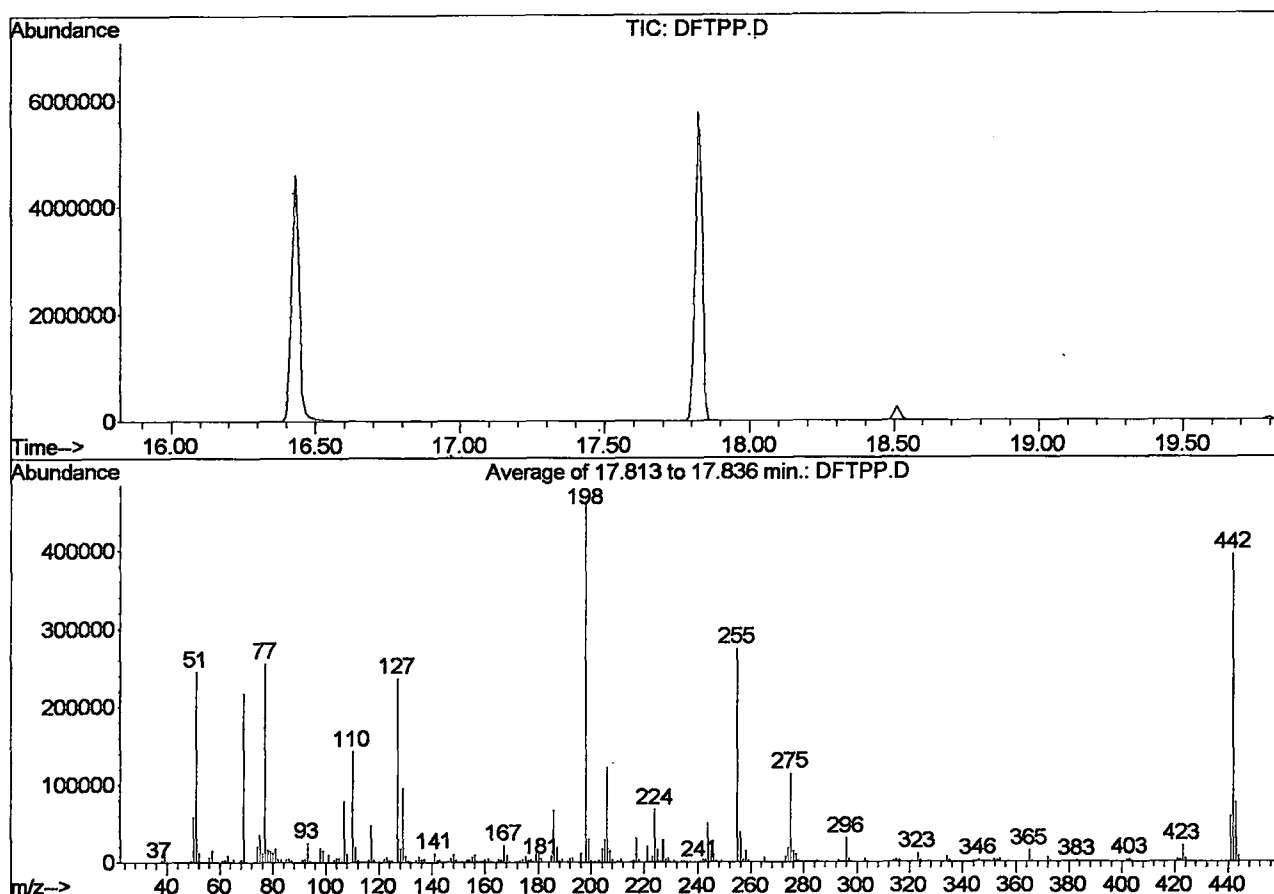

Spectrum Information: Average of 17.813 to 17.836 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	53.1	245354	PASS
68	69	0.00	2	1.6	3372	PASS
69	198	0.00	100	47.0	216938	PASS
70	69	0.00	2	0.5	1056	PASS
127	198	40	60	51.3	236800	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	461696	PASS
199	198	5	9	6.6	30413	PASS
275	198	10	30	24.7	114176	PASS
365	198	1	99	3.3	15158	PASS
441	443	1	100	76.8	58856	PASS
442	198	40	110	85.3	393856	PASS
443	442	17	23	19.4	76589	PASS

DFTPP.D SCAN020507.M

Tue May 14 14:07:53 2002