

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 05/28/2002 Time: 14:42:00

Sample: AE11310
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 5/28/02 14:41 Ended: 5/28/02 14:41 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		85		10.0

Comments for Sample AE11310 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 05-28-2002 Time: 14:42:24

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY2102\11310.D
 Acq On : 21 May 2002 11:26 pm
 Sample : EXTRACT5/14
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 22 9:13 2002

Vial: 24
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0520.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed May 22 09:03:22 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0520

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	12.14	152	470220	40.00	ug/l	0.00
10) Naphthalene-d8	15.77	136	1838353	40.00	ug/l	-0.02
17) Acenaphthene-d10	21.08	164	872120	40.00	ug/l	-0.01
30) Phenanthrene-d10	25.52	188	1114693	40.00	ug/l	-0.01
38) Chrysene-d12	33.58	240	563414	40.00	ug/l	-0.03
44) Perylene-d12	37.78	264	353634	40.00	ug/l	-0.02

System Monitoring Compounds

28) TCMX	23.22	209	148307	33.84	ug/L	-0.01
Spiked Amount	40.000		Recovery	=	84.60%	

Target Compounds

					Qvalue
2) N-nitrosodimethylamine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitrosodi-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.83	128	187	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.56	149	748	N.D.	
26) 4-Chlorophenylphenylether	23.22	204	747	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzene	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	23.22	168	404	N.D.	
32) 4-Bromophenylphenylether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	25.52	178	130	N.D.	

(#) = qualifier out of range (m) = manual integration

11310.D GCMS0520.M Wed May 22 09:14:06 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY2102\11310.D

Vial: 24

Acq On : 21 May 2002 11:26 pm

Operator:

Sample : EXTRACT5/14

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: May 22 9:13 2002

Quant Results File: GCMS0520.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed May 22 09:03:22 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0520

Compound	R.T.	QIon	Response	Conc Unit	Qvalue
35) Anthracene	0.00	178	0	N.D.	
36) Di-n-butylphthalate	27.50	149	35234	0.96 ug/l #	98
37) Fluoranthene	0.00	202	0	N.D.	
39) Pyrene	0.00	202	0	N.D.	
40) Butylbenzylphthalate	0.00	149	0	N.D.	
41) Benzo(a)anthracene	33.58	228	1416	N.D.	
42) Bis(2-ethylhexyl)phthalate	33.80	149	1153	N.D.	
43) Chrysene	33.58	228	1416	N.D.	
45) Di-n-Octylphthalate	0.00	149	0	N.D.	
46) Benzo(b)fluoranthene	0.00	252	0	N.D.	
47) Benzo(k)fluoranthene	0.00	252	0	N.D.	
48) Benzo(a)pyrene	37.78	252	1525	N.D.	
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.	
50) Dibenzo(a,h)anthracene	0.00	278	0	N.D.	
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.	

(#) = qualifier out of range (m) = manual integration

11310.D GCMS0520.M Wed May 22 09:14:07 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\MAY2102\11310.D
Acq On : 21 May 2002 11:26 pm
Sample : EXTRACT5/14
Misc :
MS Integration Params: GOOFY.P
Quant Time: May 22 9:13 2002

Vial: 24
Operator:
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0520.RES

Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed May 22 09:03:22 2002
Response via : Initial Calibration

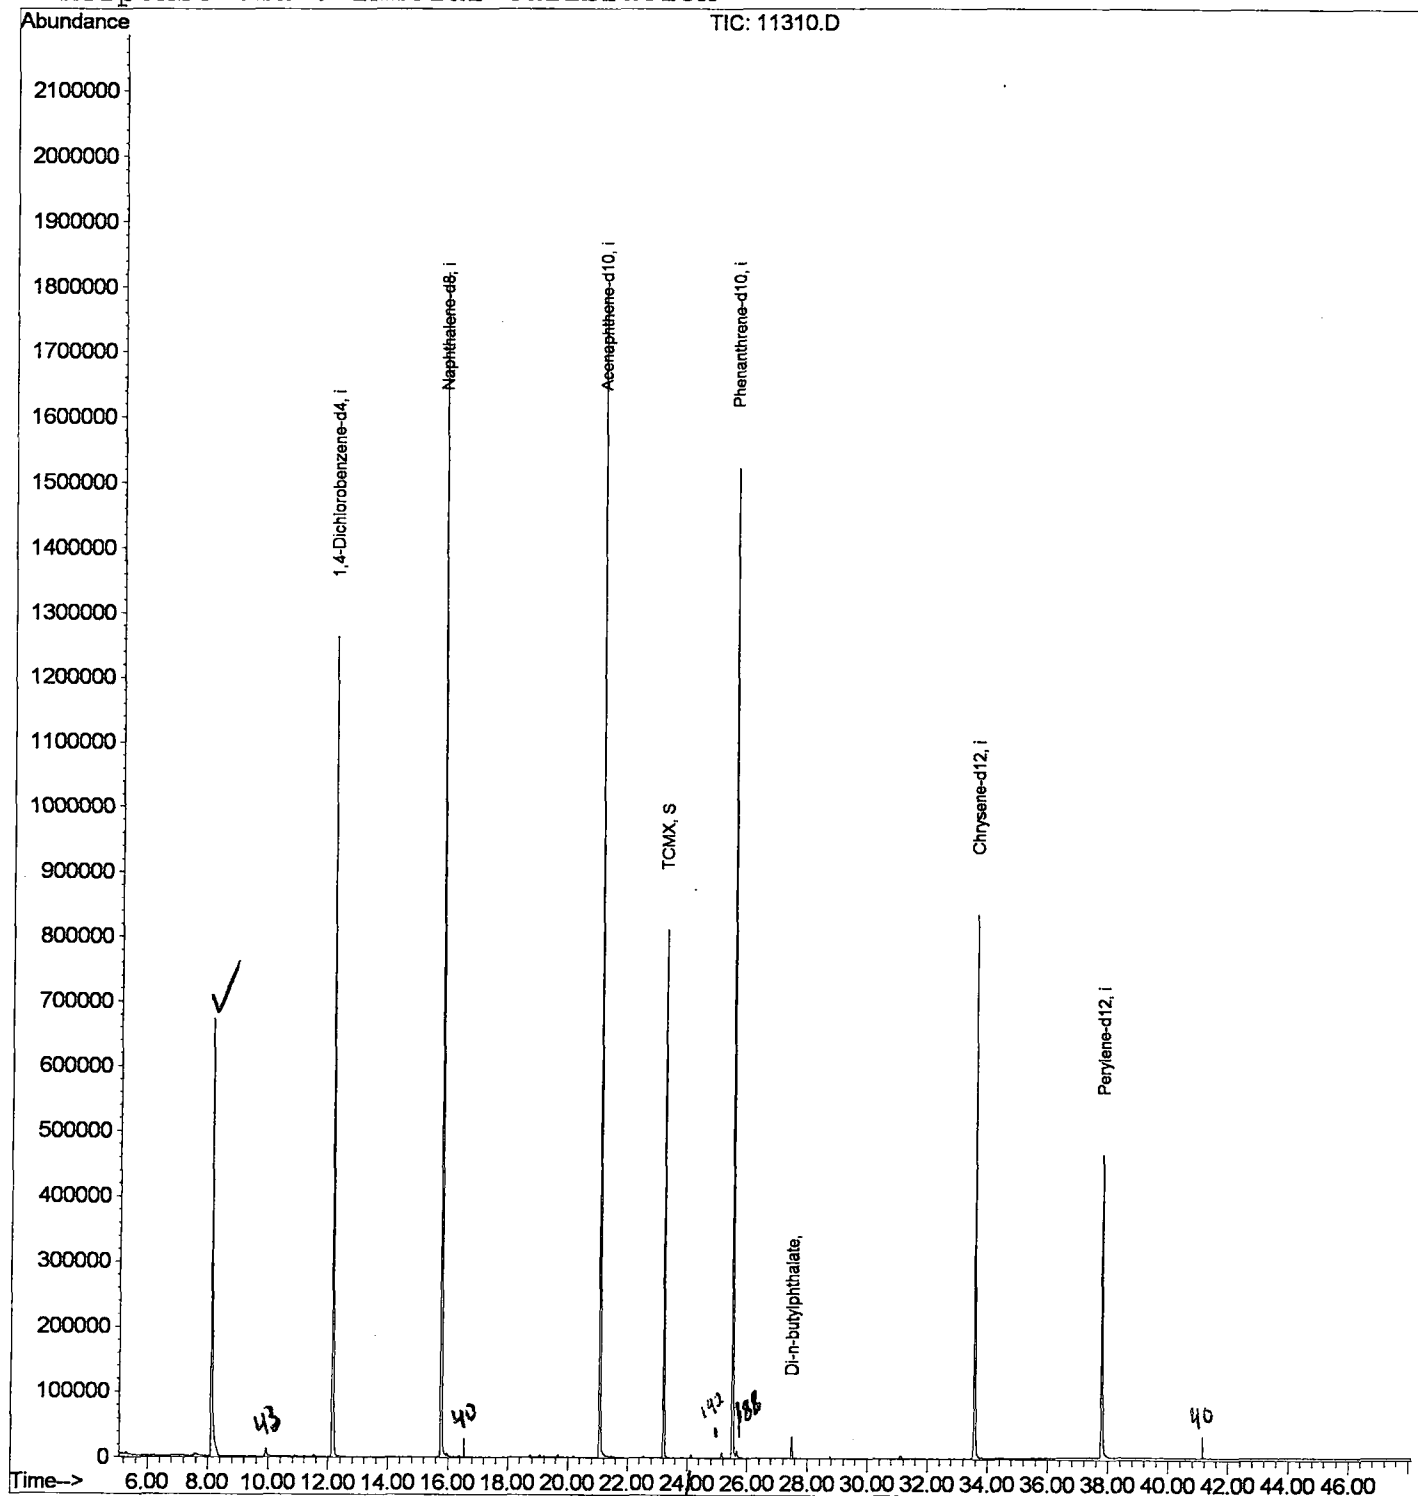

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\MAY2102\11310.D Vial: 24
 Acq On : 21 May 2002 11:26 pm Operator:
 Sample : EXTRACT5/14 Inst : 209
 Misc : Multiplr: 1.00
 MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.110	332	335	370	rVB	671356	1581028	42.22%	7.904%
2	12.142	769	775	796	rBV	1262129	2891158	77.20%	14.455%
3	15.771	1165	1171	1189	rBV	1820917	3744806	100.00%	18.722%
4	21.076	1744	1750	1766	rBV	1794264	3723459	99.43%	18.616%
5	23.221	1974	1984	1993	rBV	811082	1601746	42.77%	8.008%
6	25.521	2228	2235	2246	rBV2	1522177	3185332	85.06%	15.925%
7	27.500	2446	2451	2457	rVB	33152	61448	1.64%	0.307%
8	33.575	3107	3114	3130	rBV	835540	1846552	49.31%	9.232%
9	37.782	3565	3573	3593	rBV2	463195	1366125	36.48%	6.830%

Sum of corrected areas: 20001654

11310.D GCMS0520.M Wed May 22 09:21:42 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAY2102\11310.D
 Operator :
 Acquired : 21 May 2002 11:26 pm using AcqMethod GCMS0520
 Instrument : 209
 Sample Name: EXTRACT5/14
 Misc Info :
 Vial Number: 24
 Quant File :GCMS0520.RES (RTE Integrator)

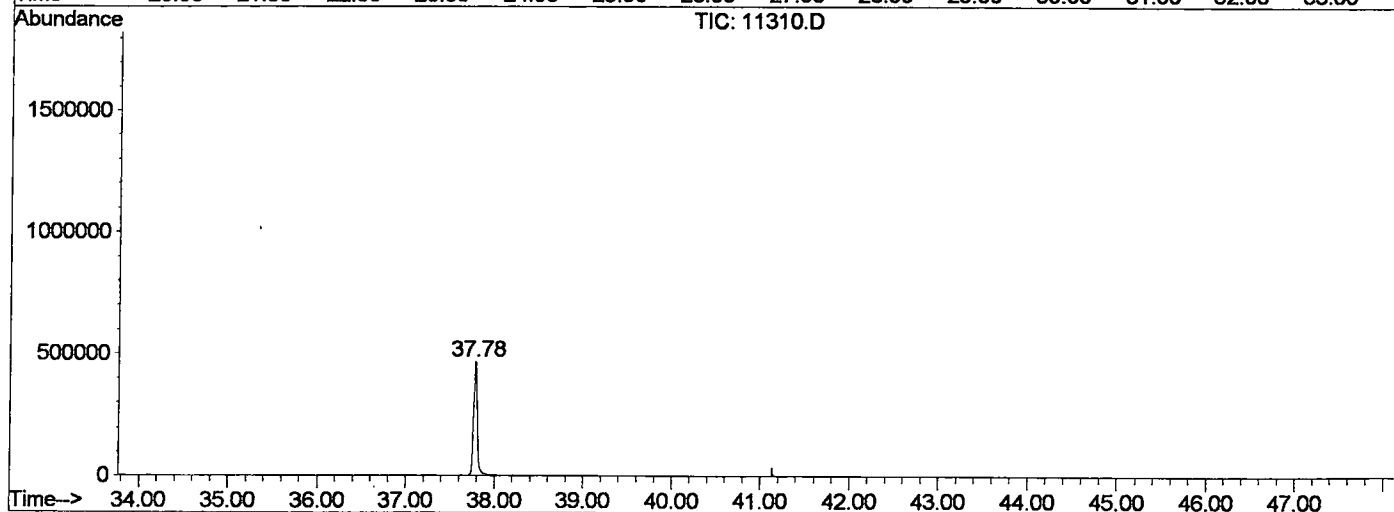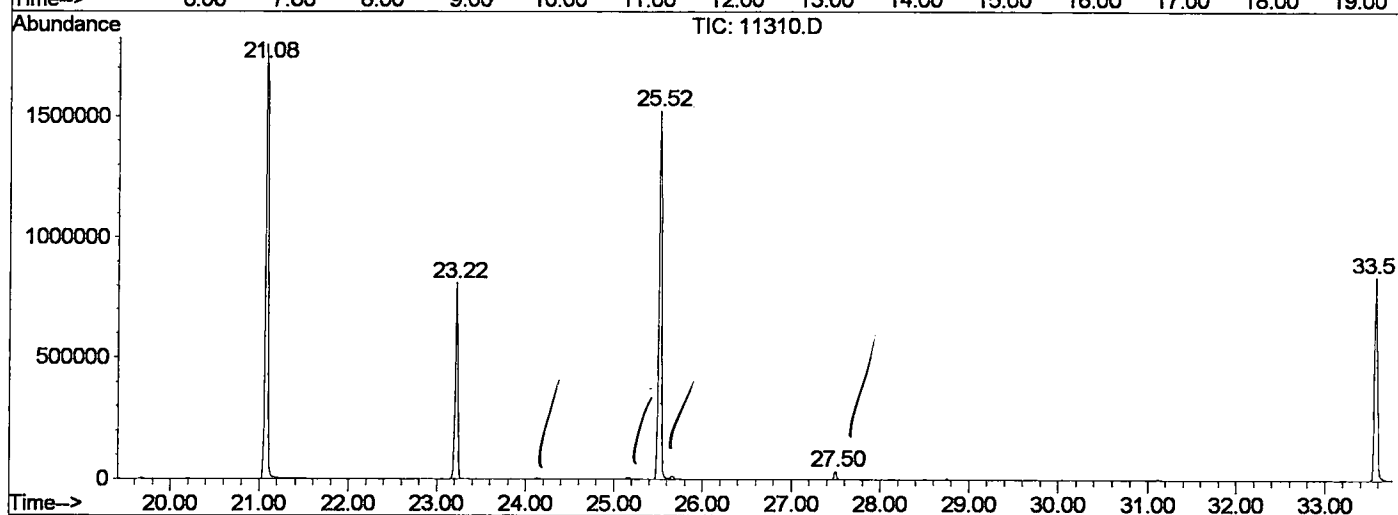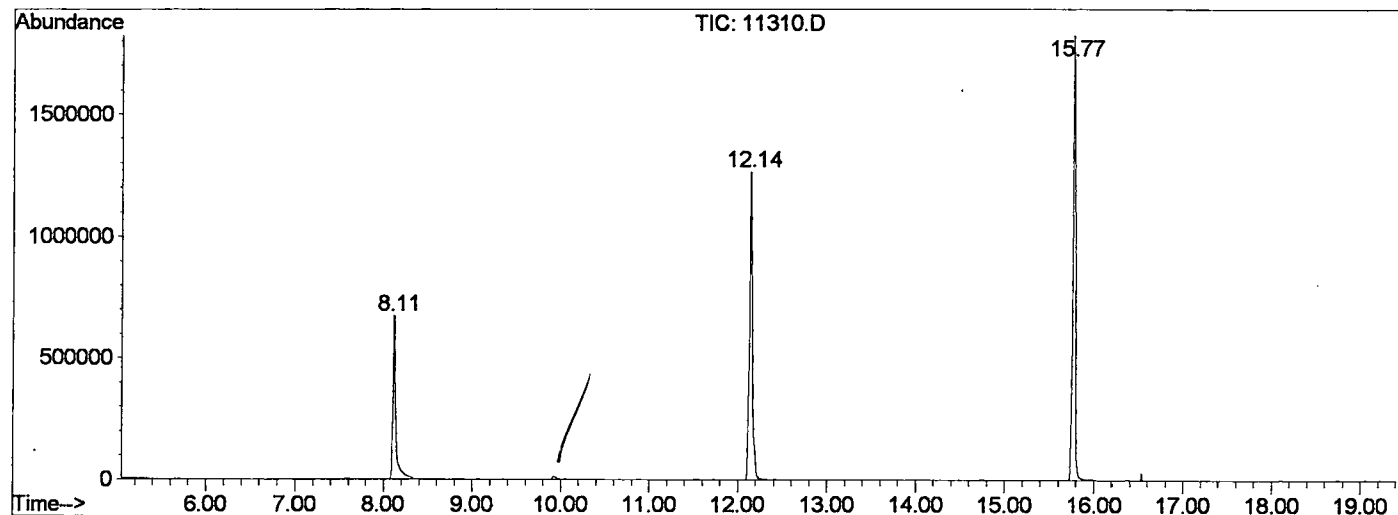

11310.D GCMS0520.M Wed May 22 09:21:43 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAY2102\11310.D
Acq On : 21 May 2002 11:26 pm
Sample : EXTRACT5/14
Misc :
MS Integration Params: LSCINT.P







Vial: 24
Operator:
Inst : 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-methyl Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.11	21.87 ug/l	1581030	1,4-Dichlorobenzene-d4	12.14

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72
2	Acetone	58	C3H6O	000067-64-1	9
3	CH2=CHCH2C(O)OCH3	100	C5H8O2	003724-55-8	9
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	7

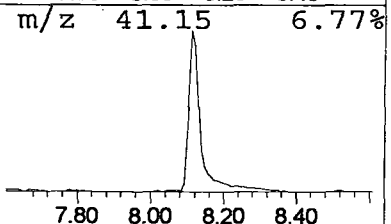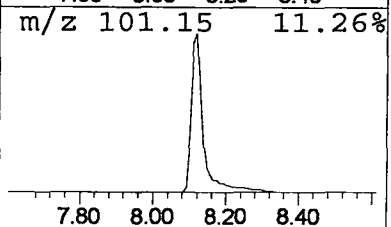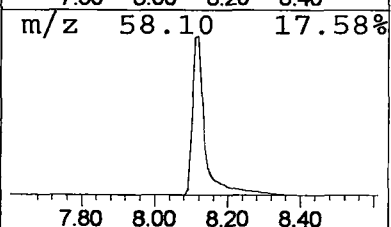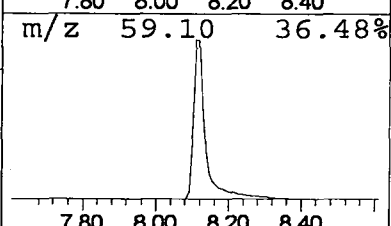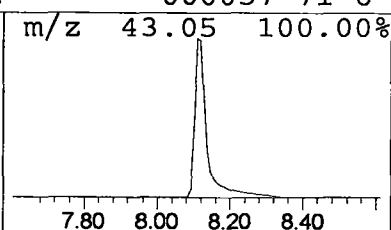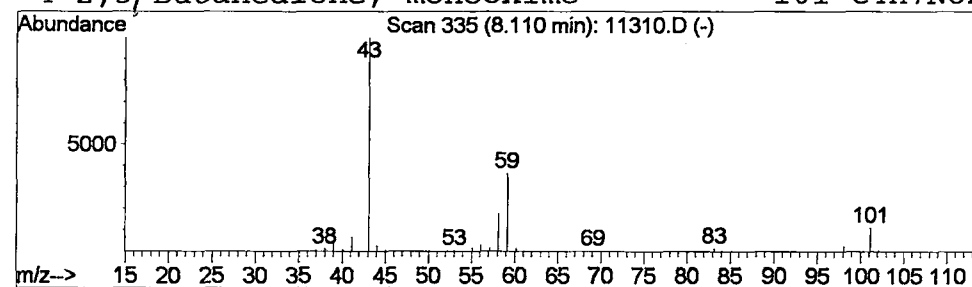

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 21 May 2002 11:26 pm
 Data File: C:\HPCHEM\1\DATA\MAY2102\11310.D
 Name: EXTRACT5/14
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.11	21.9	ug/l	1581030	ISTD01	12.14	2891160	40.0

11310.D GCMS0520.M Wed May 22 09:21:44 2002