

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 05/28/2002 Time: 14:49:27

Sample: AE11377
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 5/28/02 14:49 Ended: 5/28/02 14:49 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		86		10.0

Comments for Sample AE11377 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 05-28-2002 Time: 14:49:55

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Data File : C:\HPCHEM\1\DATA\MAY2102\11377.D
 Acq On : 22 May 2002 1:24 am
 Sample : EXTRACT5/14
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 22 9:15 2002

Vial: 26
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0520.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed May 22 09:03:22 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0520

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.14	152	429087	40.00	ug/l	0.00
10) Naphthalene-d8	15.78	136	1695111	40.00	ug/l	-0.02
17) Acenaphthene-d10	21.08	164	802499	40.00	ug/l	0.00
30) Phenanthrene-d10	25.52	188	1054648	40.00	ug/l	-0.02
38) Chrysene-d12	33.57	240	605951	40.00	ug/l	-0.04
44) Perylene-d12	37.79	264	402663	40.00	ug/l	-0.02

System Monitoring Compounds

28) TCMX	23.23	209	138708	34.39	ug/L	0.00
Spiked Amount	40.000		Recovery	=	85.97%	

Target Compounds

					Qvalue
2) N-nitrosodimethylamine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitrosodi-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.83	128	335	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.57	149	473	N.D.	
26) 4-Chlorophenylphenylether	23.23	204	606	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzene	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	23.22	168	131	N.D.	
32) 4-Bromophenylphenylether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	25.52	178	105	N.D.	

(#) = qualifier out of range (m) = manual integration

11377.D GCMS0520.M Wed May 22 09:16:07 2002

Page 1

Data File : C:\HPCHEM\1\DATA\MAY2102\11377.D

Vial: 26

Acq On : 22 May 2002 1:24 am

Operator:

Sample : EXTRACT5/14

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: May 22 9:15 2002

Quant Results File: GCMS0520.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed May 22 09:03:22 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0520

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
35) Anthracene	0.00	178	0	N.D.		
36) Di-n-butylphthalate	27.50	149	40039	1.16	ug/l	99
37) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.57	228	1466	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.80	149	715	N.D.		
43) Chrysene	33.57	228	1466	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	37.79	252	1466	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

11377.D GCMS0520.M Wed May 22 09:16:08 2002

Page 2

Quantitation Report

Data File : C:\HPCHEM\1\DATA\MAY2102\11377.D

Vial: 26

Acq On : 22 May 2002 1:24 am

Operator:

Sample : EXTRACT5/14

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: May 22 9:15 2002


Quant Results File: GCMS0520.RES

Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed May 22 09:03:22 2002

Response via : Initial Calibration

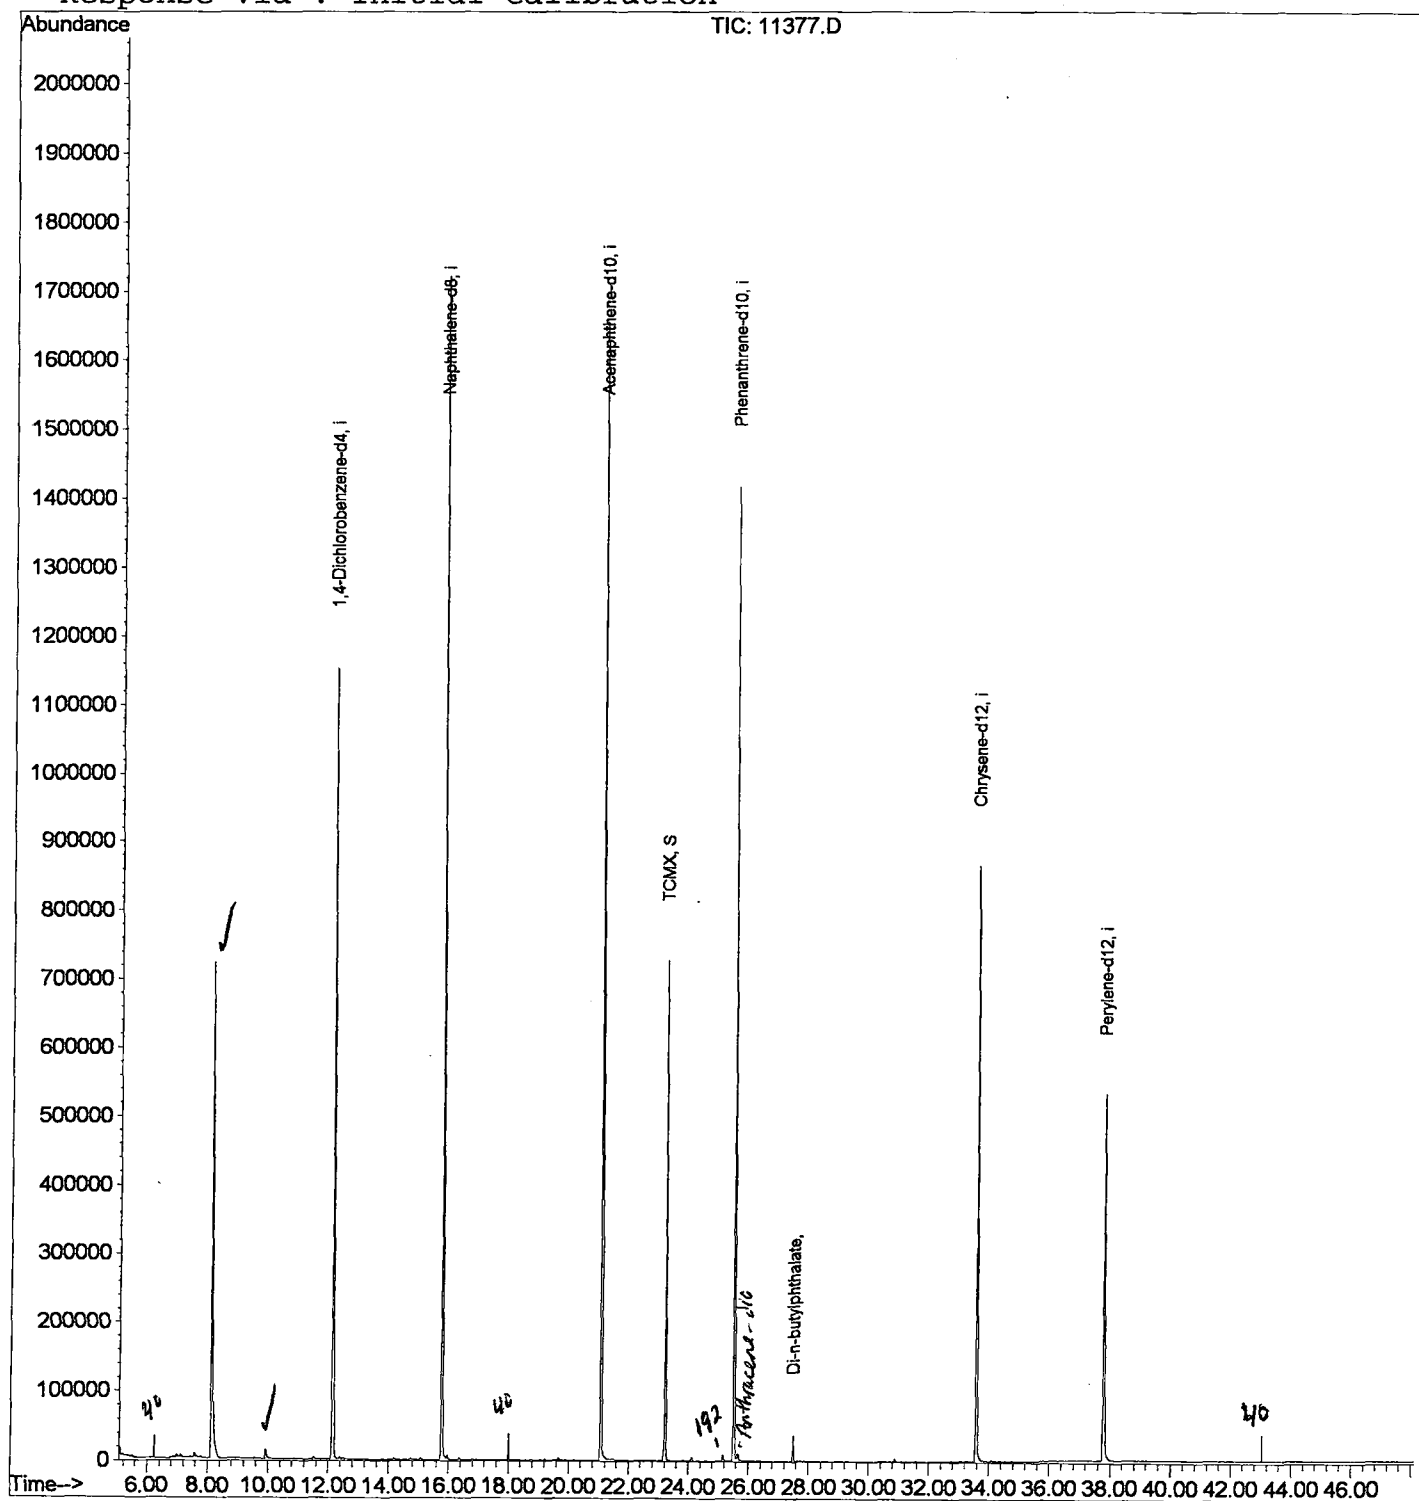

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\MAY2102\11377.D Vial: 26
 Acq On : 22 May 2002 1:24 am Operator:
 Sample : EXTRACT5/14 Inst : 209
 Misc : Multiplr: 1.00
 MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC


peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.115	331	335	341	rBV	720569	1402218	40.62%	7.345%
2	9.920	528	532	540	rBV	13751	34896	1.01%	0.183%
3	12.137	769	774	792	rBV	1151465	2645781	76.64%	13.858%
4	15.775	1165	1171	1188	rBV	1720323	3452042	100.00%	18.082%
5	21.081	1743	1750	1771	rBV	1654757	3446838	99.85%	18.054%
6	23.216	1976	1983	1994	rBV	725621	1508904	43.71%	7.904%
7	25.516	2228	2234	2244	rBV2	1416504	3004163	87.03%	15.736%
8	27.496	2445	2450	2457	rBV	37261	71758	2.08%	0.376%
9	33.571	3107	3113	3136	rBV2	864629	1981013	57.39%	10.376%
10	37.786	3565	3573	3593	rBV2	530172	1543914	44.72%	8.087%

Sum of corrected areas: 19091527

11377.D GCMS0520.M Wed May 22 09:22:06 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAY2102\11377.D
Operator :
Acquired : 22 May 2002 1:24 am using AcqMethod GCMS0520
Instrument : 209
Sample Name: EXTRACT5/14
Misc Info :
Vial Number: 26
Quant File : GCMS0520.RES (RTE Integrator)

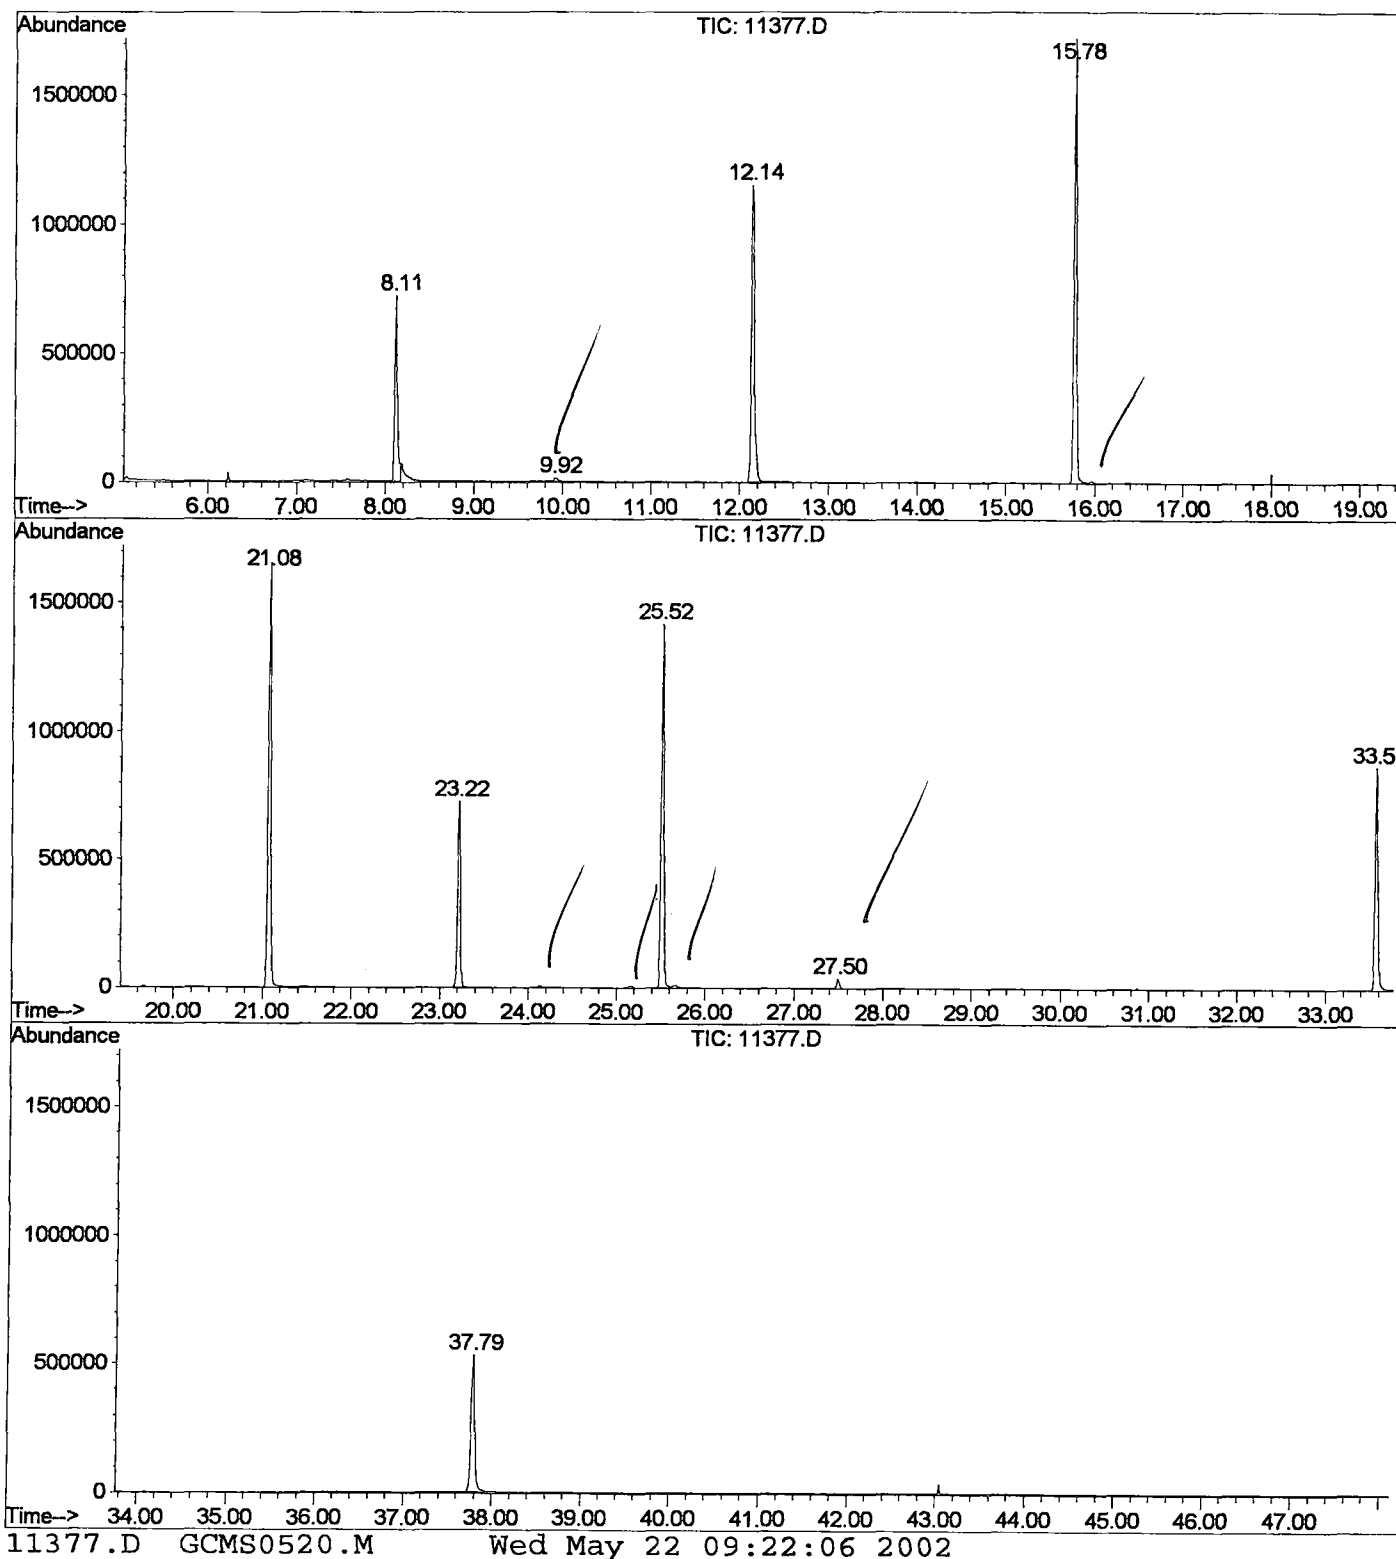

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAY2102\11377.D
Acq On : 22 May 2002 1:24 am
Sample : EXTRACT5/14
Misc :
MS Integration Params: LSCINT.P


Vial: 26
Operator:
Inst : 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-methyl Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.11	21.20 ug/l	1402220	1,4-Dichlorobenzene-d4	12.14

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72		
2	Acetone	58	C3H6O	000067-64-1	9		
3	CH2=CHCH2C(O)OCH3	100	C5H8O2	003724-55-8	9		
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	7		

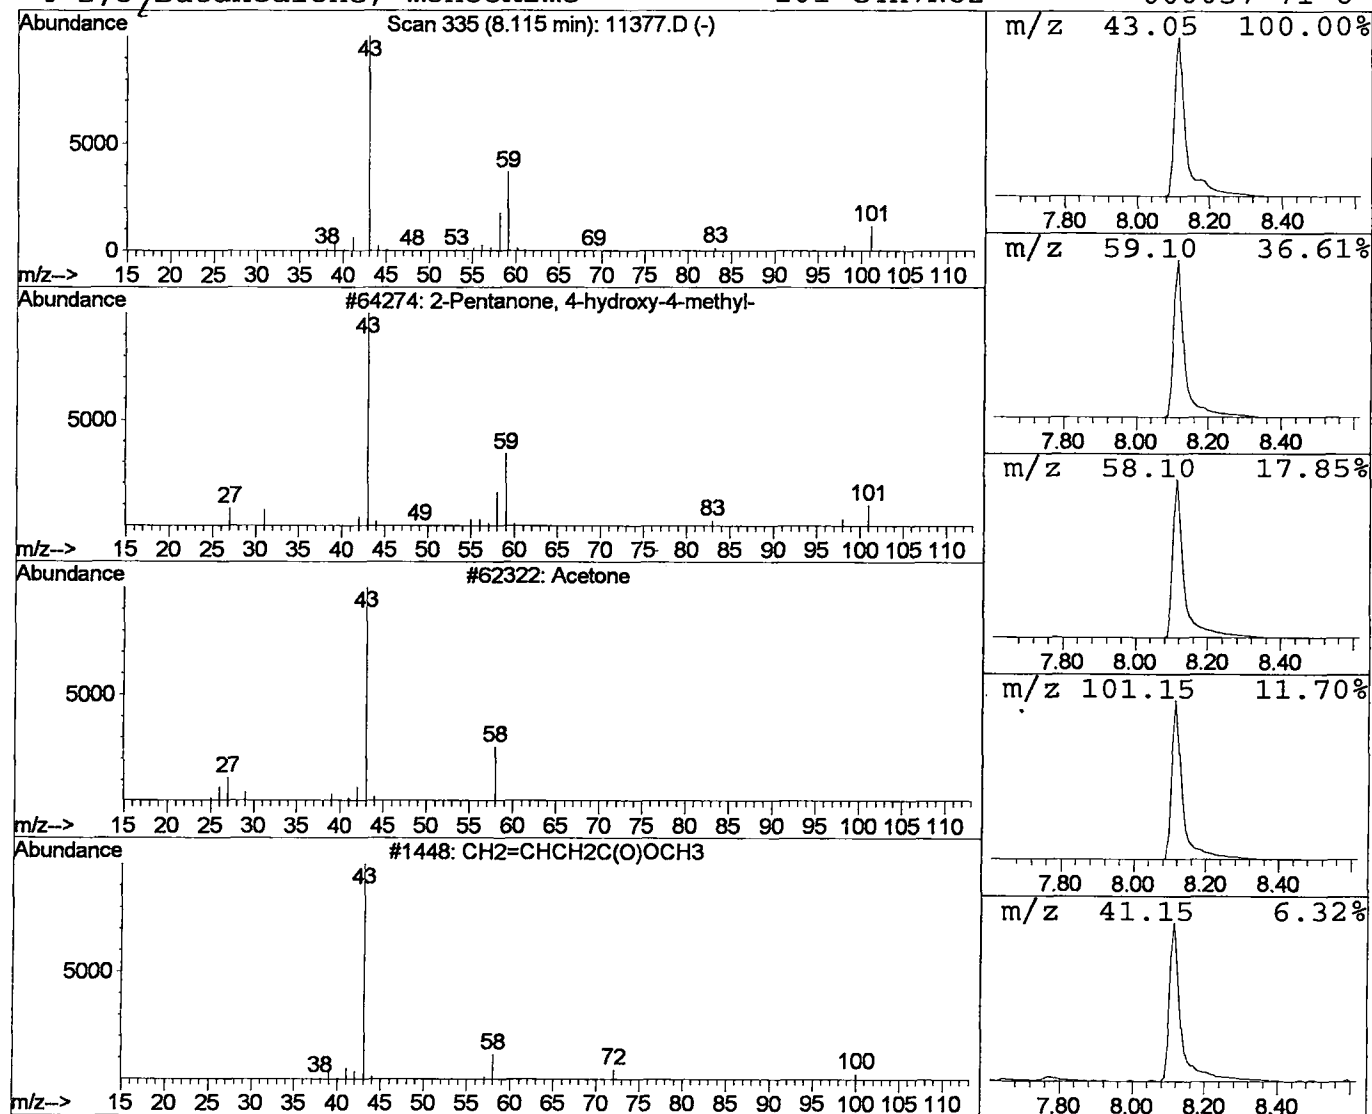

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAY2102\11377.D

Acq On : 22 May 2002 1:24 am

Sample : EXTRACT5/14

Misc :

MS Integration Params: LSCINT.P

Vial: 26

Operator:

Inst : 209

Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Library : C:\DATABASE\NBS75K.L

Peak Number 2 Acetone Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.92	0.53 ug/l	34896	1,4-Dichlorobenzene-d4	12.14

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Acetone	58	C3H6O	000067-64-1	9
2		3-Pyrrolidinol	87	C4H9NO	040499-83-0	9
3		1-Pentanamine	87	C5H13N	000110-58-7	9
4		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	9

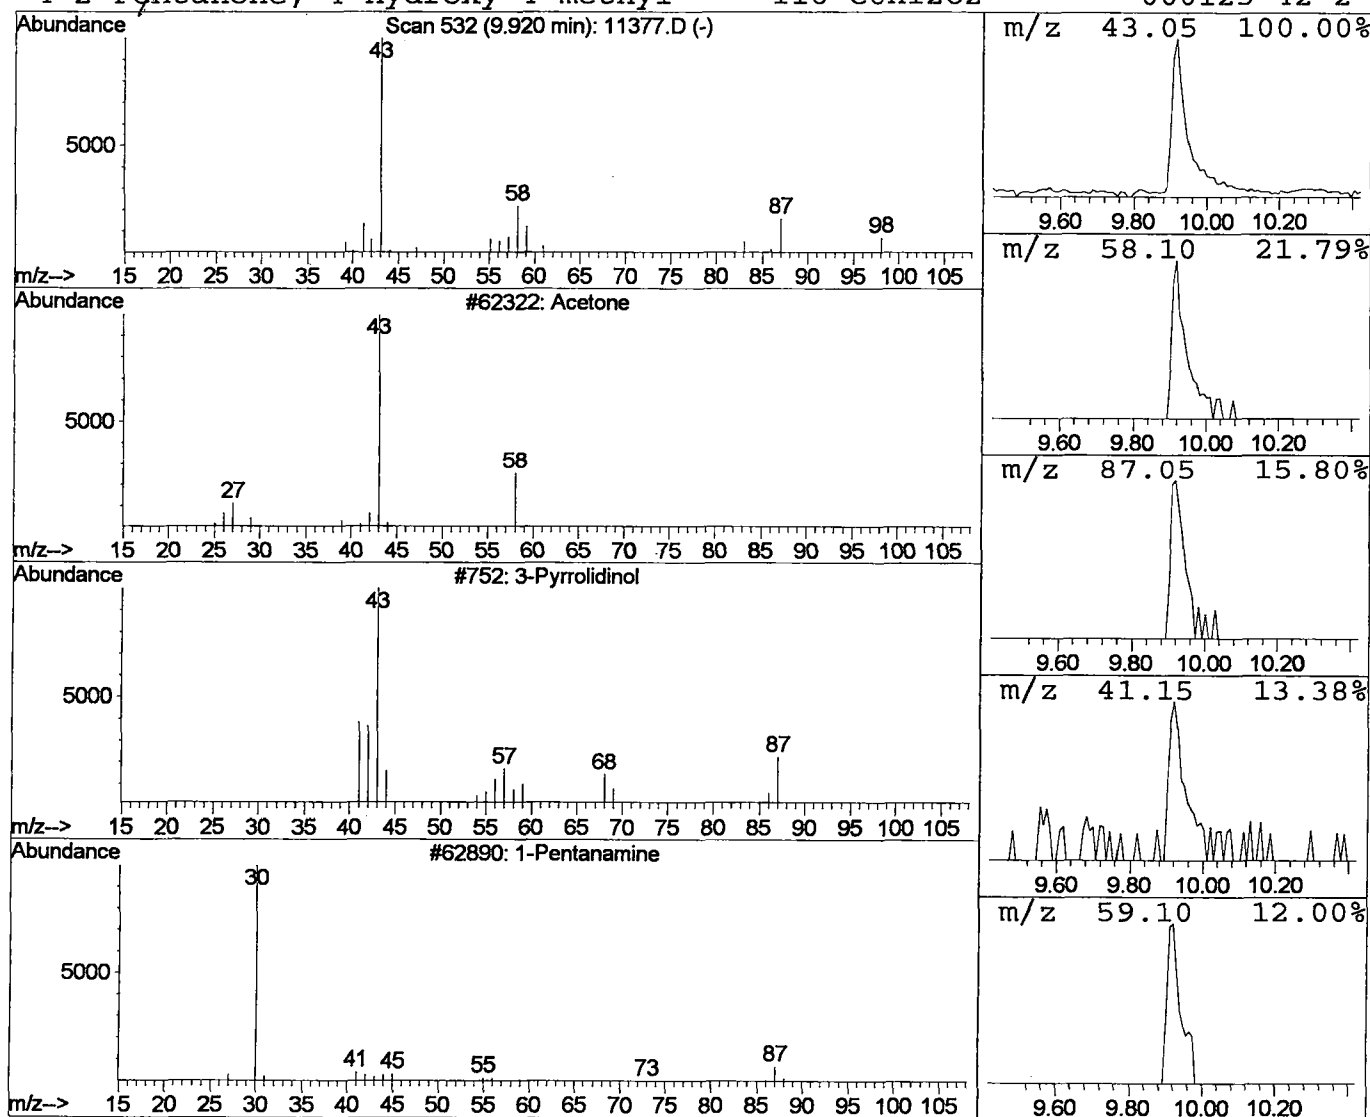

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 22 May 2002 1:24 am
Data File: C:\HPCHEM\1\DATA\MAY2102\11377.D
Name: EXTRACT5/14
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0520.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.11	21.2	ug/l	1402220	ISTD01	12.14	2645780	40.0
Acetone	9.92	0.5	ug/l	34896	ISTD01	12.14	2645780	40.0

11377.D GCMS0520.M Wed May 22 09:22:09 2002