


User: Bohlk, Ted
 Westchester Dept. of Labs & Research
 Date: 10/31/2001 Time: 11:42:58

Sample: AD23915
 Analysis: \$525 Organic Chemicals - 525.2
 Units: ug
 Started: 10/11/01 11:36 Ended: 10/23/01 11:36 Analyst: TB
 Result source: manual entry
 Page: 1

	Component Name	Vial	Result	Qualifier	MDL
1	Hexachlorocyclopentadiene		< MDL		0.10
2	Hexachlorobenzene		< MDL		0.10
3	Simazine		< MDL		0.40
4	Atrazine		< MDL		0.10
5	Alachlor		< MDL		0.20
6	bis(2-Ethylhexyl)adipate		< MDL		0.60
7	bis(2-Ethylhexyl)phthalate		0.72		0.60
8	Benzo(a)pyrene		< MDL		0.20
9	EPTC		< MDL		1.0
10	2,6-Dinitrotoluene		< MDL		2.0
11	2,4-Dinitrotoluene		< MDL		2.0
12	Molinate		< MDL		0.90
13	Terbacil		< MDL		2.0
14	Acetochlor		< MDL		2.0
15	Metribuzin		< MDL		0.15
16	Metolachlor		< MDL		0.75
17	Butachlor		< MDL		0.40
18	4,4-DDE		< MDL		0.80
19	Surr_1,3-Dimethyl-2-nitrobenze		5.2		1.0
20	Surr_Triphenyl phosphate		6.1		1.0
21	Surr_Perylene-d12		4.4		1.0

Chromatogram Plot File: E:\23915D Date: Oct-24-1991 06:40:03
 Comment: BOHLK; METHOD 525; INST 204; 10/23/01; SAMPLE 23915
 Scan No: 1 Retention Time: 0:01 RIC: 0 Mass Range: 0 - 0
 Plotted: 1 to 1860 Range: 1 to 1860 100% = 10199373

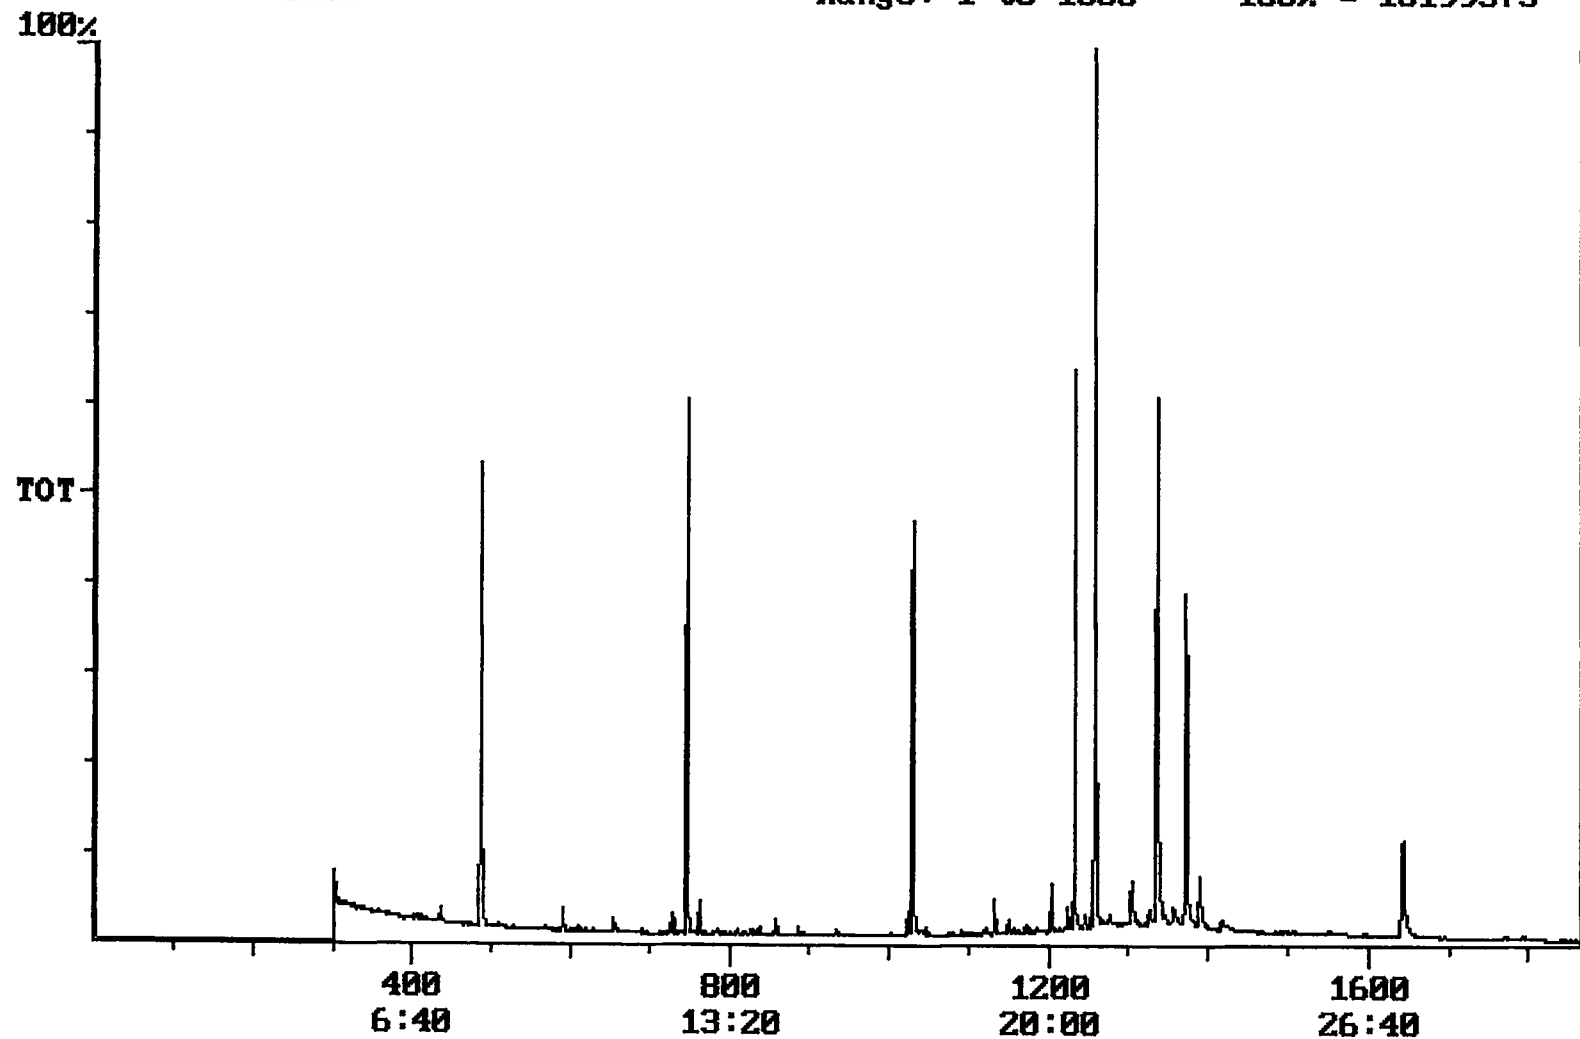

Integration Report Quanfile: 23915D Quan Entries: 14
 Comment: BOHLK; METHOD 525; INST 204; 10/23/01; SAMPLE 23915
 Sorted via: Entry Number ↑

No	Name of Compound	R Time	Scan#	Mode	Peak Area	Pk Height
1	acenaphthene d-10 (IS)	12:27	747	Auto	2,285,454	1,474,637
2	phenanthrene d-10 (IS)	17:10	1030	Auto	3,666,897	1,545,909
3	chrysene d-12 (IS)	22:52	1372	Auto	2,505,395	1,099,542
4	p-terphenyl d-14 (IS)	20:58	1258	Auto	4,465,783	3,161,833
5	acenaphthene d-10 (SURR)	12:27	747	Auto	2,285,454	1,474,637
6	phenanthrene d-10 (SURR)	17:10	1030	Auto	3,666,897	1,545,909
7	chrysene d-12 (SURR)	22:52	1372	Auto	2,505,395	1,099,542
8	1,3-dimethyl-2-nitrobenzene	8:07	487	Auto	1,403,647	831,357
9	triphenyl phosphate (S)	22:15	1335	Auto	2,012,494	941,392
10	perylene d-12 (SURR)	27:22	1642	Auto	1,373,653	254,289
11	bis(2-ethylhexyl)adipate	22:15	1335	Auto	28,746	8,868
12	bis(2-ethylhexyl)phthalate	23:10	1390	Auto	607,789	169,521
13	2,6-dinitrotoluene	12:06	726	Auto	24,180	12,944
14	2,4-dinitrotoluene	13:14	794	Auto	2,213	1,144

Quantitation Report Quanfile: 23915D Quan Entries: 14
 Comment: BOHLK; METHOD 525; INST 204; 10/23/01; SAMPLE 23915
 Sorted via: Entry Number ↑ (S) = Standard

Cal	Name of Compound	S	Scan#	R Time	Me	Calc Amt(A)	Units
1	acenaphthene d-10 (IS)	I	747	12:27	BB	5.000	UG/L
2	phenanthrene d-10 (IS)	I	1030	17:10	BV	5.000	UG/L
3	chrysene d-12 (IS)	I	1372	22:52	BB	5.000	UG/L
4	p-terphenyl d-14 (IS)	I	1258	20:58	BV	5.000	UG/L
5	acenaphthene d-10 (SURR)	A	747	12:27	BB	3.538	UG/L
6	phenanthrene d-10 (SURR)	A	1030	17:10	BV	3.919	UG/L
7	chrysene d-12 (SURR)	A	1372	22:52	BB	3.915	UG/L
8	1,3-dimethyl-2-nitrobenzene	A	487	8:07	BV	5.233	UG/L
9	triphenyl phosphate (S)	A	1335	22:15	BB	6.072	UG/L
10	perylene d-12 (SURR)	A	1642	27:22	BB	4.353	UG/L
16	bis(2-ethylhexyl)adipate	A	1335	22:15	MM	0.055	UG/L
17	bis(2-ethylhexyl)phthalate	A	1390	23:10	VB	0.716	UG/L
20	2,6-dinitrotoluene	A	726	12:06	BB	0.162	UG/L
21	2,4-dinitrotoluene	A	794	13:14	BB	0.013	UG/L

Reviewed IS/ Surrogates

Comments for Sample AD23915 - Analysis \$525

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 11-03-2001 Time: 13:01:26

The recoveries for five of the eighteen compounds in the MDL and LCS Standards were outside of their acceptance ranges. Recoveries for two of the eighteen compounds in the Spiked Sample were below their acceptance ranges. The Spiked Duplicate Sample was lost due to a laboratory accident. The level of bis(2-Ethylhexyl)phthalate in the Laboratory Blank was 24 ug/L due to a laboratory accident.