


User: Azzo Murad, Nehla
Westchester Dept. of Labs & Research
Date: 11/07/2001 Time: 10:20:34

Sample: AD24135
Analysis: \$525 Organic Chemicals - 525.2
Units: ug
Started: 10/15/01 09:43 Ended: 10/25/01 09:43 Analyst: NAM
Result source: manual entry
Page: 1

	Component Name	Vial	Result	Qualifier	MDL
1	Hexachlorocyclopentadiene		< MDL		0.10
2	Hexachlorobenzene		< MDL		0.10
3	Simazine		< MDL		0.40
4	Atrazine		< MDL		0.10
5	Alachlor		< MDL		0.20
6	bis(2-Ethylhexyl)adipate		< MDL		0.60
7	bis(2-Ethylhexyl)phthalate		< MDL		0.60
8	Benzo(a)pyrene		< MDL		0.20
9	EPTC		< MDL		1.0
10	2,6-Dinitrotoluene		< MDL		2.0
11	2,4-Dinitrotoluene		< MDL		2.0
12	Molinate		< MDL		0.90
13	Terbacil		< MDL		2.0
14	Acetochlor		< MDL		2.0
15	Metribuzin		< MDL		0.15
16	Metolachlor		< MDL		0.75
17	Butachlor		< MDL		0.40
18	4,4-DDE		< MDL		0.80
19	Surr_1,3-Dimethyl-2-nitrobenze		4.9		1.0
20	Surr_Triphenyl phosphate		5.7		1.0
21	Surr_Perylene-d12		4.3		1.0

Chromatogram Plot File: E:\24135A Date: Oct-25-1991 22:37:43
Comment: BOHLK; METHOD 525; INST 204; 10/25/01; SAMPLE 24135
Scan No: 1 Retention Time: 0:01 RIC: 0 Mass Range: 0 - 0
Plotted: 1 to 1860 Range: 1 to 1860 100% = 9808082

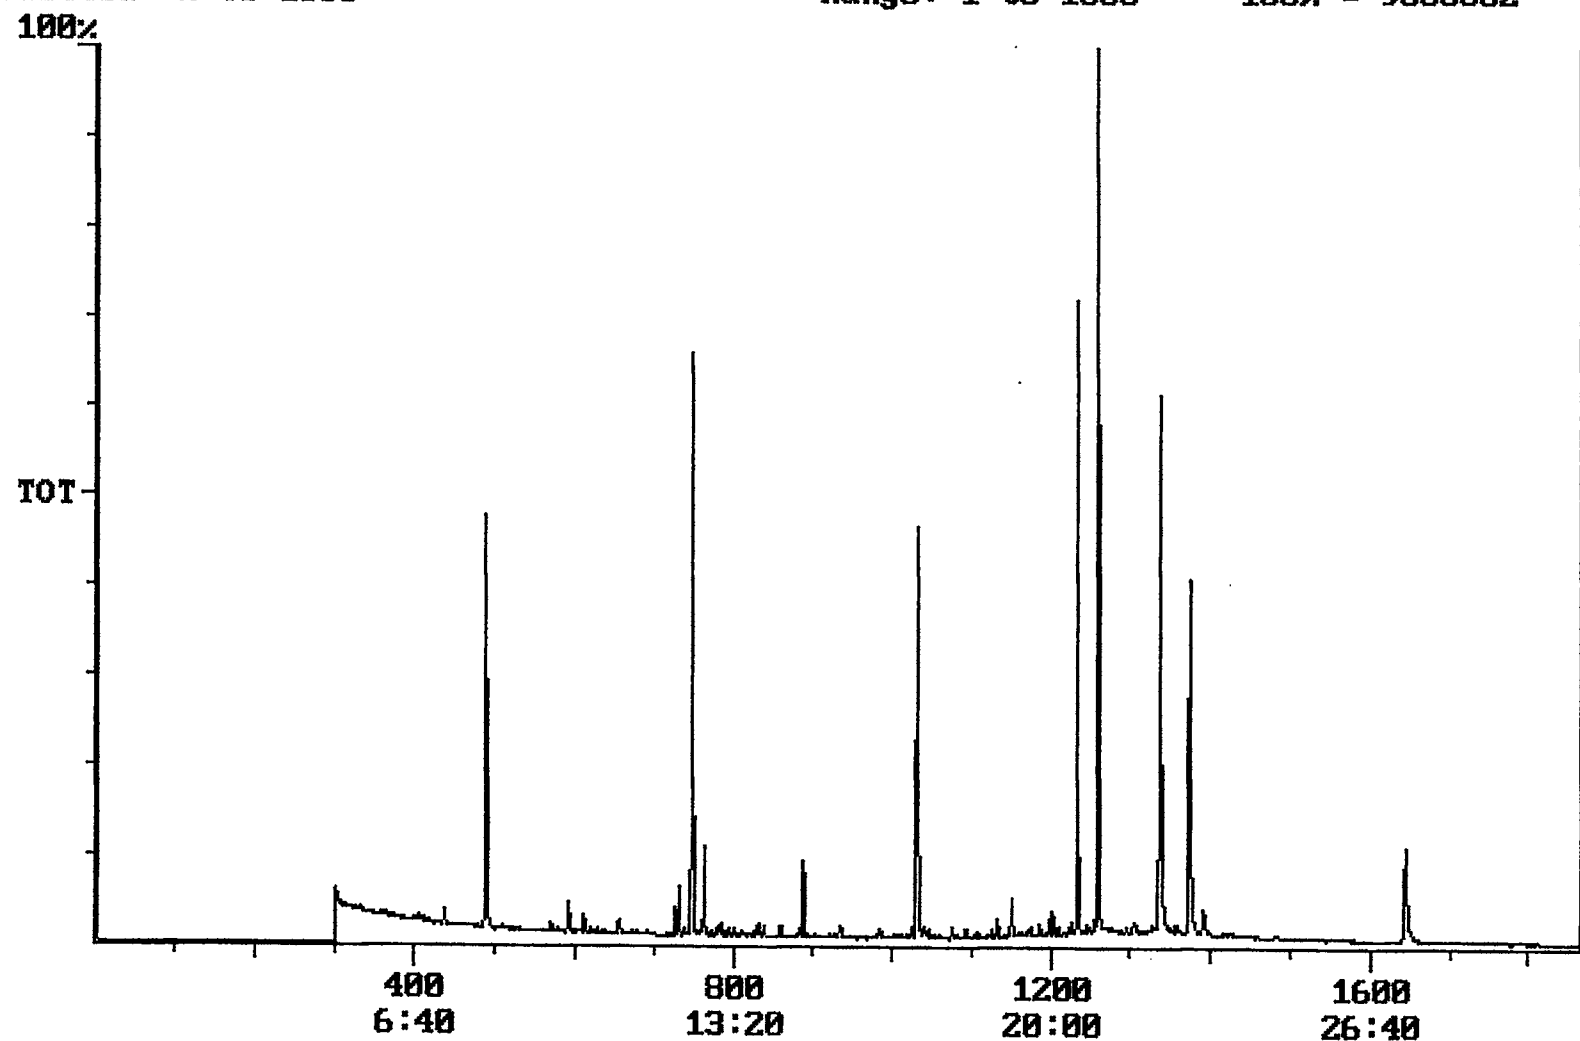

Integration Report Quanfile: 24135A Quan Entries: 14
 Comment: BOHLK; METHOD 525; INST 204; 10/25/01; SAMPLE 24135
 Sorted via: Entry Number ↑

No	Name of Compound	R Time	Scan#	Mode	Peak Area	Pk Height
1	acenaphthene d-10 (IS)	12:28	748	Auto	2,464,794	1,589,615
2	phenanthrene d-10 (IS)	17:11	1031	Auto	3,601,469	1,503,008
3	chrysene d-12 (IS)	22:53	1373	Auto	2,571,442	1,152,242
4	p-terphenyl d-14 (IS)	20:59	1259	Auto	4,055,053	2,989,008
5	acenaphthene d-10 (SURR)	12:28	748	Auto	2,464,794	1,589,615
6	phenanthrene d-10 (SURR)	17:11	1031	Auto	3,601,469	1,503,008
7	chrysene d-12 (SURR)	22:53	1373	Auto	2,571,442	1,152,242
8	1,3-dimethyl-2-nitrobenzene	8:08	488	Auto	1,415,654	697,887
9	triphenyl phosphate (S)	22:16	1336	Auto	1,924,723	904,646
10	perylene d-12 (SURR)	27:23	1643	Auto	1,380,558	259,871
11	bis(2-ethylhexyl)adipate	22:16	1336	Auto	34,486	9,615
12	bis(2-ethylhexyl)phthalate	23:11	1391	Auto	329,793	77,883
13	2,6-dinitrotoluene	12:07	727	Auto	72,524	38,103
14	2,4-dinitrotoluene	13:15	795	Auto	8,884	3,412

Quantitation Report Quanfile: 24135A Quan Entries: 14
 Comment: BOHLK; METHOD 525; INST 204; 10/25/01; SAMPLE 24135
 Sorted via: Entry Number ↑ (S) = Standard

Cal	Name of Compound	S	Scan#	R Time	Me	Calc Amt(A)	Units
1	acenaphthene d-10 (IS)	I	748	12:28	BB	5.000	UG/L
2	phenanthrene d-10 (IS)	I	1031	17:11	BV	5.000	UG/L
3	chrysene d-12 (IS)	I	1373	22:53	BB	5.000	UG/L
4	p-terphenyl d-14 (IS)	I	1259	20:59	BB	5.000	UG/L
5	acenaphthene d-10 (SURR)	A	748	12:28	BB	4.202	UG/L
6	phenanthrene d-10 (SURR)	A	1031	17:11	BV	4.239	UG/L
7	chrysene d-12 (SURR)	A	1373	22:53	BB	4.425	UG/L
8	1,3-dimethyl-2-nitrobenzene	A	488	8:08	BV	4.894	UG/L
9	triphenyl phosphate (S)	A	1336	22:16	BB	5.658	UG/L
10	perylene d-12 (SURR)	A	1643	27:23	BB	4.263	UG/L
16	bis(2-ethylhexyl)adipate	A	1336	22:16	MM	0.065	UG/L
17	bis(2-ethylhexyl)phthalate	A	1391	23:11	VV	0.375	UG/L
20	2,6-dinitrotoluene	A	727	12:07	BB	0.447	UG/L
21	2,4-dinitrotoluene	A	795	13:15	BB	0.047	UG/L

Reviewed IS/surrogates

Comments for Sample AD24135 - Analysis \$525

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 11-14-2001 Time: 11:40:11

The recovery for bis(2-Ethylhexyl)phthalate in the MDL Standard was above its acceptance range. This is probably due to laboratory contamination.