


User: Azzo Murad, Nehla
Westchester Dept. of Labs & Research
Date: 11/07/2001 Time: 10:22:19

Sample: AD24216
Analysis: \$525 Organic Chemicals - 525.2
Units: ug
Started: 10/15/01 09:43 Ended: 10/25/01 09:43 Analyst: NAM
Result source: manual entry
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Hexachlorocyclopentadiene		< MDL		0.10
2	Hexachlorobenzene		< MDL		0.10
3	Simazine		< MDL		0.40
4	Atrazine		< MDL		0.10
5	Alachlor		< MDL		0.20
6	bis(2-Ethylhexyl)adipate		< MDL		0.60
7	bis(2-Ethylhexyl)phthalate		< MDL		0.60
8	Benzo(a)pyrene		< MDL		0.20
9	EPTC		< MDL		1.0
10	2,6-Dinitrotoluene		< MDL		2.0
11	2,4-Dinitrotoluene		< MDL		2.0
12	Molinate		< MDL		0.90
13	Terbacil		< MDL		2.0
14	Acetochlor		< MDL		2.0
15	Metribuzin		< MDL		0.15
16	Metolachlor		< MDL		0.75
17	Butachlor		< MDL		0.40
18	4,4-DDE		< MDL		0.80
19	Surr_1,3-Dimethyl-2-nitrobenze		5.3		1.0
20	Surr_Triphenyl phosphate		5.2		1.0
21	Surr_Perylene-d12		4.1		1.0

Chromatogram Plot File: E:\24216D Date: Oct-26-1991 00:21:04
Comment: BOHLK; METHOD 525; INST 204; 10/25/01; SAMPLE 24216
Scan No: 1 Retention Time: 0:01 RIC: 0 Mass Range: 0 - 0
Plotted: 1 to 1859 Range: 1 to 1859 100% = 8685218

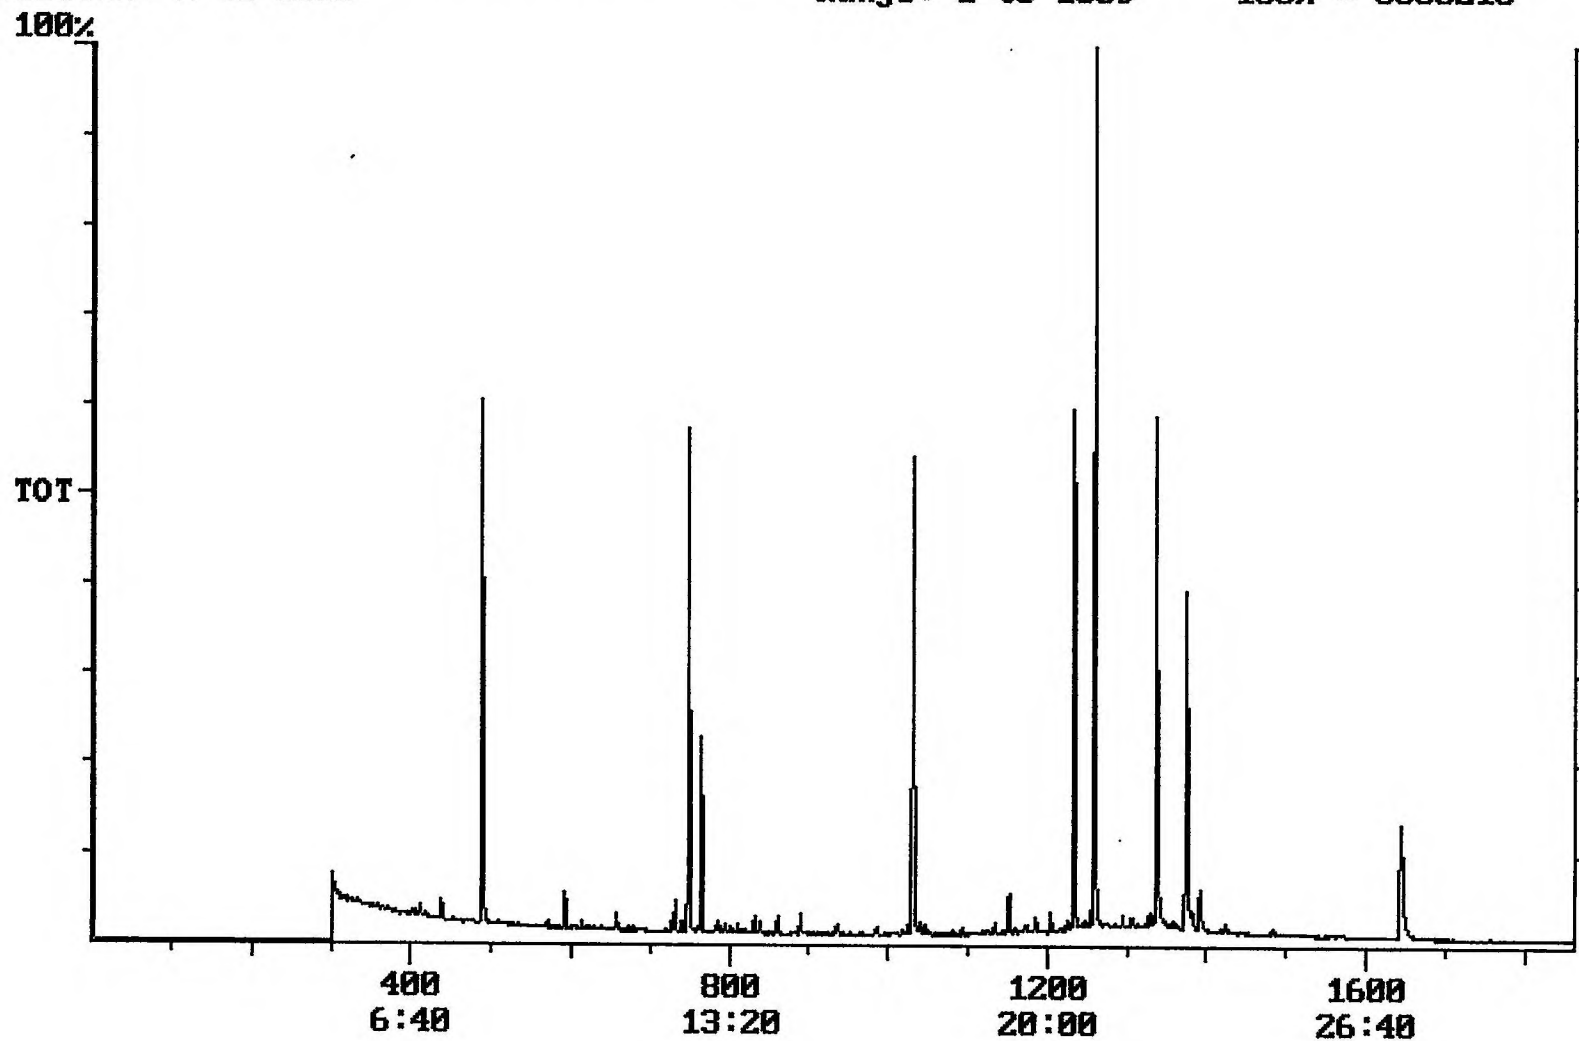

Integration Report

Quanfile: 24216D

Quan Entries: 15

Comment: BOHLK; METHOD 525; INST 204; 10/25/01; SAMPLE 24216

Sorted via: Entry Number ↑

No	Name of Compound	R Time	Scan#	Mode	Peak Area	Pk Height
1	acenaphthene d-10(IS)	12:28	748	Auto	2,248,066	1,162,352
2	phenanthrene d-10 (IS)	17:11	1031	Auto	3,468,253	1,577,152
3	chrysene d-12(IS)	22:53	1373	Auto	2,625,833	999,992
4	p-terphenyl d-14(IS)	20:59	1259	Auto	4,082,351	2,771,451
5	acenaphthene d-10(SURR	12:28	748	Auto	2,248,066	1,162,352
6	phenanthrene d-10(SURR	17:11	1031	Auto	3,468,253	1,577,152
7	chrysene d-12 (SURR)	22:53	1373	Auto	2,625,833	999,992
8	1,3-dimethyl-2-nitrobe	8:08	488	Auto	1,407,917	819,583
9	triphenyl phosphate (S	22:16	1336	Auto	1,794,573	741,655
10	perylene d-12 (SURR)	27:24	1644	Auto	1,367,021	268,356
11	hexachlorocyclopentadi	10:19	619	Auto	1,729	1,729
12	bis(2-ethylhexyl)adipa	22:16	1336	Auto	35,337	6,930
13	bis(2-ethylhexyl)phtha	23:11	1391	Auto	359,637	104,851
14	2,6-dinitrotoluene	12:08	728	Auto	36,421	17,571
15	2,4-dinitrotoluene	13:05	785	Auto	1,192	1,192

Quantitation Report

Quanfile: 24216D

Quan Entries: 15

Comment: BOHLK; METHOD 525; INST 204; 10/25/01; SAMPLE 24216

Sorted via: Entry Number ↑

(S) = Standard

Cal	Name of Compound	S	Scan#	R Time	Me	Calc Amt(A)	Units
1	acenaphthene d-10(IS)	I	748	12:28	BV	5.000	UG/L
2	phenanthrene d-10 (IS)	I	1031	17:11	BV	5.000	UG/L
3	chrysene d-12(IS)	I	1373	22:53	BB	5.000	UG/L
4	p-terphenyl d-14(IS)	I	1259	20:59	BB	5.000	UG/L
5	acenaphthene d-10(SURR	A	748	12:28	BV	3.807	UG/L
6	phenanthrene d-10(SURR	A	1031	17:11	BV	4.055	UG/L
7	chrysene d-12 (SURR)	A	1373	22:53	BB	4.488	UG/L
8	1,3-dimethyl-2-nitroben	A	488	8:08	BV	5.336	UG/L
9	triphenyl phosphate (S	A	1336	22:16	BB	5.166	UG/L
10	perylene d-12 (SURR)	A	1644	27:24	BB	4.134	UG/L
11	hexachlorocyclopentadi	A	619	10:19	BB	0.018	UG/L
16	bis(2-ethylhexyl)adipa	A	1336	22:16	MM	0.065	UG/L
17	bis(2-ethylhexyl)phtha	A	1391	23:11	VB	0.401	UG/L
20	2,6-dinitrotoluene	A	728	12:08	BB	0.248	UG/L
21	2,4-dinitrotoluene	A	785	13:05	BB	0.007	UG/L

Reviewed 10/25/01

Comments for Sample AD24216 - Analysis \$525

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 11-14-2001 Time: 11:54:54

The recovery for bis(2-Ethylhexyl)phthalate in the MDL Standard was above its acceptance range. This is probably due to laboratory contamination.