


User: Azzo Murad, Nehla
Westchester Dept. of Labs & Research
Date: 11/07/2001 Time: 10:22:34

Sample: AD24217
Analysis: \$525 Organic Chemicals - 525.2
Units: ug
Started: 10/15/01 09:43 Ended: 10/25/01 09:43 Analyst: NAM
Result source: manual entry
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Hexachlorocyclopentadiene		< MDL		0.10
2	Hexachlorobenzene		< MDL		0.10
3	Simazine		< MDL		0.40
4	Atrazine		< MDL		0.10
5	Alachlor		< MDL		0.20
6	bis(2-Ethylhexyl)adipate		< MDL		0.60
7	bis(2-Ethylhexyl)phthalate		0.78		0.60
8	Benzo(a)pyrene		< MDL		0.20
9	EPTC		< MDL		1.0
10	2,6-Dinitrotoluene		< MDL		2.0
11	2,4-Dinitrotoluene		< MDL		2.0
12	Molinate		< MDL		0.90
13	Terbacil		< MDL		2.0
14	Acetochlor		< MDL		2.0
15	Metribuzin		< MDL		0.15
16	Metolachlor		< MDL		0.75
17	Butachlor		< MDL		0.40
18	4,4-DDE		< MDL		0.80
19	Surr_1,3-Dimethyl-2-nitrobenze		5.3		1.0
20	Surr_Triphenyl phosphate		5.8		1.0
21	Surr_Perylene-d12		4.2		1.0

Chromatogram Plot File: E:\24217E Date: Oct-26-1991 00:55:32
Comment: BOHLK; METHOD 525; INST 204; 10/25/01; SAMPLE 24217
Scan No: 1 Retention Time: 0:01 RIC: 0 Mass Range: 0 - 0
Plotted: 1 to 1860 Range: 1 to 1860 100% = 7310936

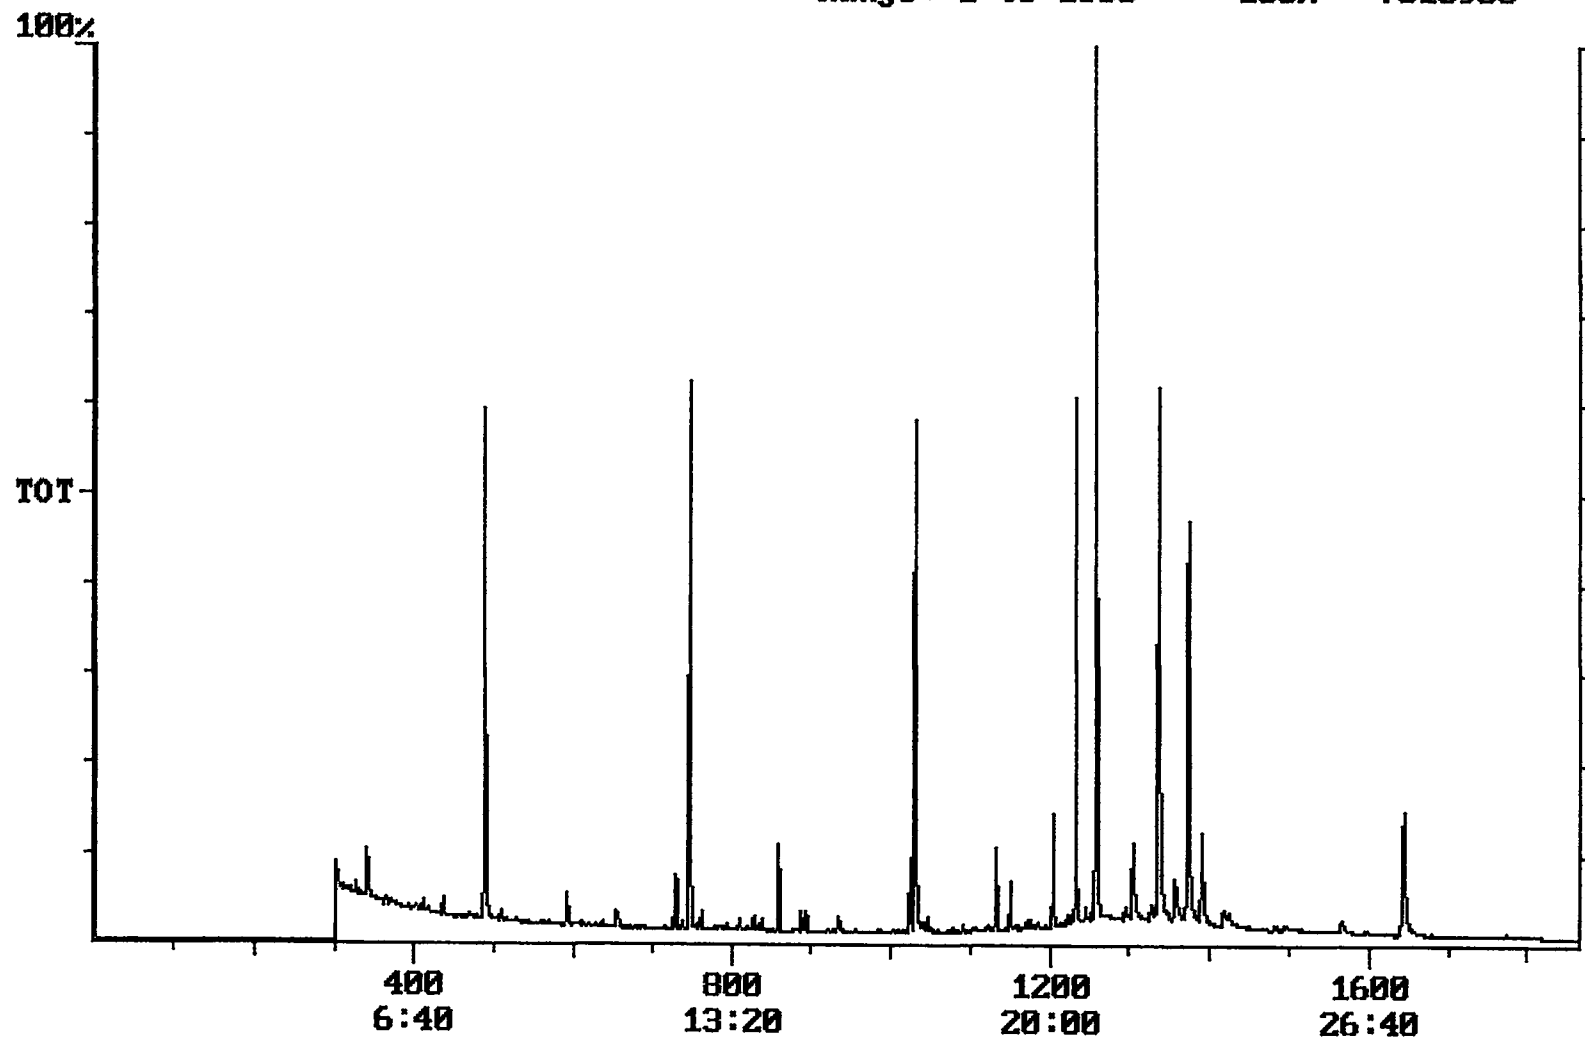

Integration Report Quanfile: 24217E Quan Entries: 15
 Comment: BOHLK; METHOD 525; INST 204; 10/25/01; SAMPLE 24217
 Sorted via: Entry Number ↑

No	Name of Compound	R Time	Scan#	Mode	Peak Area	Pk Height
1	acenaphthene d-10(IS)	12:28	748	Auto	2,141,030	1,012,087
2	phenanthrene d-10 (IS)	17:10	1030	Auto	3,339,409	1,449,838
3	chrysene d-12(IS)	22:53	1373	Auto	2,349,540	884,095
4	p-terphenyl d-14(IS)	20:58	1258	Auto	3,848,613	2,127,454
5	acenaphthene d-10(SURR)	12:28	748	Auto	2,141,030	1,012,087
6	phenanthrene d-10(SURR)	17:10	1030	Auto	3,339,409	1,449,838
7	chrysene d-12 (SURR)	22:53	1373	Auto	2,349,540	884,095
8	1,3-dimethyl-2-nitrobenzene	8:07	487	Auto	1,335,763	634,068
9	triphenyl phosphate (S)	22:16	1336	Auto	1,796,837	633,734
10	perylene d-12 (SURR)	27:23	1643	Auto	1,251,226	251,013
11	hexachlorocyclopentadiene	10:18	618	Auto	3,302	2,155
12	bis(2-ethylhexyl)adipate	22:16	1336	Auto	29,727	6,106
13	bis(2-ethylhexyl)phthalate	23:10	1390	Auto	616,937	207,860
14	2,6-dinitrotoluene	12:07	727	Auto	19,192	10,672
15	2,4-dinitrotoluene	13:14	794	Auto	6,209	3,350

Quantitation Report

Quanfile: 24217E

Quan Entries: 15

Comment: BOHLK; METHOD 525; INST 204; 10/25/01; SAMPLE 24217

Sorted via: Entry Number ↑

(S) = Standard

Cal	Name of Compound	S	Scan#	R Time	Me	Calc Amt(A)	Units
1	acenaphthene d-10(IS)	I	748	12:28	BB	5.000	UG/L
2	phenanthrene d-10 (IS)	I	1030	17:10	BV	5.000	UG/L
3	chrysene d-12(IS)	I	1373	22:53	BB	5.000	UG/L
4	p-terphenyl d-14(IS)	I	1258	20:58	BB	5.000	UG/L
5	acenaphthene d-10(SURR	A	748	12:28	BB	3.846	UG/L
6	phenanthrene d-10(SURR	A	1030	17:10	BV	4.142	UG/L
7	chrysene d-12 (SURR)	A	1373	22:53	BB	4.260	UG/L
8	1,3-dimethyl-2-nitroben	A	487	8:07	BV	5.316	UG/L
9	triphenyl phosphate (S	A	1336	22:16	BB	5.781	UG/L
10	perylene d-12 (SURR)	A	1643	27:23	BB	4.228	UG/L
11	hexachlorocyclopentadi	A	618	10:18	BB	0.035	UG/L
16	bis(2-ethylhexyl)adipa	A	1336	22:16	MM	0.061	UG/L
17	bis(2-ethylhexyl)phtha	A	1390	23:10	VV	0.776	UG/L
20	2,6-dinitrotoluene	A	727	12:07	BB	0.138	UG/L
21	2,4-dinitrotoluene	A	794	13:14	BB	0.038	UG/L

Reviewed IS/surrogates

Comments for Sample AD24217 - Analysis \$525

Westchester Dept. of Labs & Research

User: Vinci, David L.

Date: 11-14-2001 Time: 11:59:11

The recovery for bis(2-Ethylhexyl)phthalate in the MDL Standard was above its acceptance range. This is probably due to laboratory contamination.