


User: Azzo Murad, Nehla
Westchester Dept. of Labs & Research
Date: 11/07/2001 Time: 10:58:57

Sample: AD24237
Analysis: \$525 Organic Chemicals - 525.2
Units: ug
Started: 10/15/01 10:56 Ended: 10/25/01 10:56 Analyst: NAM
Result source: manual entry
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Hexachlorocyclopentadiene		< MDL		0.10
2	Hexachlorobenzene		< MDL		0.10
3	Simazine		< MDL		0.40
4	Atrazine		< MDL		0.10
5	Alachlor		< MDL		0.20
6	bis(2-Ethylhexyl)adipate		< MDL		0.60
7	bis(2-Ethylhexyl)phthalate		< MDL		0.60
8	Benzo(a)pyrene		< MDL		0.20
9	EPTC		< MDL		1.0
10	2,6-Dinitrotoluene		< MDL		2.0
11	2,4-Dinitrotoluene		< MDL		2.0
12	Molinate		< MDL		0.90
13	Terbacil		< MDL		2.0
14	Acetochlor		< MDL		2.0
15	Metribuzin		< MDL		0.15
16	Metolachlor		< MDL		0.75
17	Butachlor		< MDL		0.40
18	4,4-DDE		< MDL		0.80
19	Surr_1,3-Dimethyl-2-nitrobenze		5.6		1.0
20	Surr_Triphenyl phosphate		5.8		1.0
21	Surr_Perylene-d12		4.3		1.0

Chromatogram Plot File: F:\24237J Date: Oct-26-1991 03:47:46
Comment: BOHLK; METHOD 525; INST 204; 10/25/01; SAMPLE 24237
Scan No: 1 Retention Time: 0:01 RIC: 0 Mass Range: 0 - 0
Plotted: 1 to 1859 Range: 1 to 1859 100% = 9889920

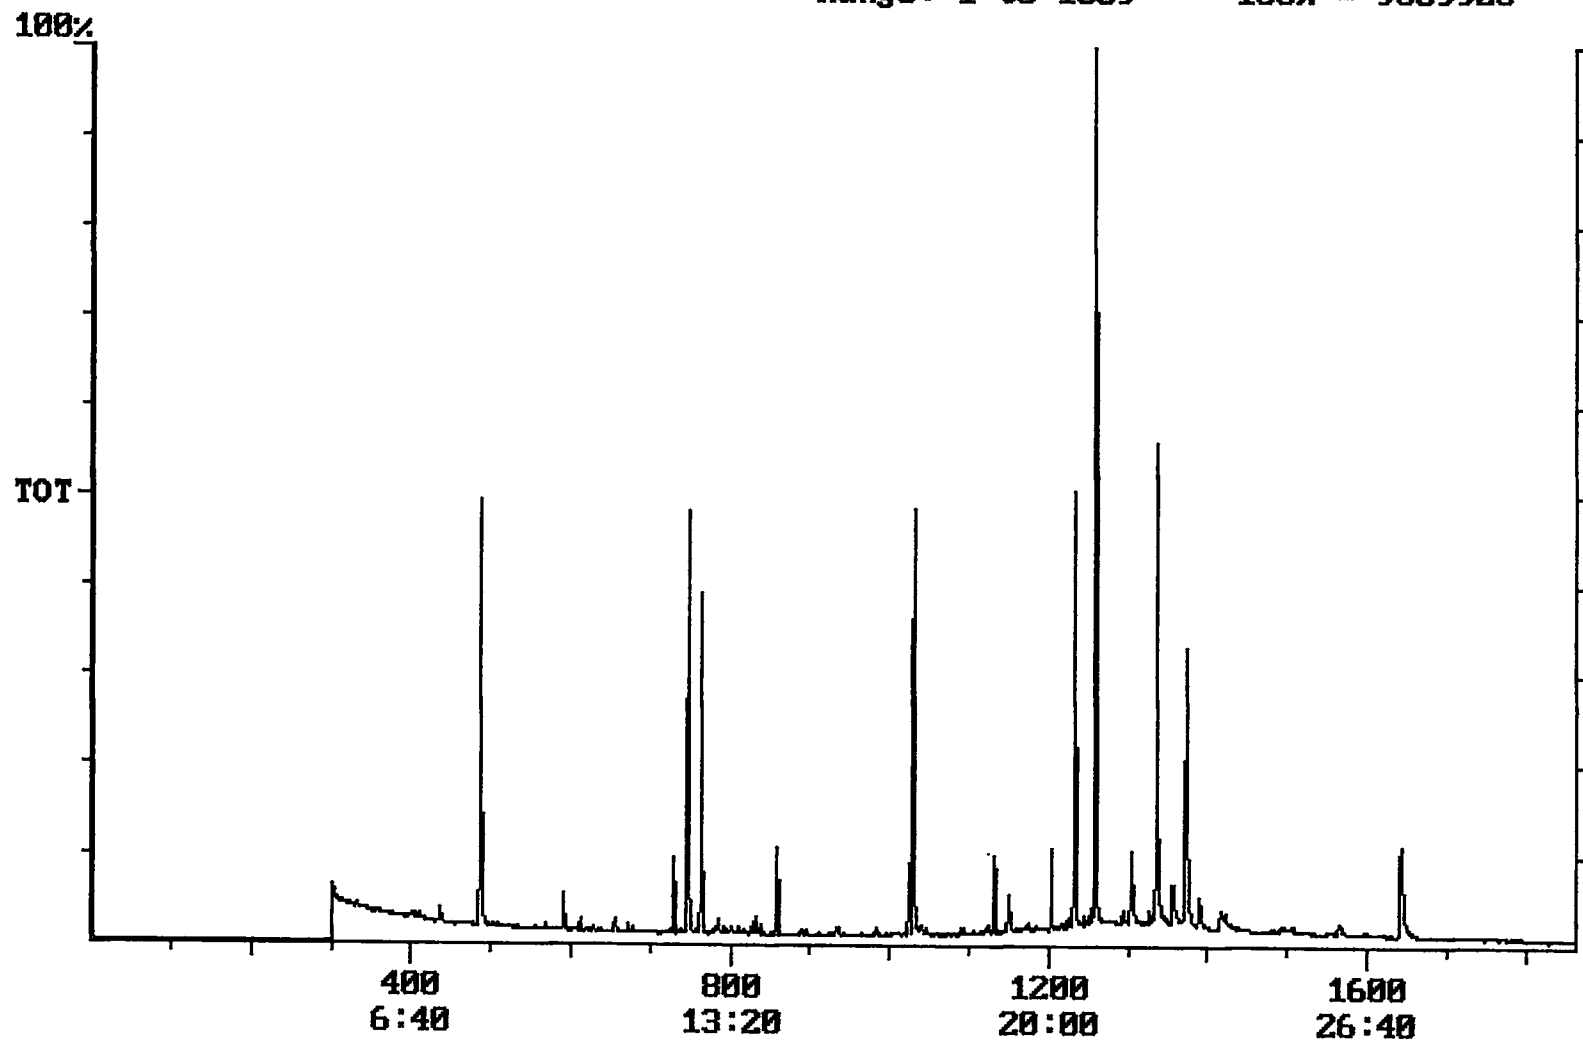

Integration Report Quanfile: 24237J Quan Entries: 14
 Comment: BOHLK; METHOD 525; INST 204; 10/25/01; SAMPLE 24237
 Sorted via: Entry Number ↑

No	Name of Compound	R Time	Scan#	Mode	Peak Area	Pk Height
1	acenaphthene d-10 (IS)	12:27	747	Auto	2,035,932	1,095,054
2	phenanthrene d-10 (IS)	17:10	1030	Auto	3,526,625	1,606,640
3	chrysene d-12 (IS)	22:52	1372	Auto	2,432,388	891,505
4	p-terphenyl d-14 (IS)	20:58	1258	Auto	4,493,034	2,942,674
5	acenaphthene d-10 (SURR)	12:27	747	Auto	2,035,932	1,095,054
6	phenanthrene d-10 (SURR)	17:10	1030	Auto	3,526,625	1,606,640
7	chrysene d-12 (SURR)	22:52	1372	Auto	2,432,388	891,505
8	1,3-dimethyl-2-nitrobenzene	8:07	487	Auto	1,340,727	737,493
9	triphenyl phosphate (S)	22:15	1335	Auto	1,866,946	820,172
10	perylene d-12 (SURR)	27:23	1643	Auto	1,324,458	261,380
11	bis(2-ethylhexyl)adipate	22:07	1327	Auto	25,187	6,315
12	bis(2-ethylhexyl)phthalate	23:10	1390	Auto	310,171	94,511
13	2,6-dinitrotoluene	12:06	726	Auto	14,486	7,100
14	2,4-dinitrotoluene	13:14	794	Auto	3,861	1,713

Quantitation Report

Quanfile: 24237J

Quan Entries: 14

Comment: BOHLK; METHOD 525; INST 204; 10/25/01; SAMPLE 24237

Sorted via: Entry Number ↑

(S) = Standard

Cal	Name of Compound	S	Scan#	R Time	Me	Calc Amt(A)	Units
1	acenaphthene d-10 (IS)	I	747	12:27	BV	5.000	UG/L
2	phenanthrene d-10 (IS)	I	1030	17:10	BV	5.000	UG/L
3	chrysene d-12 (IS)	I	1372	22:52	BB	5.000	UG/L
4	p-terphenyl d-14 (IS)	I	1258	20:58	BB	5.000	UG/L
5	acenaphthene d-10 (SURR)	A	747	12:27	BV	3.132	UG/L
6	phenanthrene d-10 (SURR)	A	1030	17:10	BV	3.747	UG/L
7	chrysene d-12 (SURR)	A	1372	22:52	BB	3.778	UG/L
8	1,3-dimethyl-2-nitrobenzene	A	487	8:07	BV	5.611	UG/L
9	triphenyl phosphate (S)	A	1335	22:15	BB	5.802	UG/L
10	perylene d-12 (SURR)	A	1643	27:23	BB	4.323	UG/L
16	bis(2-ethylhexyl)adipate	A	1327	22:07	MM	0.050	UG/L
17	bis(2-ethylhexyl)phthalate	A	1390	23:10	VB	0.373	UG/L
20	2,6-dinitrotoluene	A	726	12:06	BB	0.109	UG/L
21	2,4-dinitrotoluene	A	794	13:14	BB	0.025	UG/L

Reviewed is/surrogate

Comments for Sample AD24237 - Analysis \$525

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 11-15-2001 Time: 10:10:24

The recovery for bis(2-Ethylhexyl)phthalate in the MDL Standard was above its acceptance range. This probably due to laboratory contamination.