


User: Azzo Murad, Nehla
Westchester Dept. of Labs & Research
Date: 11/07/2001 Time: 10:17:34

Sample: AD24287
Analysis: \$525 Organic Chemicals - 525.2
Units: ug
Started: 10/15/01 10:08 Ended: 10/25/01 10:08 Analyst: NAM
Result source: manual entry
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Hexachlorocyclopentadiene		< MDL		0.10
2	Hexachlorobenzene		< MDL		0.10
3	Simazine		< MDL		0.40
4	Atrazine		< MDL		0.10
5	Alachlor		< MDL		0.20
6	bis(2-Ethylhexyl)adipate		< MDL		0.60
7	bis(2-Ethylhexyl)phthalate		1.08		0.60
8	Benzo(a)pyrene		< MDL		0.20
9	EPTC		< MDL		1.0
10	2,6-Dinitrotoluene		< MDL		2.0
11	2,4-Dinitrotoluene		< MDL		2.0
12	Molinate		< MDL		0.90
13	Terbacil		< MDL		2.0
14	Acetochlor		< MDL		2.0
15	Metribuzin		< MDL		0.15
16	Metolachlor		< MDL		0.75
17	Butachlor		< MDL		0.40
18	4,4-DDE		< MDL		0.80
19	Surr_1,3-Dimethyl-2-nitrobenze		5.1		1.0
20	Surr_Triphenyl phosphate		5.6		1.0
21	Surr_Perylene-d12		3.6		1.0

Chromatogram Plot File: F:\24287L Date: Oct-26-1991 04:56:40
Comment: BOHLK; METHOD 525; INST 204; 10/25/01; SAMPLE 24287
Scan No: 1 Retention Time: 0:01 RIC: 0 Mass Range: 0 - 0
Plotted: 1 to 1860 Range: 1 to 1860 100% = 10019933

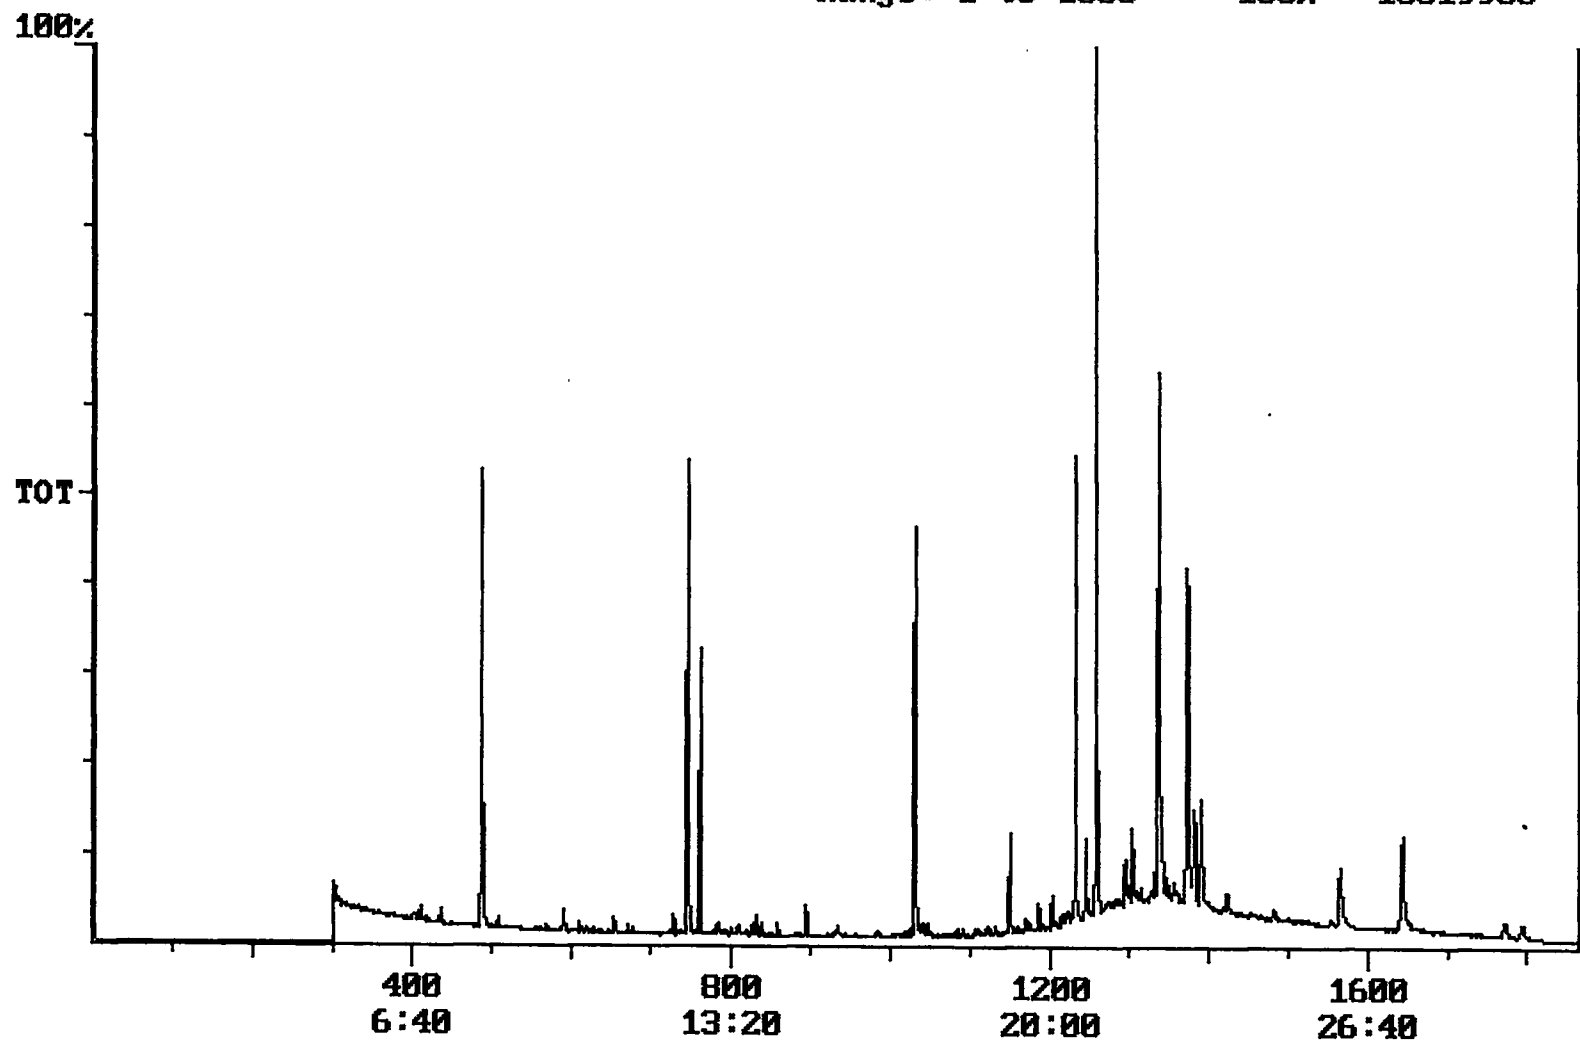

Integration Report Quanfile: 24287L Quan Entries: 14
 Comment: BOHLK; METHOD 525; INST 204; 10/25/01; SAMPLE 24287
 Sorted via: Entry Number ↑

No	Name of Compound	R Time	Scan#	Mode	Peak Area	Pk Height
1	acenaphthene d-10 (IS)	12:27	747	Auto	2,408,866	1,254,012
2	phenanthrene d-10 (IS)	17:10	1030	Auto	3,593,790	1,598,397
3	chrysene d-12 (IS)	22:52	1372	Auto	2,749,391	1,064,638
4	p-terphenyl d-14 (IS)	20:58	1258	Auto	4,269,027	3,088,193
5	acenaphthene d-10 (SURR)	12:27	747	Auto	2,408,866	1,254,012
6	phenanthrene d-10 (SURR)	17:10	1030	Auto	3,593,790	1,598,397
7	chrysene d-12 (SURR)	22:52	1372	Auto	2,749,391	1,064,638
8	1,3-dimethyl-2-nitrobenzene	8:07	487	Auto	1,441,403	795,564
9	triphenyl phosphate (S)	22:15	1335	Auto	2,030,335	930,476
10	perylene d-12 (SURR)	27:23	1643	Auto	1,252,337	243,786
11	hexachlorocyclopentadiene	10:18	618	Auto	1,031	1,031
12	bis(2-ethylhexyl)phthalate	23:10	1390	Auto	994,884	341,268
13	2,6-dinitrotoluene	12:06	726	Auto	11,470	5,988
14	2,4-dinitrotoluene	13:14	794	Auto	3,026	1,935

Quantitation Report

Quanfile: 24287L

Quan Entries: 14

Comment: BOHLK; METHOD 525; INST 204; 10/25/01; SAMPLE 24287

Sorted via: Entry Number ↑

(S) = Standard

Cal	Name of Compound	S	Scan#	R Time	Me	Calc Amt(A)	Units
1	acenaphthene d-10(IS)	I	747	12:27	BV	5.000	UG/L
2	phenanthrene d-10 (IS)	I	1030	17:10	BV	5.000	UG/L
3	chrysene d-12(IS)	I	1372	22:52	BV	5.000	UG/L
4	p-terphenyl d-14(IS)	I	1258	20:58	BV	5.000	UG/L
5	acenaphthene d-10(SURR)	A	747	12:27	BV	3.900	UG/L
6	phenanthrene d-10(SURR)	A	1030	17:10	BV	4.018	UG/L
7	chrysene d-12 (SURR)	A	1372	22:52	BV	4.494	UG/L
8	1,3-dimethyl-2-nitrobenzene	A	487	8:07	BV	5.099	UG/L
9	triphenyl phosphate (S)	A	1335	22:15	BB	5.582	UG/L
10	perylene d-12 (SURR)	A	1643	27:23	BV	3.617	UG/L
11	hexachlorocyclopentadiene	A	618	10:18	BB	0.010	UG/L
17	bis(2-ethylhexyl)phthalate	A	1390	23:10	BB	1.077	UG/L
20	2,6-dinitrotoluene	A	726	12:06	BB	0.073	UG/L
21	2,4-dinitrotoluene	A	794	13:14	BB	0.017	UG/L

Reviewed IS/surrogate

Comments for Sample AD24287 - Analysis \$525

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 11-15-2001 Time: 10:28:01

The recovery for bis(2-Ethylhexyl)phthalate in the MDL Standard was above its acceptance range. This is probably due to laboratory contamination.