


User: Bohlk, Ted
Westchester Dept. of Labs & Research
Date: 11/29/2001 Time: 10:27:08

Sample: AD25155
Analysis: \$525 Organic Chemicals - 525.2
Units: ug
Started: 10/25/01 10:24 Ended: 11/9/01 10:24 Analyst: TB
Result source: manual entry
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Hexachlorocyclopentadiene		< MDL		0.10
2	Hexachlorobenzene		< MDL		0.10
3	Simazine		< MDL		0.40
4	Atrazine		< MDL		0.20
5	Alachlor		< MDL		0.20
6	bis(2-Ethylhexyl)adipate		< MDL		0.60
7	bis(2-Ethylhexyl)phthalate		0.71		0.60
8	Benzo(a)pyrene		< MDL		0.20
9	EPTC		< MDL		1.0
10	2,6-Dinitrotoluene		< MDL		2.0
11	2,4-Dinitrotoluene		< MDL		2.0
12	Molinate		< MDL		0.90
13	Terbacil		< MDL		2.0
14	Acetochlor		< MDL		2.0
15	Metribuzin		< MDL		0.15
16	Metolachlor		< MDL		0.75
17	Butachlor		< MDL		0.40
18	4,4-DDE		< MDL		0.80
19	Surr_1,3-Dimethyl-2-nitrobenze		5.1		1.0
20	Surr_Triphenyl phosphate		5.4		1.0
21	Surr_Perylene-d12		3.4		1.0

Chromatogram Plot File: F:\251550 Date: Nov-10-1991 09:49:28
 Comment: BOHLK; METHOD 525; INST 204; 11/09/01; SAMPLE 25155
 Scan No: 1 Retention Time: 0:01 RIC: 0 Mass Range: 0 - 0
 Plotted: 1 to 1860 Range: 1 to 1860 100% = 8431779

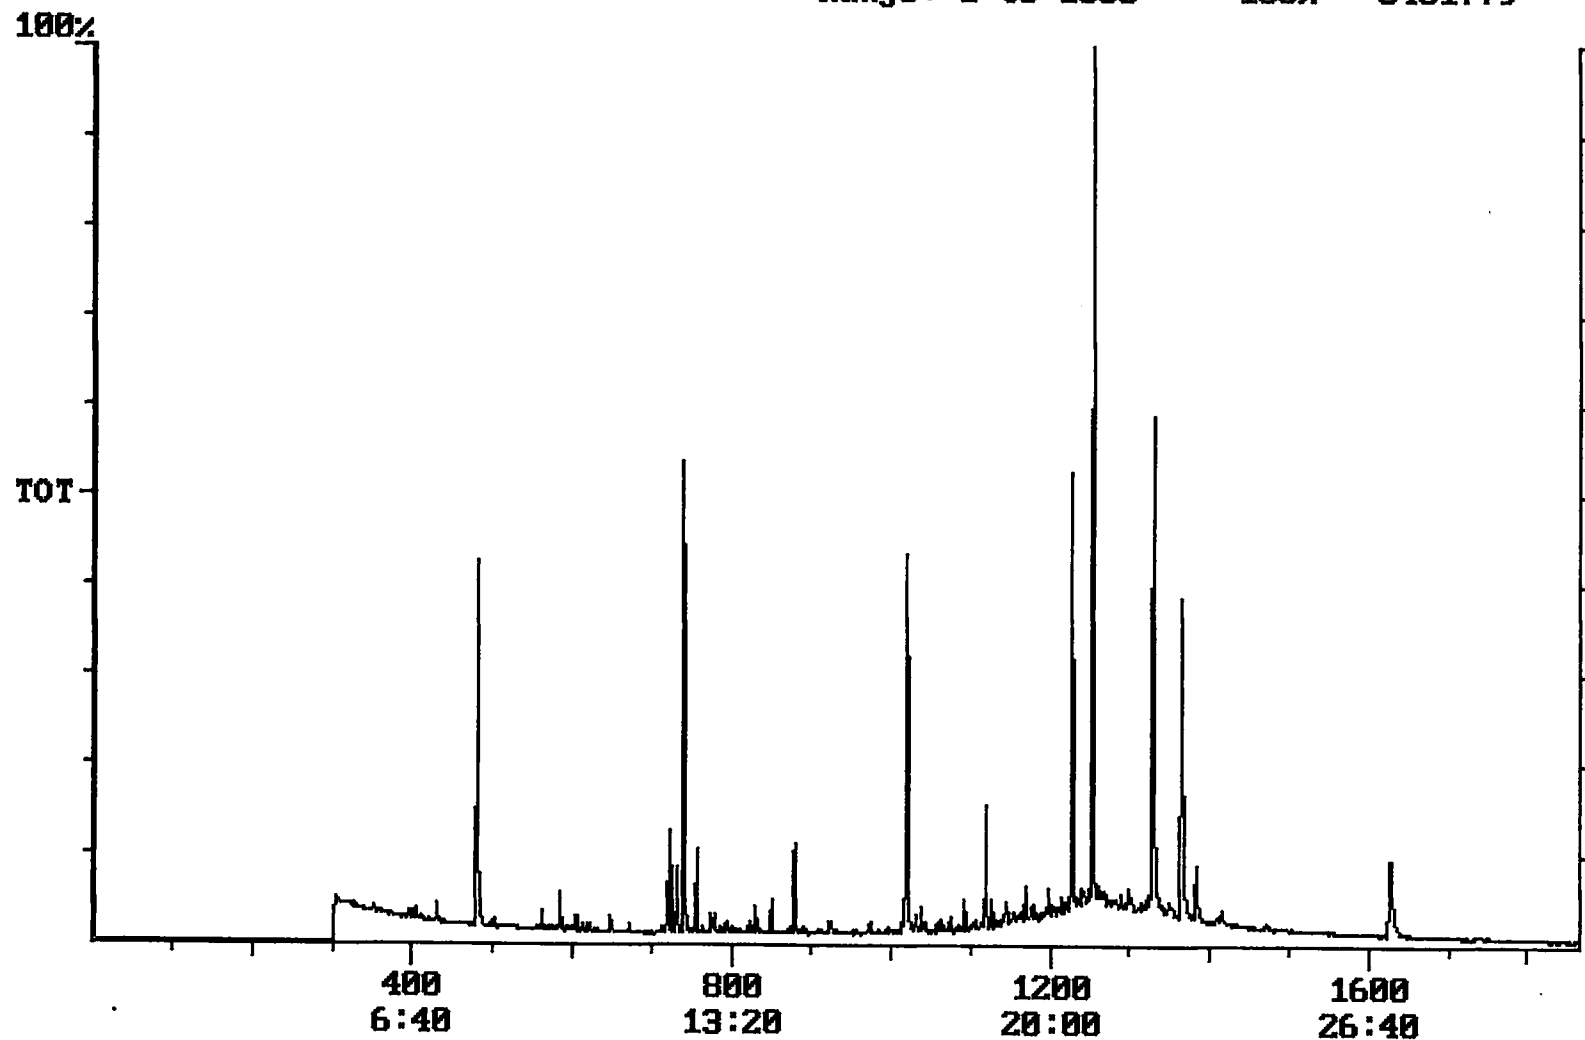

Integration Report Quanfile: 251550 Quan Entries: 15
 Comment: BOHLK; METHOD 525; INST 204; 11/09/01; SAMPLE 25155
 Sorted via: Entry Number ↑

No	Name of Compound	R Time	Scan#	Mode	Peak Area	Pk Height
1	acenaphthene d-10 (IS)	12:20	740	Auto	1,901,505	1,054,427
2	phenanthrene d-10 (IS)	17:00	1020	Auto	2,885,114	1,156,366
3	chrysene d-12 (IS)	22:45	1365	Auto	2,116,554	857,085
4	p-terphenyl d-14 (IS)	20:53	1253	Auto	3,443,935	2,476,843
5	acenaphthene d-10 (SURR)	12:20	740	Auto	1,901,505	1,054,427
6	phenanthrene d-10 (SURR)	17:00	1020	Auto	2,885,114	1,156,366
7	chrysene d-12 (SURR)	22:45	1365	Auto	2,116,554	857,085
8	1,3-dimethyl-2-nitrobenzene	8:01	481	Auto	1,210,634	569,079
9	triphenyl phosphate (S)	22:09	1329	Auto	1,503,002	675,357
10	perylene d-12 (SURR)	27:07	1627	Auto	983,138	181,515
11	bis(2-ethylhexyl)adipate	22:05	1325	Auto	48,328	4,783
12	bis(2-ethylhexyl)phthalate	23:02	1382	Auto	503,911	148,089
13	2,6-dinitrotoluene	12:00	720	Auto	95,293	59,061
14	2,4-dinitrotoluene	13:07	787	Auto	1,323	1,323
15	4,4'-dichlorodiphenyl ether	20:49	1249	Auto	4,186	1,755

reviewed IS/surr's

Quantitation Report Quanfile: 251550 Quan Entries: 15
 Comment: BOHLK; METHOD 525; INST 204; 11/09/01; SAMPLE 25155
 Sorted via: Entry Number ↑ (S) = Standard

Cal	Name of Compound	S	Scan#	R Time	Me	Calc Amt(A)	Units
1	acenaphthene d-10 (IS)	I	740	12:20	BB	5.000	UG/L
2	phenanthrene d-10 (IS)	I	1020	17:00	BV	5.000	UG/L
3	chrysene d-12 (IS)	I	1365	22:45	BB	5.000	UG/L
4	p-terphenyl d-14 (IS)	I	1253	20:53	BB	5.000	UG/L
5	acenaphthene d-10 (SURR)	A	740	12:20	BB	3.703	UG/L
6	phenanthrene d-10 (SURR)	A	1020	17:00	BV	3.737	UG/L
7	chrysene d-12 (SURR)	A	1365	22:45	BB	3.800	UG/L
8	1,3-dimethyl-2-nitrobenzene	A	481	8:01	BV	5.129	UG/L
9	triphenyl phosphate (S)	A	1329	22:09	BB	5.392	UG/L
10	perylene d-12 (SURR)	A	1627	27:07	BB	3.423	UG/L
16	bis(2-ethylhexyl)adipate	A	1325	22:05	MM	0.212	UG/L
17	bis(2-ethylhexyl)phthalate	A	1382	23:02	BV	0.714	UG/L
20	2,6-dinitrotoluene	A	720	12:00	BB	0.768	UG/L
21	2,4-dinitrotoluene	A	787	13:07	BB	0.010	UG/L
28	4,4'-dichlorodiphenyl ether	A	1249	20:49	BV	0.014	UG/L

Chromatogram Plot

File: E:\251550

Date: Nov-10-1991 09:49:28

Comment: BOHLK; METHOD 525; INST 204; 11/09/01; SAMPLE 25155

Scan No: 1245

Retention Time: 20:45


RIC: 448441

Mass Range: 45 - 330


Plotted: 1230 to 1260

Range: 1 to 1860

100% = 8431779

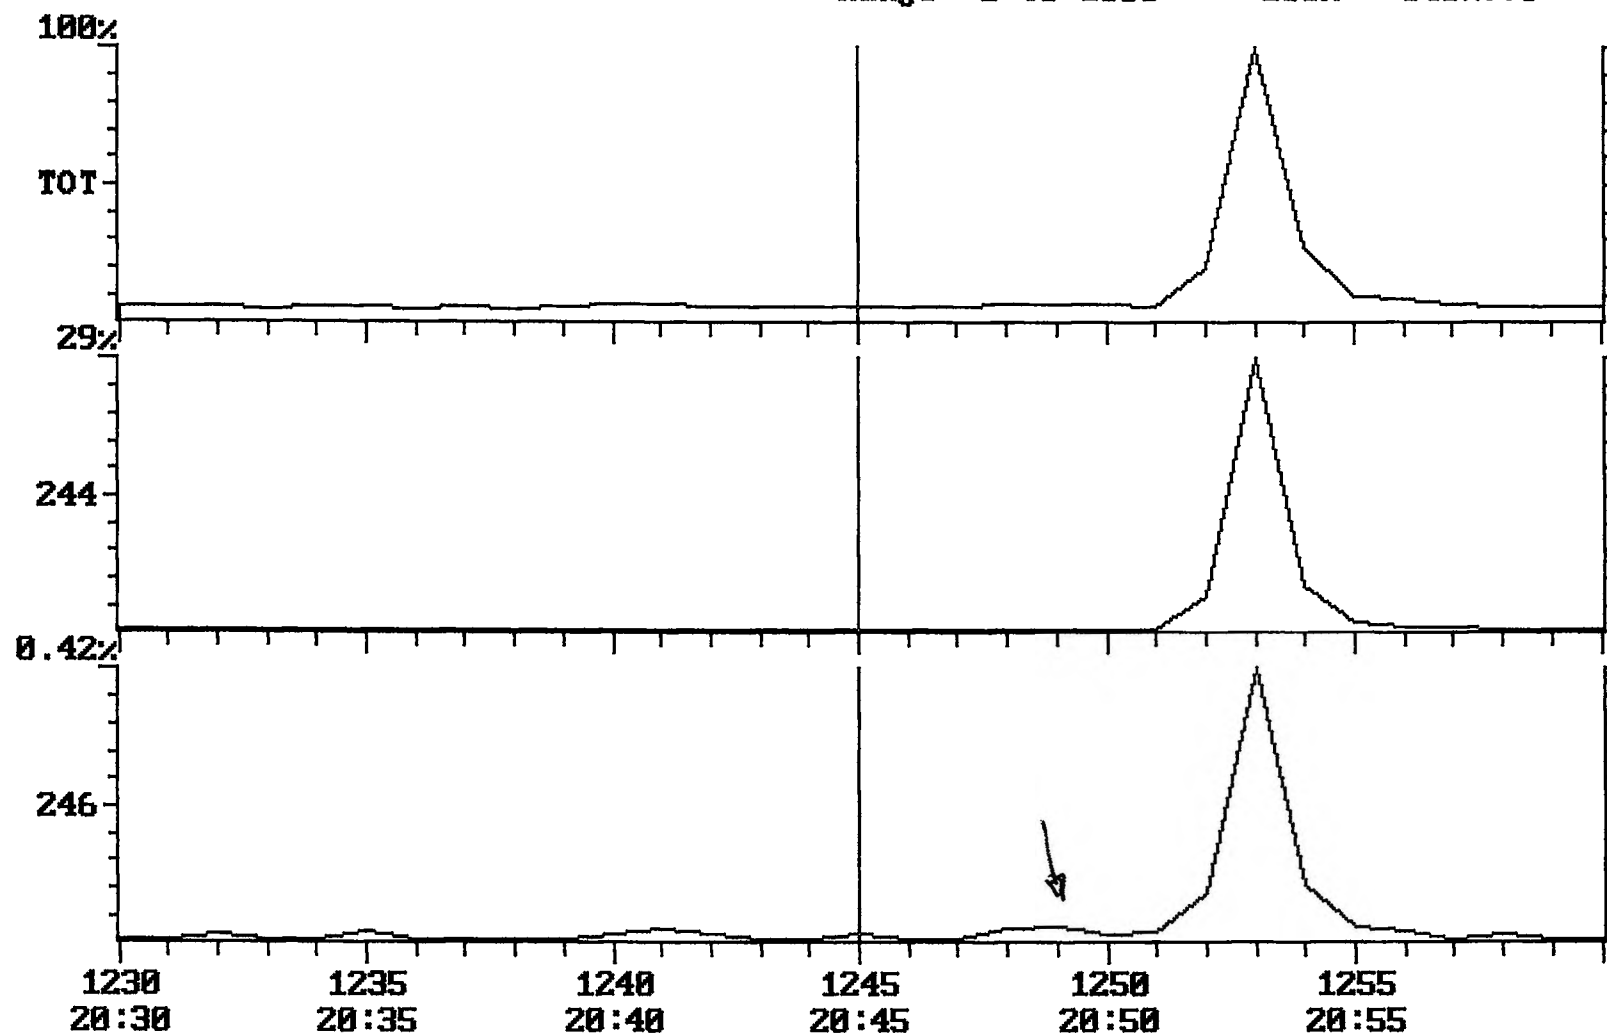

Chromatogram Plot File: E:\C2A1130 Date: Nov-30-1991 10:48:17
Comment: BOHLK; METHOD 525; INST 204; 11/30/01; C2
Scan No: 1230 Retention Time: 20:30 RIC: 37507 Mass Range: 47 - 213
Plotted: 1230 to 1260 Range: 1 to 1860 100% = 9176467

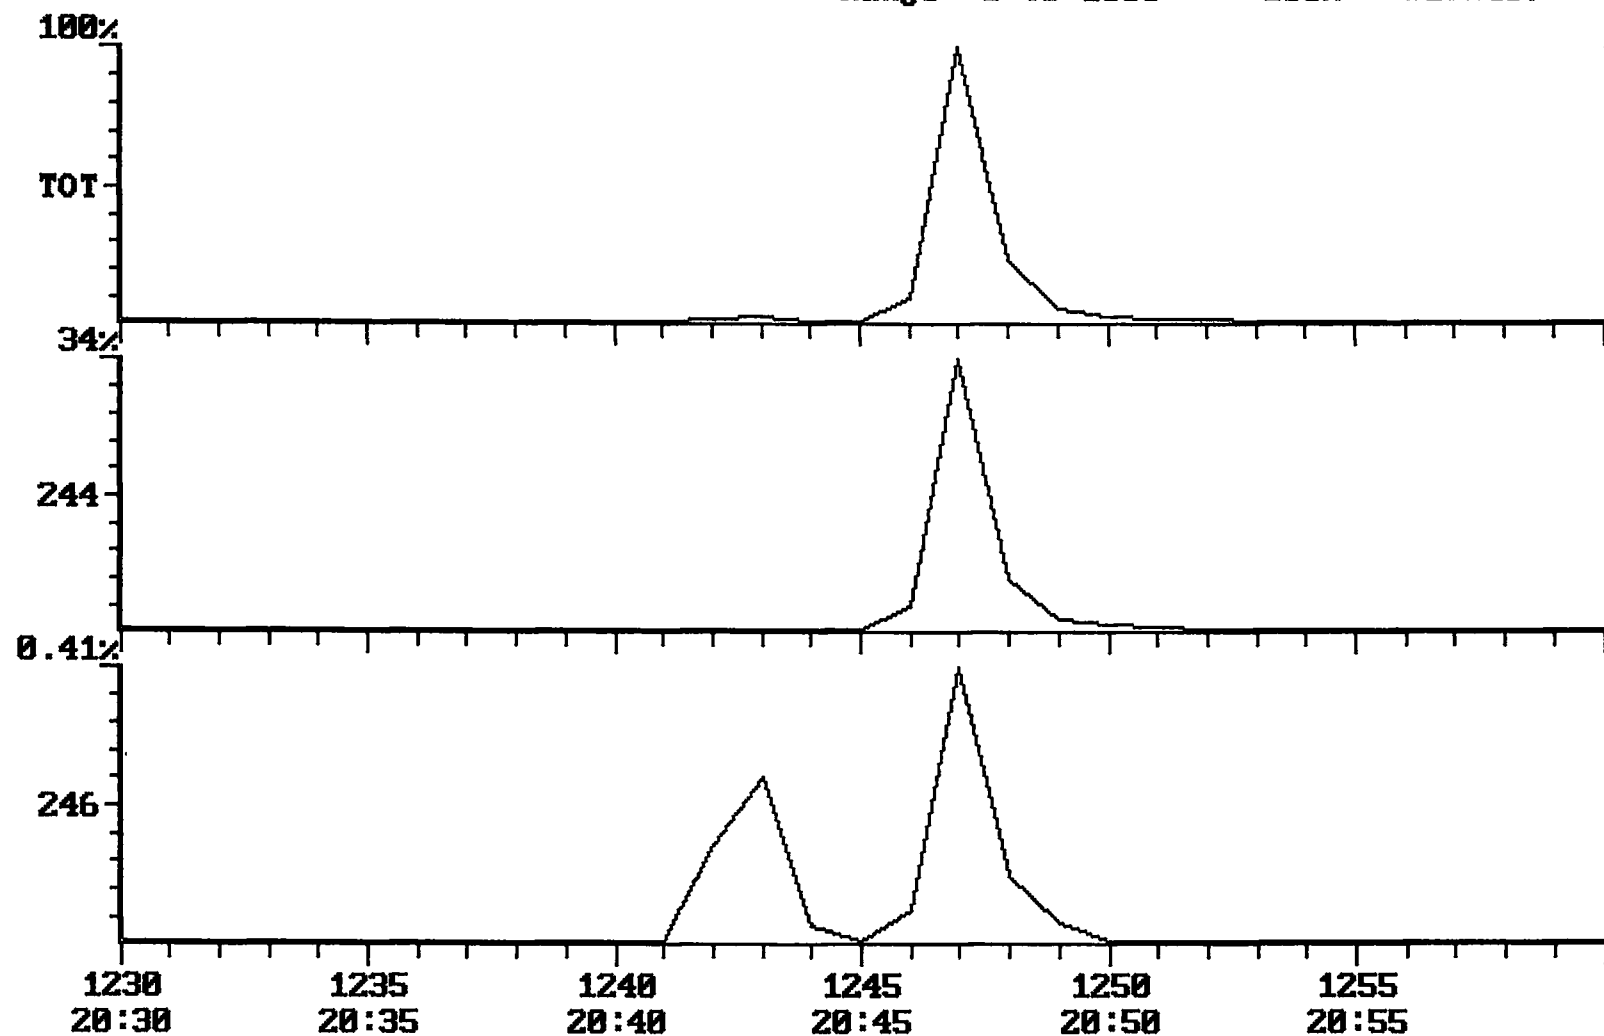

Comments for Sample AD25155 - Analysis \$525

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 12-06-2001 Time: 11:17:42

Recoveries for 3 of the 18 compounds in the MDL and LCS Standards were outside of their acceptance ranges. Recoveries for 4 of the 18 compounds in the Spiked Sample were below their acceptance ranges.