


User: Bohlk, Ted
Westchester Dept. of Labs & Research
Date: 11/30/2001 Time: 08:58:44

Sample: AD25734
Analysis: \$525 Organic Chemicals - 525.2
Units: ug
Started: 10/31/01 08:46 Ended: 11/14/01 08:46 Analyst: TB
Result source: manual entry
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Hexachlorocyclopentadiene		< MDL		0.10
2	Hexachlorobenzene		< MDL		0.10
3	Simazine		< MDL		0.40
4	Atrazine		< MDL		0.20
5	Alachlor		< MDL		0.20
6	bis(2-Ethylhexyl)adipate		< MDL		0.60
7	bis(2-Ethylhexyl)phthalate		3.1		0.60
8	Benzo(a)pyrene		< MDL		0.20
9	EPTC		< MDL		1.0
10	2,6-Dinitrotoluene		< MDL		2.0
11	2,4-Dinitrotoluene		< MDL		2.0
12	Molinate		< MDL		0.90
13	Terbacil		< MDL		2.0
14	Acetochlor		< MDL		2.0
15	Metribuzin		< MDL		0.15
16	Metolachlor		< MDL		0.75
17	Butachlor		< MDL		0.40
18	4,4-DDE		< MDL		0.80
19	Surr_1,3-Dimethyl-2-nitrobenzen		5.1		1.0
20	Surr_Triphenyl phosphate		5.7		1.0
21	Surr_Perylene-d12		3.9		1.0

Chromatogram Plot File: F:\25734H Date: Nov-15-1991 06:50:19
Comment: BOHLK; METHOD 525; INST 204; 11/14/01; SAMPLE 25734
Scan No: 1 Retention Time: 0:01 RIC: 0 Mass Range: 0 - 0
Plotted: 1 to 1860 Range: 1 to 1860 100% = 5558951

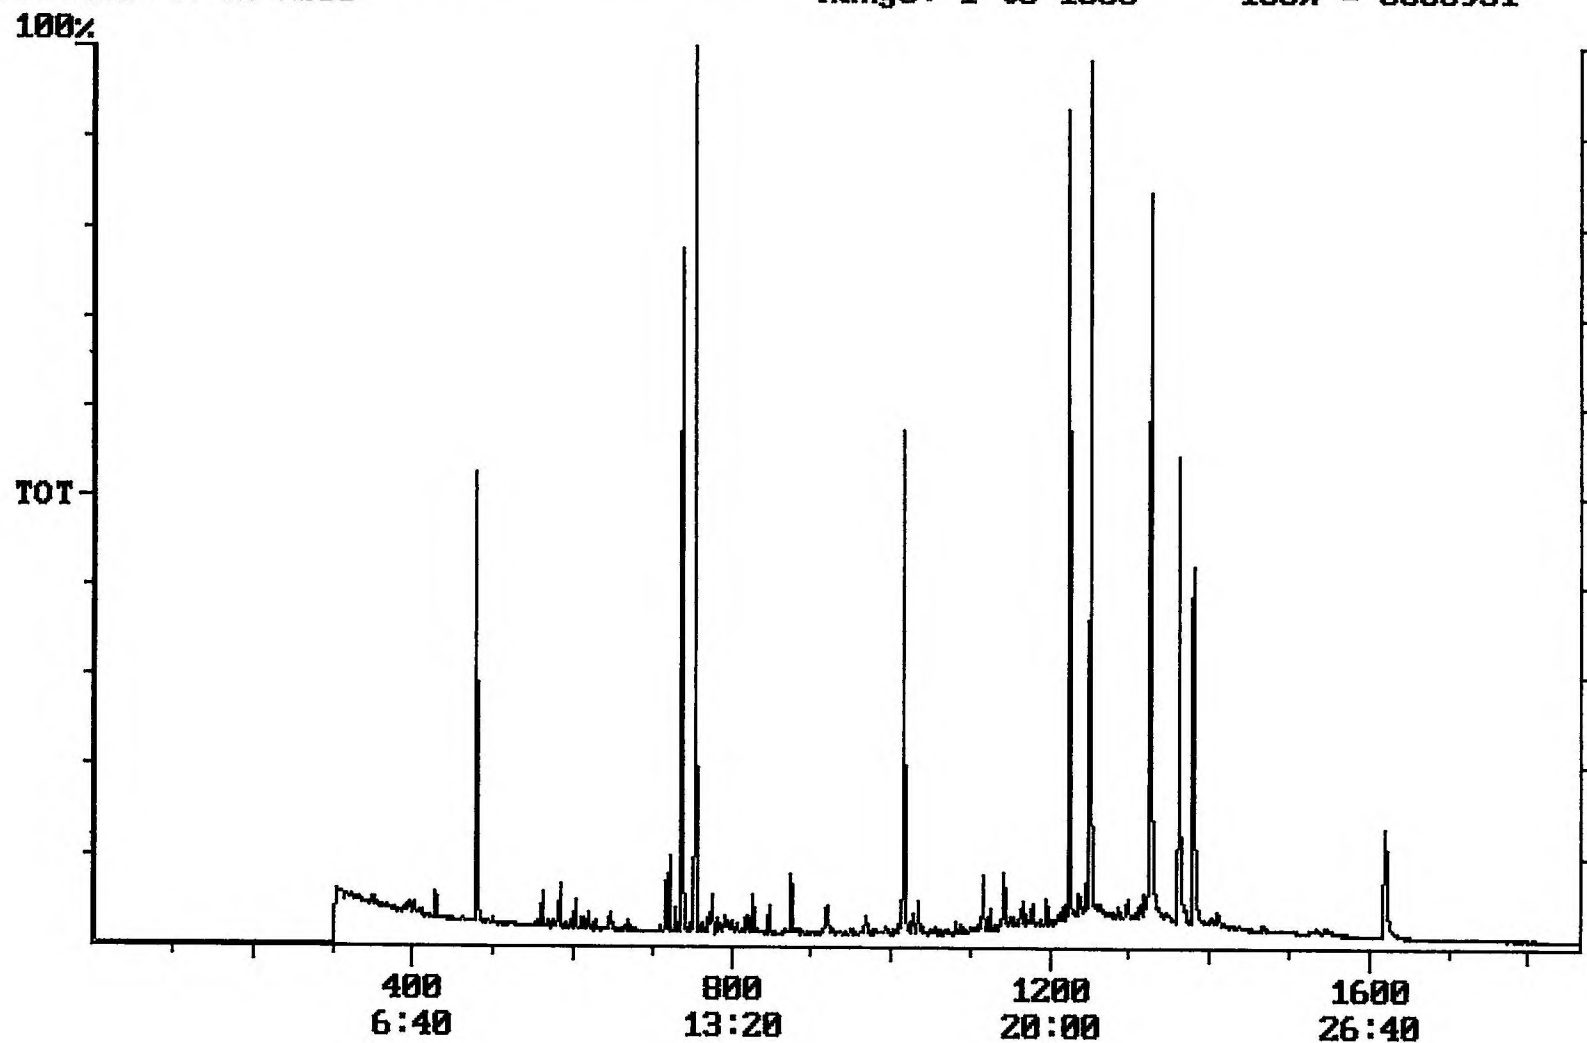

Integration Report Quanfile: 25734H Quan Entries: 17
 Comment: BOHLK; METHOD 525; INST 204; 11/14/01; SAMPLE 25734
 Sorted via: Entry Number ↑

No	Name of Compound	R Time	Scan#	Mode	Peak Area	Pk Height
1	acenaphthene d-10 (IS)	12:18	738	Auto	1,642,635	1,003,989
2	phenanthrene d-10 (IS)	16:56	1016	Auto	2,528,225	1,017,120
3	chrysene d-12 (IS)	22:41	1361	Auto	1,856,857	850,023
4	p-terphenyl d-14 (IS)	20:51	1251	Auto	3,079,535	1,546,967
5	acenaphthene d-10 (SURR)	12:18	738	Auto	1,642,635	1,003,989
6	phenanthrene d-10 (SURR)	16:56	1016	Auto	2,528,225	1,017,120
7	chrysene d-12 (SURR)	22:41	1361	Auto	1,856,857	850,023
8	1,3-dimethyl-2-nitrobenzene	7:58	478	Auto	1,053,453	440,892
9	triphenyl phosphate (S)	22:06	1326	Auto	1,521,449	679,566
10	perylene d-12 (SURR)	26:59	1619	Auto	865,398	161,915
11	hexachlorocyclopentadiene	10:09	609	Auto	1,924	1,924
12	hexachlorobenzene	15:22	922	Auto	10,405	4,085
13	simazine	16:16	976	Auto	0	0
14	bis(2-ethylhexyl)adipate	22:02	1322	Auto	53,249	4,130
15	bis(2-ethylhexyl)phthalate	22:59	1379	Auto	2,033,075	626,761
16	2,6-dinitrotoluene	11:58	718	Auto	80,714	40,858
17	4,4'-dichlorodiphenyl ether	20:46	1246	Auto	8,331	5,380

Reviewed 12/01/01

Quantitation Report Quanfile: 25734H Quan Entries: 17
 Comment: BOHLK; METHOD 525; INST 204; 11/14/01; SAMPLE 25734
 Sorted via: Entry Number ↑ (S) = Standard

Cal	Name of Compound	S	Scan#	R Time	Me	Calc Amt(A)	Units
1	acenaphthene d-10 (IS)	I	738	12:18	BV	5.000	UG/L
2	phenanthrene d-10 (IS)	I	1016	16:56	BV	5.000	UG/L
3	chrysene d-12 (IS)	I	1361	22:41	BB	5.000	UG/L
4	p-terphenyl d-14 (IS)	I	1251	20:51	BB	5.000	UG/L
5	acenaphthene d-10 (SURR)	A	738	12:18	BV	3.510	UG/L
6	phenanthrene d-10 (SURR)	A	1016	16:56	BV	3.523	UG/L
7	chrysene d-12 (SURR)	A	1361	22:41	BB	3.879	UG/L
8	1,3-dimethyl-2-nitrobenzene	A	478	7:58	BB	5.149	UG/L
9	triphenyl phosphate (S)	A	1326	22:06	BB	5.715	UG/L
10	perylene d-12 (SURR)	A	1619	26:59	BB	3.862	UG/L
11	hexachlorocyclopentadiene	A	609	10:09	BB	0.025	UG/L
12	hexachlorobenzene	A	922	15:22	BB	0.047	UG/L
13	simazine	A	976	16:16	BB	0.001	UG/L
16	bis(2-ethylhexyl)adipate	A	1322	22:02	MM	0.238	UG/L
17	bis(2-ethylhexyl)phthalate	A	1379	22:59	BB	3.089	UG/L
20	2,6-dinitrotoluene	A	718	11:58	BB	0.765	UG/L
28	4,4'-dichlorodiphenyl ether	A	1246	20:46	BB	0.039	UG/L

Comments for Sample AD25734 - Analysis \$525

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 12-07-2001 Time: 16:19:27

Recoveries for 3 of the 18 compounds in the MDL and LCS Standards were outside of their acceptance ranges. Recoveries for 4 of the 18 compounds in the Spiked Sample were outside of their acceptance ranges. The result for bis(2-Ethylhexyl)phthalate of 3.1 ug/L could be due to collection or laboratory contamination. This value is below the NYSDOH MCL.