


User: Bohlk, Ted
 Westchester Dept. of Labs & Research
 Date: 12/13/2001 Time: 18:07:04

Sample: AD25947
 Analysis: \$525 Organic Chemicals - 525.2
 Units: ug
 Started: 11/1/01 18:05 Ended: 11/17/01 18:05 Analyst: TB
 Result source: manual entry
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Hexachlorocyclopentadiene		< MDL		0.10
2	Hexachlorobenzene		< MDL		0.10
3	Simazine		< MDL		0.40
4	Atrazine		< MDL		0.20
5	Alachlor		< MDL		0.20
6	bis(2-Ethylhexyl)adipate		< MDL		0.60
7	bis(2-Ethylhexyl)phthalate		2.2		0.60
8	Benzo(a)pyrene		< MDL		0.20
9	EPTC		< MDL		1.0
10	2,6-Dinitrotoluene		< MDL		2.0
11	2,4-Dinitrotoluene		< MDL		2.0
12	Molinate		< MDL		0.90
13	Terbacil		< MDL		2.0
14	Acetochlor		< MDL		2.0
15	Metribuzin		< MDL		0.15
16	Metolachlor		< MDL		0.75
17	Butachlor		< MDL		0.40
18	4,4-DDE		< MDL		0.80
19	Surr_1,3-Dimethyl-2-nitrobenze		5.1		1.0
20	Surr_Triphenyl phosphate		5.3		1.0
21	Surr_Perylene-d12	LSPEC	3.1		1.0

Chromatogram Plot File: C:\25947D Date: Nov-17-1991 22:02:42
Comment: BOHLK; METHOD 525; INST 204; 11/17/01; SAMPLE 25947
Scan No: 1 Retention Time: 0:01 RIC: 0 Mass Range: 0 - 0
Plotted: 1 to 1860 Range: 1 to 1860 100% = 7743242

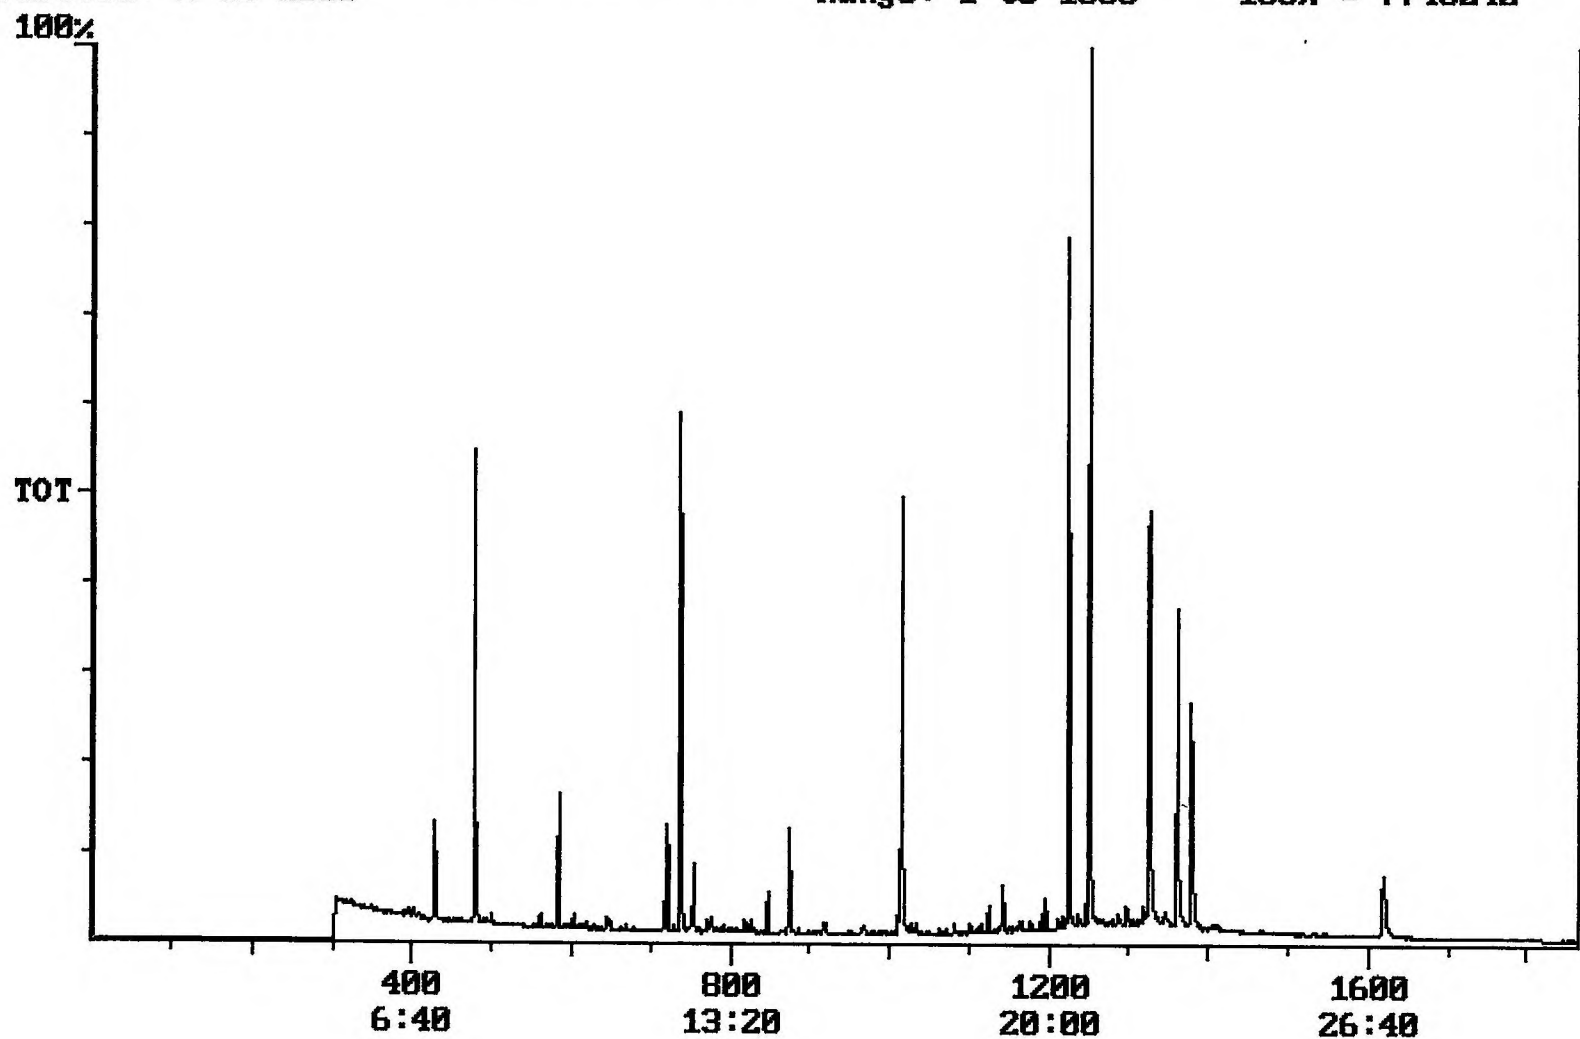

Integration Report

Quanfile: 25947D

Quan Entries: 14

Comment: BOHLK; METHOD 525; INST 204; 11/17/01; SAMPLE 25947

Sorted via: Entry Number ↑

No	Name of Compound	R Time	Scan#	Mode	Peak Area	Pk Height
1	acenaphthene d-10 (IS)	12:17	737	Auto	1,874,087	1,059,574
2	phenanthrene d-10 (IS)	16:55	1015	Auto	3,247,914	1,314,154
3	chrysene d-12 (IS)	22:41	1361	Auto	1,995,503	792,392
4	p-terphenyl d-14 (IS)	20:50	1250	Auto	3,875,347	2,515,530
5	acenaphthene d-10 (SURR)	12:17	737	Auto	1,874,087	1,059,574
6	phenanthrene d-10 (SURR)	16:55	1015	Auto	3,247,914	1,314,154
7	chrysene d-12 (SURR)	22:41	1361	Auto	1,995,503	792,392
8	1,3-dimethyl-2-nitrobenzene	7:58	478	Auto	1,200,521	658,411
9	triphenyl phosphate (S)	22:05	1325	Auto	1,512,092	516,577
10	perylene d-12 (SURR)	26:59	1619	Auto	739,908	122,895
11	bis(2-ethylhexyl)adipate	21:58	1318	Auto	40,577	5,142
12	bis(2-ethylhexyl)phthalate	22:58	1378	Auto	1,630,806	573,106
13	2,6-dinitrotoluene	11:57	717	Auto	65,643	32,863
14	2,4-dinitrotoluene	13:05	785	Auto	959	959

reversed IS/surr's

Quantitation Report

Quanfile: 25947D

Quan Entries: 14

Comment: BOHLK; METHOD 525; INST 204; 11/17/01; SAMPLE 25947

Sorted via: Entry Number ↑

(S) = Standard

Cal	Name of Compound	S	Scan#	R Time	Me	Calc Amt(A)	Units
1	acenaphthene d-10(IS)	I	737	12:17	BB	5.000	UG/L
2	phenanthrene d-10 (IS)	I	1015	16:55	BV	5.000	UG/L
3	chrysene d-12(IS)	I	1361	22:41	BB	5.000	UG/L
4	p-terphenyl d-14(IS)	I	1250	20:50	BB	5.000	UG/L
5	acenaphthene d-10(SURR)	A	737	12:17	BB	3.182	UG/L
6	phenanthrene d-10(SURR)	A	1015	16:55	BV	3.596	UG/L
7	chrysene d-12 (SURR)	A	1361	22:41	BB	3.313	UG/L
8	1,3-dimethyl-2-nitrobe	A	478	7:58	BV	5.143	UG/L
9	triphenyl phosphate (S	A	1325	22:05	BB	5.286	UG/L
10	perylene d-12 (SURR)	A	1619	26:59	BB	3.072	UG/L
16	bis(2-ethylhexyl)adipa	A	1318	21:58	MM	0.169	UG/L
17	bis(2-ethylhexyl)phtha	A	1378	22:58	BV	2.242	UG/L
20	2,6-dinitrotoluene	A	717	11:57	BB	0.542	UG/L
21	2,4-dinitrotoluene	A	785	13:05	BB	0.008	UG/L

Comments for Sample AD25947 - Analysis \$525

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 12-15-2001 Time: 11:25:23

The recovery for 1 of the 3 Surrogate Standards in this sample is below its acceptance range. Recoveries for 3 of the 18 compounds in the MDL and LCS Standards are outside of their acceptance ranges. Recoveries for 4 of the 18 compounds in the Spiked Sample are outside of their acceptance ranges. The level for bis(2-Ethylhexyl)phthalate in the Laboratory Blank is 1.2 ug/L.