


User: Bohlk, Ted
Westchester Dept. of Labs & Research
Date: 12/13/2001 Time: 18:24:39

Sample: AD26006
Analysis: \$525 Organic Chemicals - 525.2
Units: ug
Started: 11/1/01 18:15 Ended: 11/17/01 18:15 Analyst: TB
Result source: manual entry
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Hexachlorocyclopentadiene		< MDL		0.10
2	Hexachlorobenzene		< MDL		0.10
3	Simazine		< MDL		0.40
4	Atrazine		< MDL		0.20
5	Alachlor		< MDL		0.20
6	bis(2-Ethylhexyl)adipate		< MDL		0.60
7	bis(2-Ethylhexyl)phthalate		1.6		0.60
8	Benzo(a)pyrene		< MDL		0.20
9	EPTC		< MDL		1.0
10	2,6-Dinitrotoluene		< MDL		2.0
11	2,4-Dinitrotoluene		< MDL		2.0
12	Molinate		< MDL		0.90
13	Terbacil		< MDL		2.0
14	Acetochlor		< MDL		2.0
15	Metribuzin		< MDL		0.15
16	Metolachlor		< MDL		0.75
17	Butachlor		< MDL		0.40
18	4,4-DDE		< MDL		0.80
19	Surr_1,3-Dimethyl-2-nitrobenze		5.3		1.0
20	Surr_Triphenyl phosphate		5.5		1.0
21	Surr_Perylene-d12		3.3		1.0

Counted ok

Chromatogram Plot File: F:\26006H Date: Nov-18-1991 00:20:13
 Comment: BOHLK; METHOD 525; INST 204; 11/17/01; SAMPLE 26006
 Scan No: 1 Retention Time: 0:01 RIC: 0 Mass Range: 0 - 0
 Plotted: 1 to 1860 Range: 1 to 1860 100% = 6753442

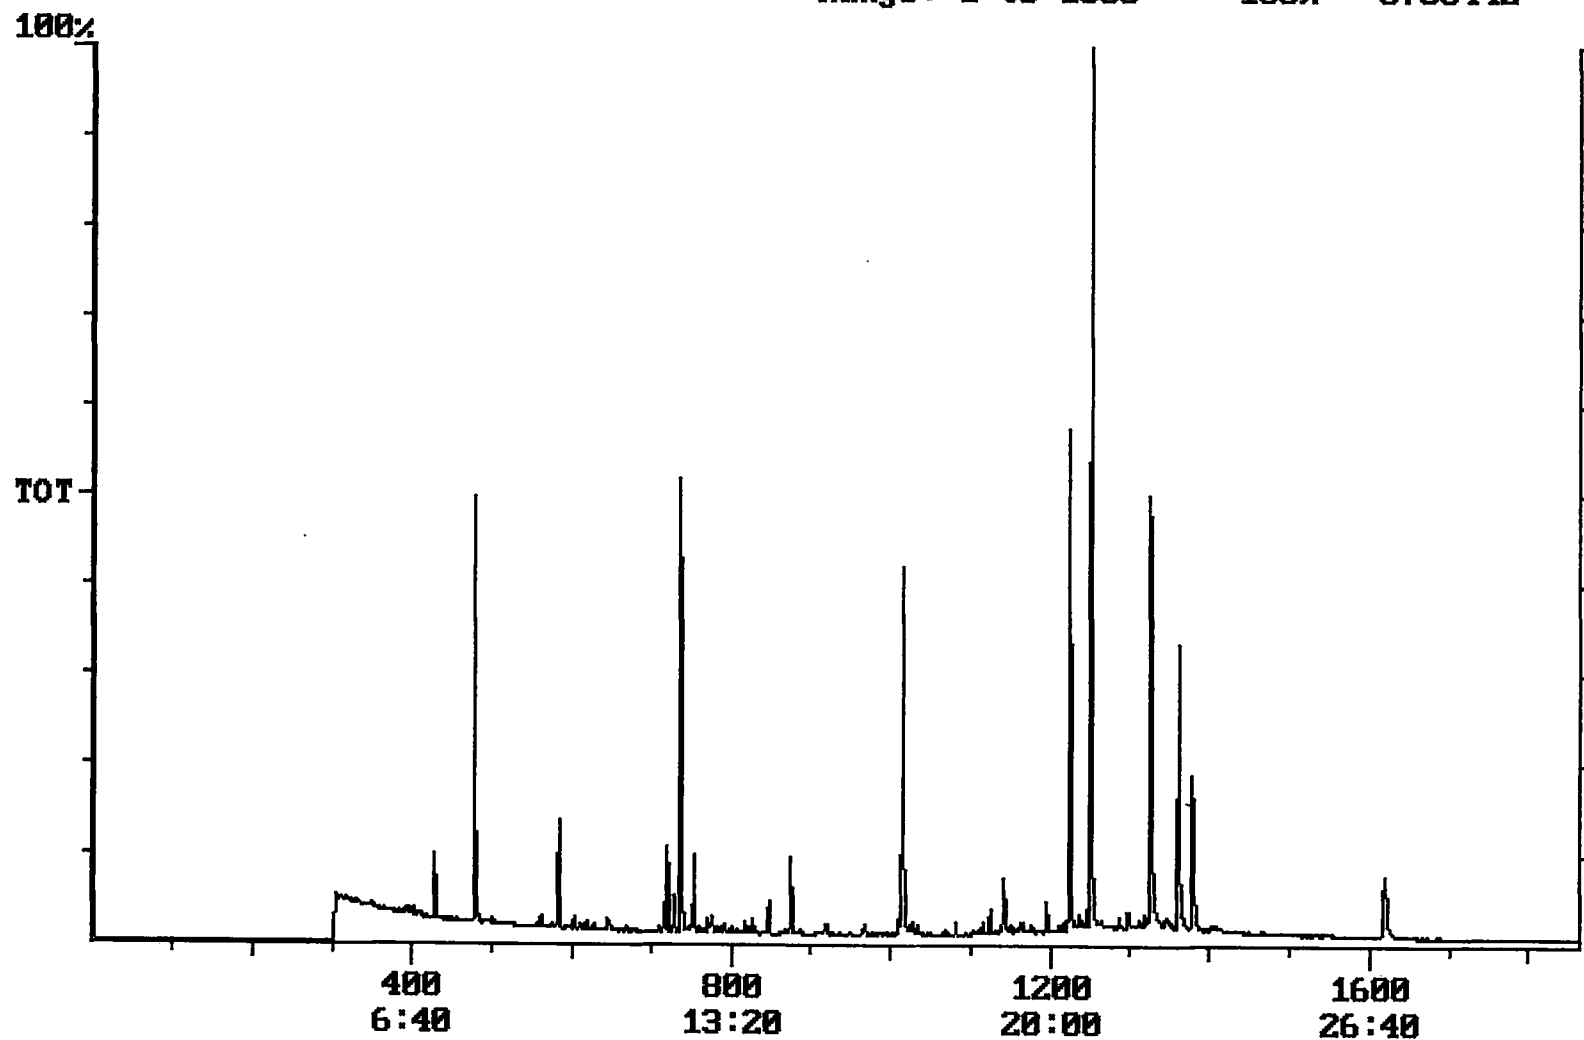

Integration Report

Quanfile: 26006H

Quan Entries: 15

Comment: BOHLK; METHOD 525; INST 204; 11/17/01; SAMPLE 26006

Sorted via: Entry Number ↑

No	Name of Compound	R Time	Scan#	Mode	Peak Area	Pk Height
1	acenaphthene d-10(IS)	12:17	737	Auto	1,421,757	763,617
2	phenanthrene d-10 (IS)	16:55	1015	Auto	2,396,900	929,035
3	chrysene d-12(IS)	22:41	1361	Auto	1,659,825	597,826
4	p-terphenyl d-14(IS)	20:50	1250	Auto	3,536,885	2,179,215
5	acenaphthene d-10(SURR)	12:17	737	Auto	1,421,757	763,617
6	phenanthrene d-10(SURR)	16:55	1015	Auto	2,396,900	929,035
7	chrysene d-12 (SURR)	22:41	1361	Auto	1,659,825	597,826
8	1,3-dimethyl-2-nitrobenzene	7:58	478	Auto	935,905	519,076
9	triphenyl phosphate (S)	22:05	1325	Auto	1,312,979	492,101
10	perylene d-12 (SURR)	26:59	1619	Auto	659,557	110,635
11	hexachlorocyclopentadiene	10:08	608	Auto	992	992
12	hexachlorobenzene	15:20	920	Auto	2,206	1,435
13	bis(2-ethylhexyl)adipate	21:58	1318	Auto	30,862	2,895
14	bis(2-ethylhexyl)phthalate	22:58	1378	Auto	1,002,676	334,821
15	2,6-dinitrotoluene	11:57	717	Auto	53,217	28,029

reversed IS/SURR's

Quantitation Report

Quanfile: 26006H

Quan Entries: 15

Comment: BOHLK; METHOD 525; INST 204; 11/17/01; SAMPLE 26006

Sorted via: Entry Number ↑

(S) = Standard

Cal	Name of Compound	S	Scan#	R Time	Me	Calc Amt(A)	Units
1	acenaphthene d-10(IS)	I	737	12:17	BB	5.000	UG/L
2	phenanthrene d-10 (IS)	I	1015	16:55	BV	5.000	UG/L
3	chrysene d-12(IS)	I	1361	22:41	BV	5.000	UG/L
4	p-terphenyl d-14(IS)	I	1250	20:50	BB	5.000	UG/L
5	acenaphthene d-10(SURR	A	737	12:17	BB	2.645	UG/L
6	phenanthrene d-10(SURR	A	1015	16:55	BV	2.908	UG/L
7	chrysene d-12 (SURR)	A	1361	22:41	BV	3.019	UG/L
8	1,3-dimethyl-2-nitrobe	A	478	7:58	BB	5.285	UG/L
9	triphenyl phosphate (S	A	1325	22:05	BB	5.518	UG/L
10	perylene d-12 (SURR)	A	1619	26:59	BB	3.293	UG/L
11	hexachlorocyclopentadi	A	608	10:08	BB	0.015	UG/L
12	hexachlorobenzene	A	920	15:20	BB	0.012	UG/L
16	bis(2-ethylhexyl)adipa	A	1318	21:58	MM	0.155	UG/L
17	bis(2-ethylhexyl)phtha	A	1378	22:58	BB	1.620	UG/L
20	2,6-dinitrotoluene	A	717	11:57	BB	0.580	UG/L

Comments for Sample AD26006 - Analysis \$525

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 12-15-2001 Time: 11:32:42

The recovery for 1 of the 3 Surrogate Standards in this sample is below its acceptance range. Recoveries for 3 of the 18 compounds in the MDL and LCS Standards are outside of their acceptance ranges. Recoveries for 4 of the 18 compounds in the Spiked Sample are outside of their acceptance ranges. The level for bis(2-Ethylhexyl)phthalate in the Laboratory Blank is 1.2 ug/L.