

DFTPP

Data File : C:\HPCHEM\1\DATA\NOV2001\DFTPP.D

Vial: 1

Acq On : 20 Nov 2001 12:35 pm

Operator: 209 GALOS

Sample :

Inst : GC/MS 209


Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)

Title : 209 625/TCLP calibration table

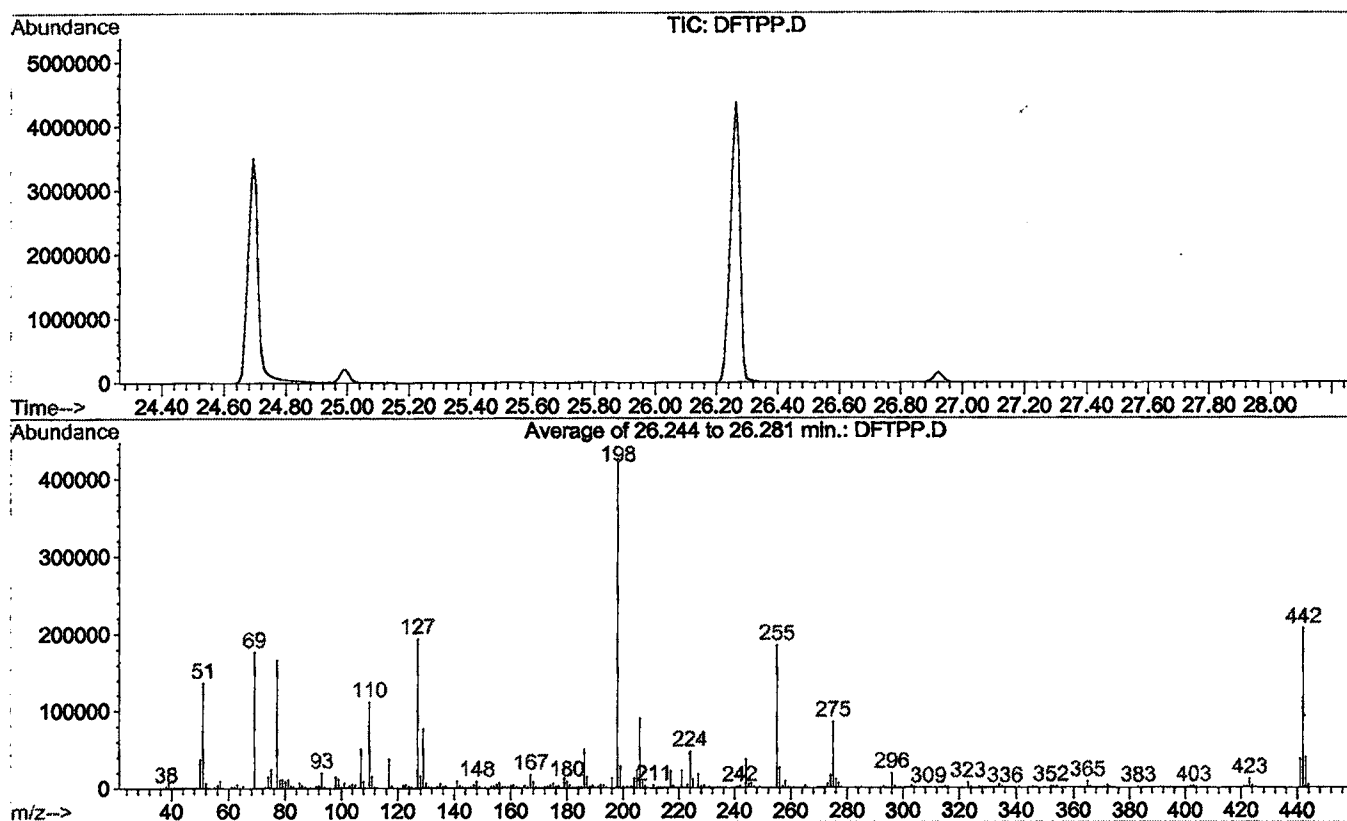

Spectrum Information: Average of 26.244 to 26.281 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	32.1	136810	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.6	176992	PASS
70	69	0.00	2	0.1	259	PASS
127	198	40	60	45.5	193813	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	425907	PASS
199	198	5	9	6.6	28067	PASS
275	198	10	30	20.1	85534	PASS
365	198	1	100	1.8	7837	PASS
441	443	0.01	100	94.9	37318	PASS
442	198	40	110	48.5	206709	PASS
443	442	17	23	19.0	39312	PASS

DFTPP.D NP103001.M

Mon Dec 10 14:59:44 2001

Page 1

GCMs^D

[illegible]

Analyst Cm/AD/mL
revision 4/12/01

Verified by _____

Reviewed by 07/11
Date 12/31

Sequence Name: C:\HPCHEM\1\SEQUENCE\NOV2001.S

Comment: INST 209; 30Mx0.25umX0.50

Operator: 209 GALOS

Data Path: C:\HPCHEM\1\data\nov2001\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch


☒ Full Method☒ Inject Anyway☐ Reprocessing Only☐ Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	NYCREF	NP103001	11/19 new ref 5ug/l
2	Sample	1	DFTPP	NP103001	
3	Sample	2	26009✓	NP103001	gc/ms unknown
4	Sample	3	26010✓	NP103001	gc/ms unknown
5	Sample	4	26011✓	NP103001	gc/ms unknown
6	Sample	5	25873✓	NP103001	gc/ms unknown
7	Sample	6	26078✓	NP103001	gc/ms unknown

DFTPP

Data File : C:\HPCHEM\1\DATA\NOV2101\DFTPP.D
 Acq On : 21 Nov 2001 11:32 am
 Sample :
 Misc :
 MS Integration Params: RTEINT.P
 Method : C:\HPCHEM\1\METHODS\NP103001.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

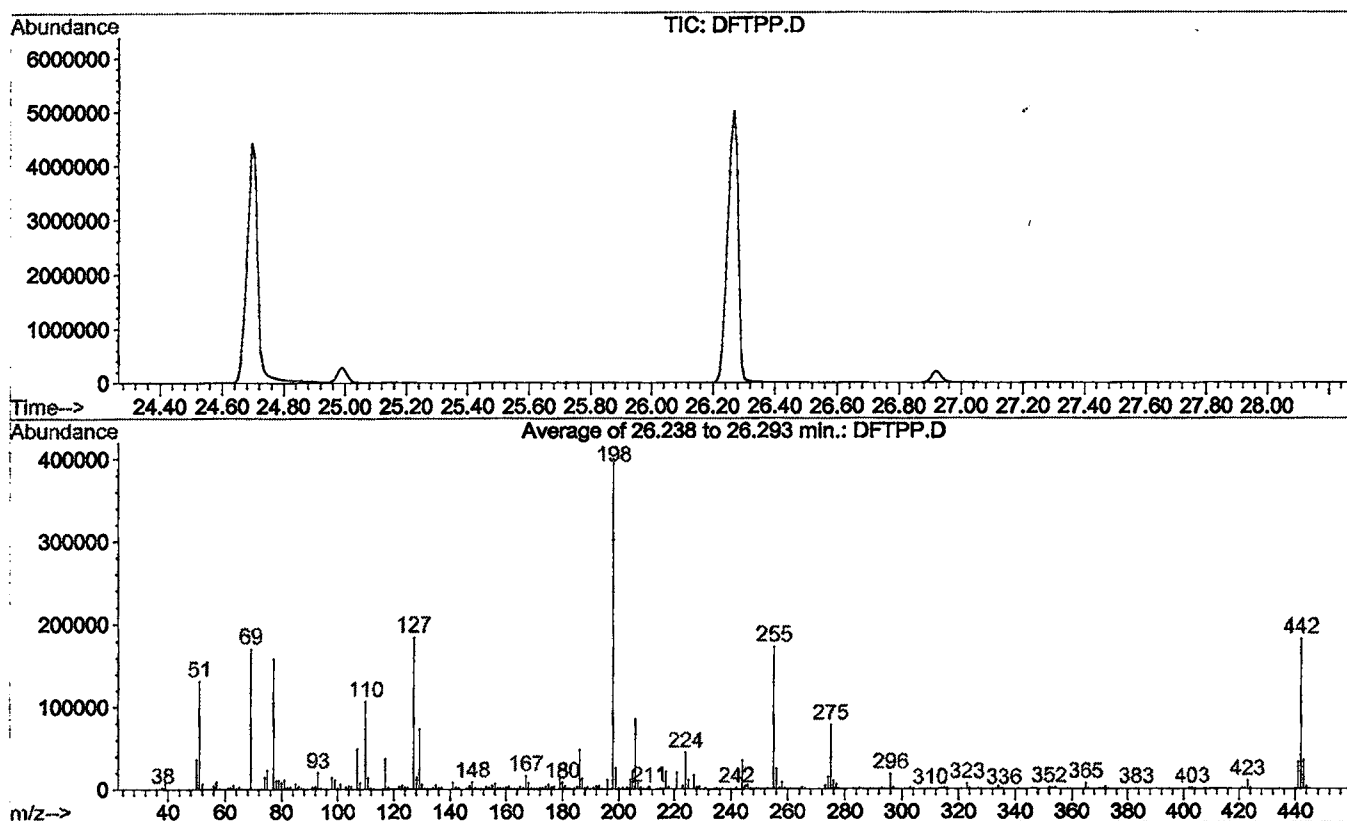

Spectrum Information: Average of 26.238 to 26.293 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	33.0	131821	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.8	171304	PASS
70	69	0.00	2	0.0	57	PASS
127	198	40	60	46.3	185221	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	399776	PASS
199	198	5	9	6.6	26517	PASS
275	198	10	30	19.5	78115	PASS
365	198	1	100	1.9	7446	PASS
441	443	0.01	100	94.0	32848	PASS
442	198	40	110	45.7	182586	PASS
443	442	17	23	19.1	34963	PASS