

Sequence Name: C:\HPCHEM\1\SEQUENCE\NOV3001.S
 Comment: INST 209; 30Mx0.25umX0.50
 Operator: 209 GALOS
 Data Path: C:\HPCHEM\1\data\nov3001\
 Pre-Seq Cmd:
 Post-Seq Cmd:

Method Sections To Run On A Barcode Mismatch
 (X) Full Method (X) Inject Anyway
 () Reprocessing Only () Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP1	GCMS1126	
2	Sample	3	CALI25A	GCMS1126	calib 25
3	Sample	32	28275A	GCMS1126	11/21 scan
4	Sample	49	28651	GCMS1126	11/23 scan
5	Sample	51	LBD	NP112601	lb 11/2 gc/ms
6	Sample	52	LBE	NP112601	lb 11/2 gc/ms
7	Sample	53	26079	NP112601	11/2 gc/ms
8	Sample	54	26707	NP112601	11/2 gc/ms
9	Sample	55	26208	NP112601	11/2 gc/ms
10	Sample	56	26206	NP112601	11/2 gc/ms
11	Sample	57	26251	NP112601	11/2 gc/ms
12	Sample	58	26080	NP112601	11/2 gc/ms
13	Sample	59	26133	NP112601	11/2 gc/ms
14	Sample	60	26163	NP112601	11/2 gc/ms
15	Sample	61	26164	NP112601	11/2 gc/ms
16	Sample	62	26165	NP112601	11/2 gc/ms
17	Sample	63	26127	NP112601	11/2 gc/ms
18	Sample	64	26132	NP112601	11/2 gc/ms
19	Sample	65	26128	NP112601	11/2 gc/ms
20	Sample	66	26129	NP112601	11/2 gc/ms
21	Sample	67	26130	NP112601	11/2 gc/ms
22	Sample	1	DFTPP2	GCMS1126	
23	Sample	68	26205	NP112601	11/2 gc/ms
24	Sample	69	26204	NP112601	11/2 gc/ms
25	Sample	70	26131	NP112601	11/2 gc/ms
26	Sample	71	26202	NP112601	11/2 gc/ms
27	Sample	2	CALI40	GCMS1126	
28	Sample	3	LBF	GCMS1126	lb 11/24
29	Sample	4	28267	GCMS1126	gcms 11/24
30	Sample	5	28694	GCMS1126	gcms 11/24
31	Sample	6	28688	GCMS1126	gcms 11/24
32	Sample	7	28471	GCMS1126	gcms 11/24
33	Sample	8	28693	GCMS1126	gcms 11/24
34	Sample	9	28669	GCMS1126	gcms 11/24
35	Sample	10	28695	GCMS1126	gcms 11/24
36	Sample	11	28691	GCMS1126	gcms 11/24
37	Sample	12	28430	GCMS1126	gcms 11/24
38	Sample	13	28677	GCMS1126	gcms 11/24
39	Sample	14	28689	GCMS1126	gcms 11/24
40	Sample	15	28662	GCMS1126	gcms 11/24
41	Sample	16	28678	GCMS1126	gcms 11/24
42	Sample	17	28663	GCMS1126	gcms 11/24
43	Sample	18	28664	GCMS1126	gcms 11/24

Sequence Name: C:\HPCHEM\1\SEQUENCE\NOV3001.S

Line Type	Vial	DataFile	Method	Sample Name
44 Sample	19 2869A	GCMS1126	gcms	11/24
45 Sample	20 2869B	GCMS1126	gcms	11/24
46 Sample	21 REF	GCMS1126	gcms	11/24

DFTPP

Data File : C:\HPCHEM\1\DATA\NOV3001\DFTPP1.D

Acq On : 30 Nov 2001 11:46 am

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP112601.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

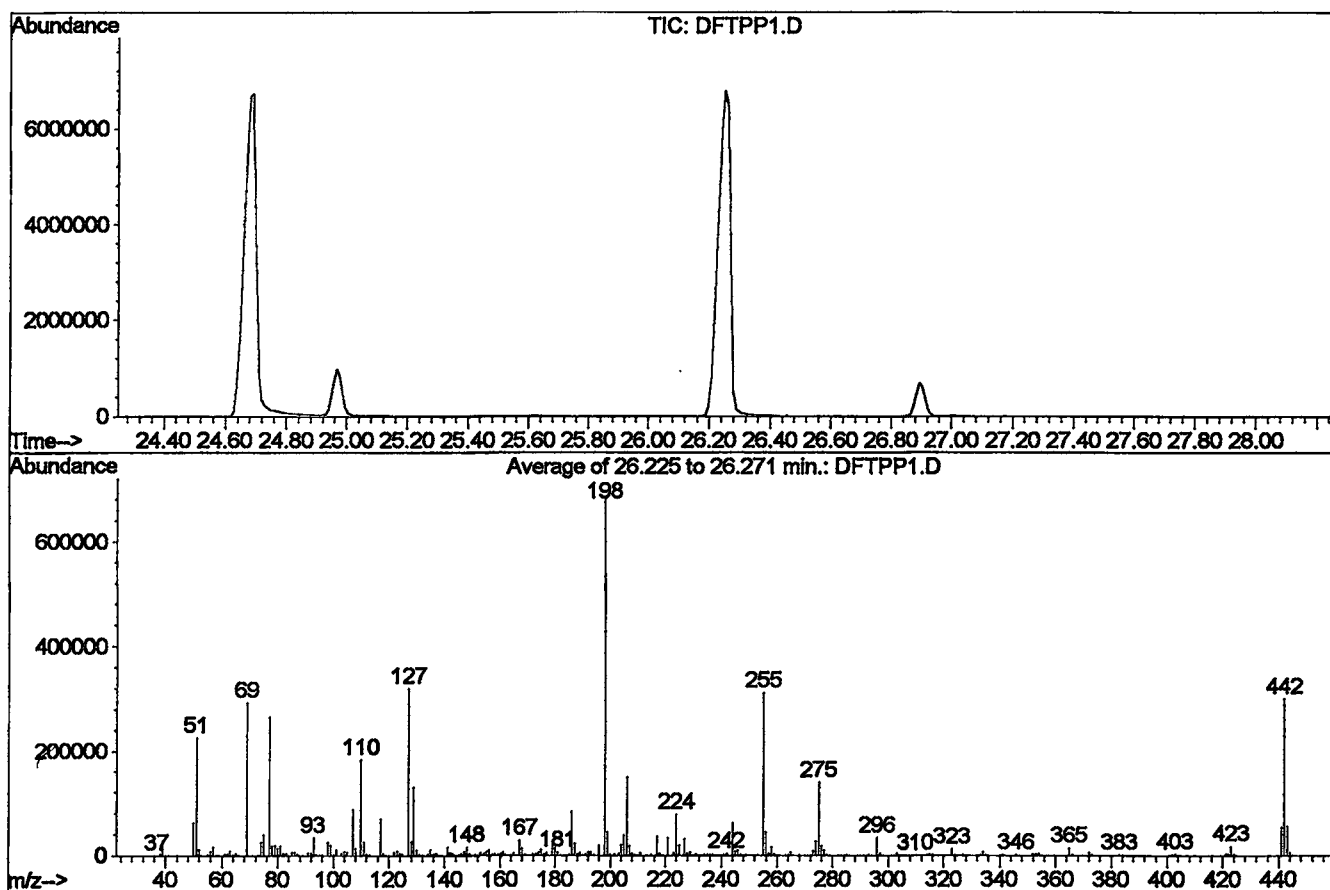

Spectrum Information: Average of 26.225 to 26.271 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	33.0	226344	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.7	292767	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	46.6	319531	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	685472	PASS
199	198	5	9	6.7	45641	PASS
275	198	10	30	20.5	140344	PASS
365	198	1	100	2.1	14410	PASS
441	443	0.01	100	94.5	54483	PASS
442	198	40	110	43.7	299499	PASS
443	442	17	23	19.2	57635	PASS