

Method

508

Date Extracted

11/3/01

Page

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
	LB ✓	500m		1m			2m		7			
	CAO Net				1m							
	Pest Net											
	Tox Net											
26252	spr CAO											
26252	spr Dup CAO											
26253	spr Pest											
26253	spr Dup Pest											
26315	spr Tox											
26315	spr Dup Tox											
	26252 ✓											
	26253 ✓											
	26315 ✓											
	26316 ✓											
	26317 ✓											
	26318 ✓											
	26319 -											
	26320 ✓											
	26321 ✓											
*	26333											
Remarks												
* Is it a NYC Sample												
Reviewed by.												
2/19/02												
drip rate must be between 5-15 ml/min for liq-liq extractors												
drip rate -												
Extraction type - Septum												
Solv. lot# V42 E17												
NaCl lot# V11599												
Na2SO4 lot# V32603												
STANDARD	INT STD LOG#											
CALIBRATION												
REF/SPIKE	1992	20626	1993									
MDL/MDRF												
Q. CHECK												
INT. STD.												
SURROGATE	18396											
LPC												
ENDRIN/DDT												

Analyst

C.M.

revision 4/12/01

Verified by

Reviewed by

Date

Sequence Name: C:\HPCHEM\1\SEQUENCE\NOV3001.S

Comment: 208

Operator: GALOS

Data Path: C:\HPCHEM\1\DATA\nov3001\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch

(X) Full Method

(X) Inject Anyway

() Reprocessing Only

() Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
------	------	------	----------	--------	-------------

1	Sample	1	DFTPP	NP112701	
2	Sample	2	LB	NP112701	lb 11/3
3	Sample	3	26393	NP112701	gc/ms unknown 11/3
4	Sample	4	26390	NP112701	gc/ms unknown 11/3
5	Sample	5	26392	NP112701	gc/ms unknown 11/3
6	Sample	6	26389	NP112701	gc/ms unknown 11/3
7	Sample	7	26391	NP112701	gc/ms unknown 11/3
8	Sample	8	26474	NP112701	gc/ms unknown 11/3
9	Sample	9	26473	NP112701	gc/ms unknown 11/3
10	Sample	10	26472	NP112701	gc/ms unknown 11/3
11	Sample	11	26471	NP112701	gc/ms unknown 11/3
12	Sample	12	26386	NP112701	gc/ms unknown 11/3
13	Sample	13	26387	NP112701	gc/ms unknown 11/3
14	Sample	14	26388	NP112701	gc/ms unknown 11/3
15	Sample	15	LBA	NP112701	lb 11/5
16	Sample	16	26317	NP112701	gc/ms unknown 11/3
17	Sample	17	26355	NP112701	gc/ms unknown 11/3
18	Sample	18	26252	NP112701	gc/ms unknown 11/3
19	Sample	19	26320	NP112701	gc/ms unknown 11/3
20	Sample	20	26394	NP112701	gc/ms unknown 11/3
21	Sample	21	26433	NP112701	gc/ms unknown 11/3
22	Sample	22	26434	NP112701	gc/ms unknown 11/3
23	Sample	23	26470	NP112701	gc/ms unknown 11/3
24	Sample	24	26315	NP112701	gc/ms unknown 11/3
25	Sample	25	26337	NP112701	gc/ms unknown 11/3
26	Sample	26	26203	NP112701	gc/ms unknown 11/3 reext
27	Sample	27	26316	NP112701	gc/ms unknown 11/3
28	Sample	28	26318	NP112701	gc/ms unknown 11/3
29	Sample	29	26333	NP112701	gc/ms unknown 11/3
30	Sample	30	26336	NP112701	gc/ms unknown 11/3
31	Sample	31	26321	NP112701	gc/ms unknown 11/3
32	Sample	32	26253	NP112701	gc/ms unknown 11/3 +26319

DFTPP

Data File : C:\HPCHEM\1\DATA\NOV3001\DFTPP.D

Acq On : 30 Nov 2001 8:10 am

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)


Title : 208 625/TCLP calibration table

Vial: 1

Operator: GALOS

Inst : GC/MS Ins

Multiplr: 1.00

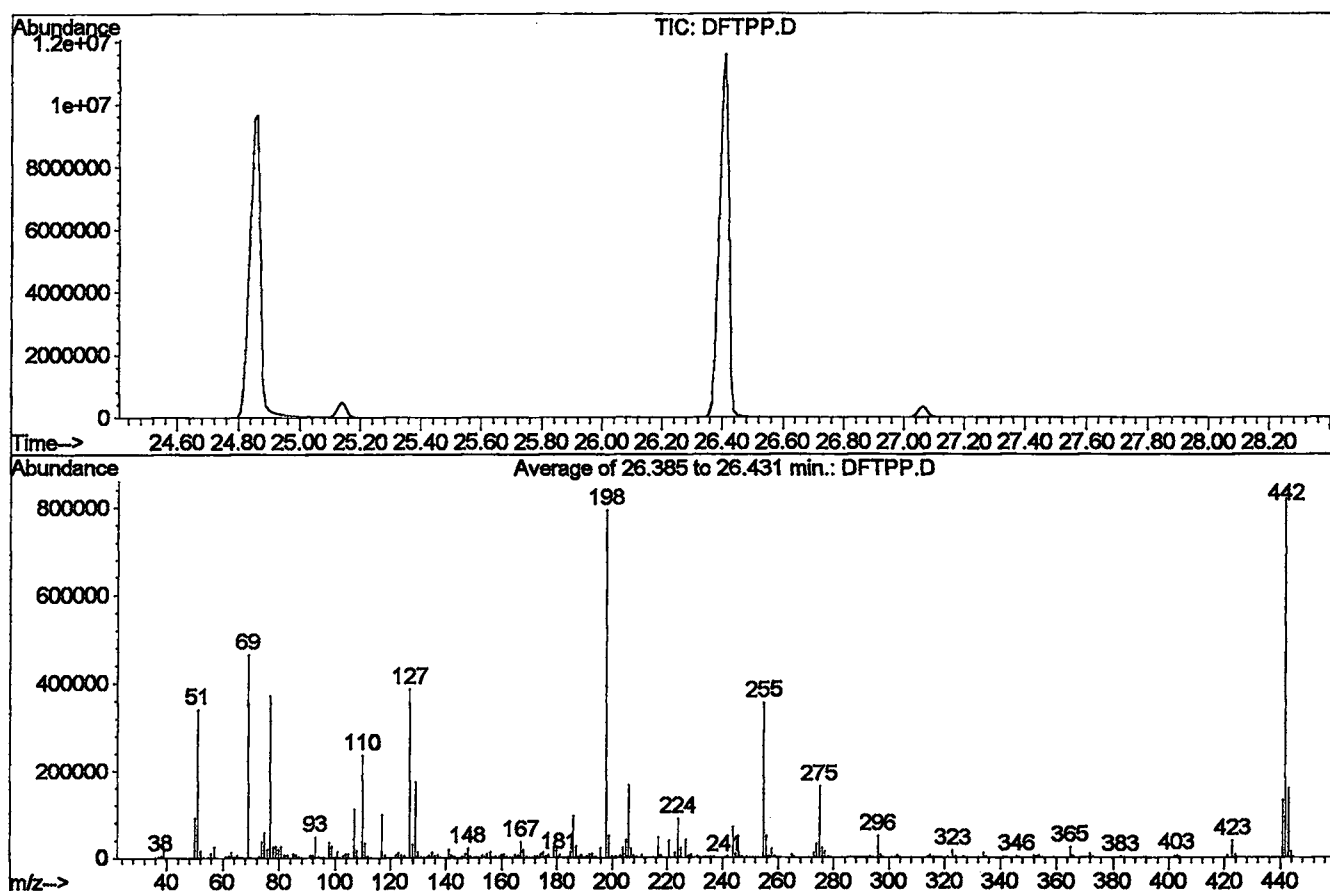

Spectrum Information: Average of 26.385 to 26.431 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	42.9	340988	PASS
68	69	0.00	2	0.0	108	PASS
69	198	0.00	100	58.7	466187	PASS
70	69	0.00	2	0.4	1766	PASS
127	198	40	60	48.8	387268	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	794315	PASS
199	198	5	9	6.5	51786	PASS
275	198	10	30	20.5	162656	PASS
365	198	1	99	3.0	23964	PASS
441	443	1	99	83.1	131785	PASS
442	198	40	110	103.3	820491	PASS
443	442	17	23	19.3	158596	PASS