

Method 308 CCMS Date Extracted 11/5/01 Page

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
	Lab Blue/soot			1ml			2ml					
	Ref 10xaph											
	Ref Pat + chlor											
	P21 122											
	26203 ✓									1		
	26335 ✓									2		
	26336 ✓									3		
	26337 ✓									4		
	26386 ✓									5		
	26387 ✓									6		
	26388 ✓									7		
	26389 ✓									8		
	26390 ✓									9		
	26391 ✓									10		
	Spike Chlor + dmp			1ml								
	Spike 10x + dmp											
	Spike Peot + dmp											
	26392 ✓									1		
	26393 ✓									2		
	26394 ✓									3		
	26433 ✓									4		
	26434 ✓									5		
	26470 ✓									6		
	26471 ✓									7		
	26472 ✓									8		
	26473 ✓									9		
	26474 ✓									10		
Remarks												
26203 re extracted												
Reviewed by, <u>CB 2/14/02</u>												
drip rate must be between 5-15 ml/min for liq-liq extractors												
drip rate -												
Extraction type -		Solv. lot#		NaCl lot#		Na2SO4 lot#						
STANDARD	INT STD LOG#											
CALIBRATION												
REF/SPIKE												
MDL/MDRF												
Q. CHECK												
INT. STD.												
SURROGATE												
LPC												
ENDRIN/DDT												

Analyst CM/BD/ML
revision 4/12/01

Verified by

Reviewed by
Date 12/10/11

DFTPP

Data File : C:\HPCHEM\1\DATA\NOV3001\DFTPP.D

Acq On : 30 Nov 2001 8:10 am

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)


Title : 208 625/TCLP calibration table

Vial: 1

Operator: GALOS

Inst : GC/MS Ins

Multiplr: 1.00

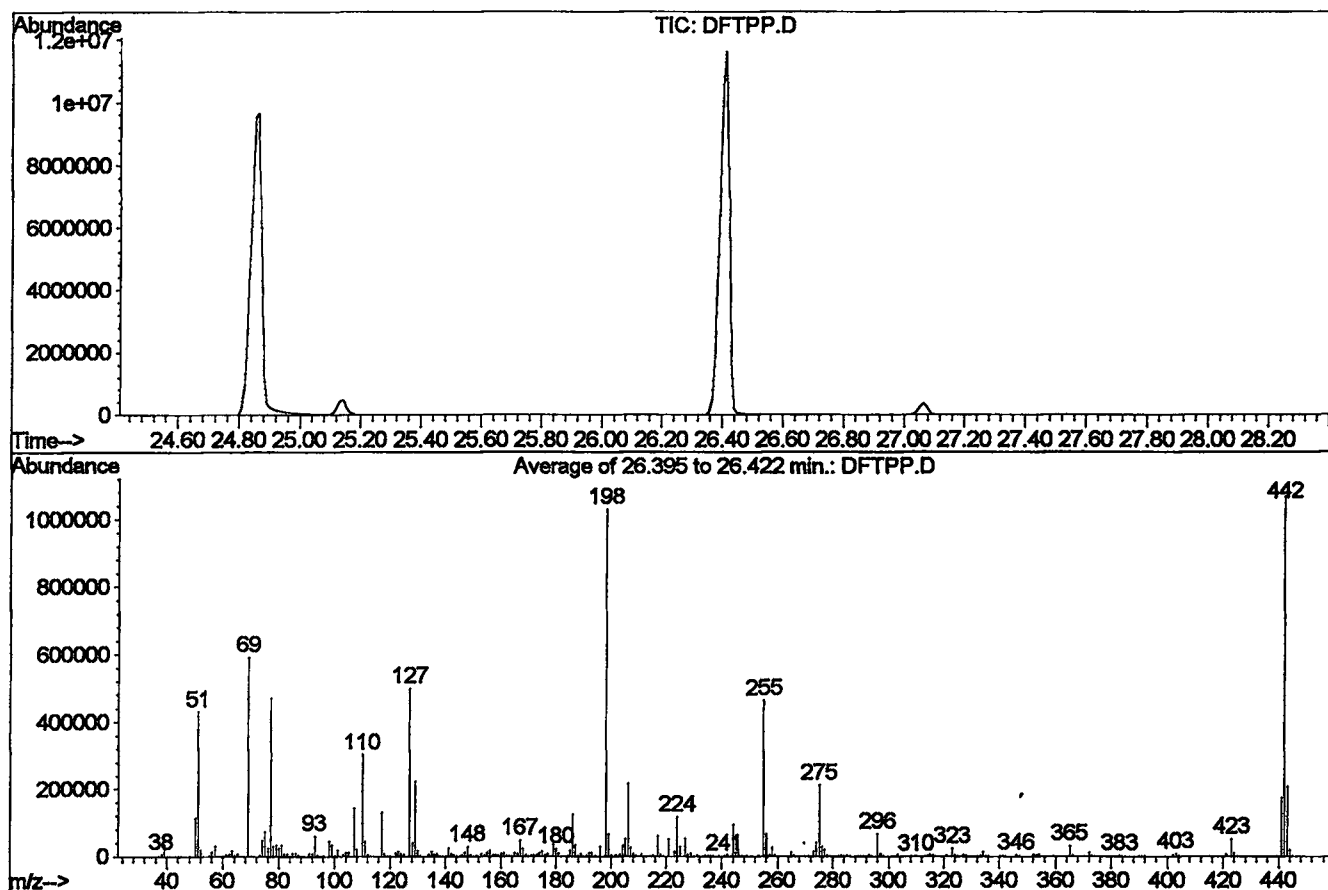

Spectrum Information: Average of 26.395 to 26.422 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	41.9	431552	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	57.5	592752	PASS
70	69	0.00	2	0.4	2260	PASS
127	198	40	60	48.5	499632	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	1030256	PASS
199	198	5	9	6.5	66662	PASS
275	198	10	30	20.6	212432	PASS
365	198	1	99	3.1	31782	PASS
441	443	1	99	83.5	172760	PASS
442	198	40	110	103.7	1068048	PASS
443	442	17	23	19.4	206814	PASS

DFTPP.D NP112701.M

Tue Dec 04 14:58:47 2001