

Method 508 GEMS Date Extracted 11/6/01Page

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH = 7	Count
✓	LAB BLANK	50mL	✓	1mL			2mL			
	Ref ChL + Pest									
	Ref Tox									
	PKL 1232									
26530	S ChL				1mL					
26532	SD ChL									
26533	S Tox									
26533	SD Tox									
26536	S Pest									
26536	SD Pest									
✓	26475-									1
✓	26476-									2
✓	26477									3
✓	26478									4
✓	26532-									5
✓	26533-									6
✓	26534									7
✓	26535									8
✓	26536									9
✓	26537									10
Remarks										
Reviewed by, <i>[Signature]</i> 2/19/02										
drip rate must be between 5-15 ml/min for liq-liq extractors										
drip rate -										
Extraction type - <u>See funnel</u> Solv. lot# <u>V42E17</u> NaCl lot# <u>V11599</u> Na2SO4 lot# <u>V32603</u>										
STANDARD	INT STD LOG#									
CALIBRATION										
REF/SPIKE	<u>Tox: 1992</u>	<u>ChL: 1993</u>	<u>Pest: 2006</u>							
MDL/MDRF										
Q. CHECK										
INT. STD.										
SURROGATE	<u>1839b</u>									
LPC										
ENDRIN/DDT										

Analyst ML/AD
revision 4/12/01Verified by Reviewed by [Signature]
Date 12/16/01

Sequence Name: C:\HPCHEM\1\SEQUENCE\DEC0601.S

Comment: 208

Operator: GALOS

Data Path: C:\HPCHEM\1\DATA\dec0701\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch

☒ Full Method☒ Inject Anyway☐ Reprocessing Only☐ Don't Inject

Line Type	Vial	DataFile	Method	Sample Name
1 Sample	1	DFTPP	NP112701	
2 Sample	34	27010	NP112701	gc/ms unknown
3 Sample	2	LB	NP112701	gc/ms unknown 11/6
4 Sample	3	26478	NP112701	gc/ms unknown 11/6
5 Sample	4	26537	NP112701	gc/ms unknown 11/6
6 Sample	5	26475	NP112701	gc/ms unknown 11/6
7 Sample	6	26476	NP112701	gc/ms unknown 11/6
8 Sample	7	26533	NP112701	gc/ms unknown 11/6
9 Sample	8	26532	NP112701	gc/ms unknown 11/6
10 Sample	9	26534	NP112701	gc/ms unknown 11/6
11 Sample	10	26535	NP112701	gc/ms unknown 11/6
12 Sample	11	26536	NP112701	gc/ms unknown 11/6
13 Sample	12	LBB	NP112701	gc/ms unknown 11/13
14 Sample	13	27545	NP112701	gc/ms unknown 11/13
15 Sample	14	27116	NP112701	gc/ms unknown 11/13
16 Sample	15	26830	NP112701	gc/ms unknown 11/13
17 Sample	16	27190	NP112701	gc/ms unknown 11/13
18 Sample	17	27191	NP112701	gc/ms unknown 11/13
19 Sample	18	27117	NP112701	gc/ms unknown 11/13
20 Sample	19	27118	NP112701	gc/ms unknown 11/13
21 Sample	20	27142	NP112701	gc/ms unknown 11/13
22 Sample	21	27141	NP112701	gc/ms unknown 11/13
23 Sample	22	27141A	NP112701	gc/ms unknown 11/13
24 Sample	23	27188	NP112701	gc/ms unknown 11/13
25 Sample	24	27115	NP112701	gc/ms unknown 11/13
26 Sample	25	27143	NP112701	gc/ms unknown 11/13
27 Sample	26	27114	NP112701	gc/ms unknown 11/13
28 Sample	27	27146	NP112701	gc/ms unknown 11/13
29 Sample	28	27140	NP112701	gc/ms unknown 11/13
30 Sample	29	27189	NP112701	gc/ms unknown 11/13
31 Sample	30	27192	NP112701	gc/ms unknown 11/13
32 Sample	31	27490	NP112701	gc/ms unknown 11/13
33 Sample	32	27491	NP112701	gc/ms unknown 11/13
34 Sample	33	27491A	NP112701	gc/ms unknown 11/13
35 Sample	35	27390	NP112701	gc/ms unknown 11/13
36 Sample	36	27391	NP112701	gc/ms unknown 11/13
37 Sample	37	27393	NP112701	gc/ms unknown 11/13
38 Sample	38	27392	NP112701	gc/ms unknown 11/13
39 Sample	39	27394	NP112701	gc/ms unknown 11/13
40 Sample	40	27395	NP112701	gc/ms unknown 11/13

*do
inject on
12/20/01*

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC0701\DFTPP.D

Vial: 1

Acq On : 7 Dec 2001 5:12 pm

Operator: GALOS

Sample :

Inst : GC/MS Ins


Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)

Title : 208 625/TCLP calibration table

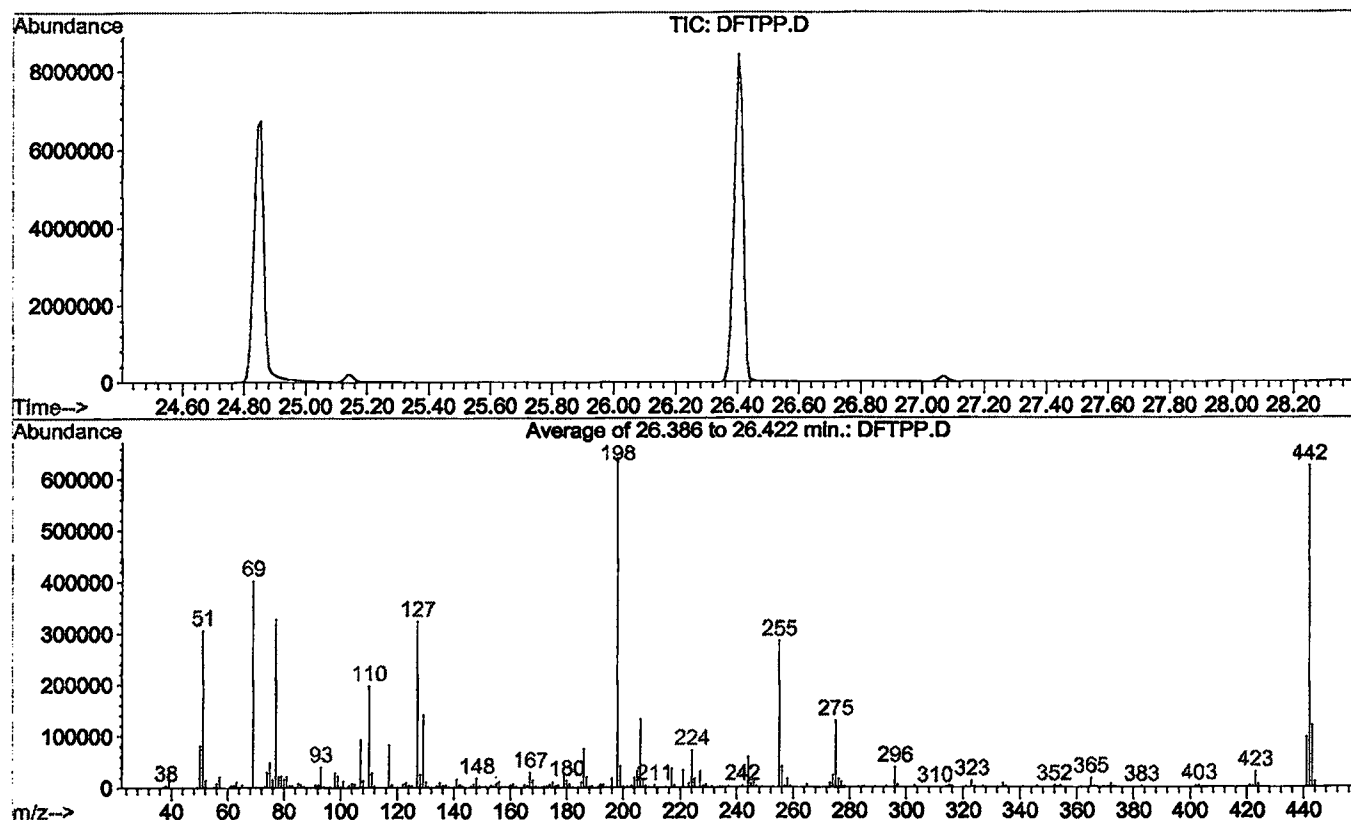

Spectrum Information: Average of 26.386 to 26.422 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	47.8	306971	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	62.8	403187	PASS
70	69	0.00	2	0.4	1624	PASS
127	198	40	60	50.3	323034	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	641907	PASS
199	198	5	9	6.5	42021	PASS
275	198	10	30	20.2	129642	PASS
365	198	1	99	2.8	18020	PASS
441	443	1	99	81.0	97307	PASS
442	198	40 ⁵⁰	110	97.5 ✓	625549	PASS
443	442	17	23	19.2	120126	PASS

DFTPP.D NP112701.M

Mon Dec 10 09:25:21 2001